

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082221\
 Data File : PL069370.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2021 07:45
 Operator : AR\AJ
 Sample : M3468-07
 Misc :
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SAMPLE-2-(161.00)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 09:08:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 21 02:23:37 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.634	5.568	8830694	26759419	19.140	18.680
28)	SA Decachlor...	10.402	11.491	8596332	16414393	12.736	13.393
Target Compounds							
7)	B delta-BHC	0.000	7.043f	0	2713150	N.D.	1.469 #
10)	B gamma-Chl...	0.000	8.295	0	2785465	N.D.	1.811 #
13)	MA Dieldrin	7.735f	0.000	1021726	0	1.683	N.D. #
25)	Chlordane-3	0.000	8.295	0	2785465	N.D.	13.007 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082221\
Data File : PL069370.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2021 07:45
Operator : AR\AJ
Sample : M3468-07
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SAMPLE-2-(161.00)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 09:08:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
Quant Title : GC Extractables
QLast Update : Sat Aug 21 02:23:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

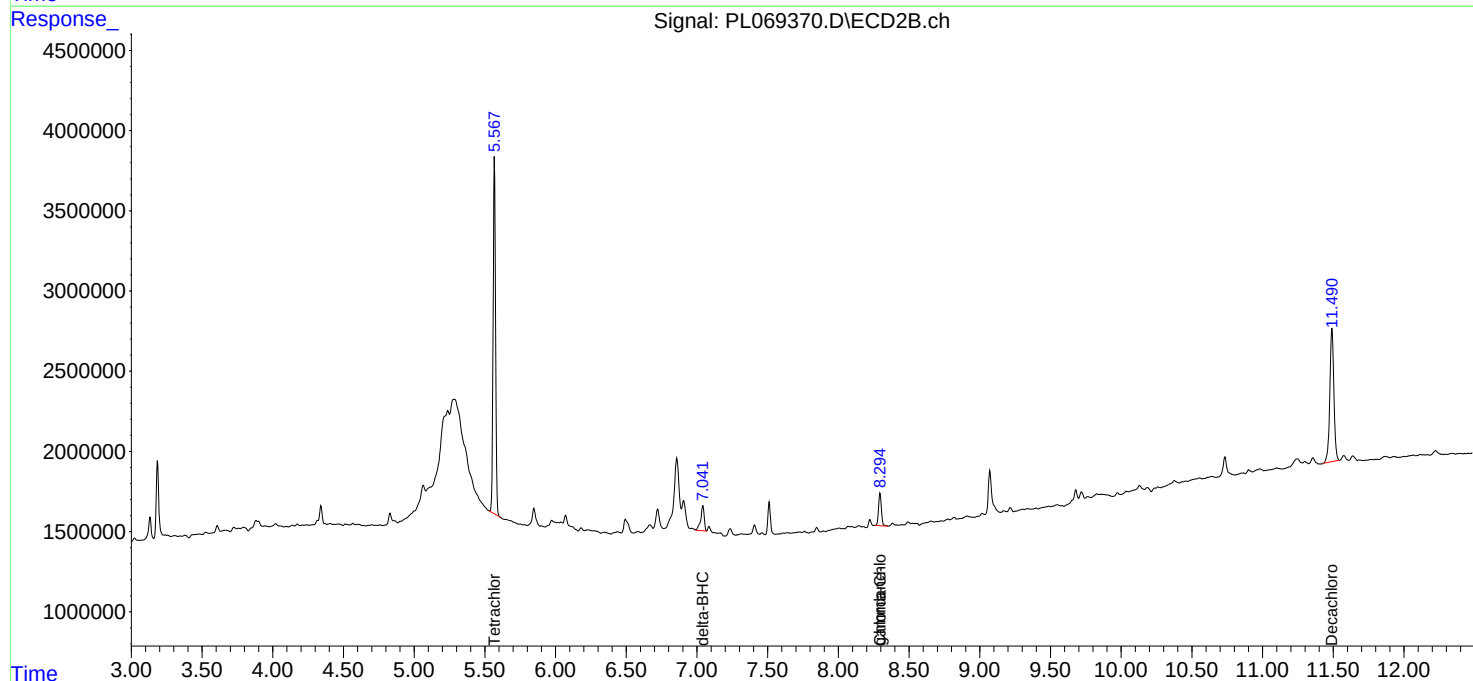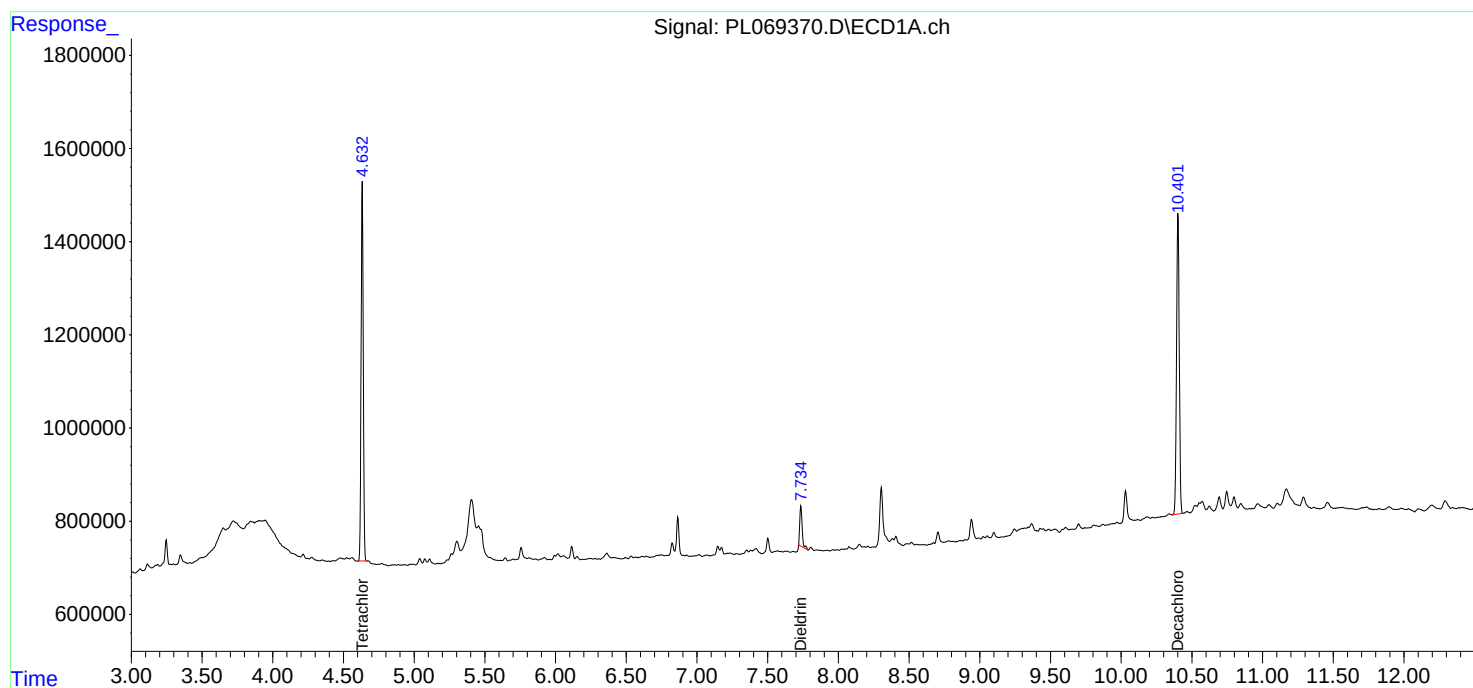


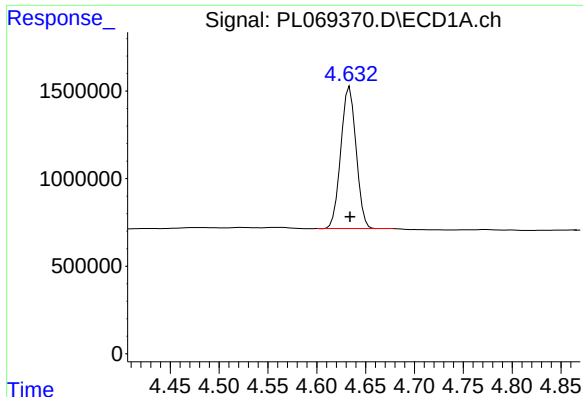

#1 Tetrachloro-m-xylene


R.T.: 4.634 min
Delta R.T.: 0.000 min
Response: 8830694
Conc: 19.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
SAMPLE-2-(161.00)

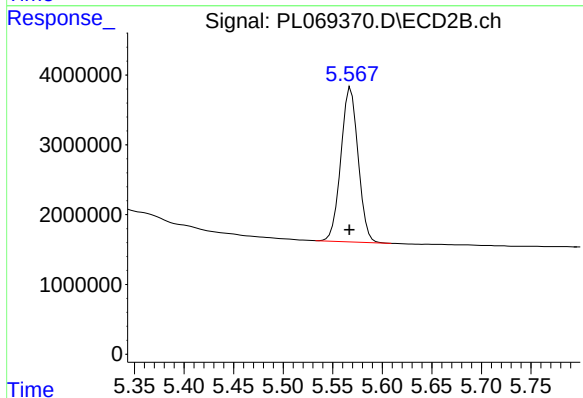


#1 Tetrachloro-m-xylene

R.T.: 5.568 min
Delta R.T.: 0.001 min
Response: 26759419
Conc: 18.68 ng/ml

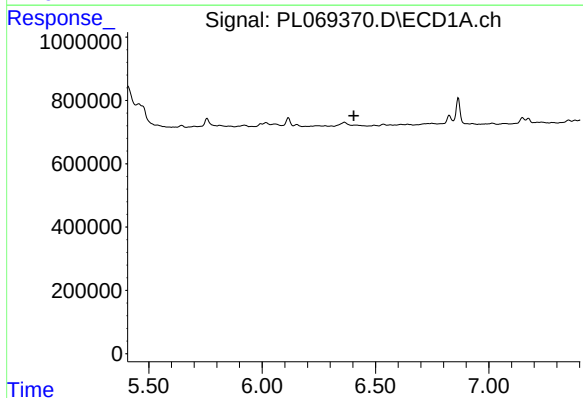


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.404 min
Response: 0
Conc: N.D.

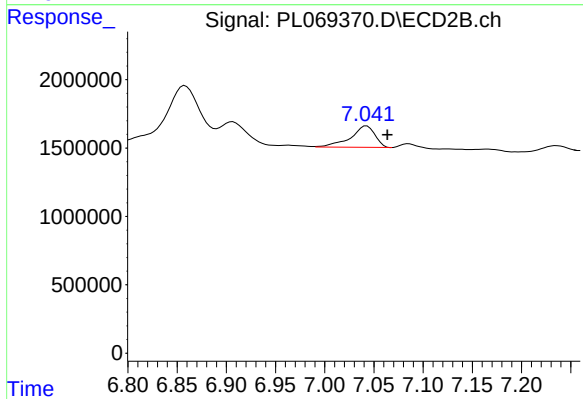

#7 delta-BHC


R.T.: 7.043 min
Delta R.T.: -0.021 min
Response: 2713150
Conc: 1.47 ng/ml

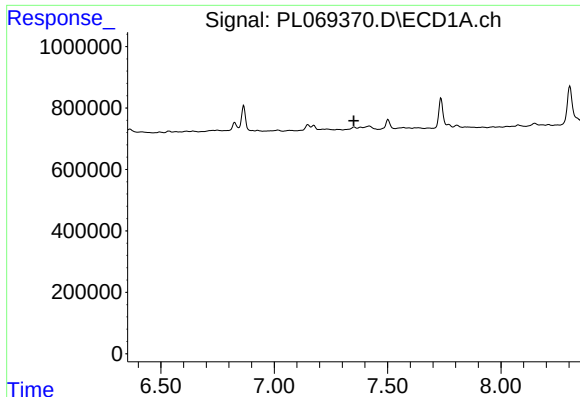

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.352 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SAMPLE-2-(161.00)

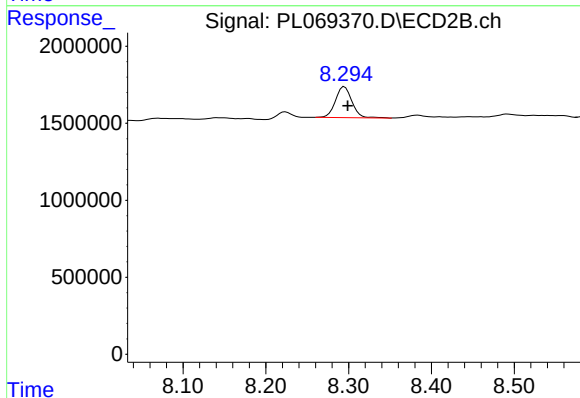


#10 gamma-Chlordane

R.T.: 8.295 min
Delta R.T.: -0.004 min
Response: 2785465
Conc: 1.81 ng/ml

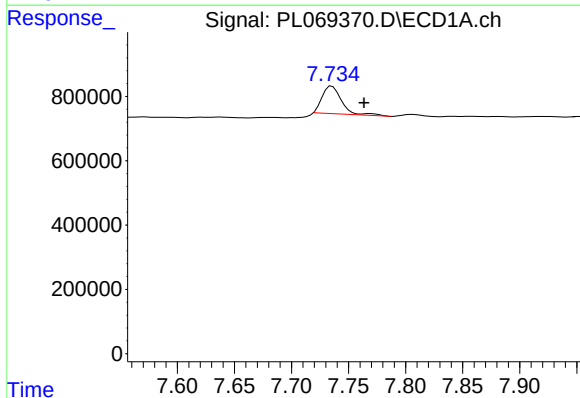


#13 Dieldrin

R.T.: 7.735 min
Delta R.T.: -0.028 min
Response: 1021726
Conc: 1.68 ng/ml

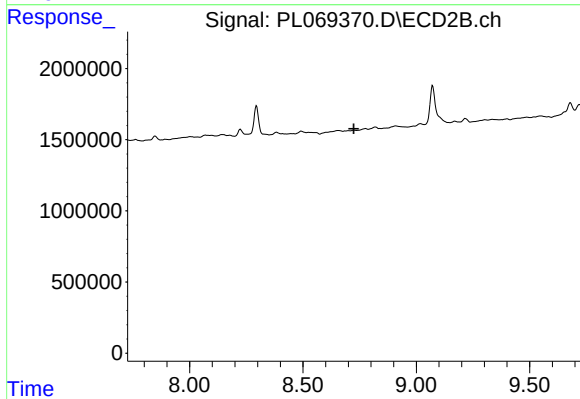

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 8.725 min
Response: 0
Conc: N.D.

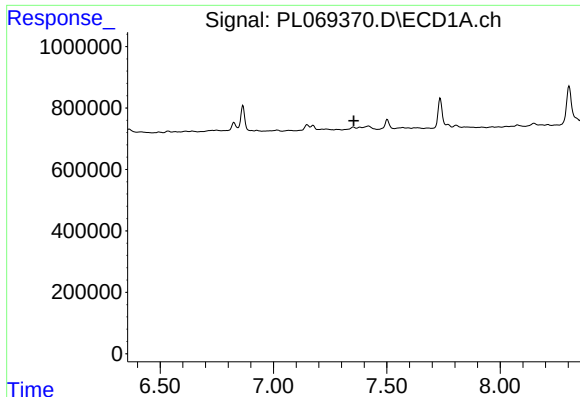

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.354 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SAMPLE-2-(161.00)

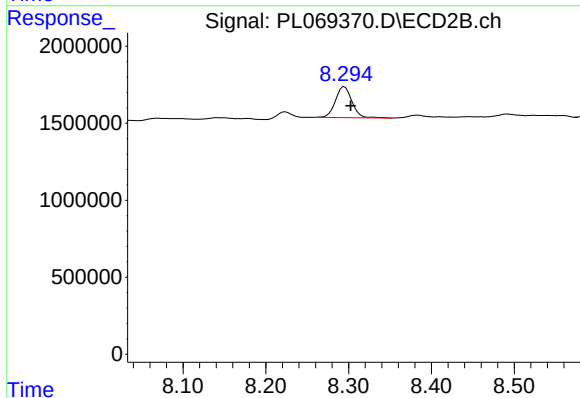


#25 Chlordane-3

R.T.: 8.295 min
Delta R.T.: -0.008 min
Response: 2785465
Conc: 13.01 ng/ml

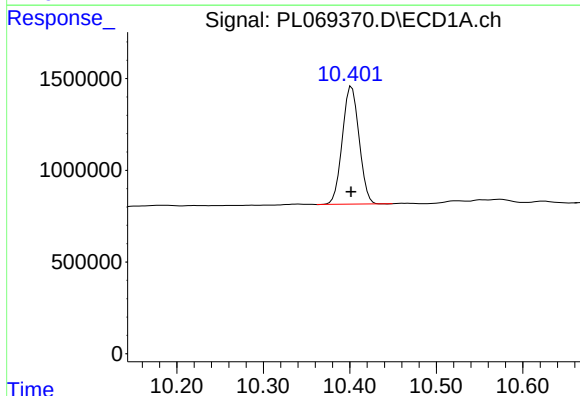

#28 Decachlorobiphenyl

R.T.: 10.402 min
Delta R.T.: 0.000 min
Response: 8596332
Conc: 12.74 ng/ml

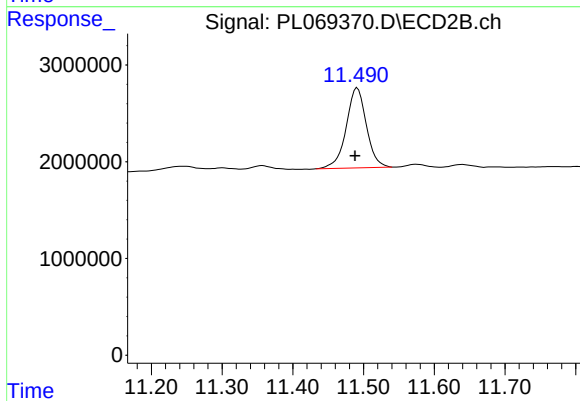

#28 Decachlorobiphenyl

R.T.: 11.491 min
Delta R.T.: 0.003 min
Response: 16414393
Conc: 13.39 ng/ml