

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082221\
 Data File : PL069373.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2021 08:35
 Operator : AR\AJ
 Sample : M3468-10
 Misc :
 ALS Vial : 78 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SAMPLE-5-(184.50)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 09:09:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 21 02:23:37 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.634	5.586f	8490236	24511259	18.402	17.111
28)	SA Decachlor...	10.403	11.509f	11236726	18766439	16.648	15.312
Target Compounds							
7)	B delta-BHC	0.000	7.061	0	4207489	N.D.	2.278 #
10)	B gamma-Chl...	0.000	8.312	0	1118387	N.D.	0.727 #
16)	A 4,4'-DDD	0.000	9.090f	0	4769612	N.D.	3.888 #
20)	A Methoxychlor	0.000	9.883f	0	1863885	N.D.	2.903 #
25)	Chlordane-3	0.000	8.312	0	1118387	N.D.	5.223 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082221\
Data File : PL069373.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2021 08:35
Operator : AR\AJ
Sample : M3468-10
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SAMPLE-5-(184.50)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 09:09:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
Quant Title : GC Extractables
QLast Update : Sat Aug 21 02:23:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

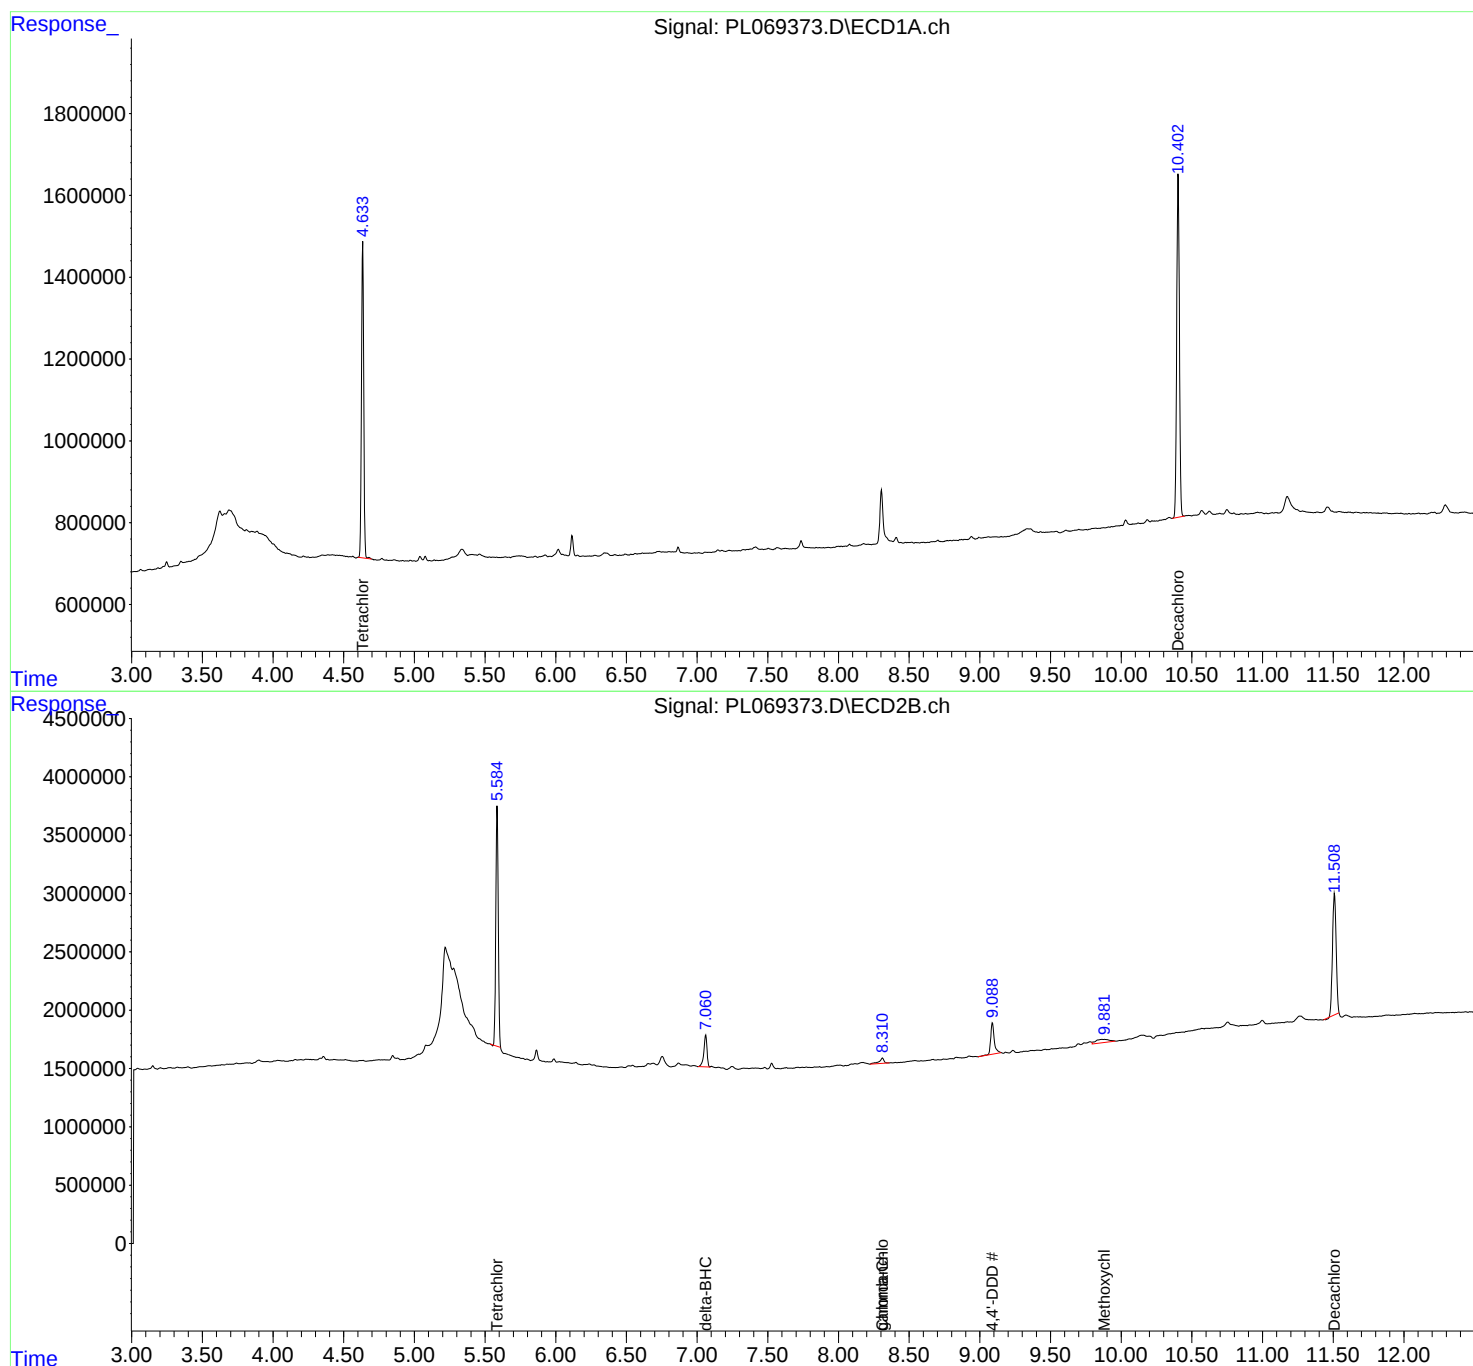


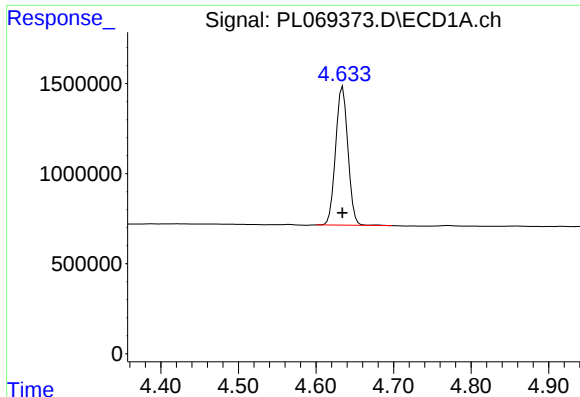

#1 Tetrachloro-m-xylene


R.T.: 4.634 min
Delta R.T.: 0.000 min
Response: 8490236
Conc: 18.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
SAMPLE-5-(184.50)

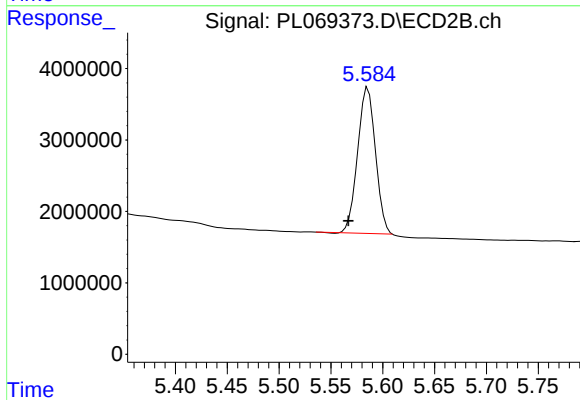


#1 Tetrachloro-m-xylene

R.T.: 5.586 min
Delta R.T.: 0.019 min
Response: 24511259
Conc: 17.11 ng/ml

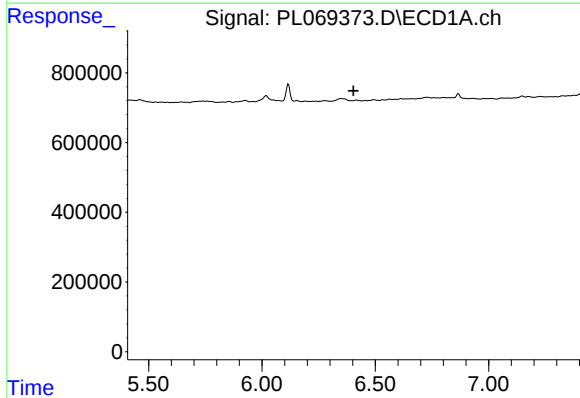


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.404 min
Response: 0
Conc: N.D.

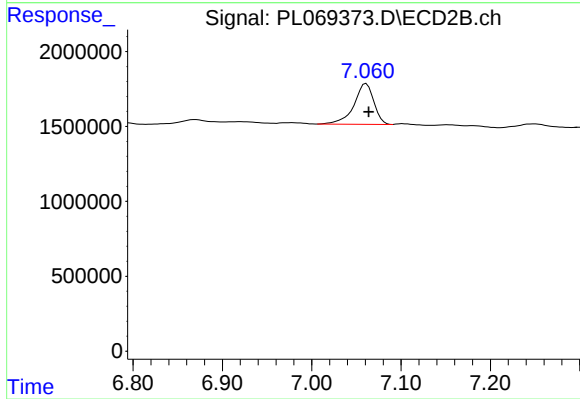

#7 delta-BHC


R.T.: 7.061 min
Delta R.T.: -0.003 min
Response: 4207489
Conc: 2.28 ng/ml

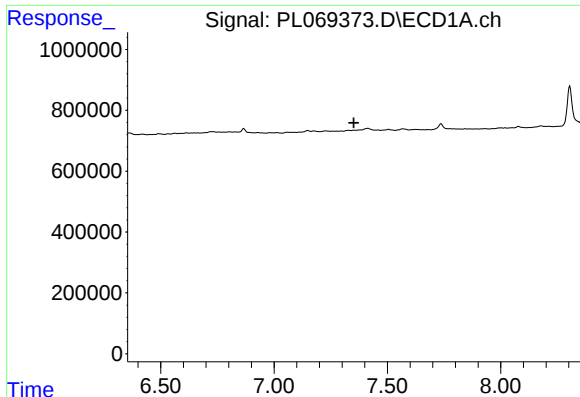

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.352 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SAMPLE-5-(184.50)

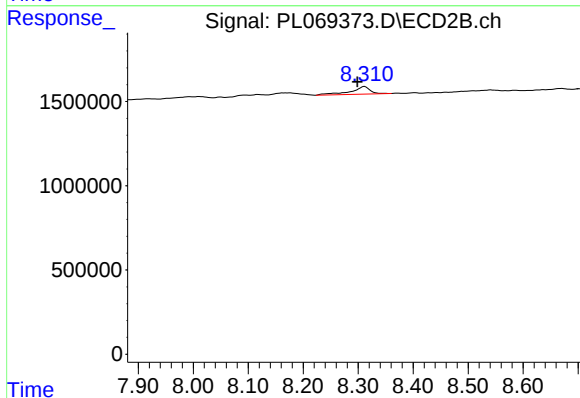


#10 gamma-Chlordane

R.T.: 8.312 min
Delta R.T.: 0.013 min
Response: 1118387
Conc: 0.73 ng/ml

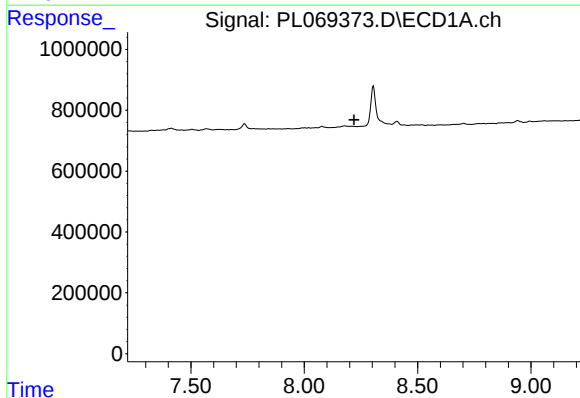


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.220 min
Response: 0
Conc: N.D.

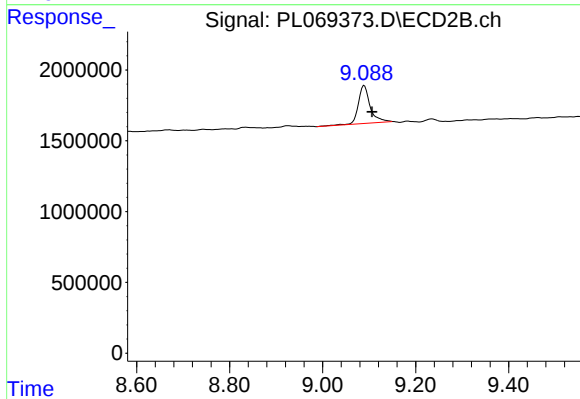

#16 4,4'-DDD


R.T.: 9.090 min
Delta R.T.: -0.017 min
Response: 4769612
Conc: 3.89 ng/ml

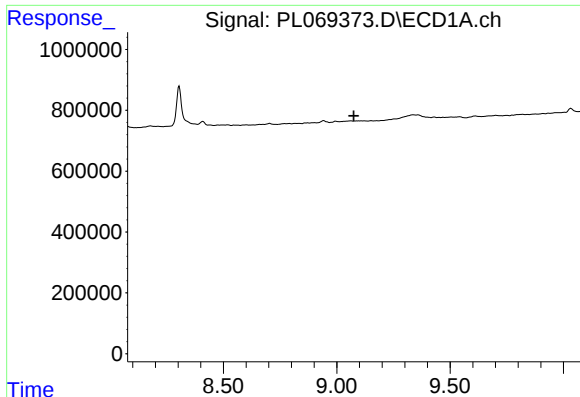

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 9.075 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SAMPLE-5-(184.50)

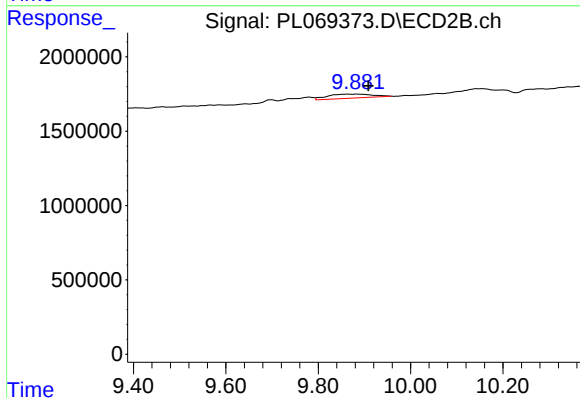


#20 Methoxychlor

R.T.: 9.883 min
Delta R.T.: -0.026 min
Response: 1863885
Conc: 2.90 ng/ml

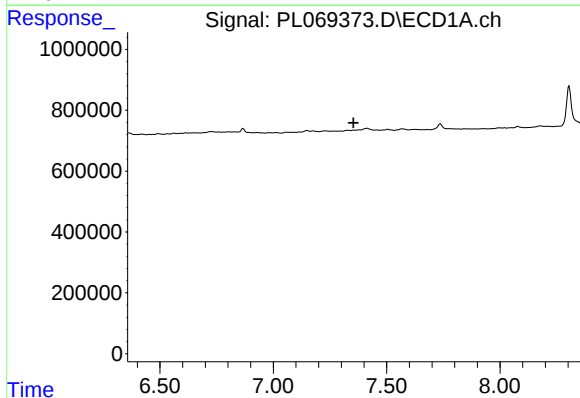


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.354 min
Response: 0
Conc: N.D.

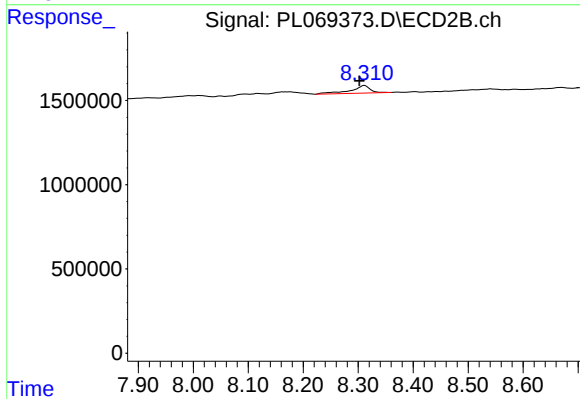

#25 Chlordane-3


R.T.: 8.312 min
Delta R.T.: 0.009 min
Response: 1118387
Conc: 5.22 ng/ml

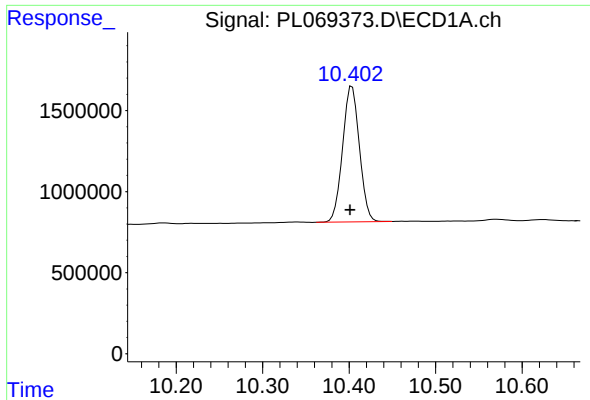

#28 Decachlorobiphenyl

R.T.: 10.403 min
Delta R.T.: 0.002 min
Response: 11236726
Conc: 16.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
SAMPLE-5-(184.50)

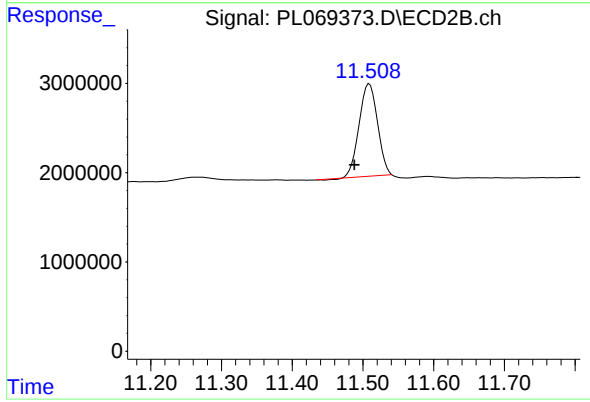

#28 Decachlorobiphenyl

R.T.: 11.509 min
Delta R.T.: 0.021 min
Response: 18766439
Conc: 15.31 ng/ml