

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082221\
 Data File : PL069376.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2021 09:25
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 12:25:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 21 02:23:37 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.633	5.567	11647556	34684662	25.245	24.213
28)	SA Decachlor...	10.402	11.491	16148806	28908951	23.926	23.588
Target Compounds							
4)	MA Heptachlor	6.150f	0.000	831870	0	1.201	N.D. #
7)	B delta-BHC	0.000	7.036f	0	4575368	N.D.	2.477 #
8)	B Heptachlo...	0.000	8.036	0	1583265	N.D.	1.053 #
10)	B gamma-Chl...	0.000	8.284	0	893309	N.D.	0.581 #
14)	MA Endrin	8.077f	0.000	826708	0	1.431	N.D. #
25)	Chlordane-3	0.000	8.284f	0	893309	N.D.	4.171 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082221\
Data File : PL069376.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2021 09:25
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 12:25:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
Quant Title : GC Extractables
QLast Update : Sat Aug 21 02:23:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

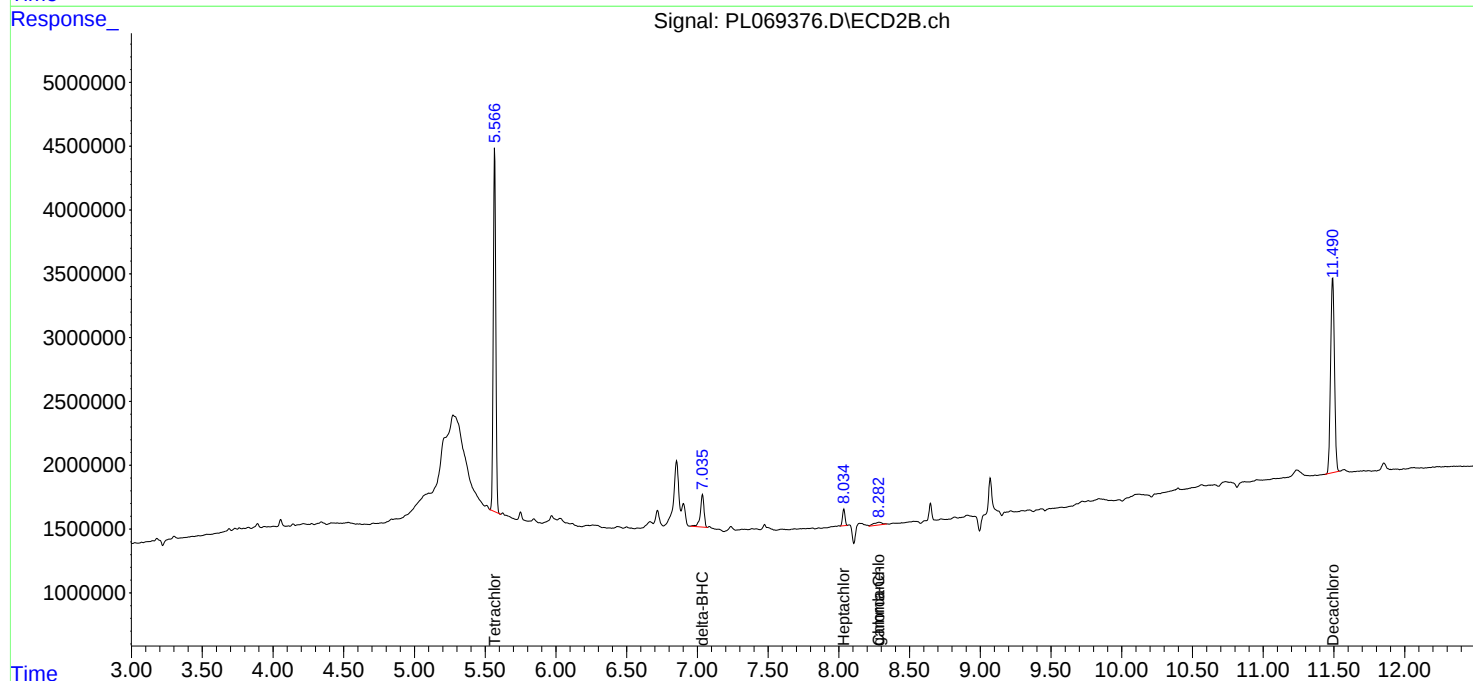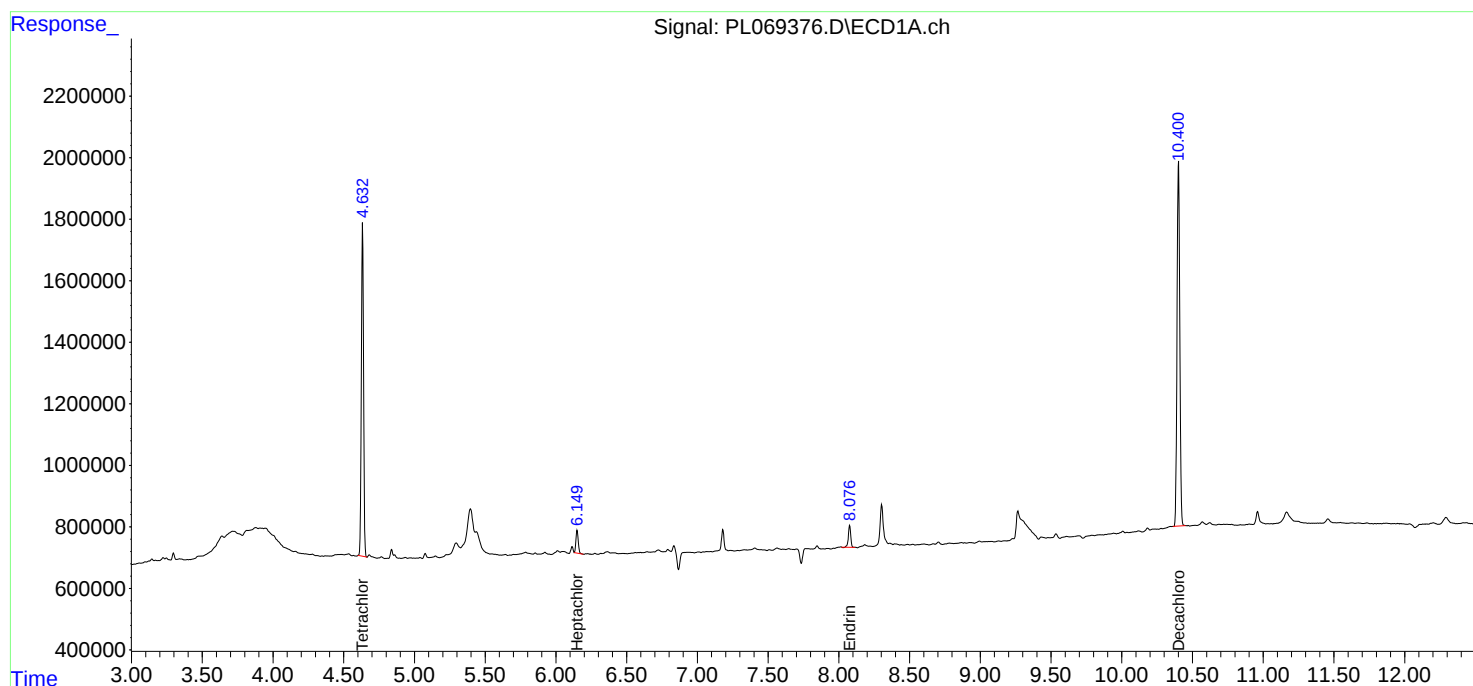


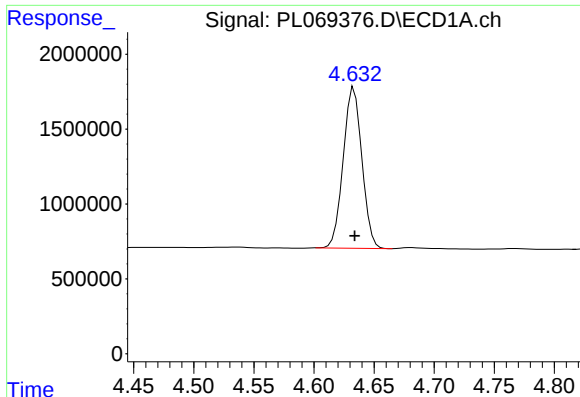

#1 Tetrachloro-m-xylene


R.T.: 4.633 min
Delta R.T.: 0.000 min
Response: 11647556
Conc: 25.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

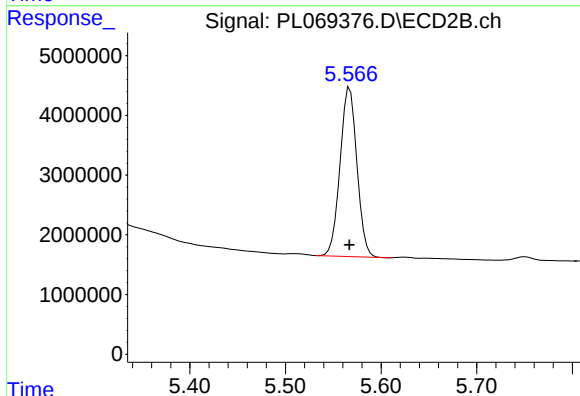


#1 Tetrachloro-m-xylene

R.T.: 5.567 min
Delta R.T.: 0.000 min
Response: 34684662
Conc: 24.21 ng/ml

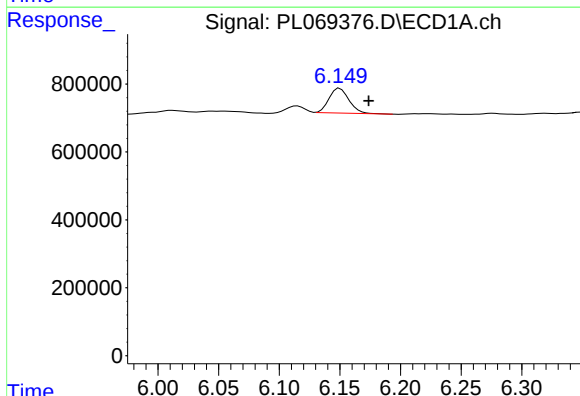


#4 Heptachlor

R.T.: 6.150 min
Delta R.T.: -0.024 min
Response: 831870
Conc: 1.20 ng/ml

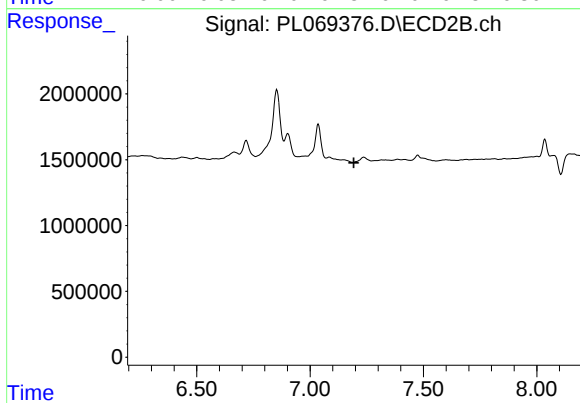

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 7.193 min
Response: 0
Conc: N.D.

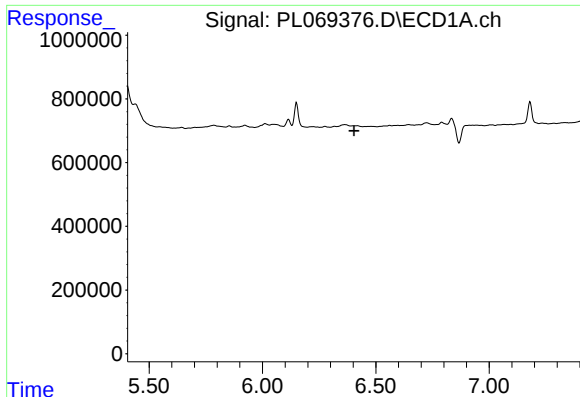

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.404 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

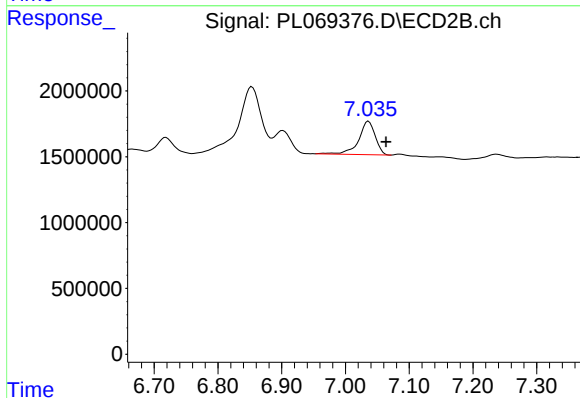


#7 delta-BHC

R.T.: 7.036 min
Delta R.T.: -0.028 min
Response: 4575368
Conc: 2.48 ng/ml

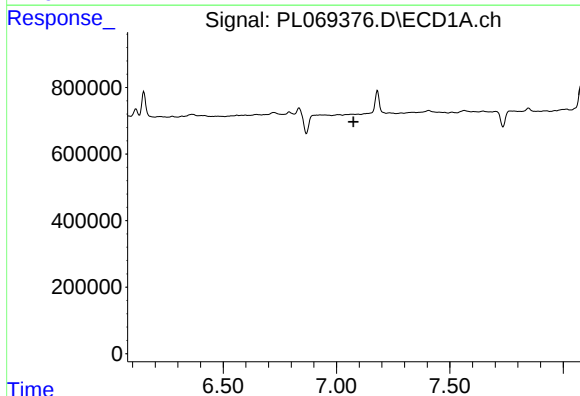


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 7.075 min
Response: 0
Conc: N.D.

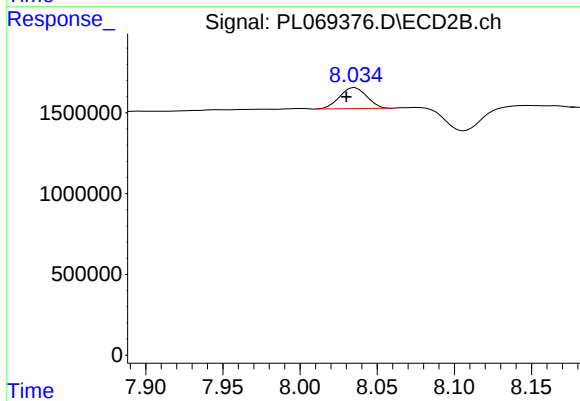

#8 Heptachlor epoxide


R.T.: 8.036 min
Delta R.T.: 0.006 min
Response: 1583265
Conc: 1.05 ng/ml

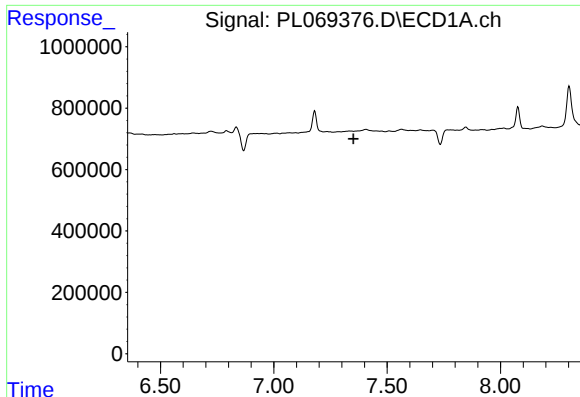

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.352 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

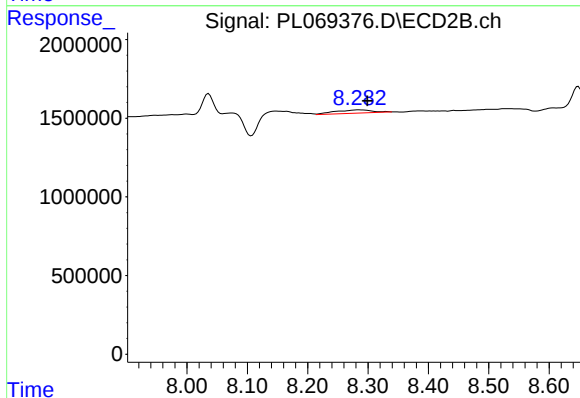


#10 gamma-Chlordane

R.T.: 8.284 min
Delta R.T.: -0.015 min
Response: 893309
Conc: 0.58 ng/ml

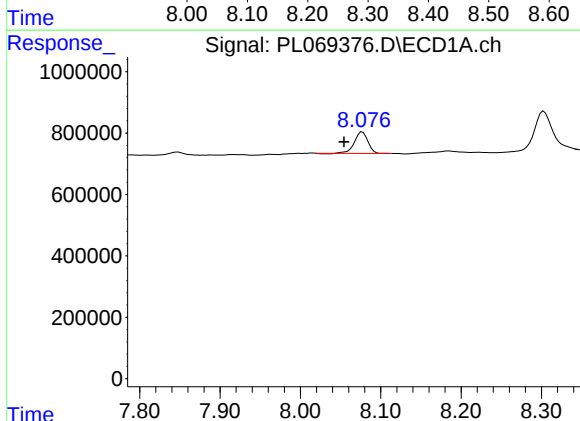


#14 Endrin

R.T.: 8.077 min
Delta R.T.: 0.023 min
Response: 826708
Conc: 1.43 ng/ml

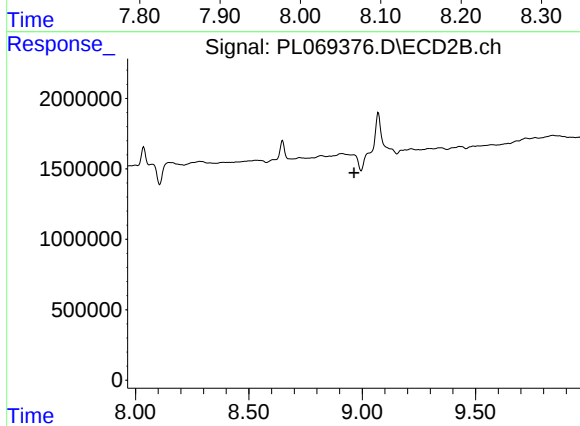

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 8.964 min
Response: 0
Conc: N.D.

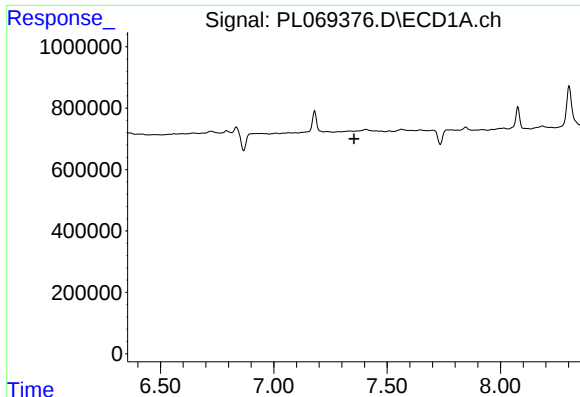

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.354 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

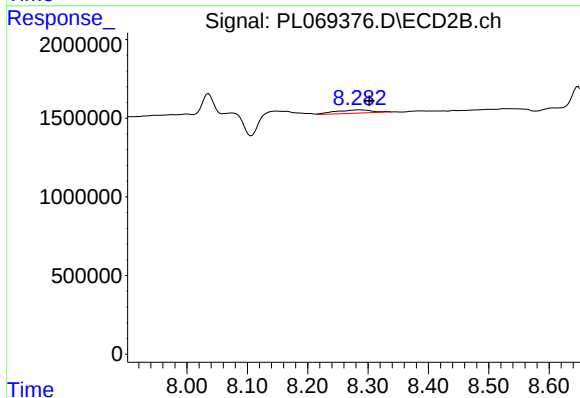


#25 Chlordane-3

R.T.: 8.284 min
Delta R.T.: -0.018 min
Response: 893309
Conc: 4.17 ng/ml

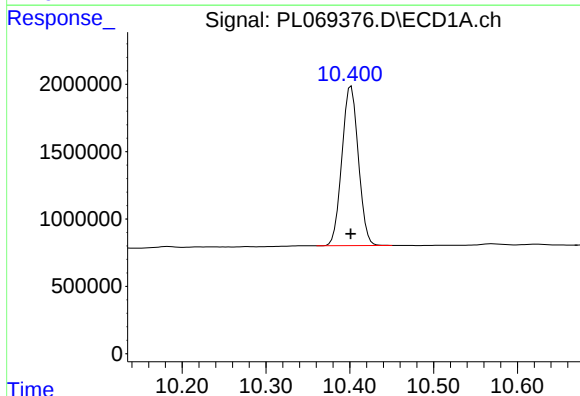

#28 Decachlorobiphenyl

R.T.: 10.402 min
Delta R.T.: 0.000 min
Response: 16148806
Conc: 23.93 ng/ml

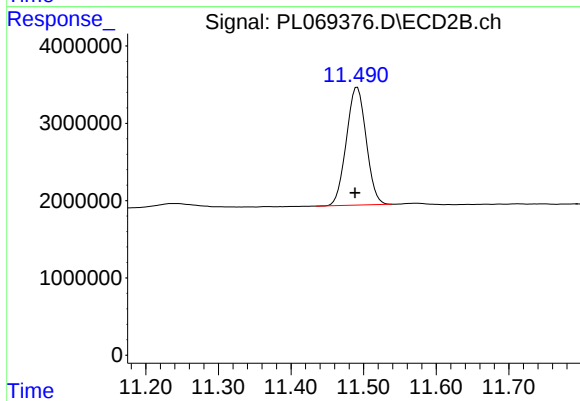

#28 Decachlorobiphenyl

R.T.: 11.491 min
Delta R.T.: 0.003 min
Response: 28908951
Conc: 23.59 ng/ml