

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082222\
 Data File : PL077245.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Aug 2022 17:53
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 22 19:08:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082222.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 22 19:07:18 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.415	2.630	129.3E6	341.2E6	100.493	98.364
28)	SA Decachlor...	8.905	7.734	101.0E6	252.2E6	94.610	96.385
Target Compounds							
23)	Chlordane-1	4.575	3.609	44560975	80958799	1002.323	913.366
24)	Chlordane-2	5.109	4.179	44786130	103.4E6	979.741	955.766
25)	Chlordane-3	5.821	4.803	188.9E6	312.6E6	1032.303	990.010
26)	Chlordane-4	5.898	4.865	227.4E6	322.9E6	1017.579	995.111
27)	Chlordane-5	6.758	5.529	36594646	85967553	976.097	982.801



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082222\
Data File : PL077245.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2022 17:53
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 22 19:08:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082222.M
Quant Title : GC Extractables
QLast Update : Mon Aug 22 19:07:18 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

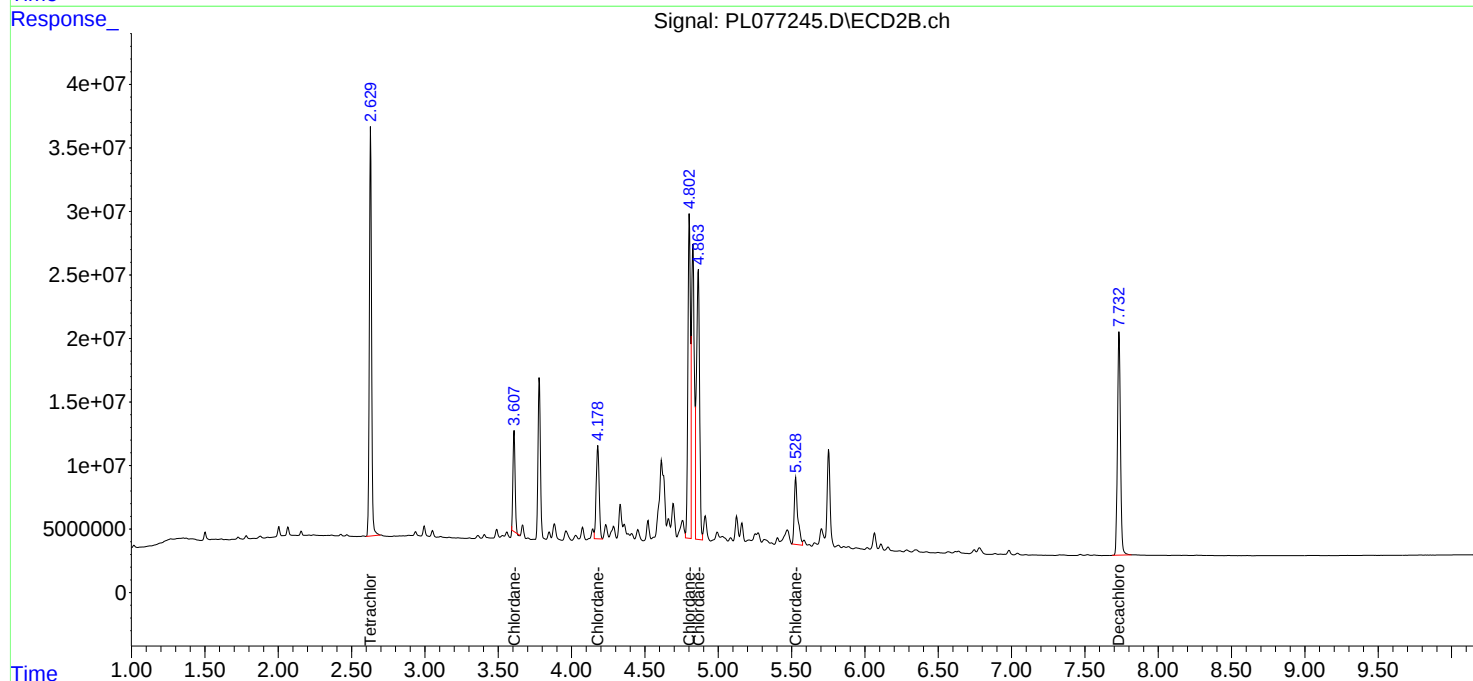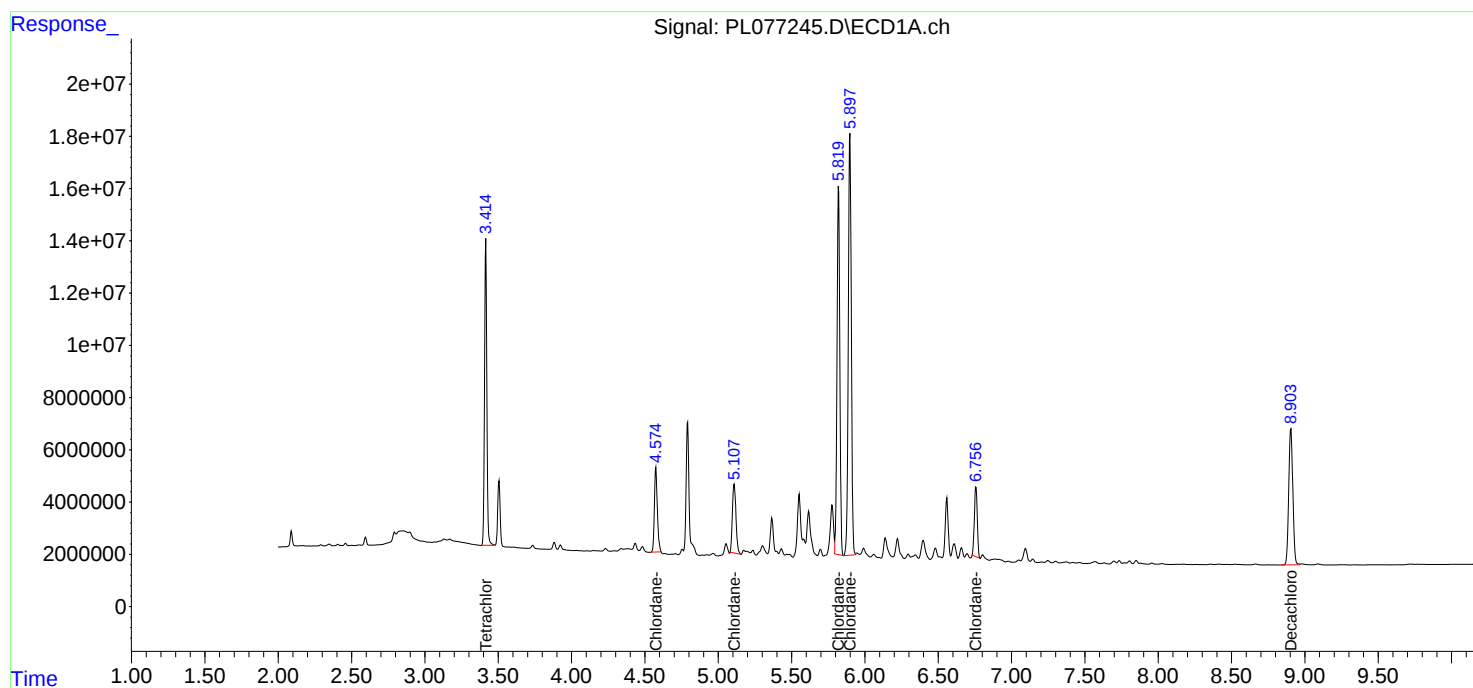


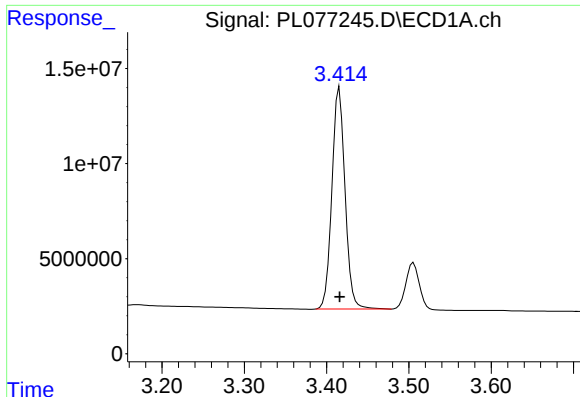

#1 Tetrachloro-m-xylene


R.T.: 3.415 min
Delta R.T.: 0.000 min
Response: 129309197
Conc: 100.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

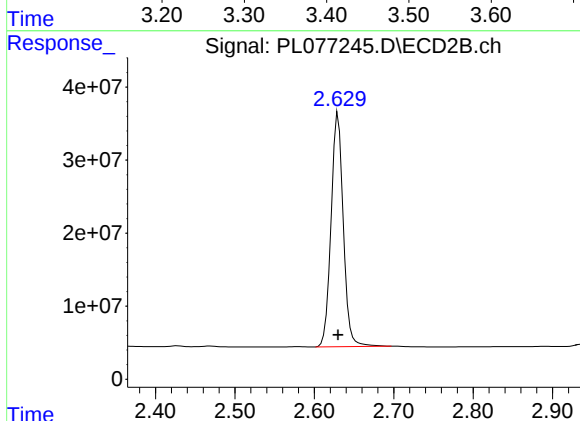


#1 Tetrachloro-m-xylene

R.T.: 2.630 min
Delta R.T.: 0.000 min
Response: 341242477
Conc: 98.36 ng/ml

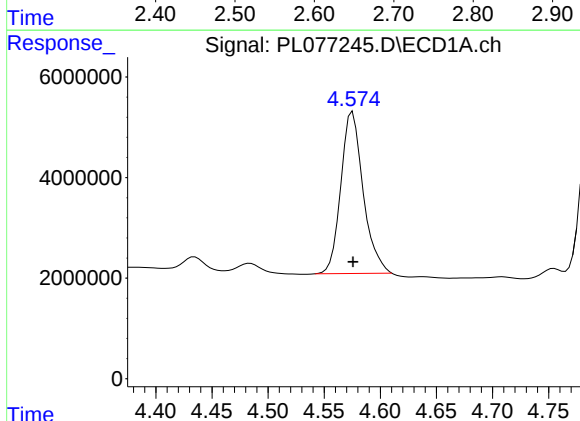


#23 Chlordane-1

R.T.: 4.575 min
Delta R.T.: 0.000 min
Response: 44560975
Conc: 1002.32 ng/ml

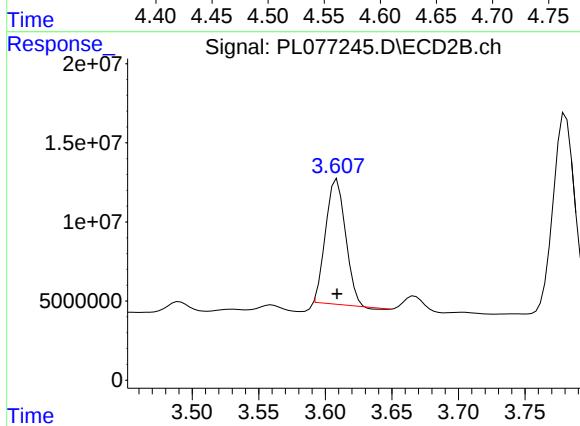

#23 Chlordane-1


R.T.: 3.609 min
Delta R.T.: 0.000 min
Response: 80958799
Conc: 913.37 ng/ml

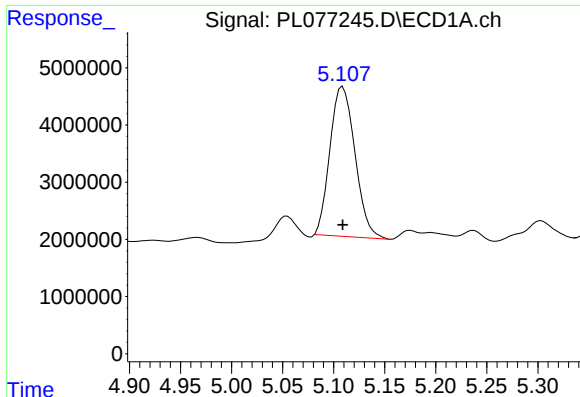

#24 Chlordane-2


R.T.: 5.109 min
Delta R.T.: 0.000 min
Response: 44786130
Conc: 979.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

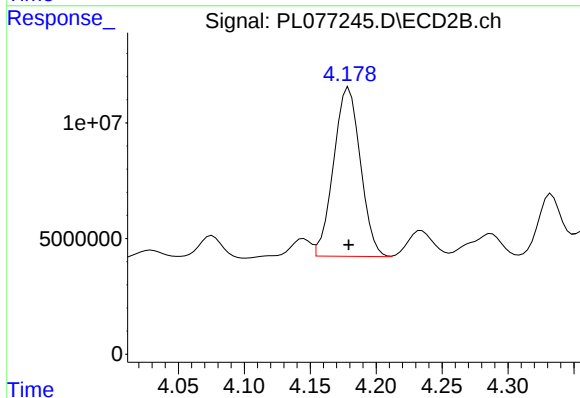


#24 Chlordane-2

R.T.: 4.179 min
Delta R.T.: 0.000 min
Response: 103449439
Conc: 955.77 ng/ml

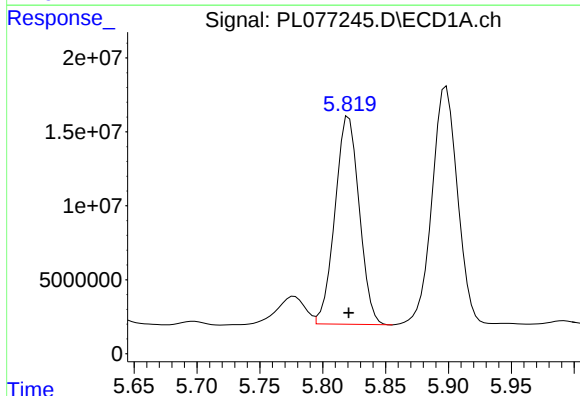


#25 Chlordane-3

R.T.: 5.821 min
Delta R.T.: 0.000 min
Response: 188898880
Conc: 1032.30 ng/ml

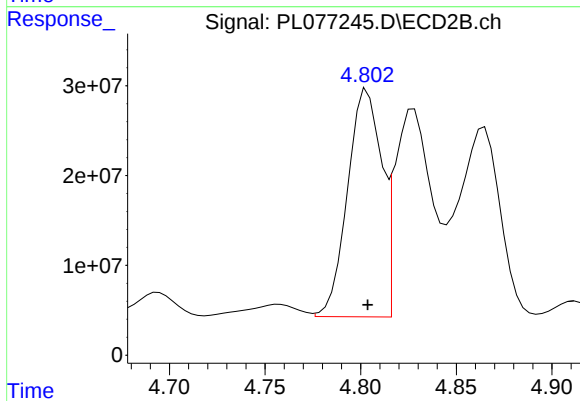

#25 Chlordane-3


R.T.: 4.803 min
Delta R.T.: 0.000 min
Response: 312590494
Conc: 990.01 ng/ml

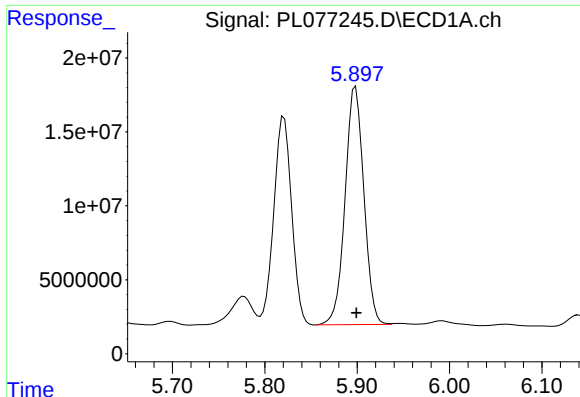

#26 Chlordane-4


R.T.: 5.898 min
Delta R.T.: 0.000 min
Response: 227408276
Conc: 1017.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

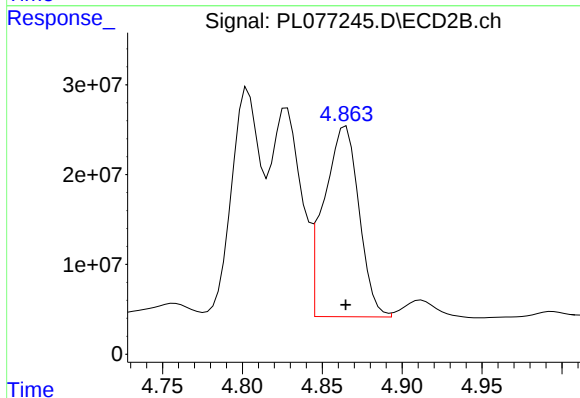


#26 Chlordane-4

R.T.: 4.865 min
Delta R.T.: 0.000 min
Response: 322882872
Conc: 995.11 ng/ml

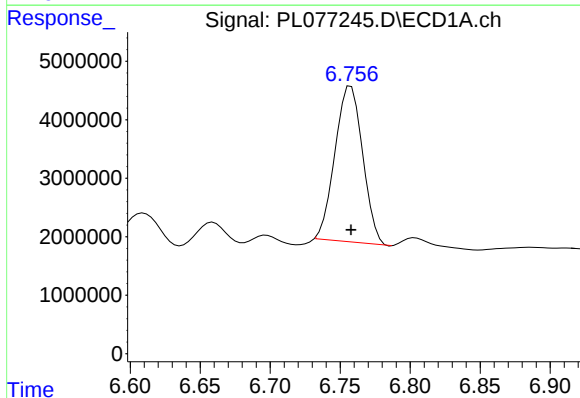


#27 Chlordane-5

R.T.: 6.758 min
Delta R.T.: 0.000 min
Response: 36594646
Conc: 976.10 ng/ml

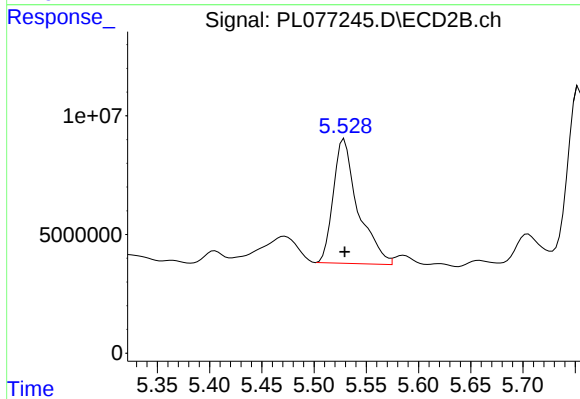

#27 Chlordane-5


R.T.: 5.529 min
Delta R.T.: 0.000 min
Response: 85967553
Conc: 982.80 ng/ml

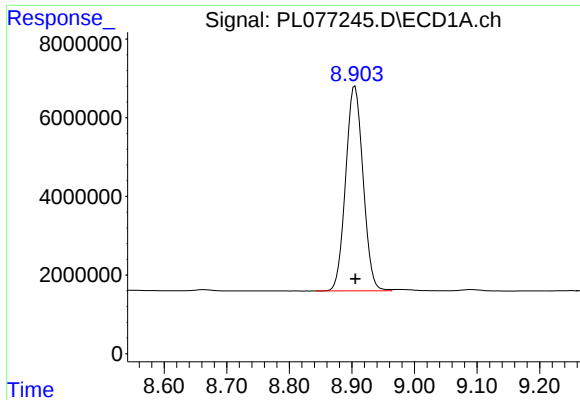

#28 Decachlorobiphenyl

R.T.: 8.905 min
Delta R.T.: 0.000 min
Response: 101009980
Conc: 94.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

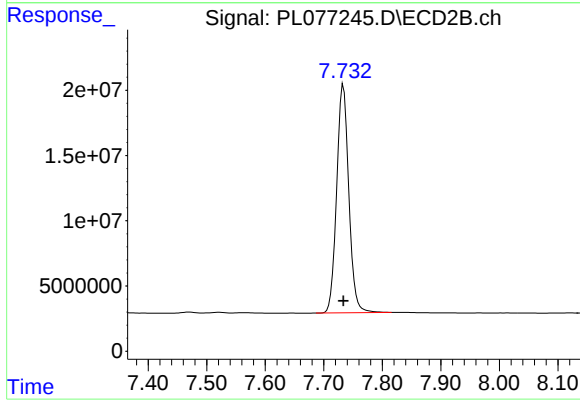

#28 Decachlorobiphenyl

R.T.: 7.734 min
Delta R.T.: 0.000 min
Response: 252227260
Conc: 96.38 ng/ml