

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082222\
 Data File : PL077246.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Aug 2022 18:07
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 22 19:08:38 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082222.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 22 19:07:18 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.416	2.630	95607853	254.4E6	74.302	73.318
28)	SA Decachlor...	8.905	7.734	77241886	190.1E6	72.348	72.650
Target Compounds							
23)	Chlordane-1	4.576	3.609	32856509	64501827	739.051	727.701
24)	Chlordane-2	5.109	4.180	34314354	77599487	750.661	716.939
25)	Chlordane-3	5.820	4.804	136.6E6	231.2E6	746.492	732.269
26)	Chlordane-4	5.899	4.865	165.4E6	238.9E6	740.321	736.251
27)	Chlordane-5	6.757	5.529	27633506	63610348	737.075	727.208



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082222\
Data File : PL077246.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2022 18:07
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 22 19:08:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082222.M
Quant Title : GC Extractables
QLast Update : Mon Aug 22 19:07:18 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

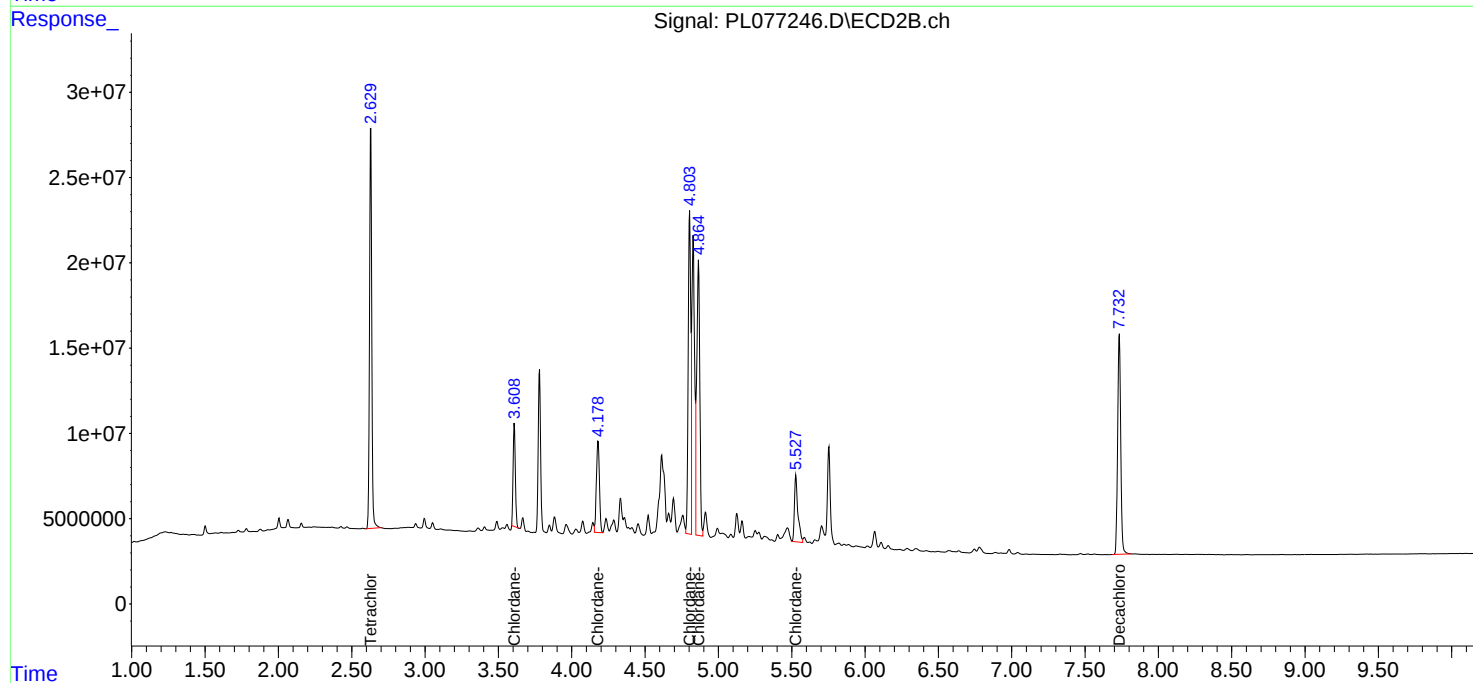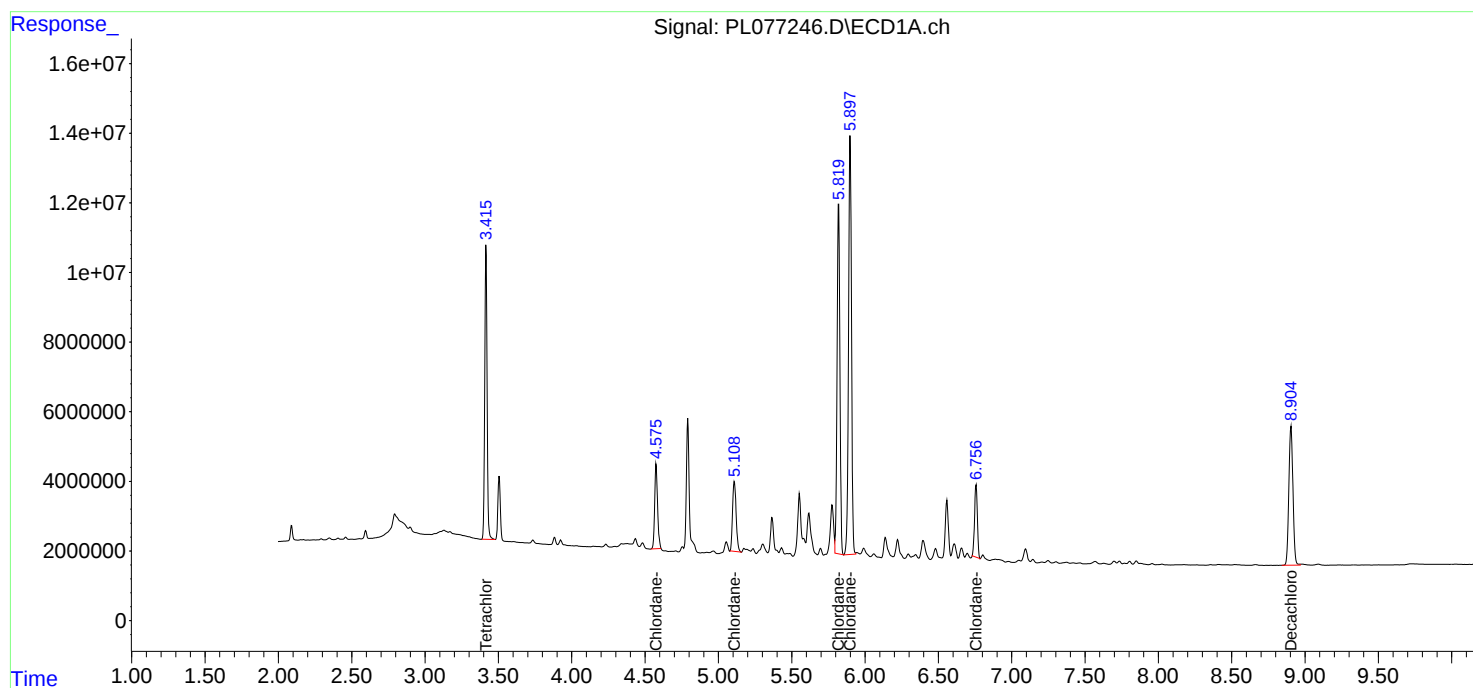


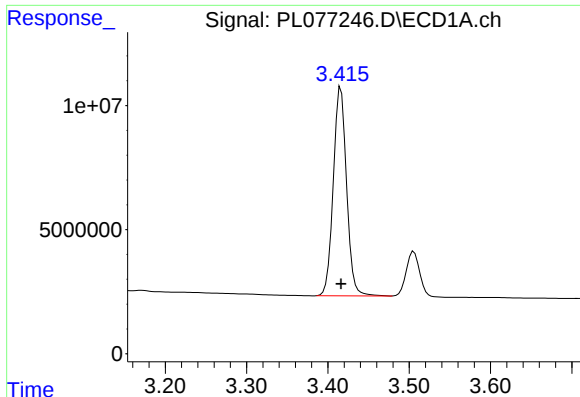

#1 Tetrachloro-m-xylene


R.T.: 3.416 min
Delta R.T.: 0.000 min
Response: 95607853
Conc: 74.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

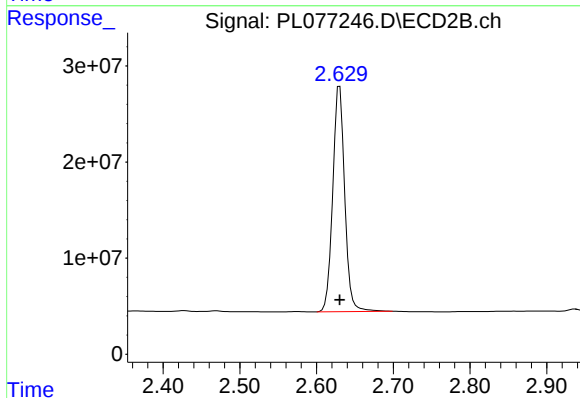


#1 Tetrachloro-m-xylene

R.T.: 2.630 min
Delta R.T.: 0.000 min
Response: 254354331
Conc: 73.32 ng/ml

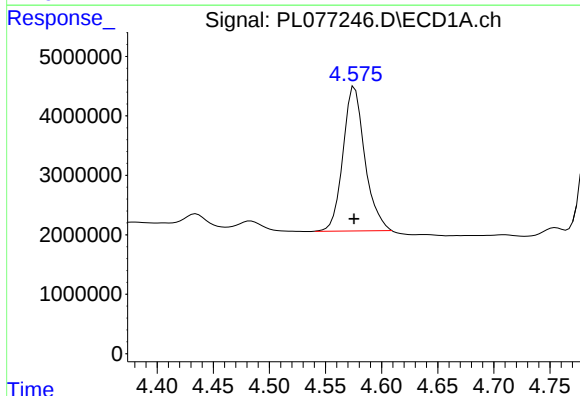


#23 Chlordane-1

R.T.: 4.576 min
Delta R.T.: 0.000 min
Response: 32856509
Conc: 739.05 ng/ml

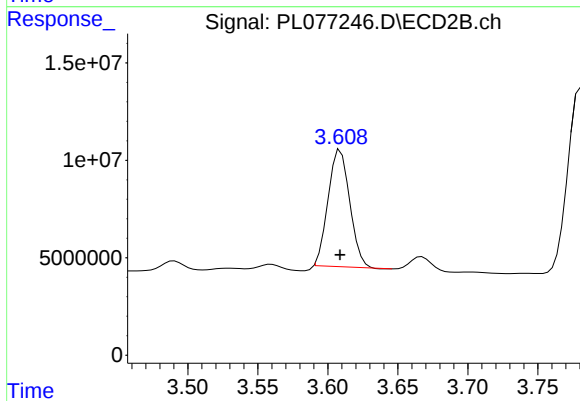

#23 Chlordane-1


R.T.: 3.609 min
Delta R.T.: 0.000 min
Response: 64501827
Conc: 727.70 ng/ml

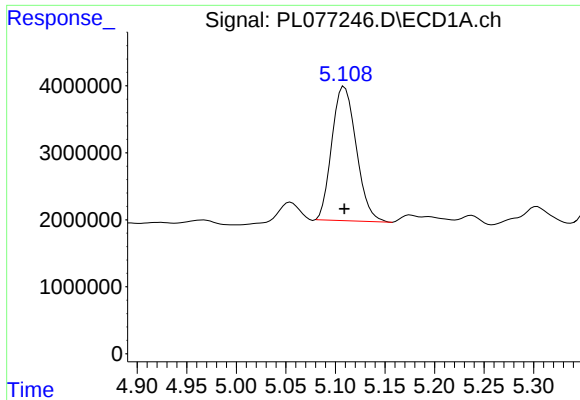

#24 Chlordane-2


R.T.: 5.109 min
Delta R.T.: 0.000 min
Response: 34314354
Conc: 750.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

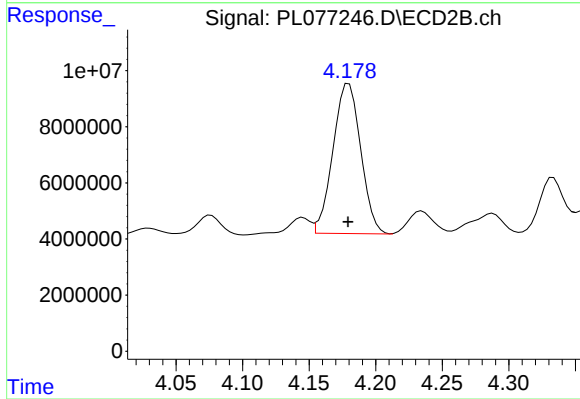


#24 Chlordane-2

R.T.: 4.180 min
Delta R.T.: 0.000 min
Response: 77599487
Conc: 716.94 ng/ml

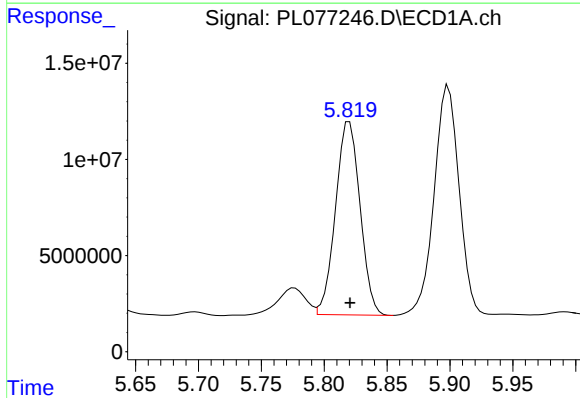


#25 Chlordane-3

R.T.: 5.820 min
Delta R.T.: 0.000 min
Response: 136598920
Conc: 746.49 ng/ml

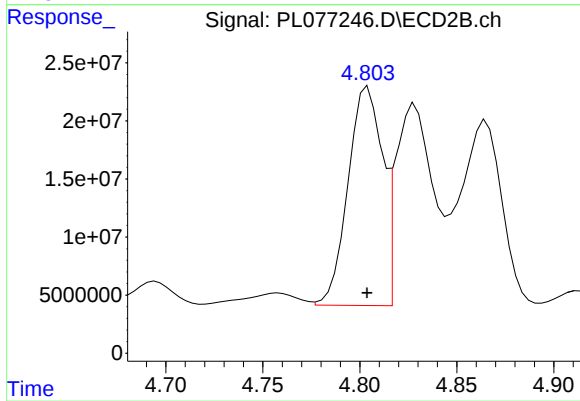

#25 Chlordane-3


R.T.: 4.804 min
Delta R.T.: 0.000 min
Response: 231209901
Conc: 732.27 ng/ml

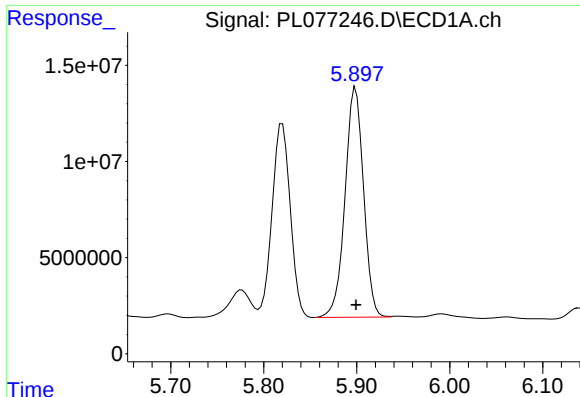

#26 Chlordane-4


R.T.: 5.899 min
Delta R.T.: 0.000 min
Response: 165446713
Conc: 740.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

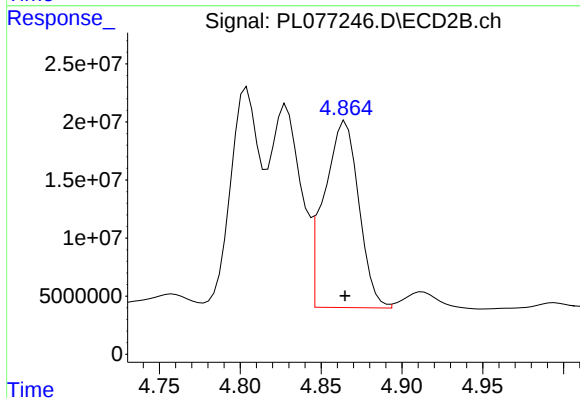


#26 Chlordane-4

R.T.: 4.865 min
Delta R.T.: 0.000 min
Response: 238890817
Conc: 736.25 ng/ml

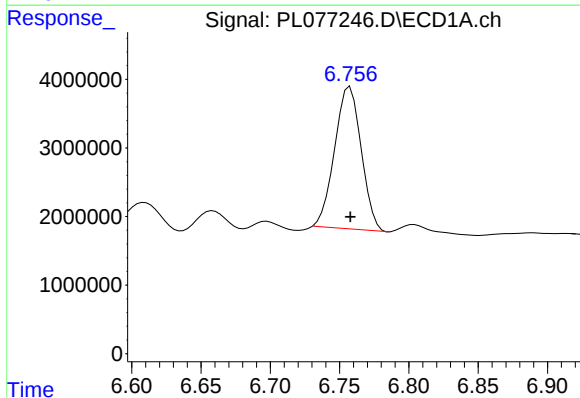


#27 Chlordane-5

R.T.: 6.757 min
Delta R.T.: 0.000 min
Response: 27633506
Conc: 737.07 ng/ml

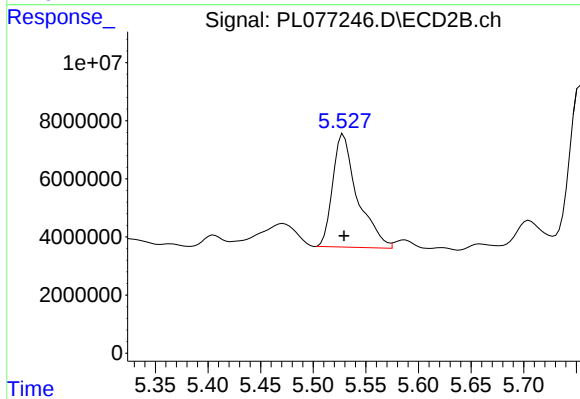

#27 Chlordane-5


R.T.: 5.529 min
Delta R.T.: 0.000 min
Response: 63610348
Conc: 727.21 ng/ml

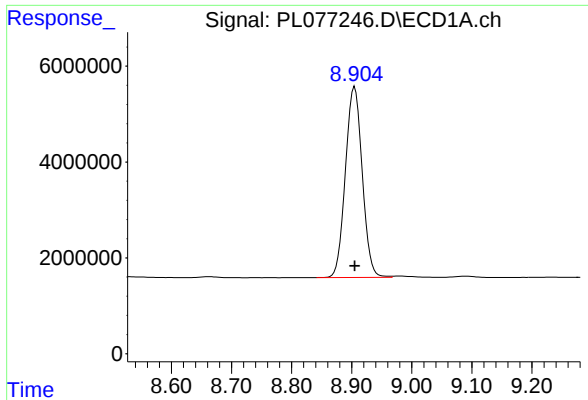

#28 Decachlorobiphenyl

R.T.: 8.905 min
Delta R.T.: 0.000 min
Response: 77241886
Conc: 72.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

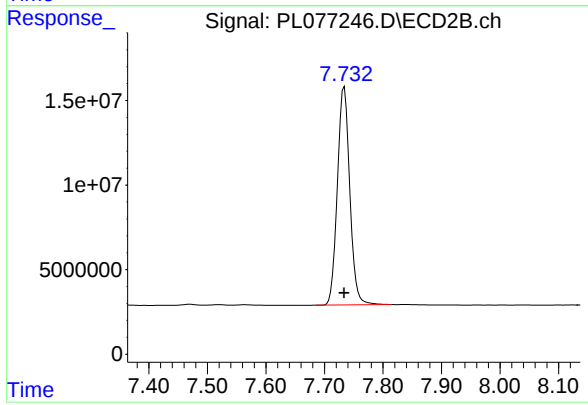

#28 Decachlorobiphenyl

R.T.: 7.734 min
Delta R.T.: 0.000 min
Response: 190116592
Conc: 72.65 ng/ml