

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082222\
 Data File : PL077248.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Aug 2022 18:35
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 22 19:09:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082222.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 22 19:07:18 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.417	2.631	29852774	81550601	23.200	23.507
28)	SA Decachlor...	8.910	7.738	26456878	63812462	24.781	24.385
Target Compounds							
23)	Chlordane-1	4.577	3.610	10151773	20686035	228.347	233.377
24)	Chlordane-2	5.111	4.181	11346489	25916566	248.216	239.442
25)	Chlordane-3	5.824	4.806	40885984	71942682	223.435	227.851
26)	Chlordane-4	5.902	4.867	50514727	75594229	226.037	232.978
27)	Chlordane-5	6.761	5.531	8879170	20886663	236.836	238.781



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082222\
Data File : PL077248.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2022 18:35
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 22 19:09:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082222.M
Quant Title : GC Extractables
QLast Update : Mon Aug 22 19:07:18 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

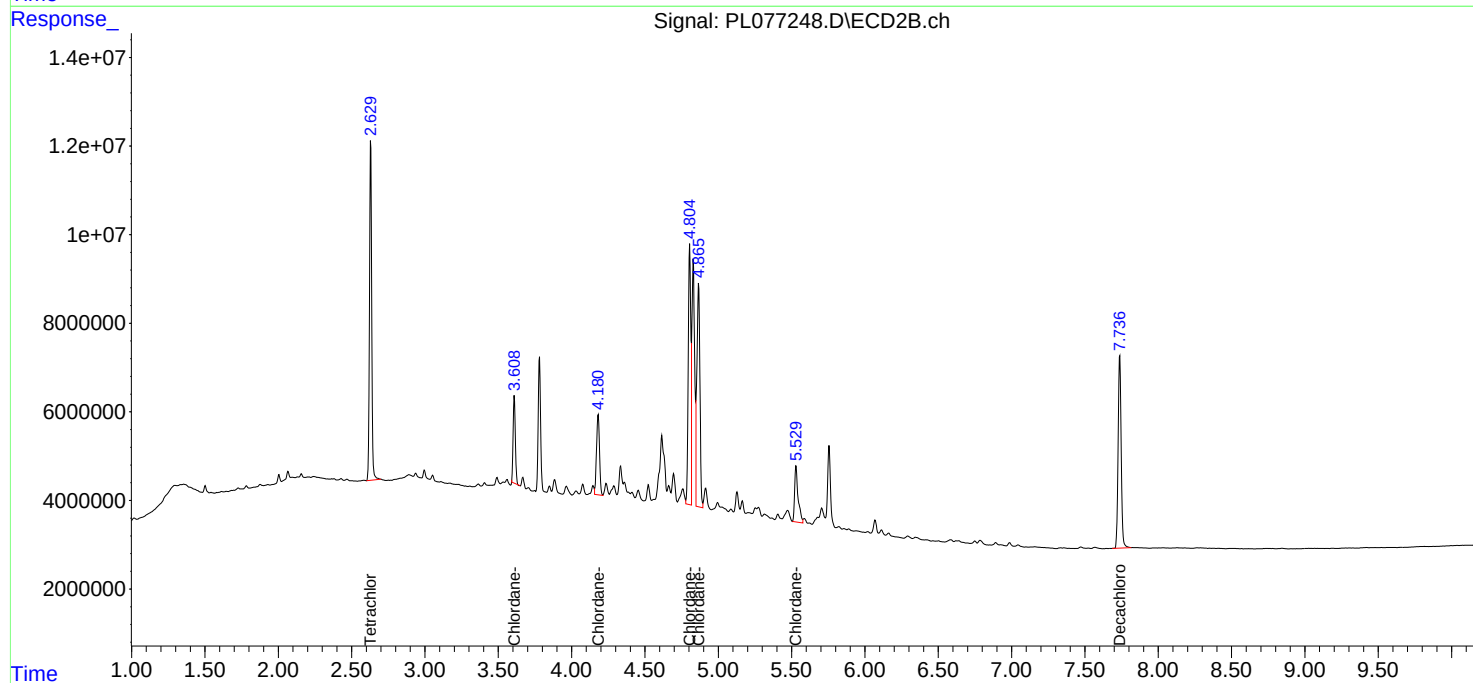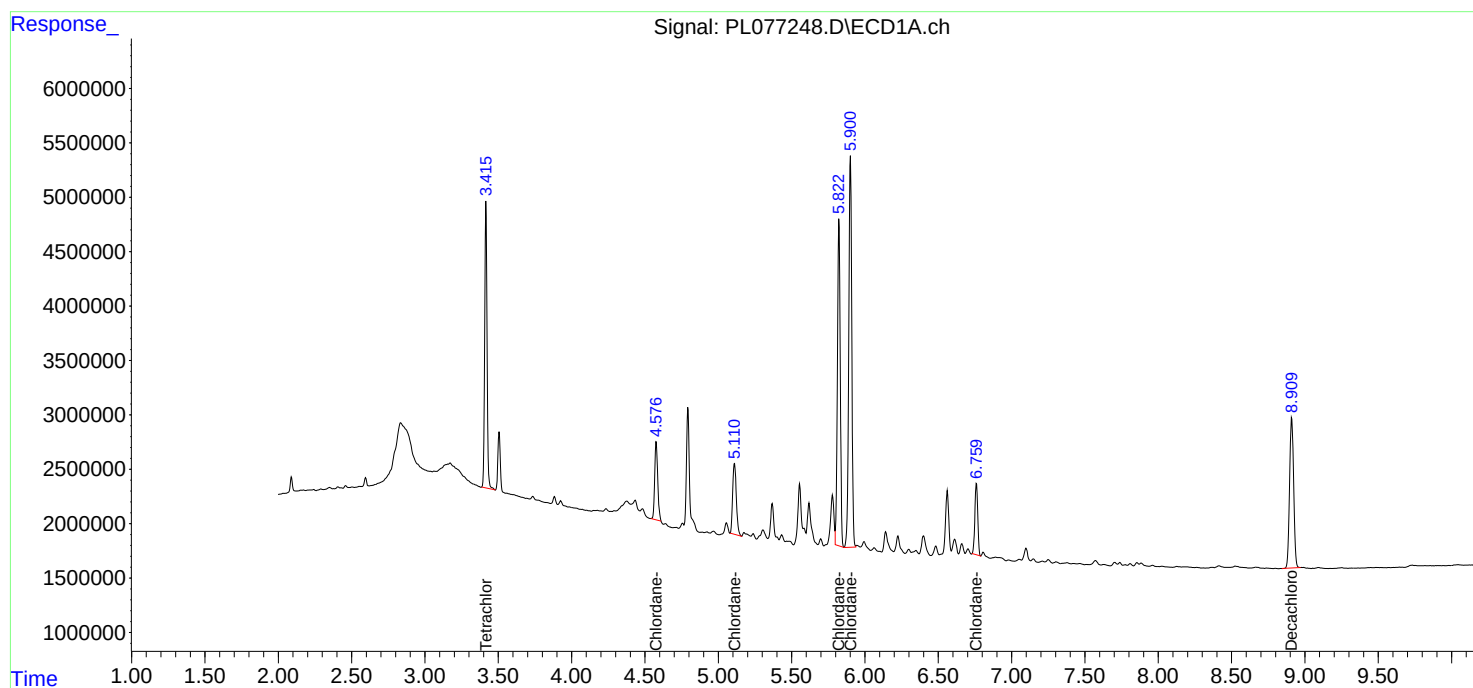


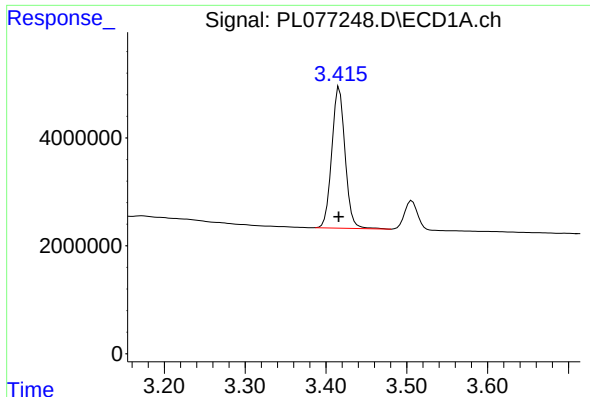

#1 Tetrachloro-m-xylene


R.T.: 3.417 min
Delta R.T.: 0.000 min
Response: 29852774
Conc: 23.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

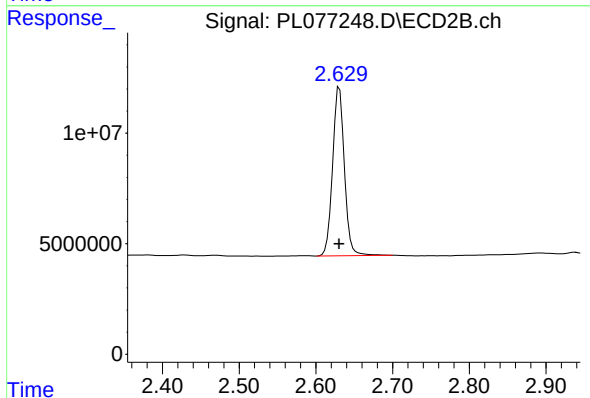


#1 Tetrachloro-m-xylene

R.T.: 2.631 min
Delta R.T.: 0.000 min
Response: 81550601
Conc: 23.51 ng/ml

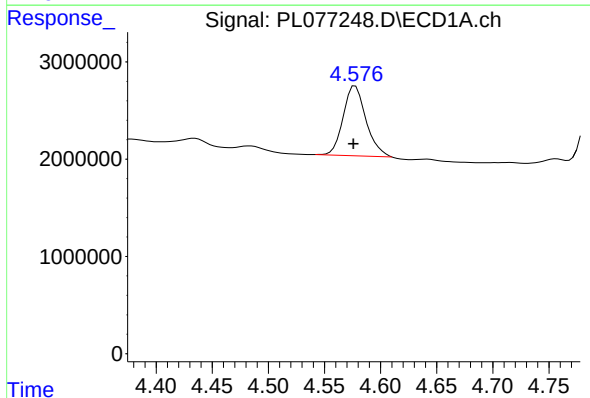


#23 Chlordane-1

R.T.: 4.577 min
Delta R.T.: 0.002 min
Response: 10151773
Conc: 228.35 ng/ml

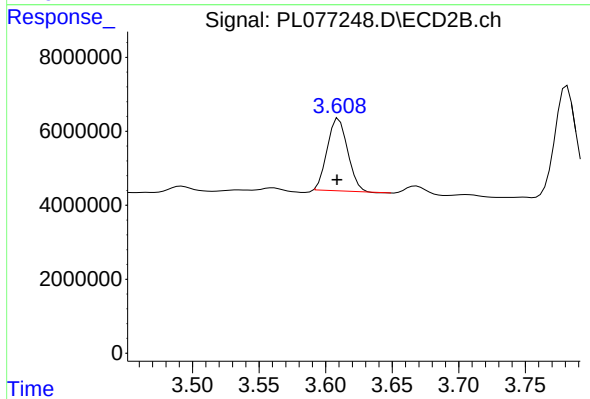

#23 Chlordane-1


R.T.: 3.610 min
Delta R.T.: 0.001 min
Response: 20686035
Conc: 233.38 ng/ml

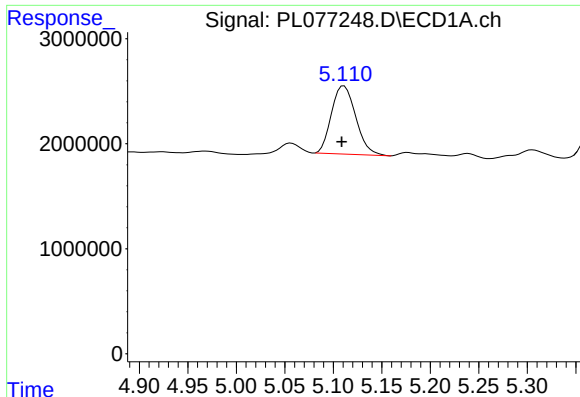

#24 Chlordane-2


R.T.: 5.111 min
Delta R.T.: 0.002 min
Response: 11346489
Conc: 248.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

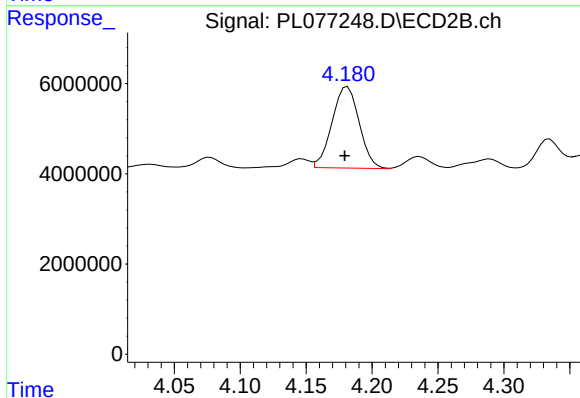


#24 Chlordane-2

R.T.: 4.181 min
Delta R.T.: 0.002 min
Response: 25916566
Conc: 239.44 ng/ml

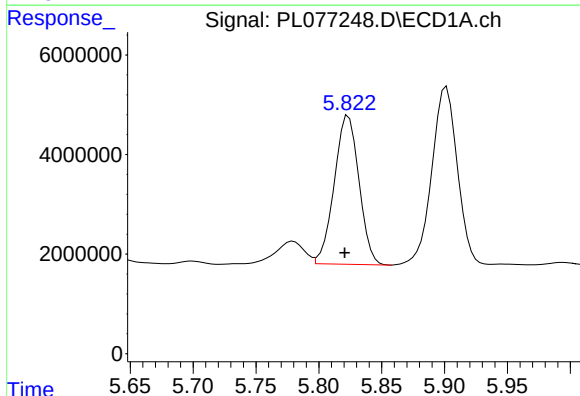


#25 Chlordane-3

R.T.: 5.824 min
Delta R.T.: 0.003 min
Response: 40885984
Conc: 223.44 ng/ml

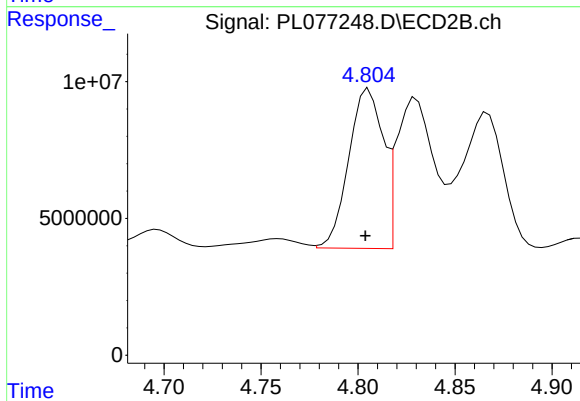

#25 Chlordane-3


R.T.: 4.806 min
Delta R.T.: 0.002 min
Response: 71942682
Conc: 227.85 ng/ml

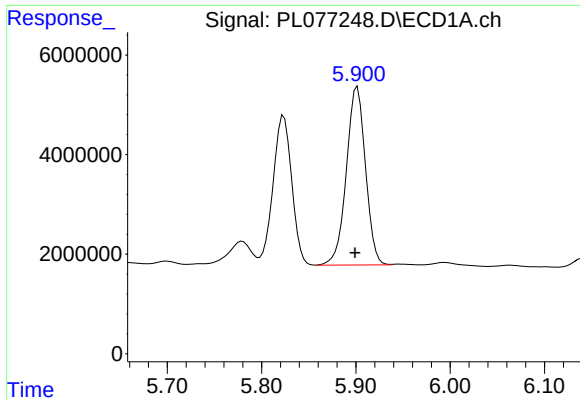

#26 Chlordane-4


R.T.: 5.902 min
Delta R.T.: 0.002 min
Response: 50514727
Conc: 226.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

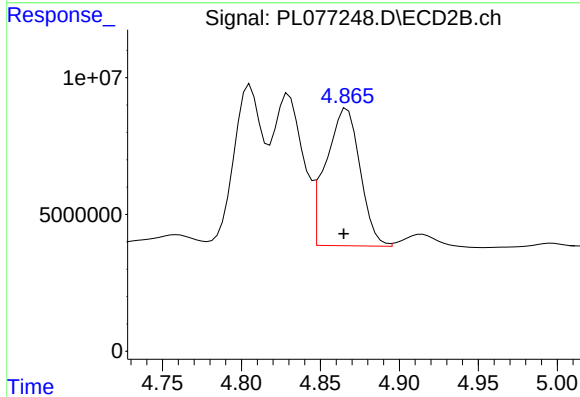


#26 Chlordane-4

R.T.: 4.867 min
Delta R.T.: 0.002 min
Response: 75594229
Conc: 232.98 ng/ml

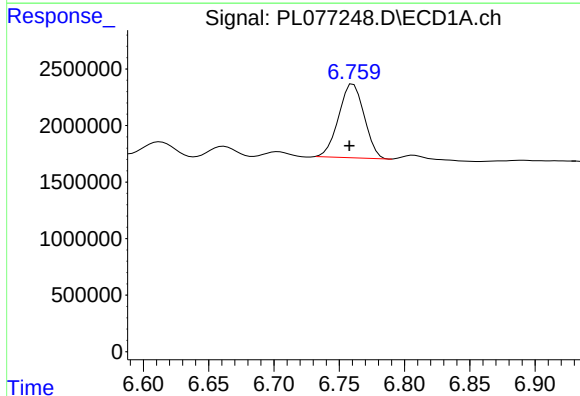


#27 Chlordane-5

R.T.: 6.761 min
Delta R.T.: 0.003 min
Response: 8879170
Conc: 236.84 ng/ml

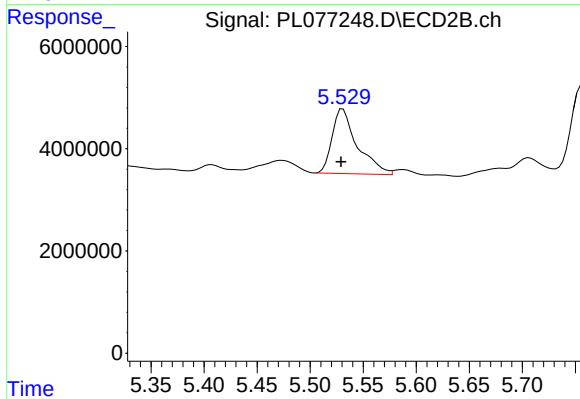

#27 Chlordane-5


R.T.: 5.531 min
Delta R.T.: 0.002 min
Response: 20886663
Conc: 238.78 ng/ml

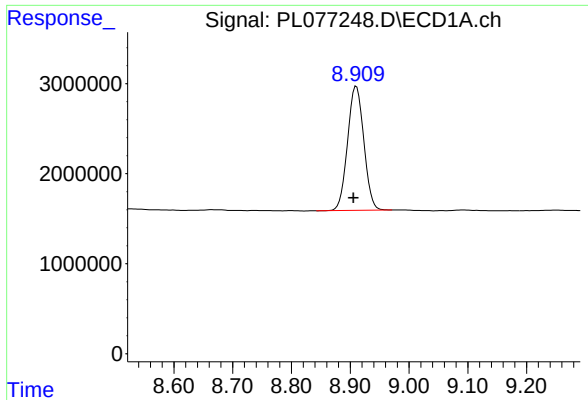

#28 Decachlorobiphenyl

R.T.: 8.910 min
Delta R.T.: 0.005 min
Response: 26456878
Conc: 24.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

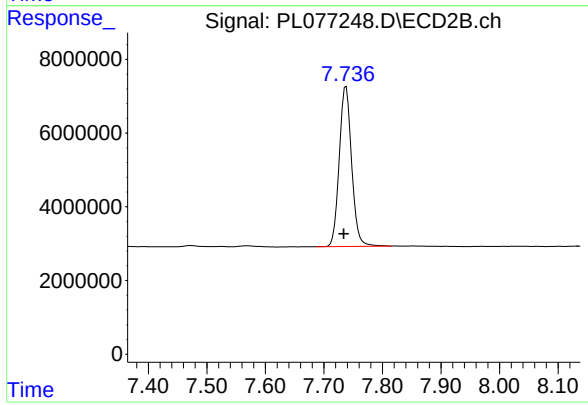

#28 Decachlorobiphenyl

R.T.: 7.738 min
Delta R.T.: 0.004 min
Response: 63812462
Conc: 24.38 ng/ml