

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082222\
 Data File : PL077256.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Aug 2022 20:26
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL082222CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 05:34:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082222.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 23 05:30:43 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.415	2.630	66968287	178.0E6	53.439	52.740
28)	SA Decachlor...	8.906	7.734	55168687	136.3E6	50.986	52.160
Target Compounds							
23)	Chlordane-1	4.575	3.608	22982697	44869817	537.204	537.653
24)	Chlordane-2	5.109	4.179	24207126	56016990	523.483	522.939
25)	Chlordane-3	5.821	4.803	95829575	161.8E6	538.747	529.748
26)	Chlordane-4	5.899	4.865	116.9E6	167.7E6	537.370	529.859
27)	Chlordane-5	6.758	5.529	19329783	46361850	529.399	529.529



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082222\
Data File : PL077256.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2022 20:26
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL082222CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 05:34:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082222.M
Quant Title : GC Extractables
QLast Update : Tue Aug 23 05:30:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

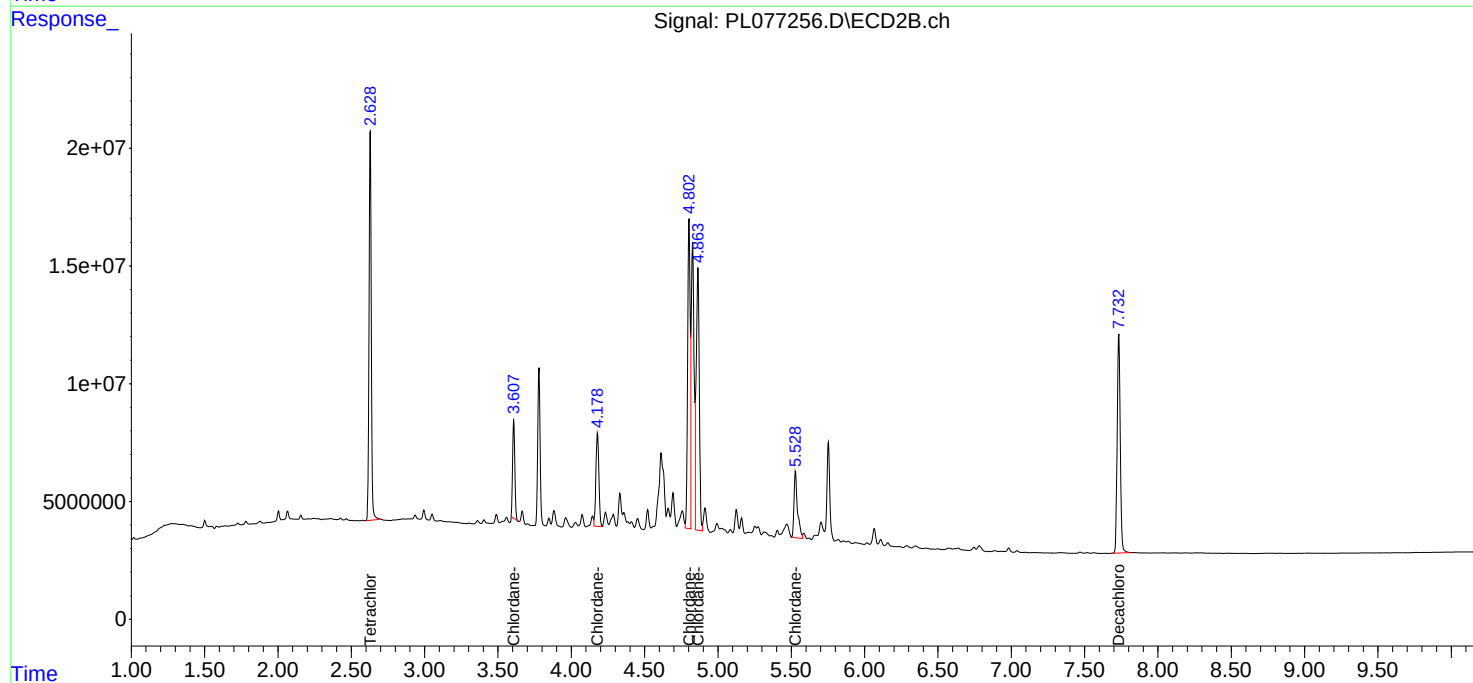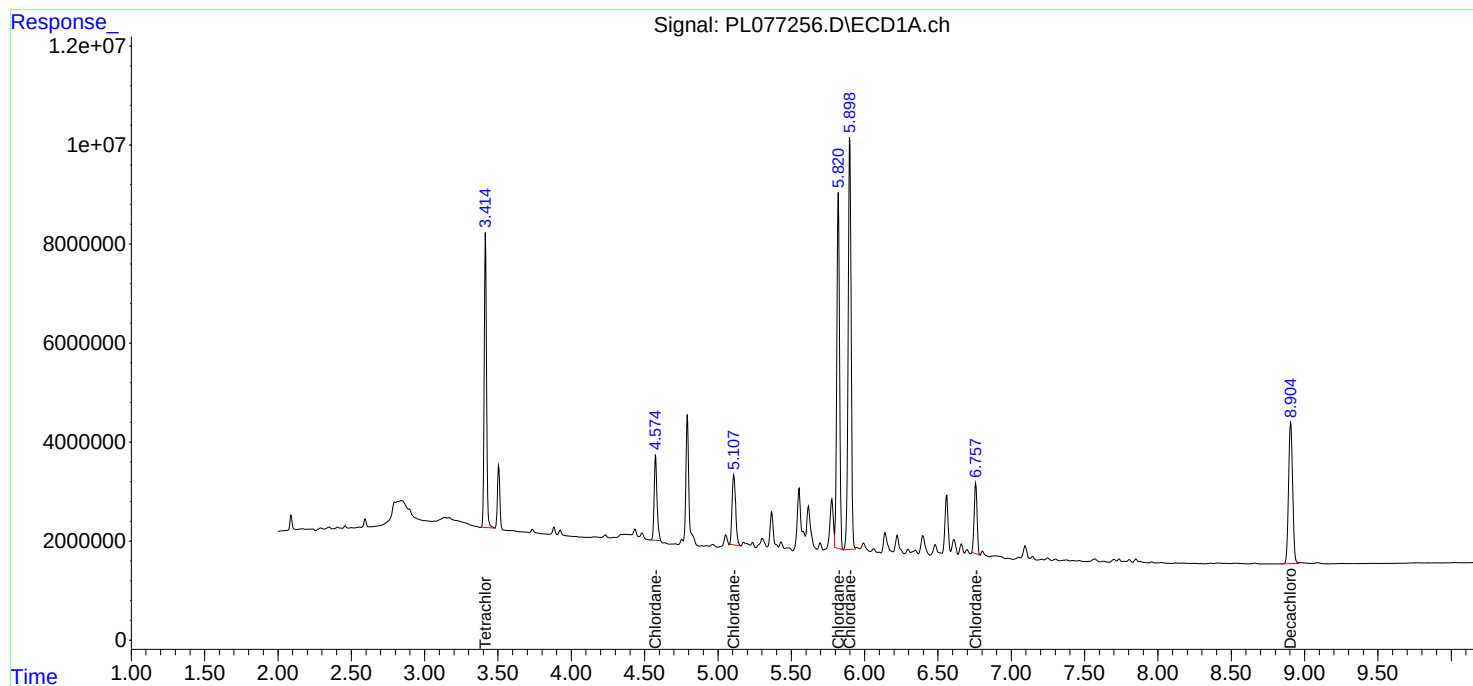


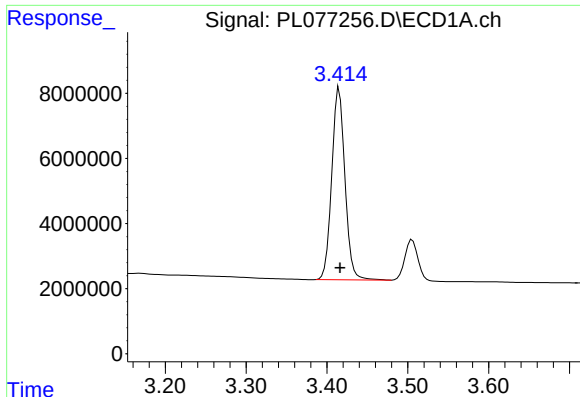

#1 Tetrachloro-m-xylene


R.T.: 3.415 min
Delta R.T.: 0.000 min
Response: 66968287
Conc: 53.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL082222CHLOR

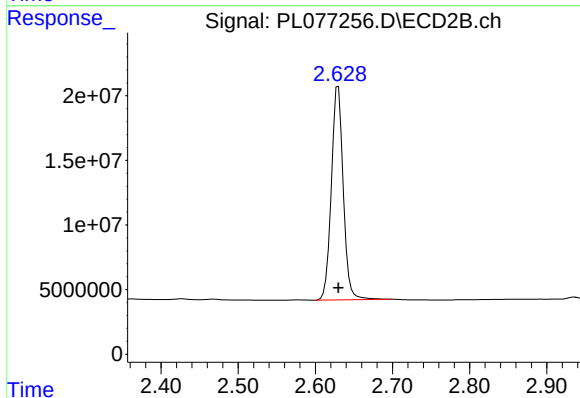


#1 Tetrachloro-m-xylene

R.T.: 2.630 min
Delta R.T.: 0.000 min
Response: 177973454
Conc: 52.74 ng/ml

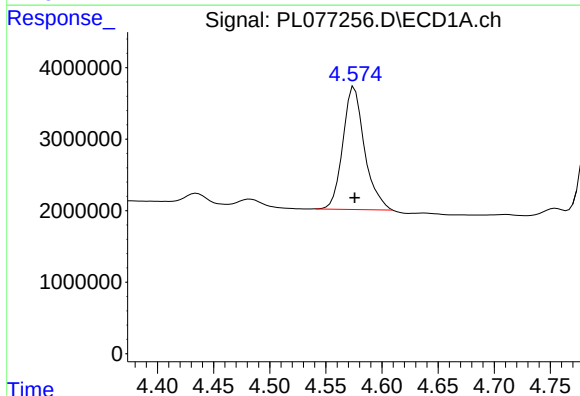


#23 Chlordane-1

R.T.: 4.575 min
Delta R.T.: 0.000 min
Response: 22982697
Conc: 537.20 ng/ml

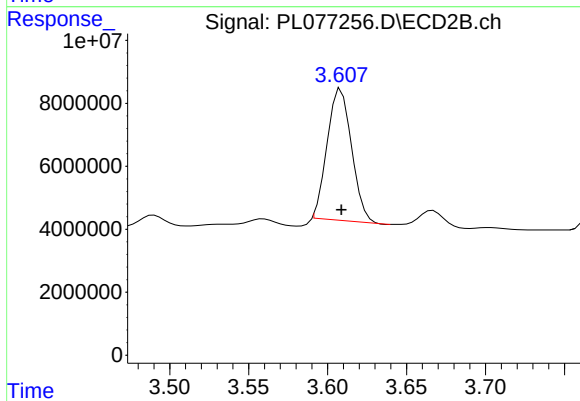

#23 Chlordane-1


R.T.: 3.608 min
Delta R.T.: 0.000 min
Response: 44869817
Conc: 537.65 ng/ml

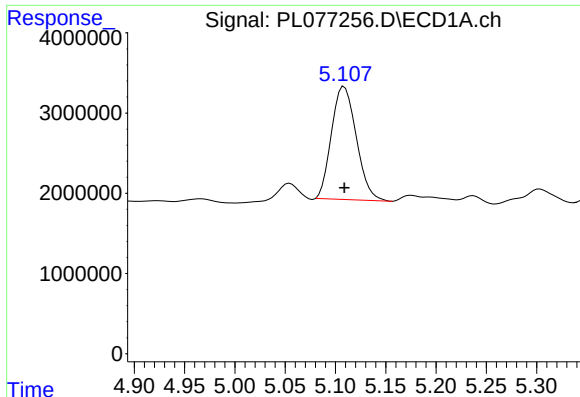

#24 Chlordane-2


R.T.: 5.109 min
Delta R.T.: 0.000 min
Response: 24207126
Conc: 523.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL082222CHLOR

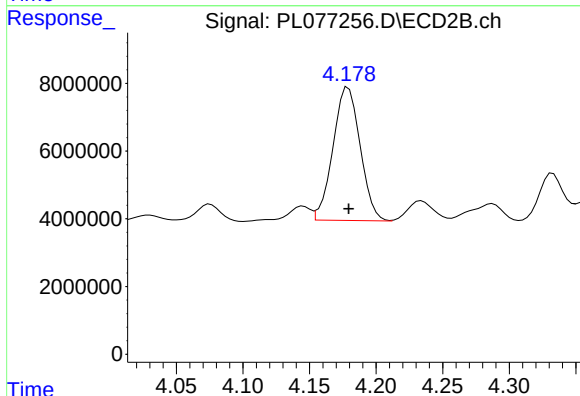


#24 Chlordane-2

R.T.: 4.179 min
Delta R.T.: 0.000 min
Response: 56016990
Conc: 522.94 ng/ml

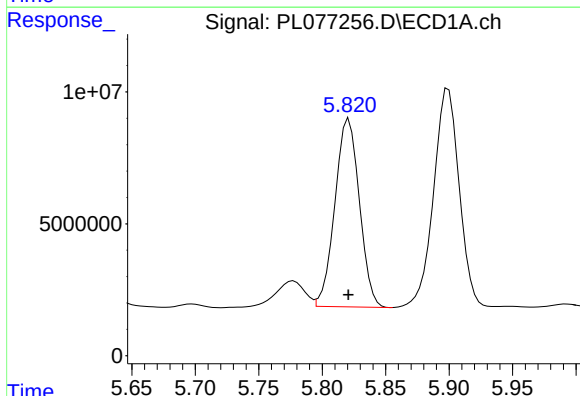


#25 Chlordane-3

R.T.: 5.821 min
Delta R.T.: 0.000 min
Response: 95829575
Conc: 538.75 ng/ml

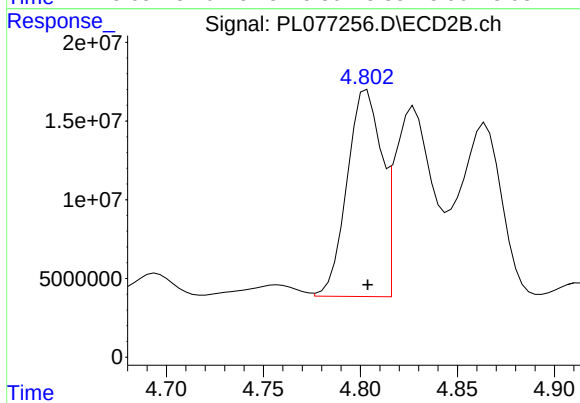

#25 Chlordane-3


R.T.: 4.803 min
Delta R.T.: 0.000 min
Response: 161756188
Conc: 529.75 ng/ml

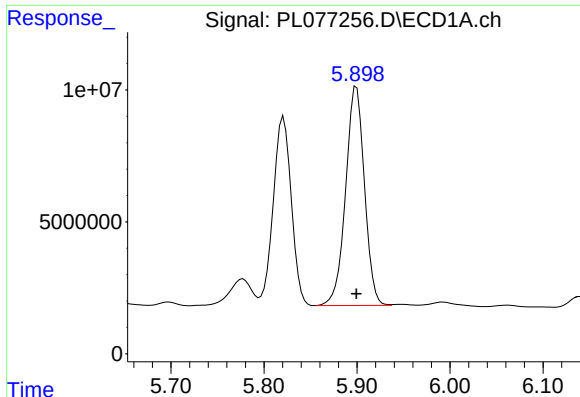

#26 Chlordane-4


R.T.: 5.899 min
Delta R.T.: 0.000 min
Response: 116888838
Conc: 537.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL082222CHLOR

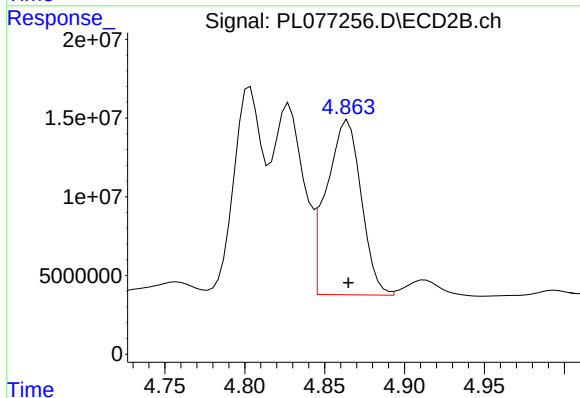


#26 Chlordane-4

R.T.: 4.865 min
Delta R.T.: 0.000 min
Response: 167685391
Conc: 529.86 ng/ml

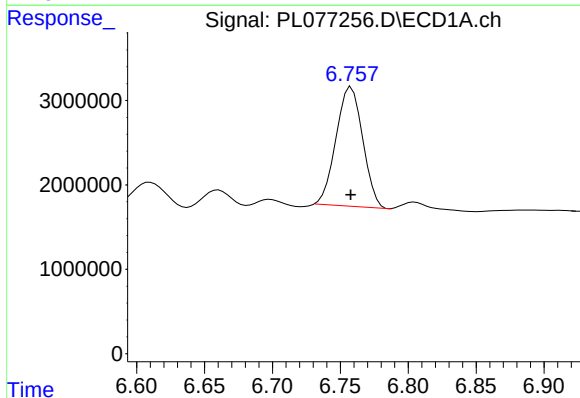


#27 Chlordane-5

R.T.: 6.758 min
Delta R.T.: 0.000 min
Response: 19329783
Conc: 529.40 ng/ml

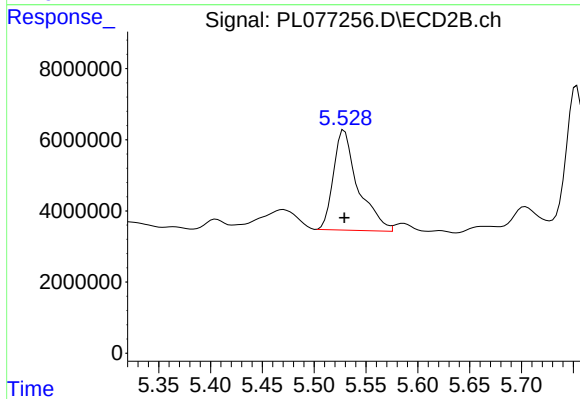

#27 Chlordane-5


R.T.: 5.529 min
Delta R.T.: 0.000 min
Response: 46361850
Conc: 529.53 ng/ml

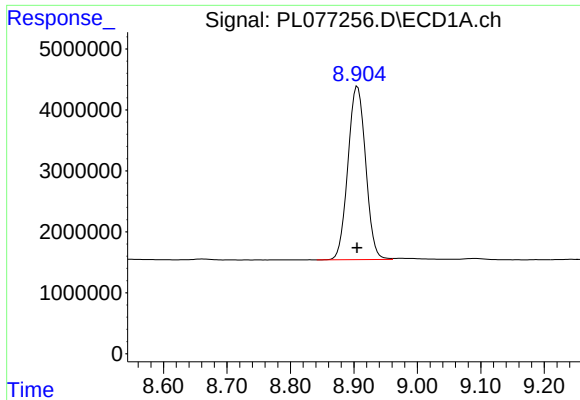

#28 Decachlorobiphenyl

R.T.: 8.906 min
Delta R.T.: 0.000 min
Response: 55168687
Conc: 50.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL082222CHLOR

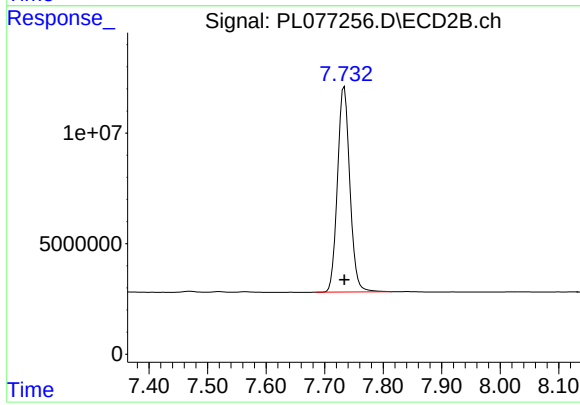

#28 Decachlorobiphenyl

R.T.: 7.734 min
Delta R.T.: 0.000 min
Response: 136315829
Conc: 52.16 ng/ml