

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082223\
 Data File : PL084907.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Aug 2023 09:41
 Operator : AR\AJ
 Sample : PB154795BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 00:48:47 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 05:52:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	2.686	42809688	19725119	17.076	16.709
27)	SA Decachlor...	9.036	7.868	56430790	43946005	32.928	32.447
Target Compounds							
2)	A alpha-BHC	3.903f	0.000	169893	0	<MDL	N.D. #
7)	B delta-BHC	4.726	0.000	194300	0	<MDL	N.D. #
20)	A Methoxychlor	7.518f	0.000	1649059	0	1.700	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082223\
Data File : PL084907.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2023 09:41
Operator : AR\AJ
Sample : PB154795BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 00:48:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

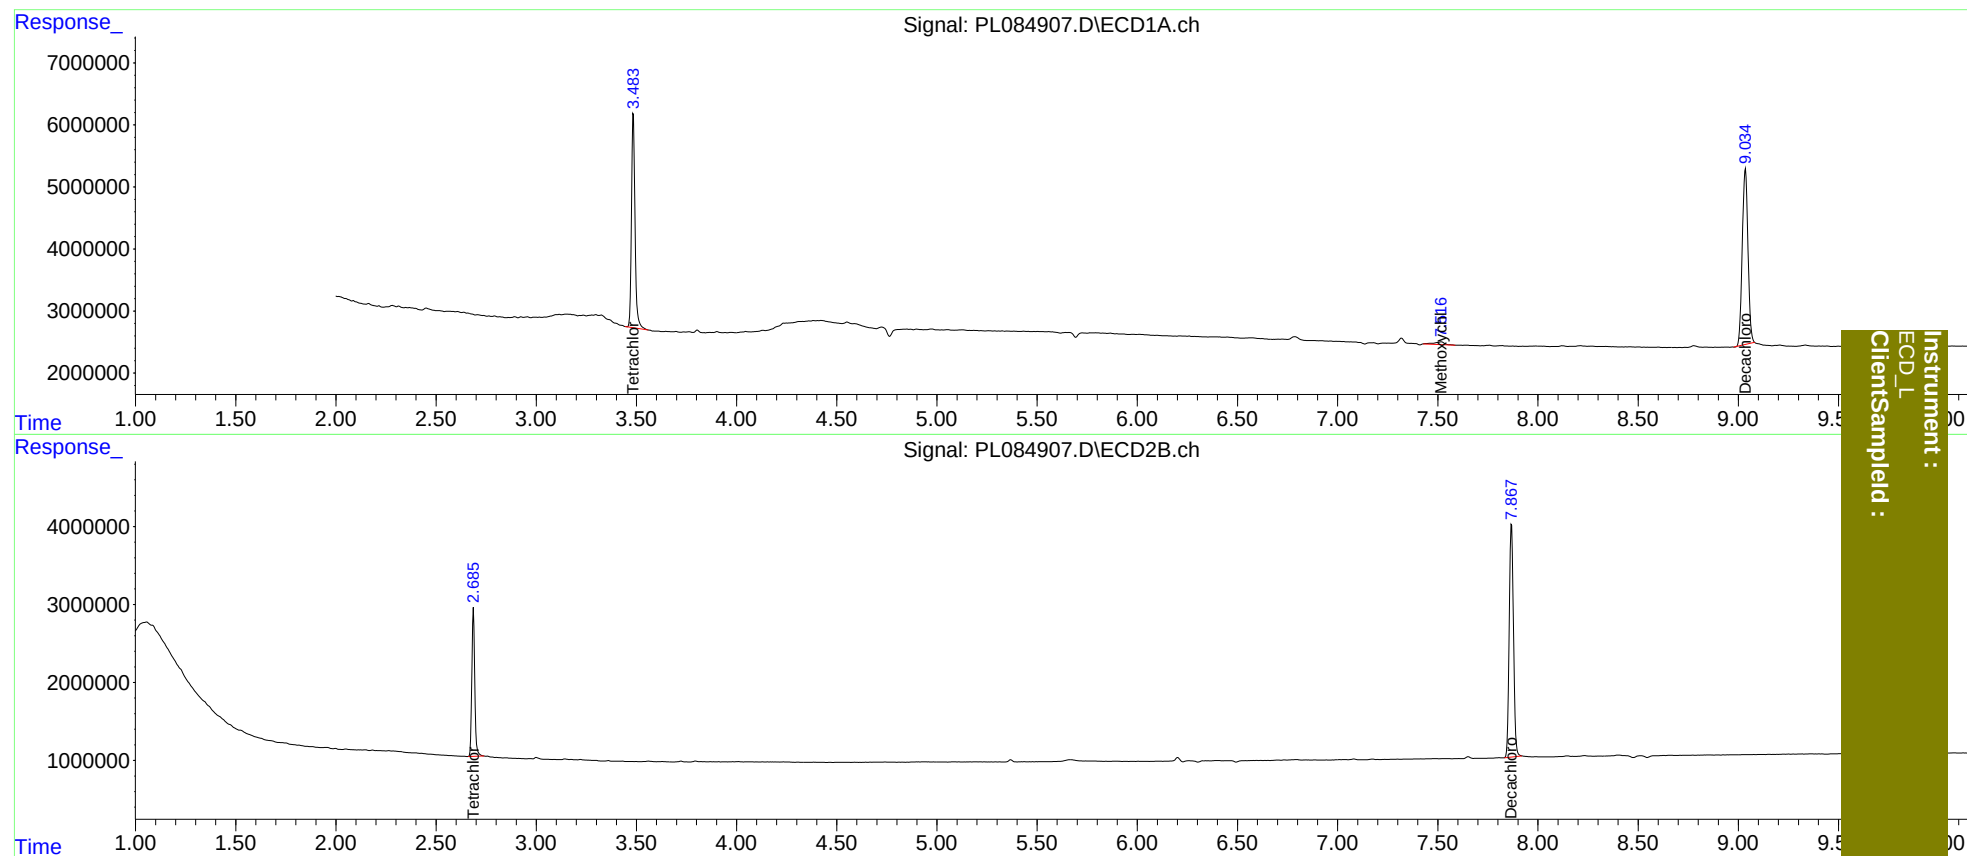


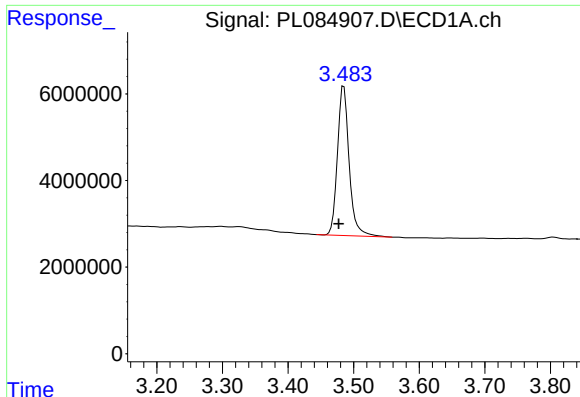

#1 Tetrachloro-m-xylene


R.T.: 3.485 min
Delta R.T.: 0.008 min
Response: 42809688
Conc: 17.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

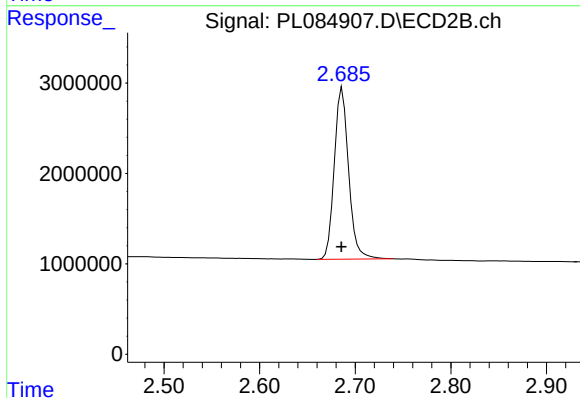


#1 Tetrachloro-m-xylene

R.T.: 2.686 min
Delta R.T.: 0.000 min
Response: 19725119
Conc: 16.71 ng/ml

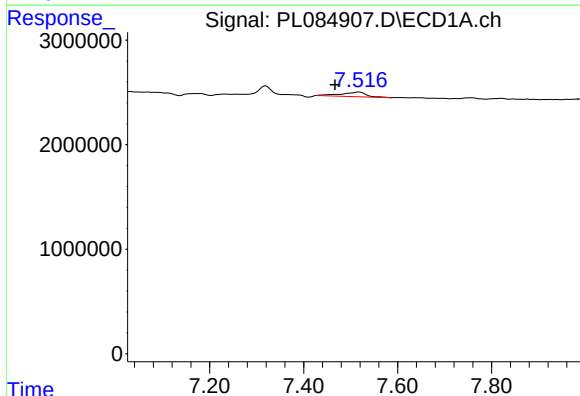


#20 Methoxychlor

R.T.: 7.518 min
Delta R.T.: 0.051 min
Response: 1649059
Conc: 1.70 ng/ml

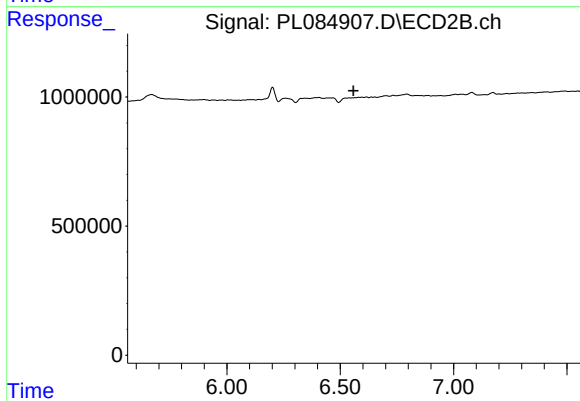

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 6.559 min
Response: 0
Conc: N.D.

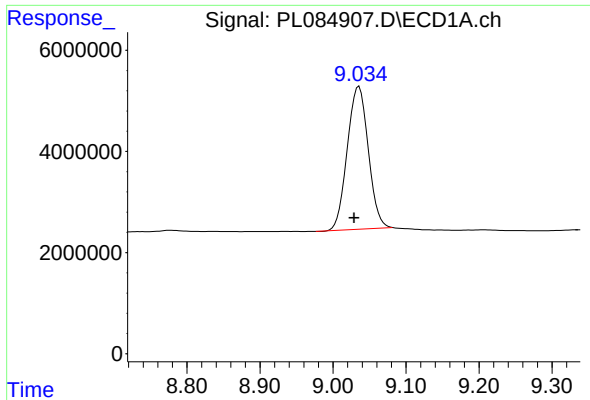

#27 Decachlorobiphenyl

R.T.: 9.036 min
Delta R.T.: 0.007 min
Response: 56430790
Conc: 32.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

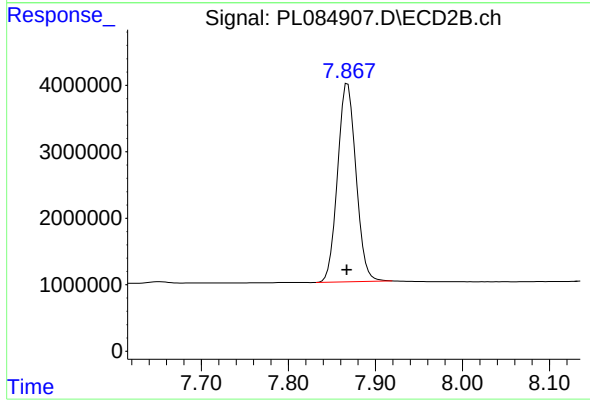

#27 Decachlorobiphenyl

R.T.: 7.868 min
Delta R.T.: 0.001 min
Response: 43946005
Conc: 32.45 ng/ml