

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082223\
 Data File : PL084915.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Aug 2023 11:32
 Operator : AR\AJ
 Sample : 04049-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 00:51:32 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 05:52:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.477	2.685	53725930	24423834	21.431	20.689
27)	SA Decachlor...	9.026	7.865	48462935	37449590	28.279	27.650
Target Compounds							
2)	A alpha-BHC	3.962f	0.000	448439	0	0.124	N.D. #
3)	MA gamma-BHC...	4.254	0.000	383659	0	0.111	N.D. #
6)	B beta-BHC	4.491	0.000	339121	0	0.192	N.D. #
16)	A 4,4'-DDD	6.621f	0.000	111365	0	<MDL	N.D. #
20)	A Methoxychlor	7.472	0.000	217908	0	0.225	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082223\
Data File : PL084915.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2023 11:32
Operator : AR\AJ
Sample : 04049-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 00:51:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

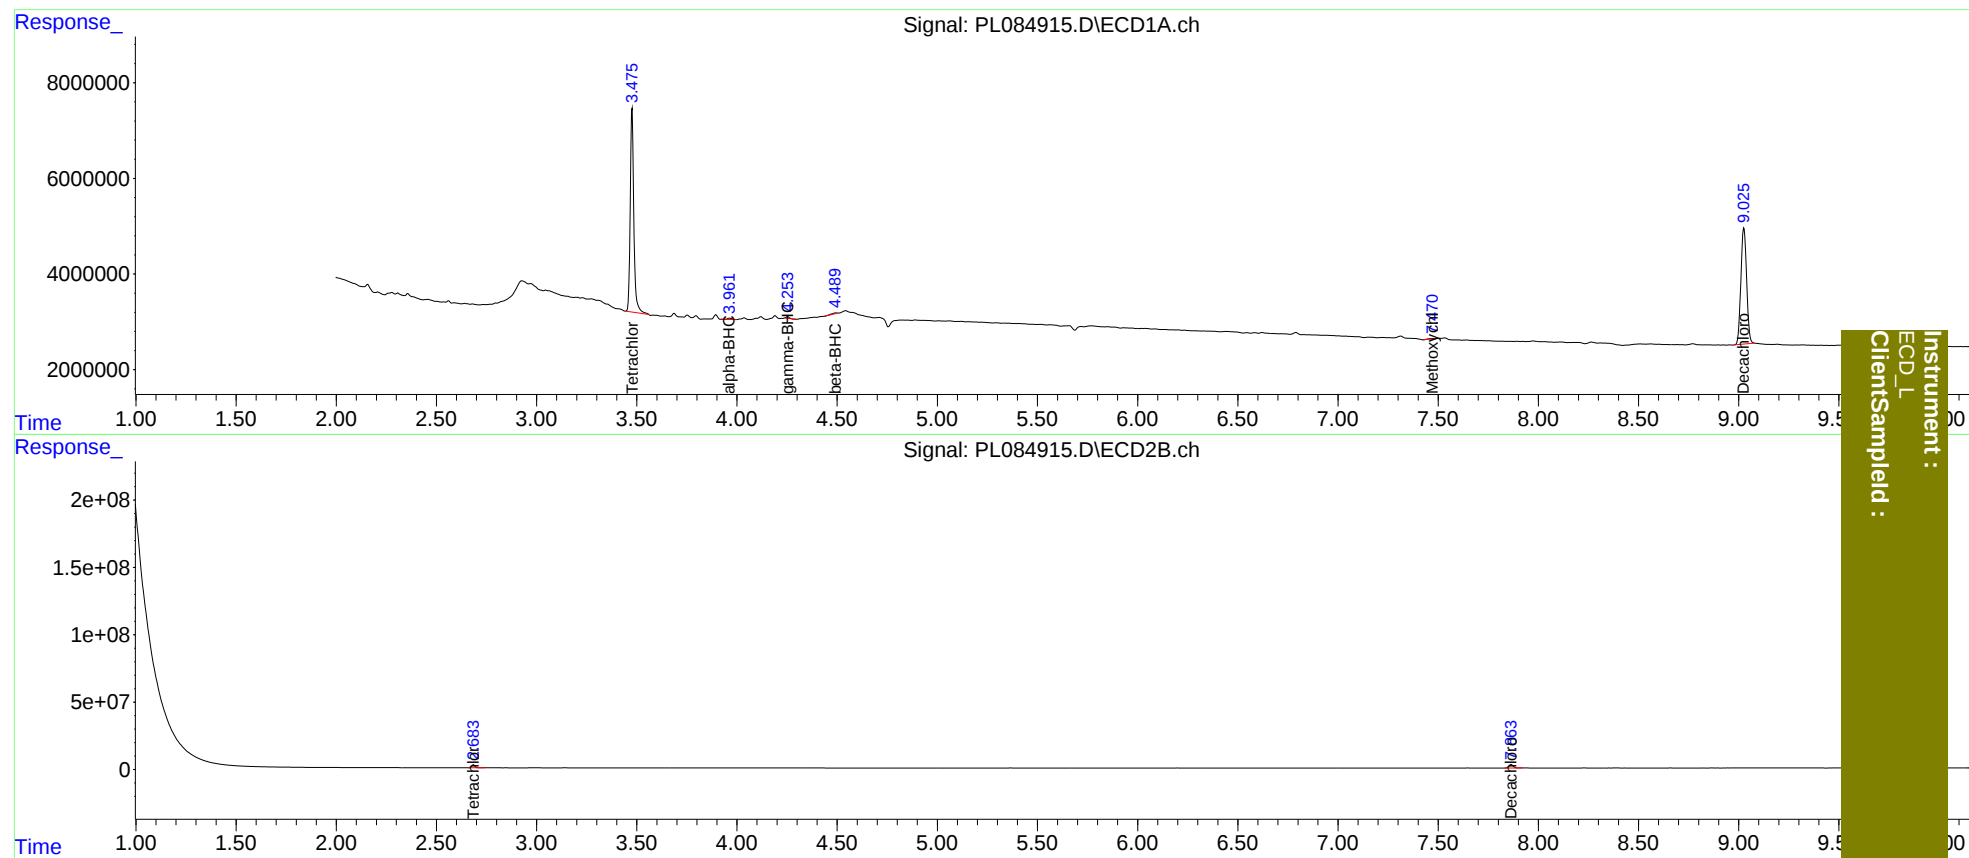


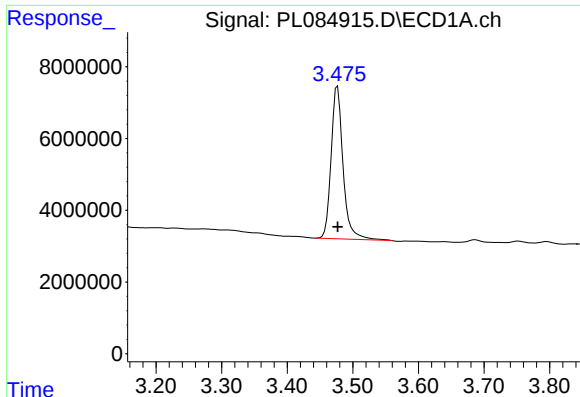

#1 Tetrachloro-m-xylene


R.T.: 3.477 min
Delta R.T.: 0.000 min
Response: 53725930
Conc: 21.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

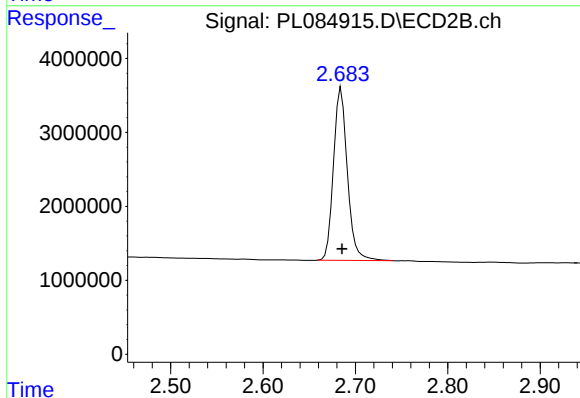


#1 Tetrachloro-m-xylene

R.T.: 2.685 min
Delta R.T.: 0.000 min
Response: 24423834
Conc: 20.69 ng/ml

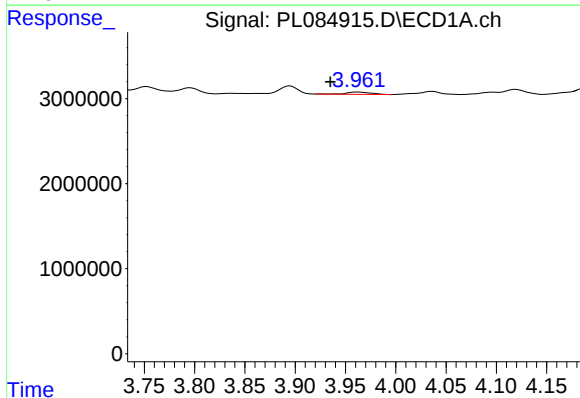


#2 alpha-BHC

R.T.: 3.962 min
Delta R.T.: 0.027 min
Response: 448439
Conc: 0.12 ng/ml

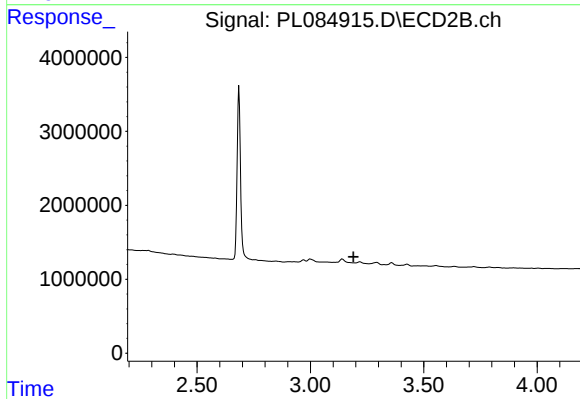

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 3.190 min
Response: 0
Conc: N.D.

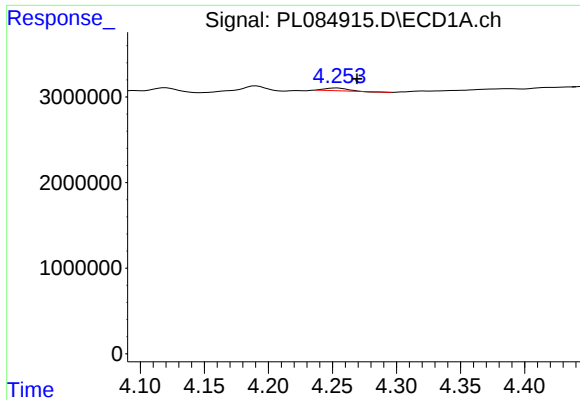

#3 gamma-BHC (Lindane)


R.T.: 4.254 min
Delta R.T.: -0.016 min
Response: 383659
Conc: 0.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

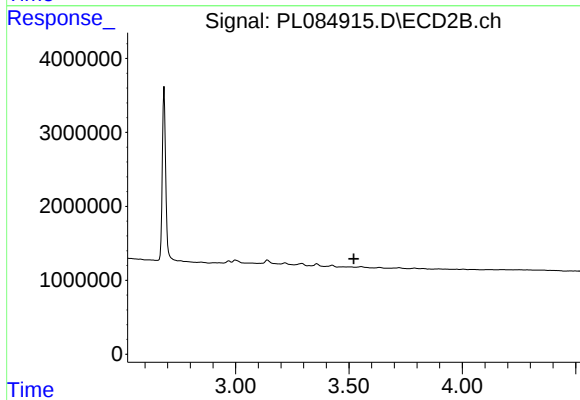


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 3.521 min
Response: 0
Conc: N.D.

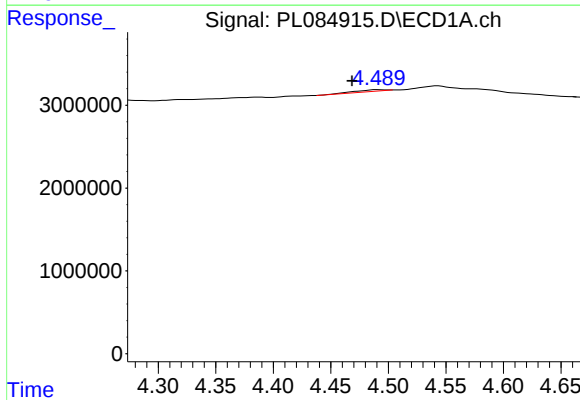


#6 beta-BHC

R.T.: 4.491 min
Delta R.T.: 0.023 min
Response: 339121
Conc: 0.19 ng/ml

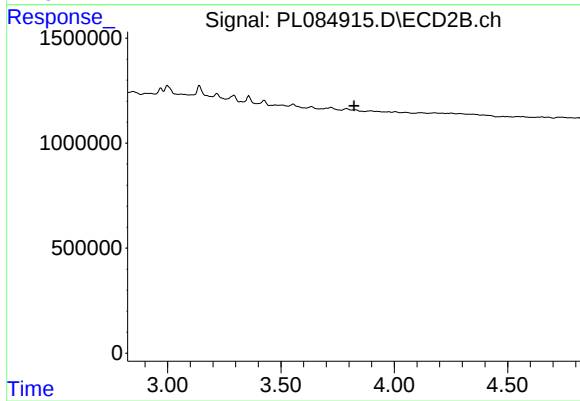

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 3.822 min
Response: 0
Conc: N.D.

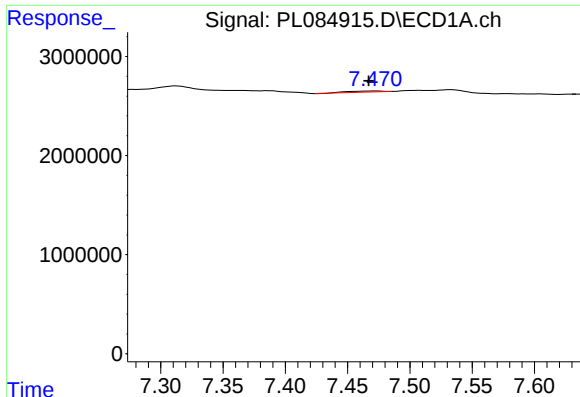

#20 Methoxychlor


R.T.: 7.472 min
Delta R.T.: 0.005 min
Response: 217908
Conc: 0.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

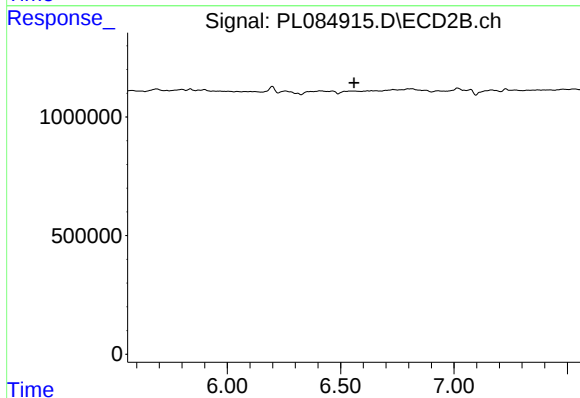


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.559 min
Response: 0
Conc: N.D.

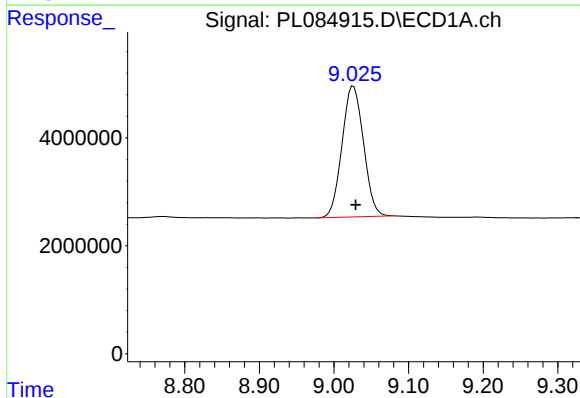

#27 Decachlorobiphenyl

R.T.: 9.026 min
Delta R.T.: -0.003 min
Response: 48462935
Conc: 28.28 ng/ml

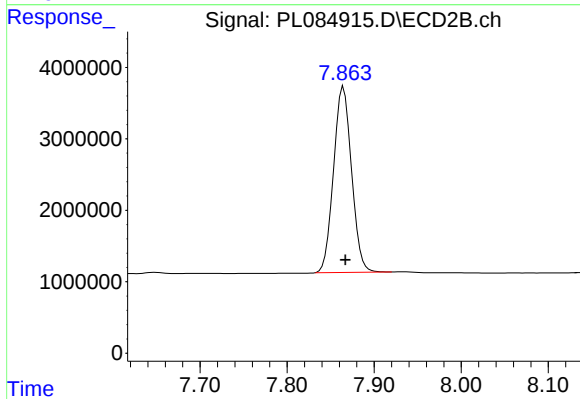

#27 Decachlorobiphenyl

R.T.: 7.865 min
Delta R.T.: -0.002 min
Response: 37449590
Conc: 27.65 ng/ml