

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082223\
Data File : PL084905.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2023 09:07
Operator : AR\AJ
Sample : 03573-02
Misc : PEST MDL WATER
ALS Vial : 6 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
MDL-WATER-QT3-2023-06

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 08/23/2023
Supervised By :Ankita Jodhani 08/23/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 00:48:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

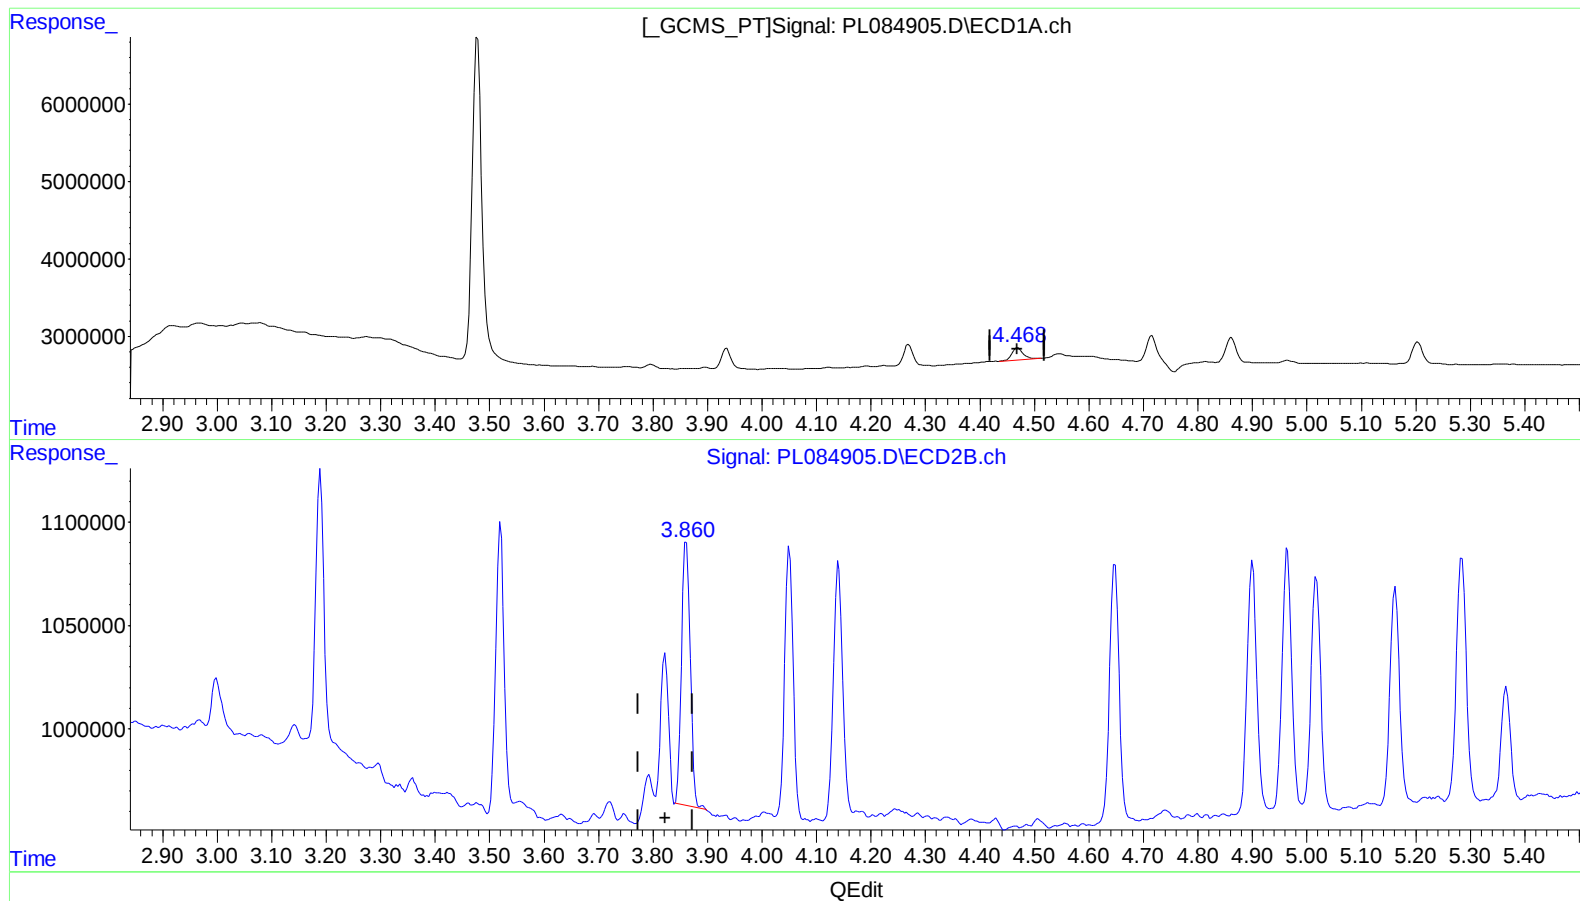

(6) beta-BHC (B)

4.469min 1.267 ng/ml

response 2237844

(6) beta-BHC #2 (B)

3.861min 1.746 ng/ml

response 1434719

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082223\
Data File : PL084905.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2023 09:07
Operator : AR\AJ
Sample : 03573-02
Misc : PEST MDL WATER
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MDL-WATER-QT3-2023-06

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 08/23/2023
Supervised By :Ankita Jodhani 08/23/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 00:48:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

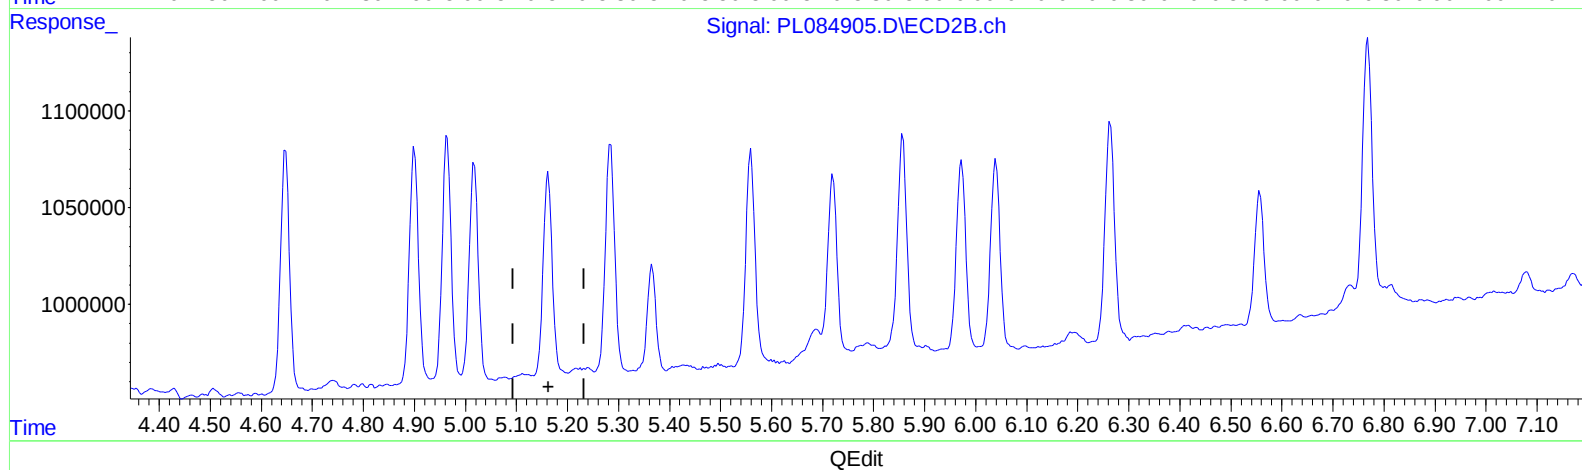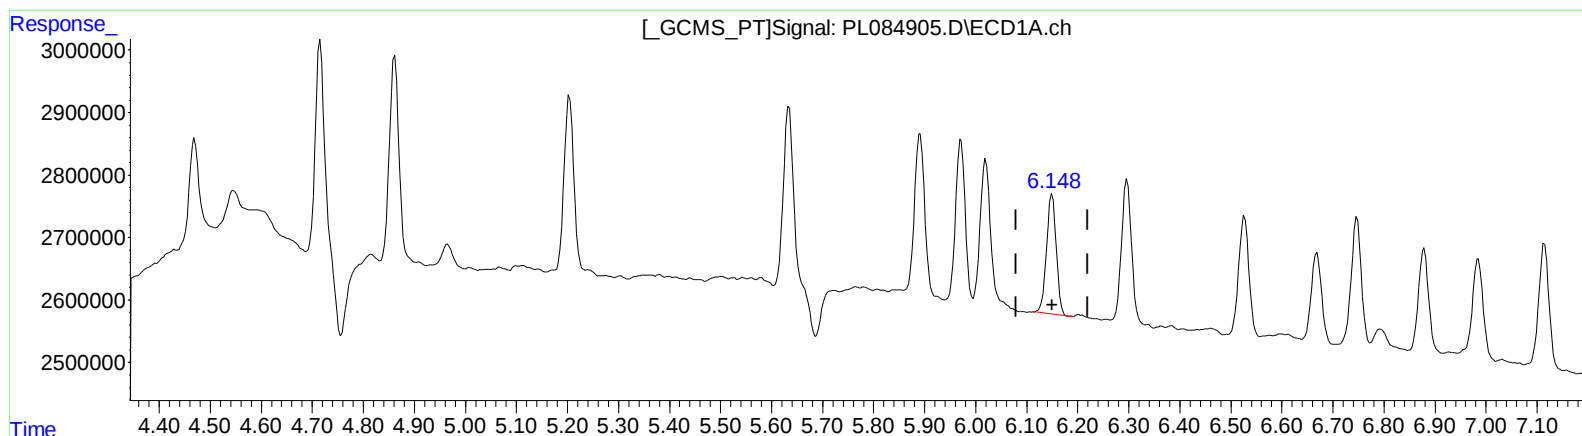

(12) 4,4'-DDE (B)
6.150min 0.952 ng/ml
response 2518933

(12) 4,4'-DDE #2 (B)
0.000min 0.000 ng/ml
response 0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082223\
Data File : PL084905.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2023 09:07
Operator : AR\AJ
Sample : 03573-02
Misc : PEST MDL WATER
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MDL-WATER-QT3-2023-06

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 08/23/2023
Supervised By :Ankita Jodhani 08/23/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 00:48:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

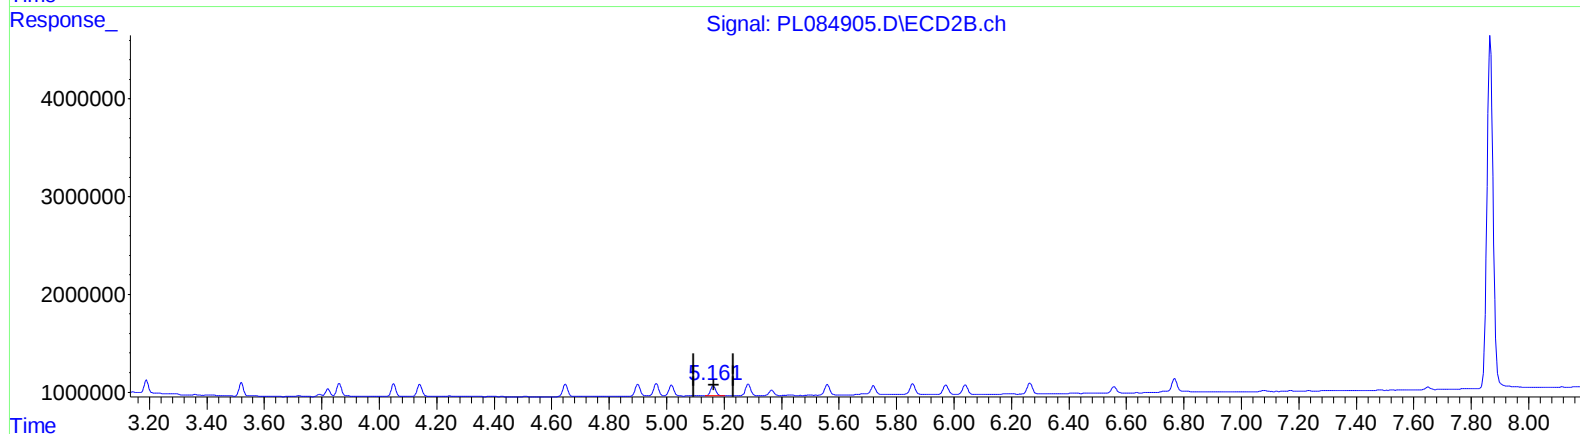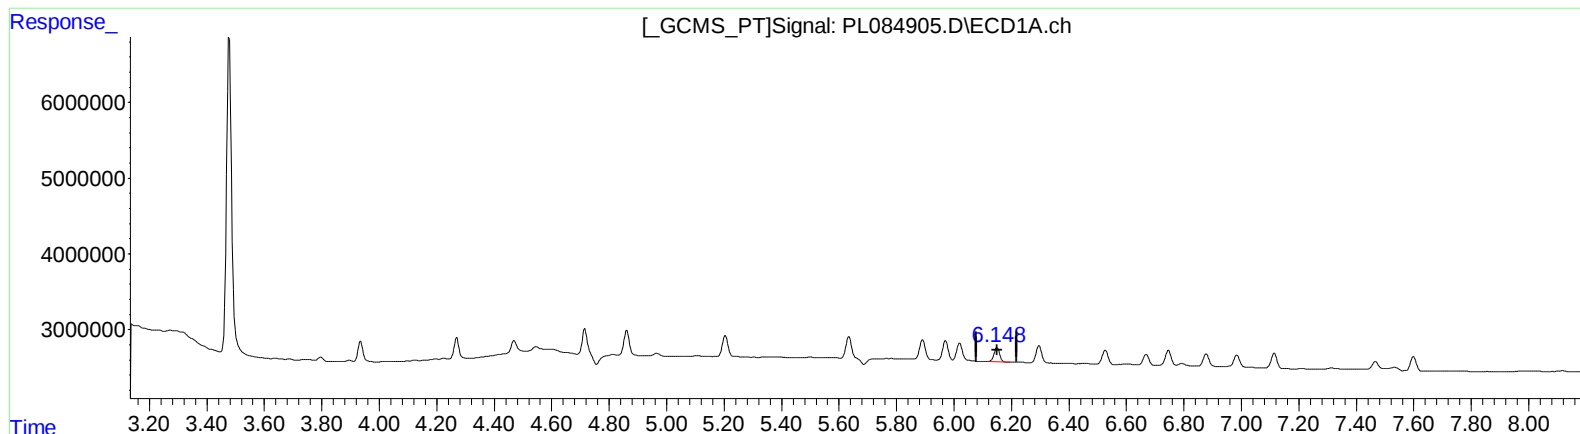

QEdit

(12) 4,4'-DDE (B)

6.150min 0.952 ng/ml

response 2518933

(12) 4,4'-DDE #2 (B)

5.161min 0.887 ng/ml m

response 1299572

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082223\
Data File : PL084905.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2023 09:07
Operator : AR\AJ
Sample : 03573-02
Misc : PEST MDL WATER
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MDL-WATER-QT3-2023-06

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 08/23/2023
Supervised By :Ankita Jodhani 08/23/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 00:48:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

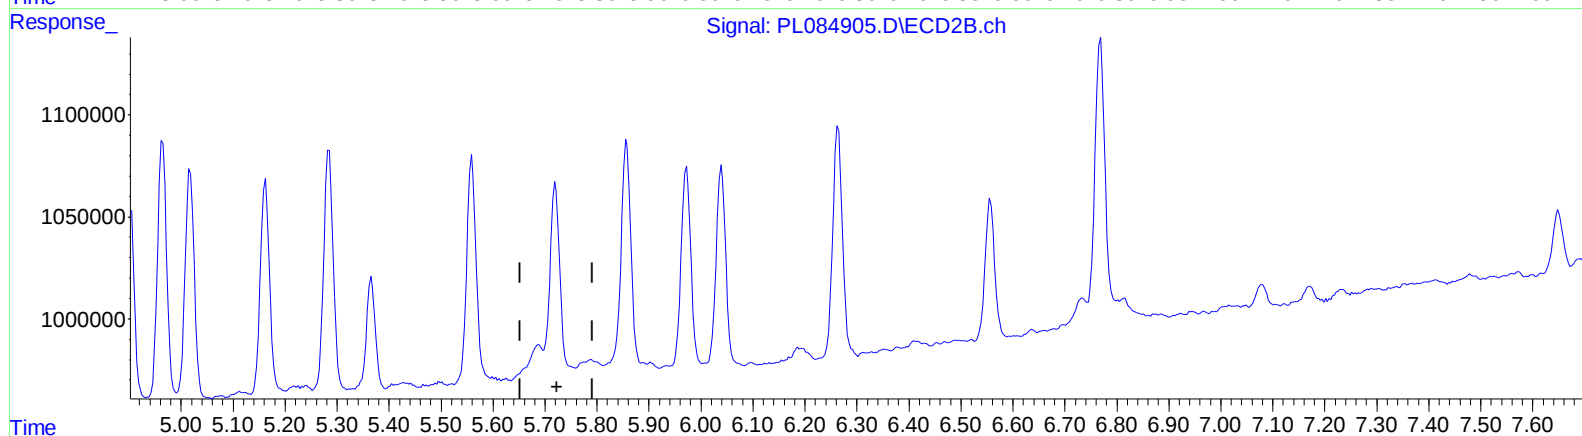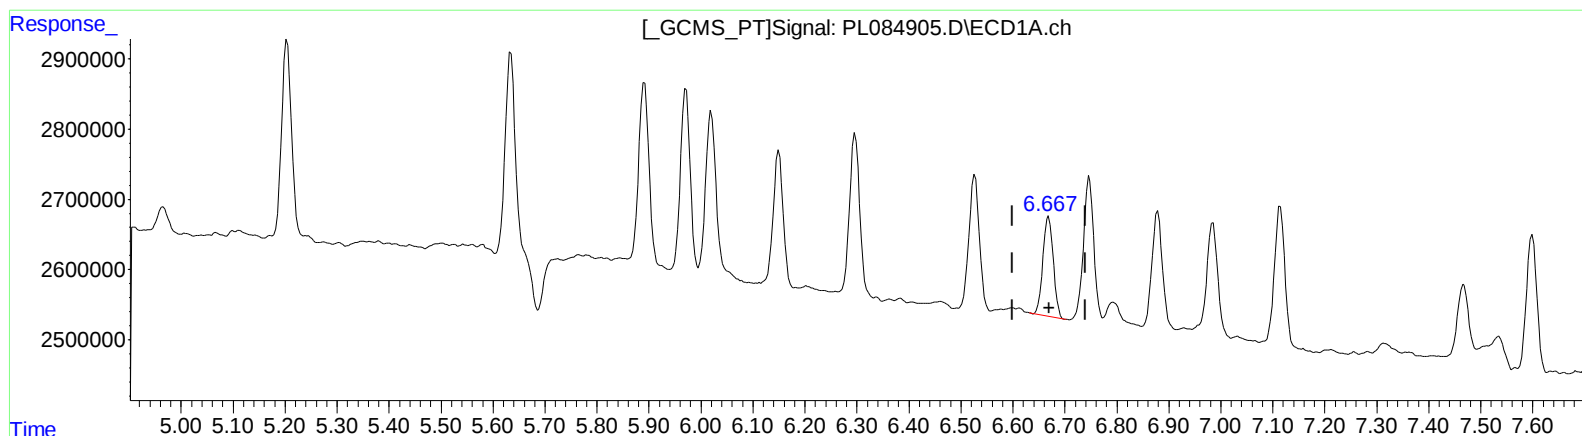

QEdit

(16) 4,4'-DDD (A)
6.669min 1.044 ng/ml
response 1975764

(16) 4,4'-DDD #2 (A)
0.000min 0.000 ng/ml
response 0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082223\
Data File : PL084905.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2023 09:07
Operator : AR\AJ
Sample : 03573-02
Misc : PEST MDL WATER
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MDL-WATER-QT3-2023-06

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 08/23/2023
Supervised By :Ankita Jodhani 08/23/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 00:48:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

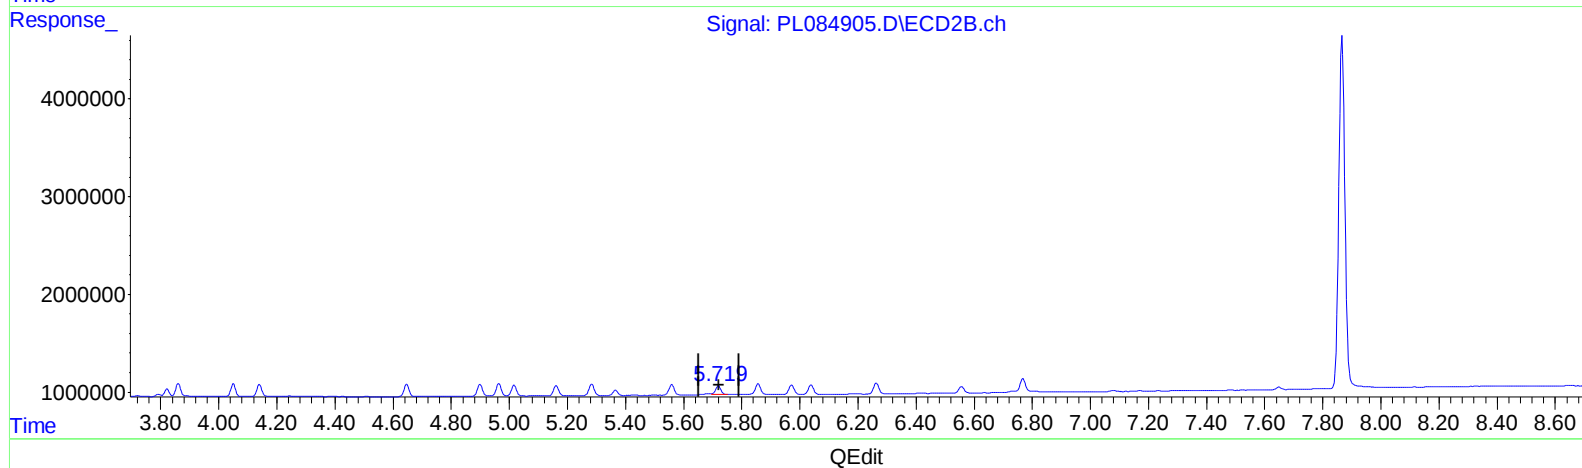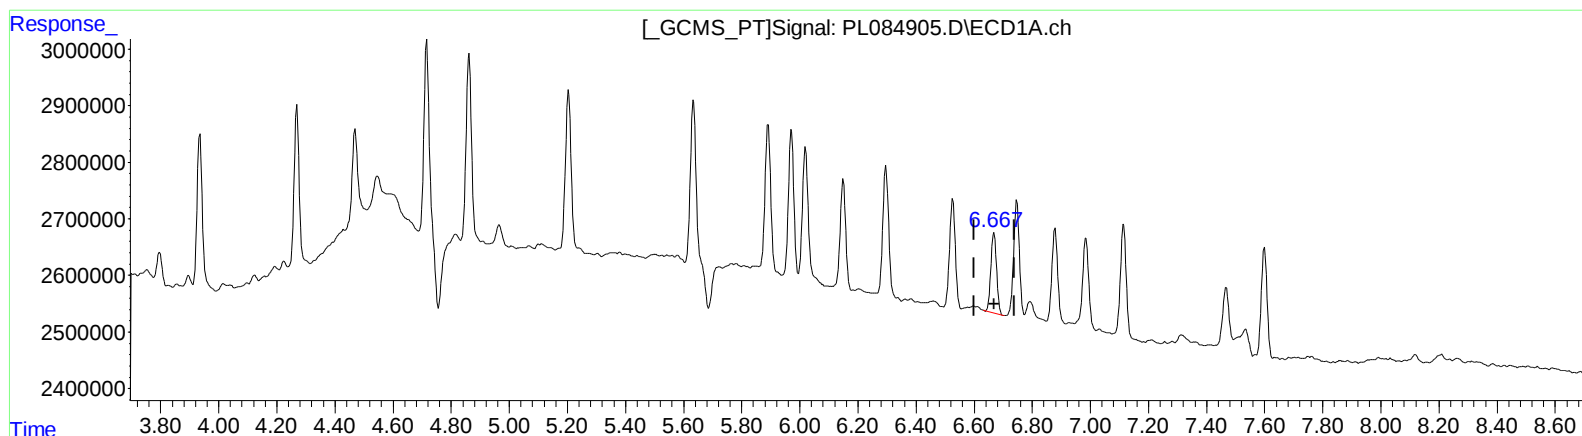

(16) 4,4'-DDD (A)
6.669min 1.044 ng/ml
response 1975764

(16) 4,4'-DDD #2 (A)
5.719min 0.943 ng/ml m
response 1127474

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082223\
Data File : PL084905.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2023 09:07
Operator : AR\AJ
Sample : 03573-02
Misc : PEST MDL WATER
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MDL-WATER-QT3-2023-06

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 08/23/2023
Supervised By :Ankita Jodhani 08/23/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 00:48:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

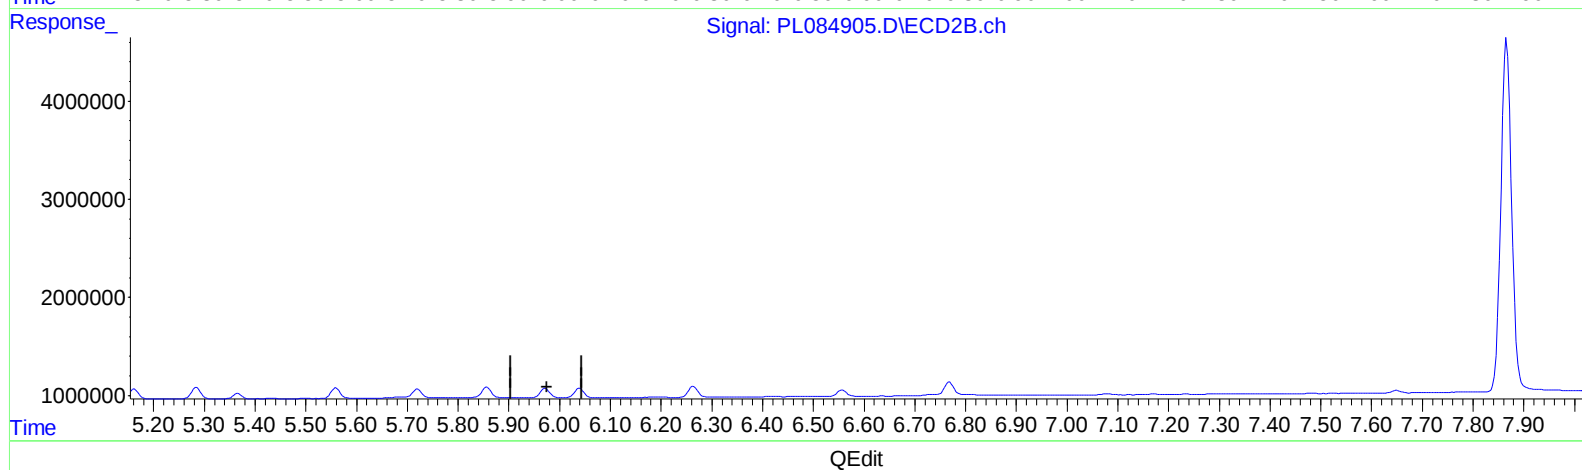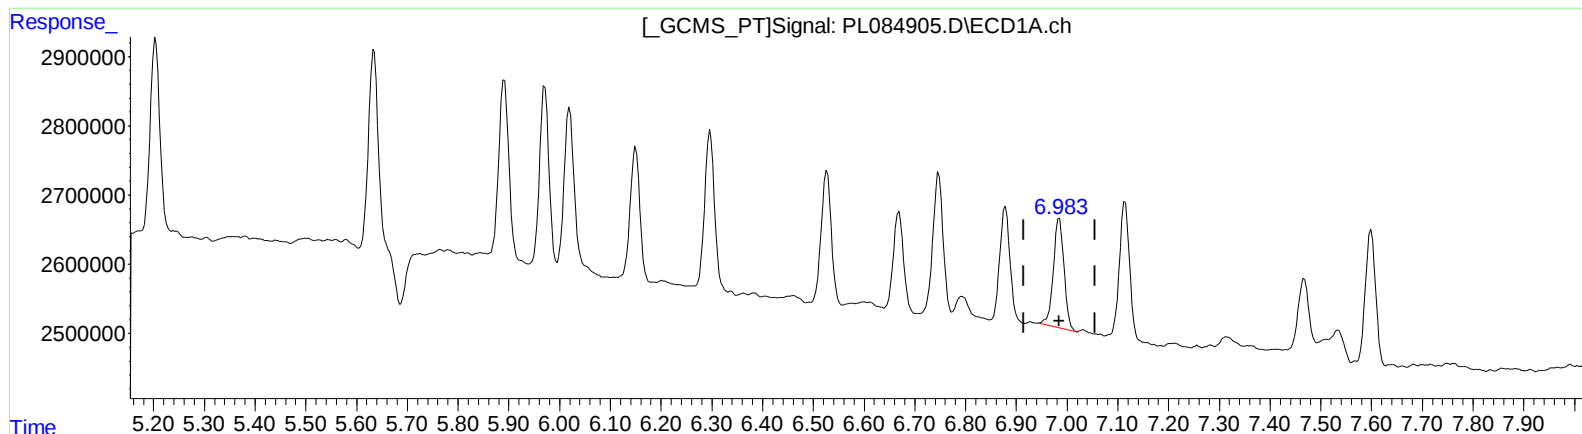

(17) 4,4'-DDT (MA)
6.985min 1.192 ng/ml
response 2298001

(17) 4,4'-DDT #2 (MA)
0.000min 0.000 ng/ml
response 0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082223\
Data File : PL084905.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2023 09:07
Operator : AR\AJ
Sample : 03573-02
Misc : PEST MDL WATER
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MDL-WATER-QT3-2023-06

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 08/23/2023
Supervised By :Ankita Jodhani 08/23/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 00:48:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

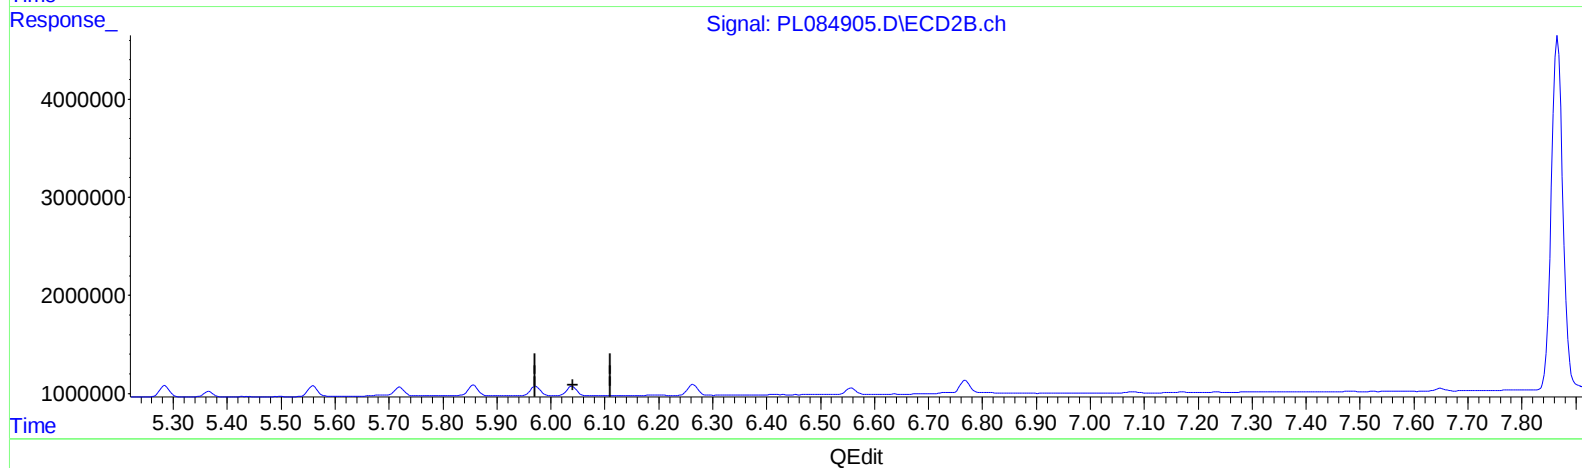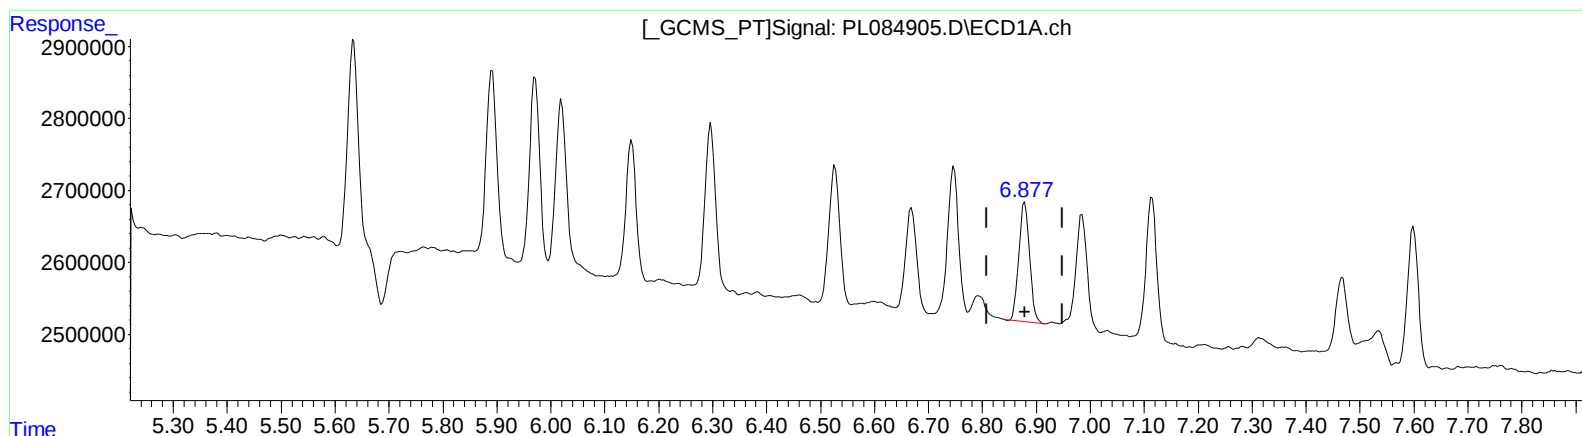

(18) Endrin aldehyde (B)
6.879min 1.232 ng/ml
response 2291645

(18) Endrin aldehyde #2 (B)
0.000min 0.000 ng/ml
response 0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082223\
Data File : PL084905.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2023 09:07
Operator : AR\AJ
Sample : 03573-02
Misc : PEST MDL WATER
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MDL-WATER-QT3-2023-06

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 08/23/2023
Supervised By :Ankita Jodhani 08/23/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 00:48:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

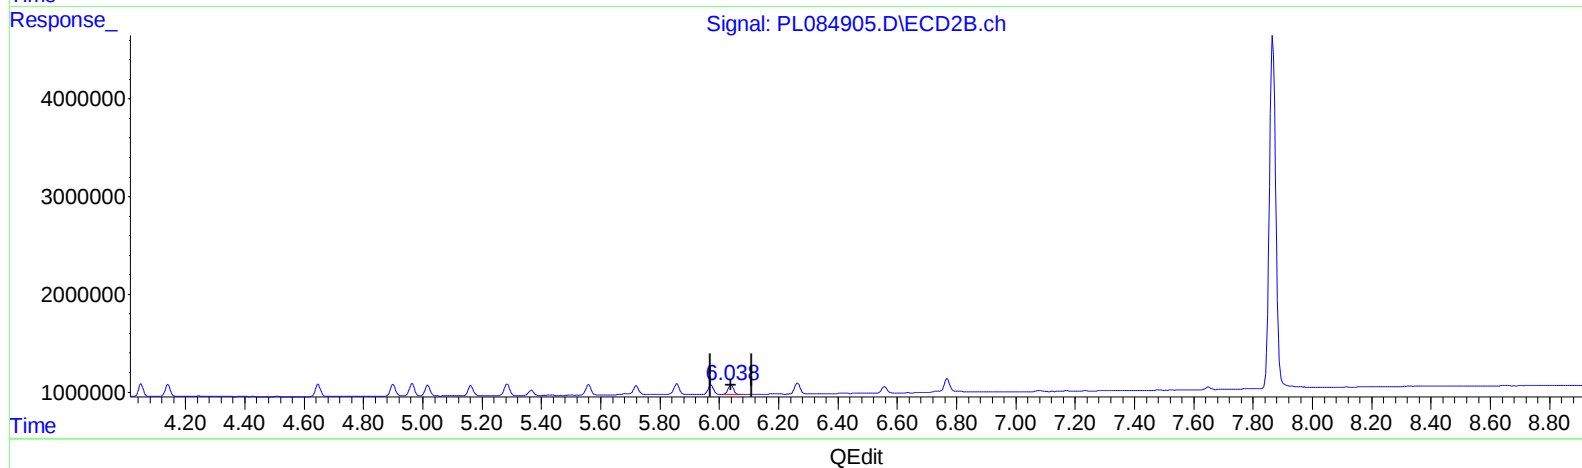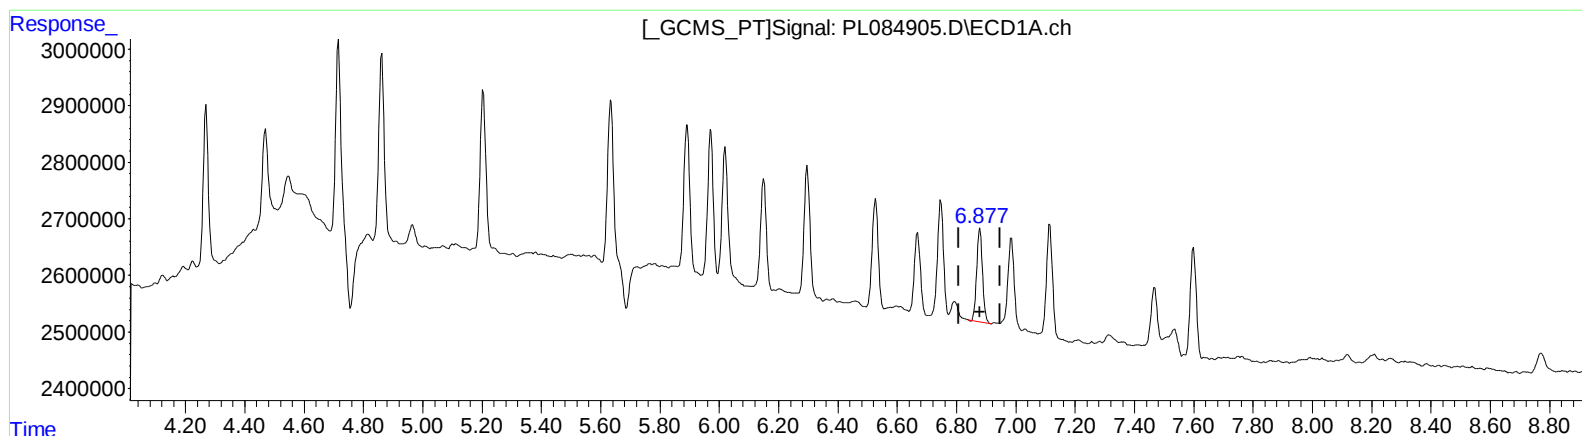

(18) Endrin aldehyde (B)

6.879min 1.232 ng/ml

response 2291645

(18) Endrin aldehyde #2 (B)

6.038min 1.082 ng/ml m

response 1229777

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082223\
Data File : PL084905.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2023 09:07
Operator : AR\AJ
Sample : 03573-02
Misc : PEST MDL WATER
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MDL-WATER-QT3-2023-06

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 08/23/2023
Supervised By :Ankita Jodhani 08/23/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 00:48:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

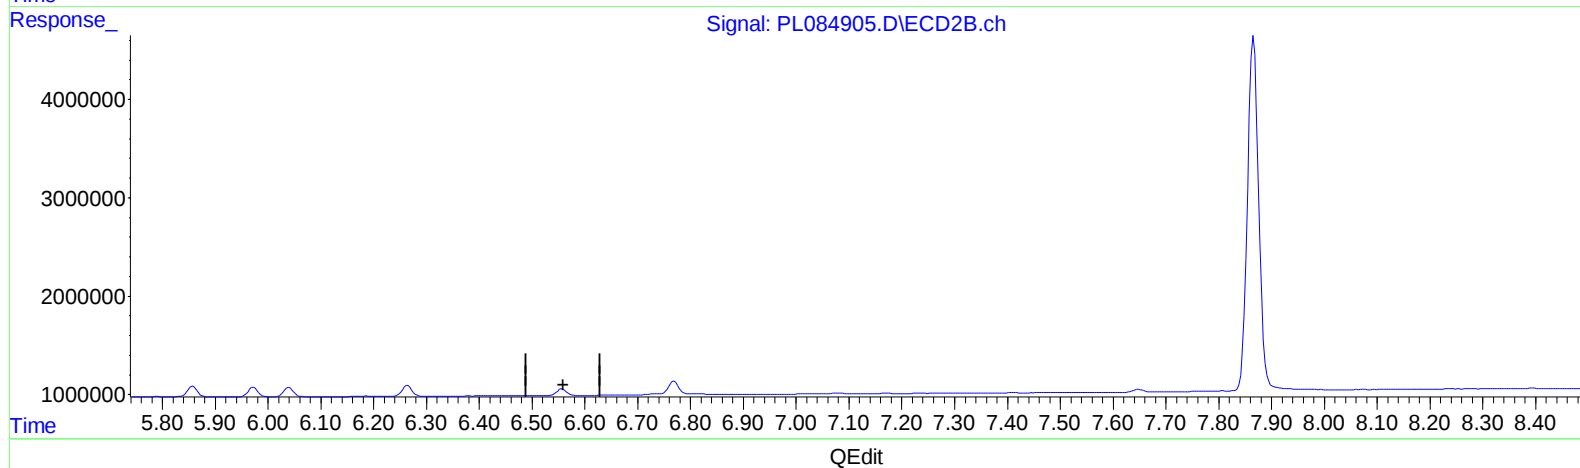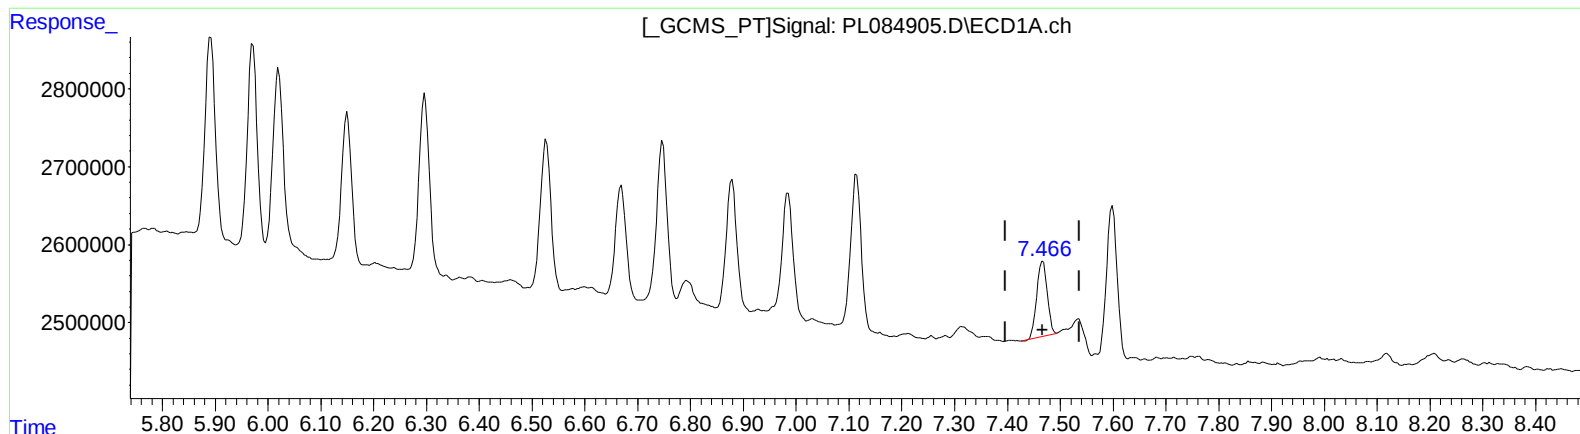

(20) Methoxychlor (A)

7.467min 1.363 ng/ml

response 1322011

(20) Methoxychlor #2 (A)

0.000min 0.000 ng/ml

response 0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082223\
 Data File : PL084905.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Aug 2023 09:07
 Operator : AR\AJ
 Sample : 03573-02
 Misc : PEST MDL WATER
 ALS Vial : 6 Sample Multiplier: 1



Instrument :
 ECD_L
 ClientSampleId :
 MDL-WATER-QT3-2023-06

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 08/23/2023
 Supervised By :Ankita Jodhani 08/23/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 00:48:07 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 05:52:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

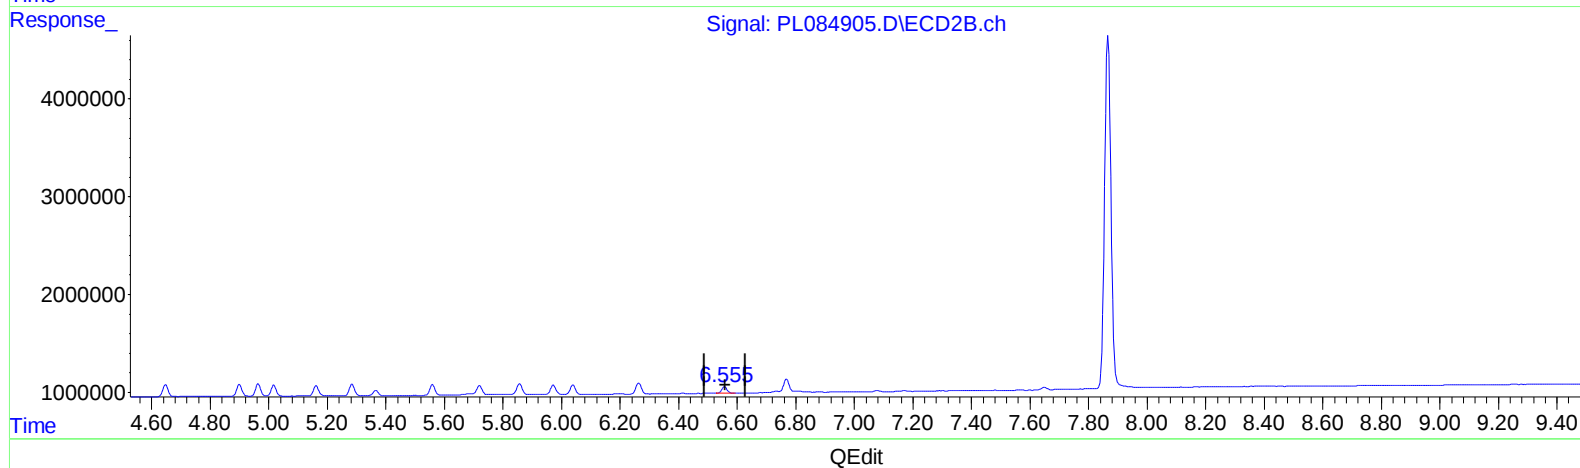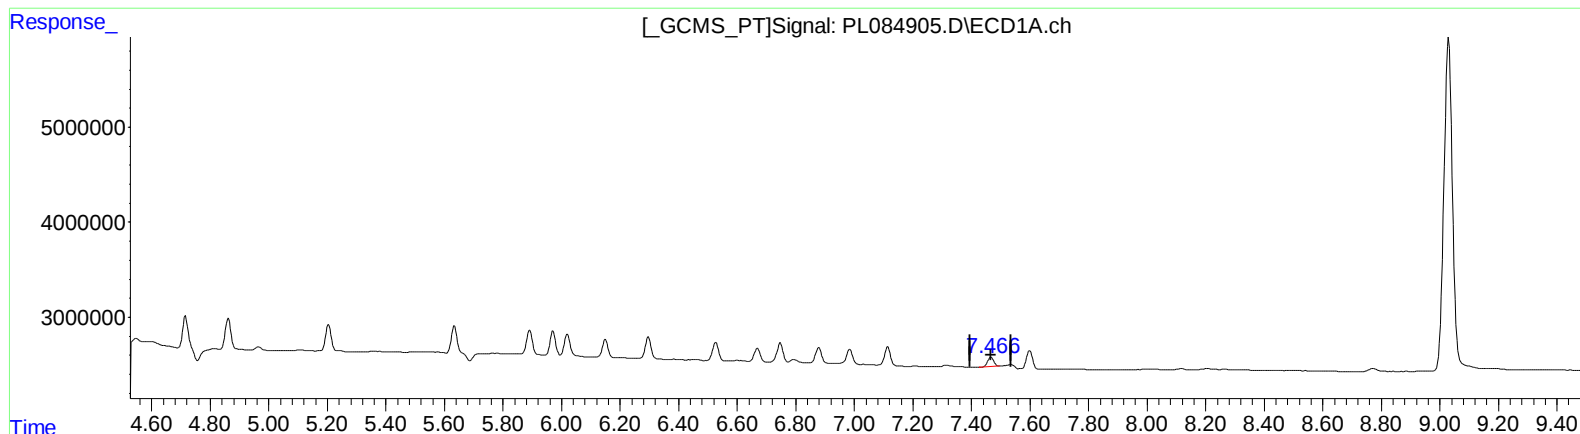

(20) Methoxychlor (A)

7.467min 1.363 ng/ml

response 1322011

(20) Methoxychlor #2 (A)

6.555min 1.244 ng/ml m

response 880630