

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082318\
 Data File : PL039464.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2018 14:49
 Operator : AJ\SJ
 Sample : J4606-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 24 03:38:31 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.303	3.906	151.4E6	65877755	21.658	24.573
28)	SA Decachlor...	7.959	8.893	103.7E6	43704695	14.767	18.833 #
Target Compounds							
6)	B beta-BHC	4.217f	0.000	9095561	0	1.958	N.D. #
7)	B delta-BHC	0.000	4.956	0	6948813	N.D.	1.745 #
8)	B Heptachlo...	4.915f	0.000	1670948	0	0.175	N.D. #
23)	Chlordane-1	4.158	0.000	10988243	0	34.708	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082318\
Data File : PL039464.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2018 14:49
Operator : AJ\SJ
Sample : J4606-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 03:38:31 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

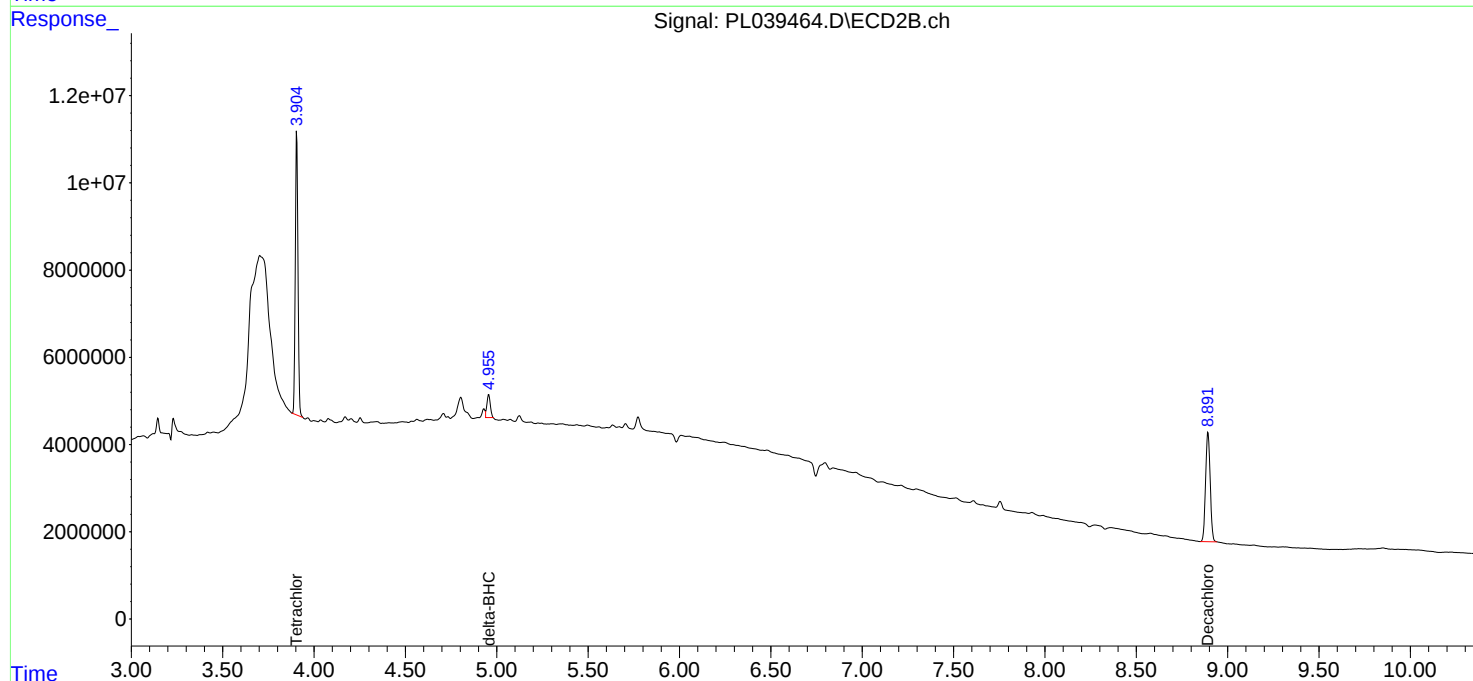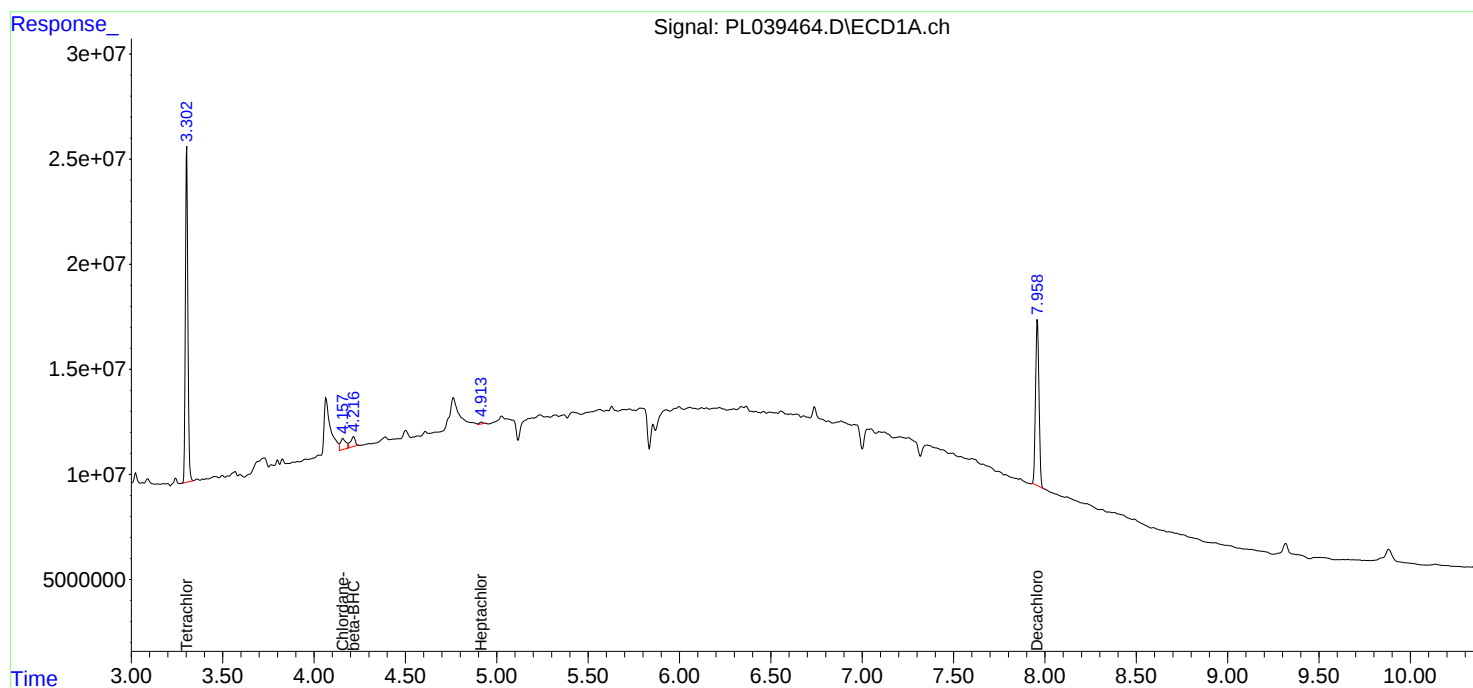


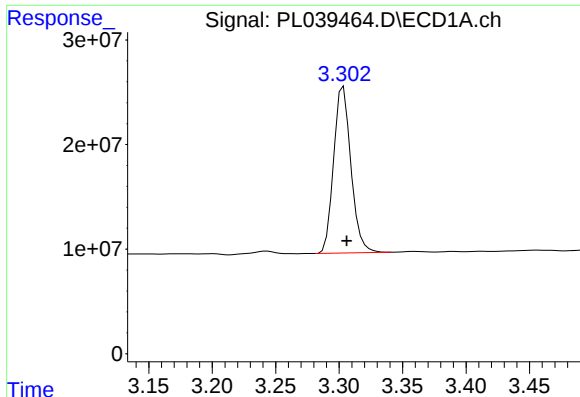

#1 Tetrachloro-m-xylene


R.T.: 3.303 min
Delta R.T.: -0.003 min
Response: 151398980
Conc: 21.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

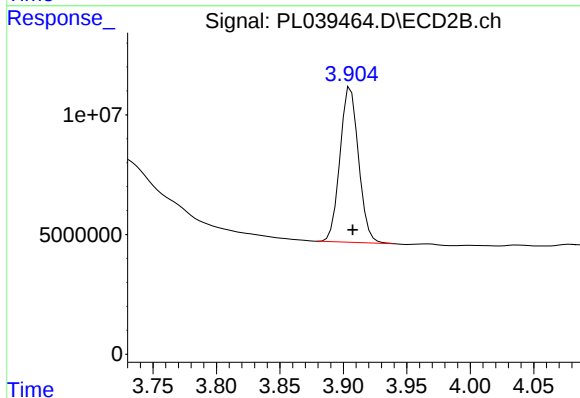


#1 Tetrachloro-m-xylene

R.T.: 3.906 min
Delta R.T.: -0.001 min
Response: 65877755
Conc: 24.57 ng/ml

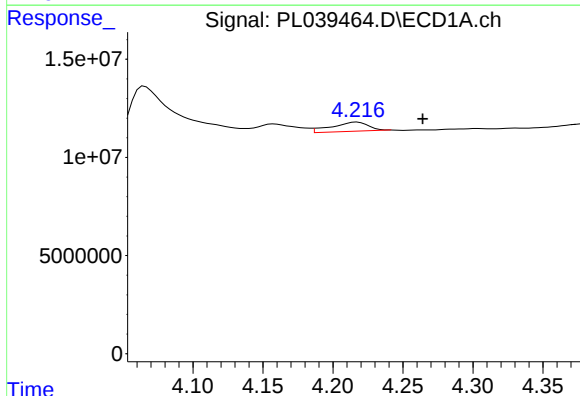


#6 beta-BHC

R.T.: 4.217 min
Delta R.T.: -0.047 min
Response: 9095561
Conc: 1.96 ng/ml

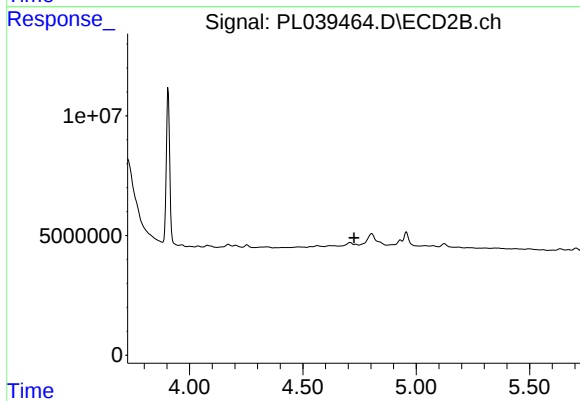

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.726 min
Response: 0
Conc: N.D.

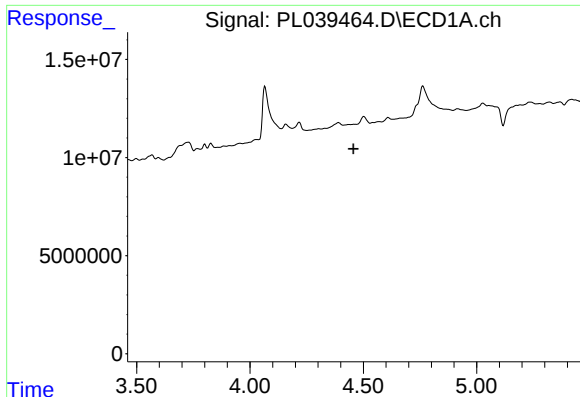

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.457 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

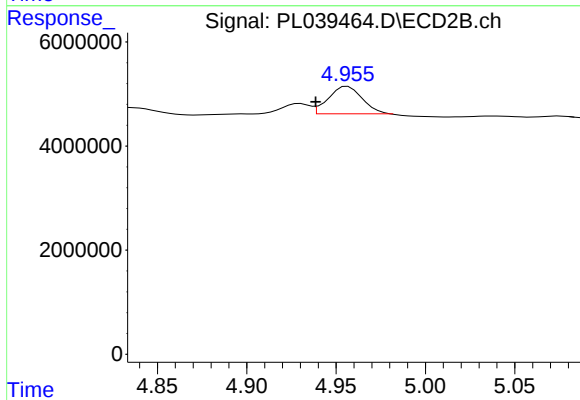


#7 delta-BHC

R.T.: 4.956 min
Delta R.T.: 0.018 min
Response: 6948813
Conc: 1.75 ng/ml

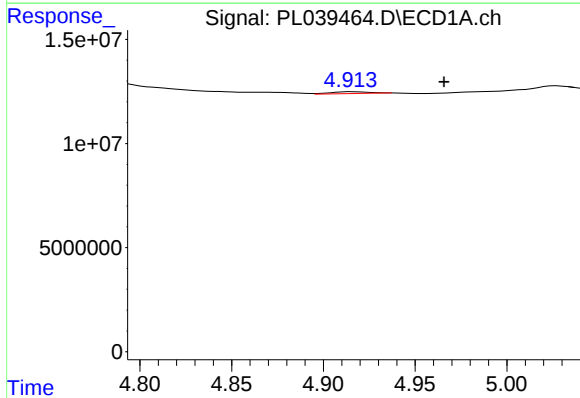


#8 Heptachlor epoxide

R.T.: 4.915 min
Delta R.T.: -0.050 min
Response: 1670948
Conc: 0.17 ng/ml

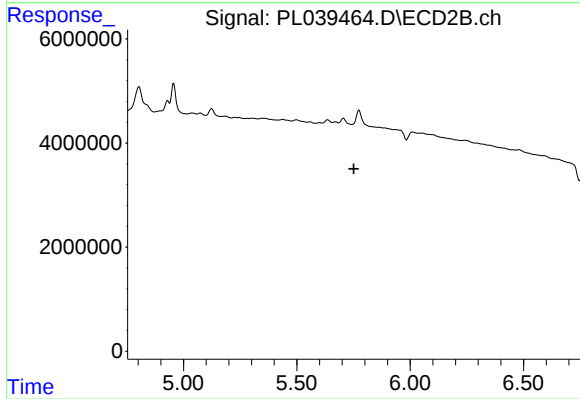

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.751 min
Response: 0
Conc: N.D.

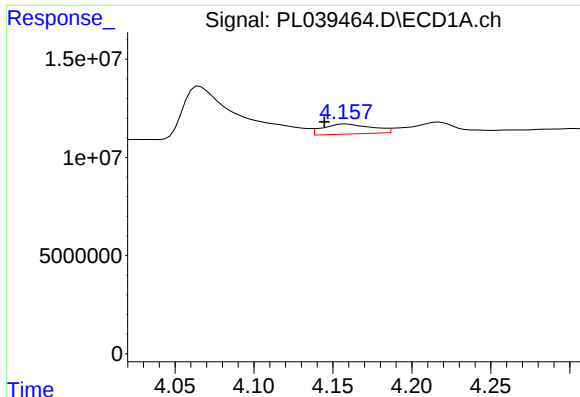

#23 Chlordane-1


R.T.: 4.158 min
Delta R.T.: 0.013 min
Response: 10988243
Conc: 34.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

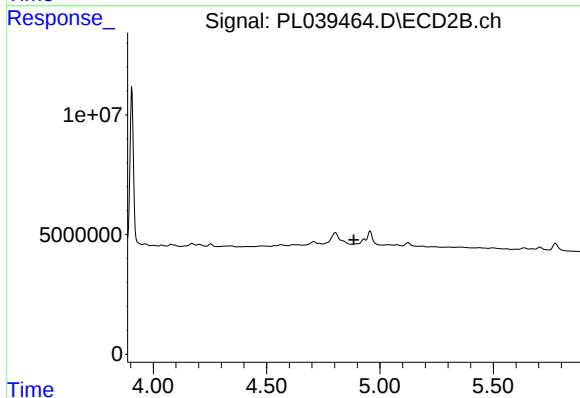


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.885 min
Response: 0
Conc: N.D.

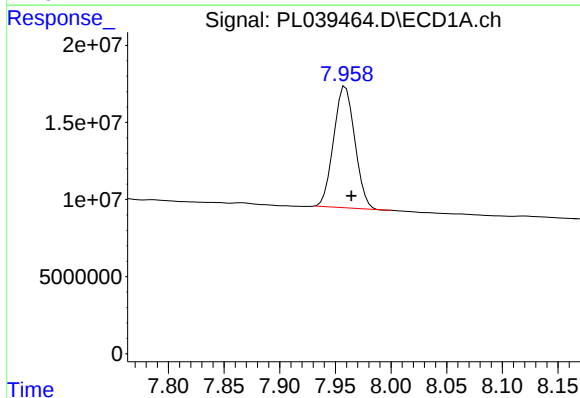

#28 Decachlorobiphenyl

R.T.: 7.959 min
Delta R.T.: -0.005 min
Response: 103715428
Conc: 14.77 ng/ml

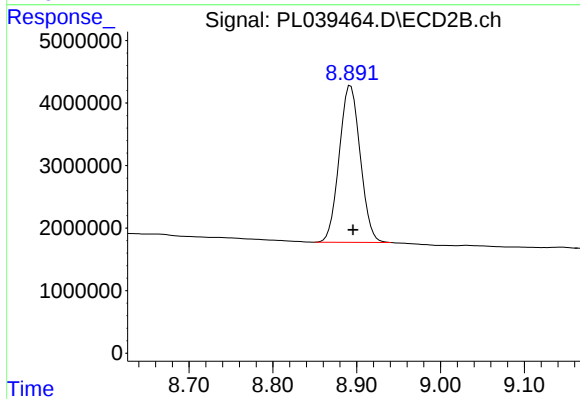

#28 Decachlorobiphenyl

R.T.: 8.893 min
Delta R.T.: -0.003 min
Response: 43704695
Conc: 18.83 ng/ml