

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082318\
 Data File : PL039468.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2018 15:45
 Operator : AJ\SJ
 Sample : J4608-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 24 03:40:02 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.304	3.906	149.3E6	64360552	21.358	24.007
28)	SA Decachlor...	7.959	8.894	107.8E6	43702369	15.348	18.832
Target Compounds							
5)	MB Aldrin	4.514	0.000	11513468	0	1.150	N.D. #
6)	B beta-BHC	4.216f	0.000	10008317	0	2.154	N.D. #
7)	B delta-BHC	0.000	4.956	0	9604462	N.D.	2.412 #
12)	B 4,4'-DDE	5.409	0.000	6017449	0	0.628	N.D. #
16)	A 4,4'-DDD	5.920	0.000	5509845	0	0.691	N.D. #
17)	MA 4,4'-DDT	6.148	0.000	5855919	0	0.772	N.D. #
20)	A Methoxychlor	6.673	0.000	11205419	0	2.738	N.D. #
23)	Chlordane-1	4.165	0.000	9915742	0	31.321	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082318\
Data File : PL039468.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2018 15:45
Operator : AJ\SJ
Sample : J4608-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 03:40:02 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

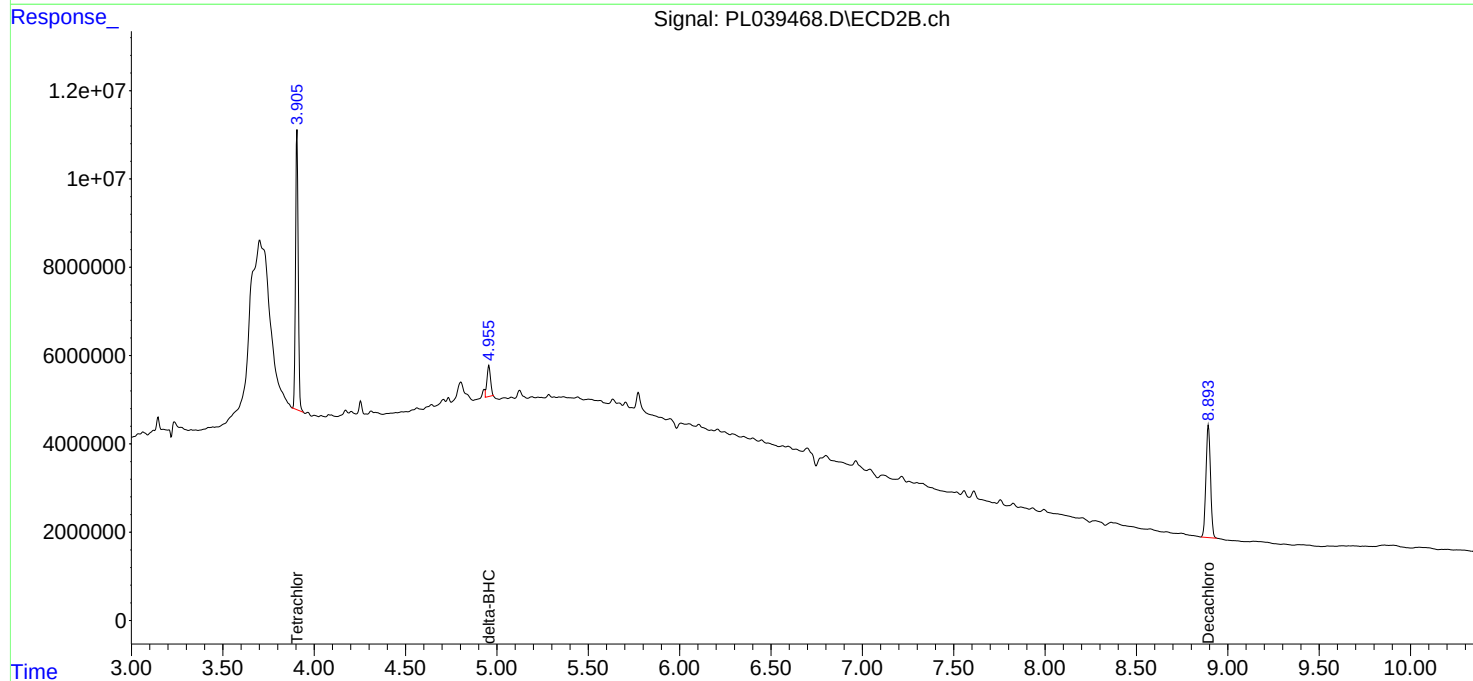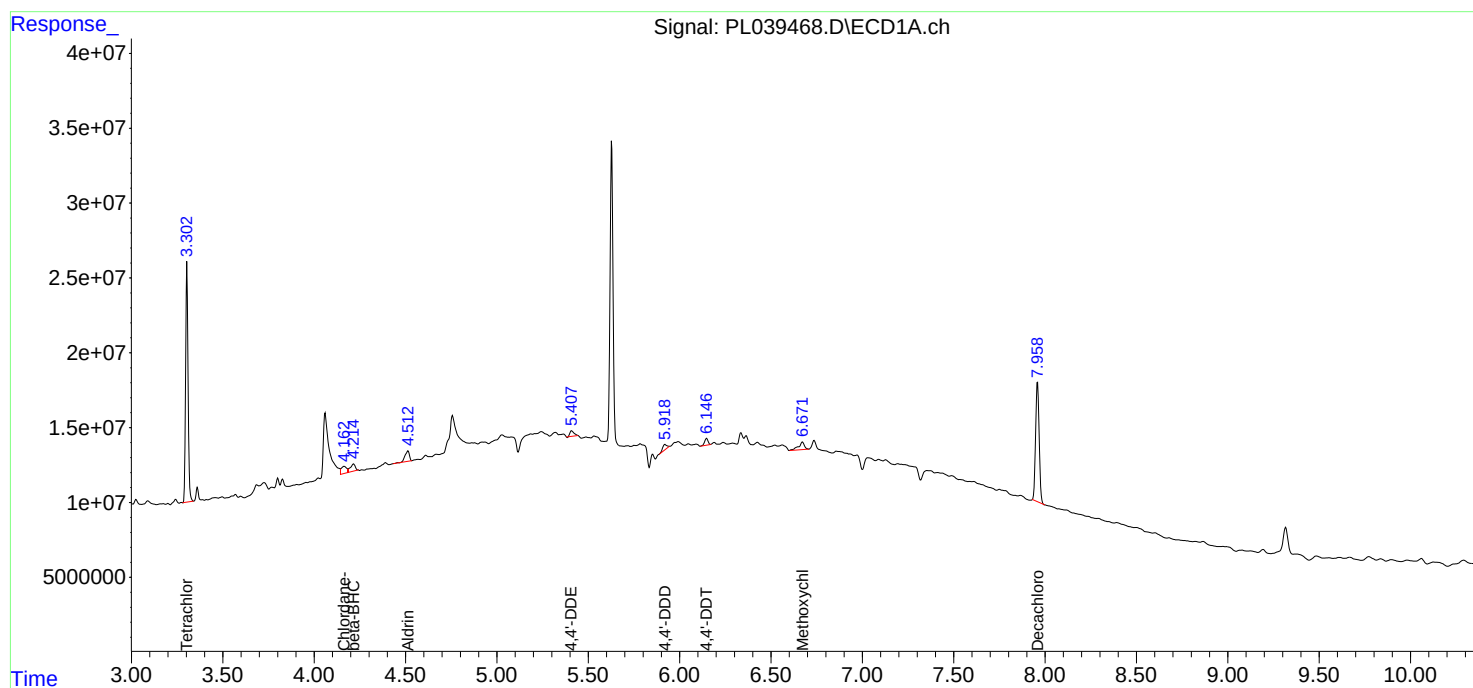


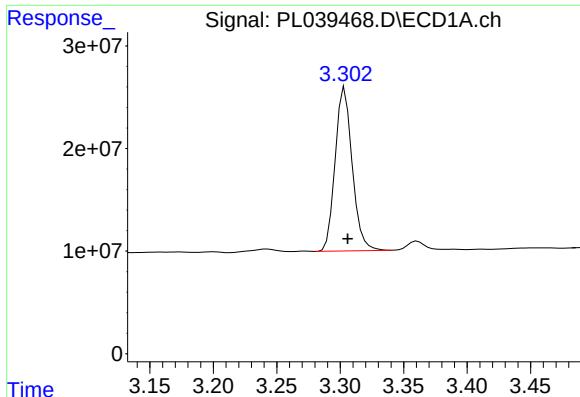

#1 Tetrachloro-m-xylene


R.T.: 3.304 min
Delta R.T.: -0.002 min
Response: 149300808
Conc: 21.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

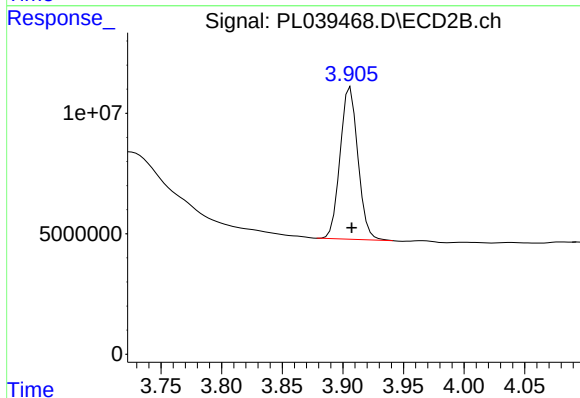


#1 Tetrachloro-m-xylene

R.T.: 3.906 min
Delta R.T.: -0.001 min
Response: 64360552
Conc: 24.01 ng/ml

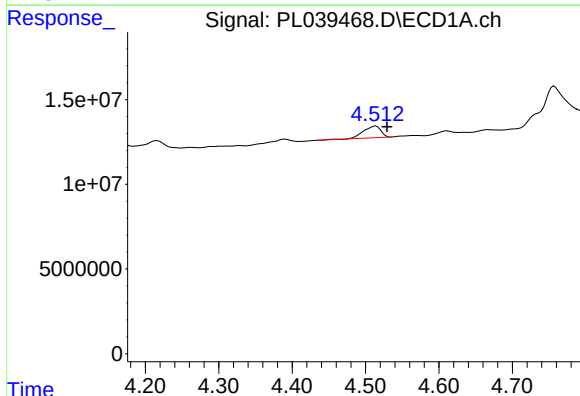


#5 Aldrin

R.T.: 4.514 min
Delta R.T.: -0.015 min
Response: 11513468
Conc: 1.15 ng/ml

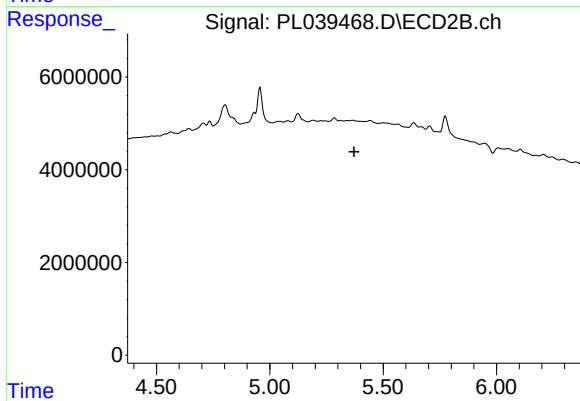

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.372 min
Response: 0
Conc: N.D.

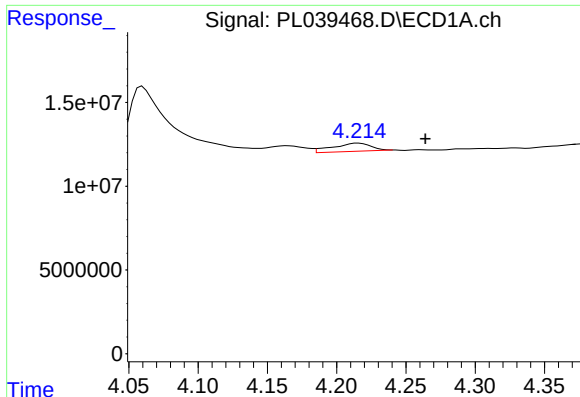

#6 beta-BHC


R.T.: 4.216 min
Delta R.T.: -0.048 min
Response: 10008317
Conc: 2.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

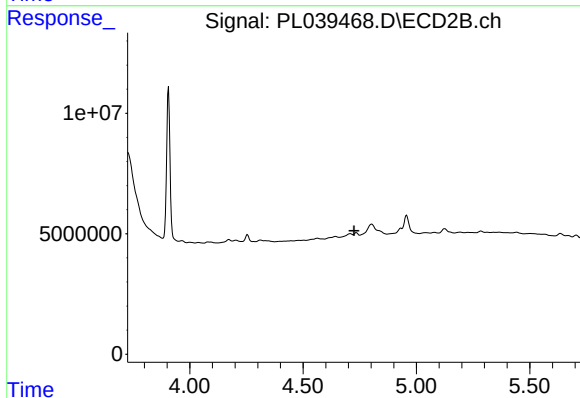


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

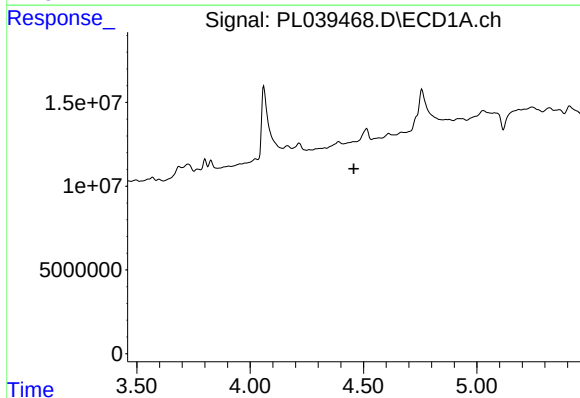


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.457 min
Response: 0
Conc: N.D.

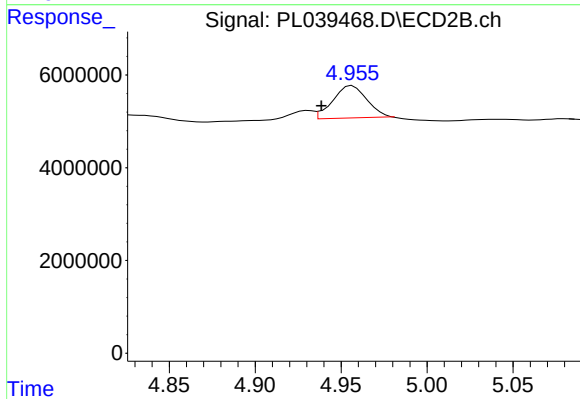

#7 delta-BHC


R.T.: 4.956 min
Delta R.T.: 0.018 min
Response: 9604462
Conc: 2.41 ng/ml

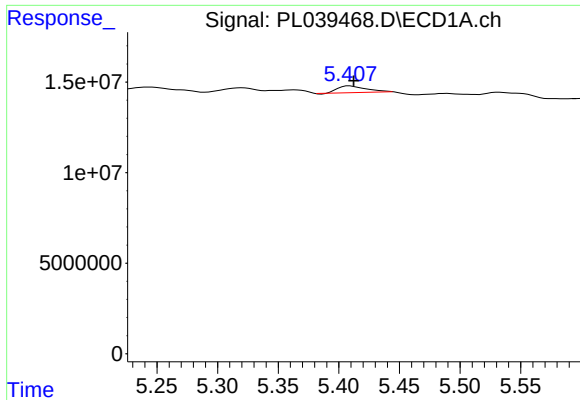

#12 4,4'-DDE


R.T.: 5.409 min
Delta R.T.: -0.003 min
Response: 6017449
Conc: 0.63 ng/ml

Instrument :
ECD_L
ClientSampleId :

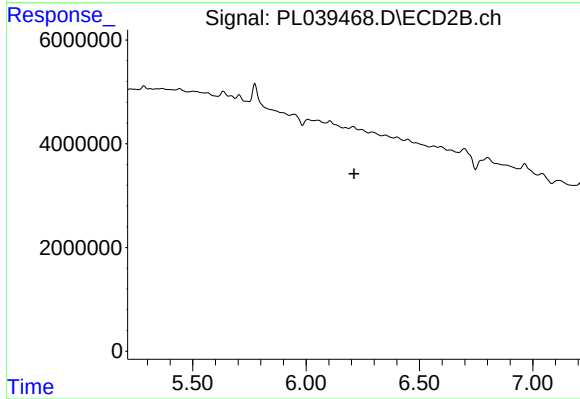


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.212 min
Response: 0
Conc: N.D.

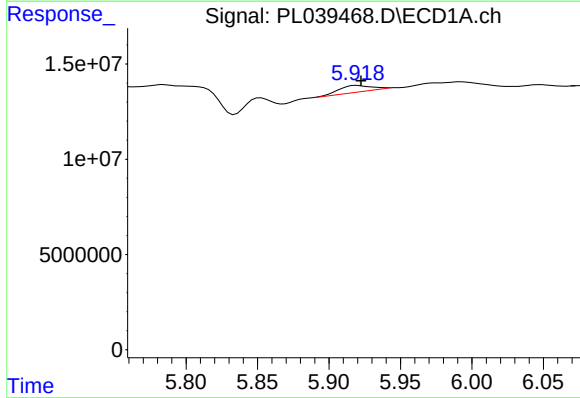


#16 4,4'-DDD

R.T.: 5.920 min
Delta R.T.: -0.003 min
Response: 5509845
Conc: 0.69 ng/ml

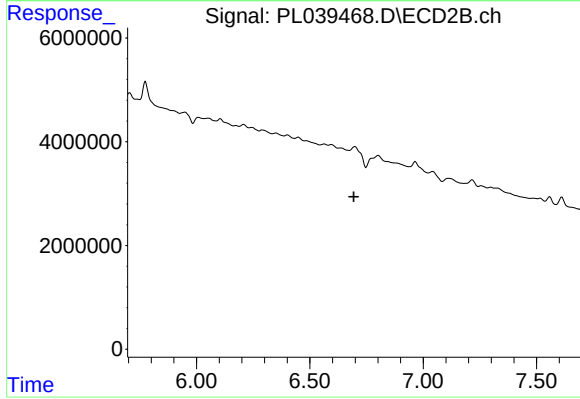

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.693 min
Response: 0
Conc: N.D.

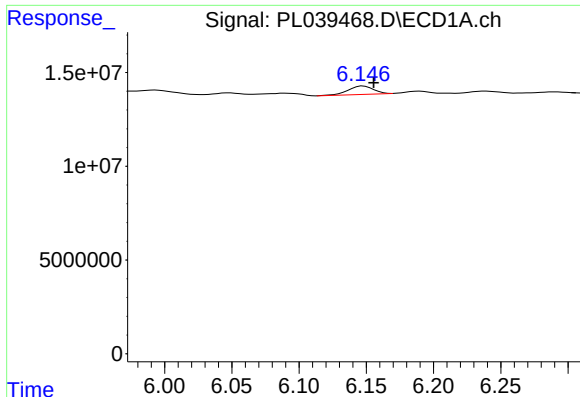

#17 4,4'-DDT


R.T.: 6.148 min
Delta R.T.: -0.008 min
Response: 5855919
Conc: 0.77 ng/ml

Instrument :
ECD_L
ClientSampleId :

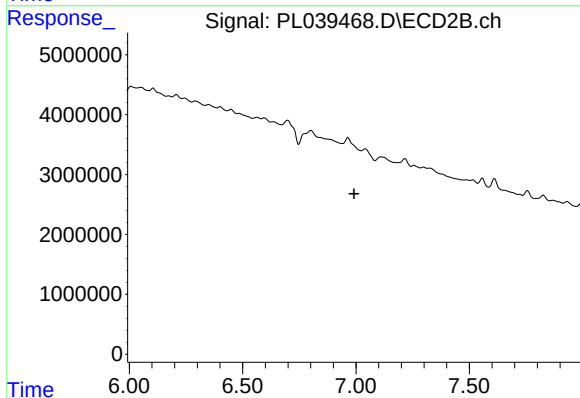


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.991 min
Response: 0
Conc: N.D.

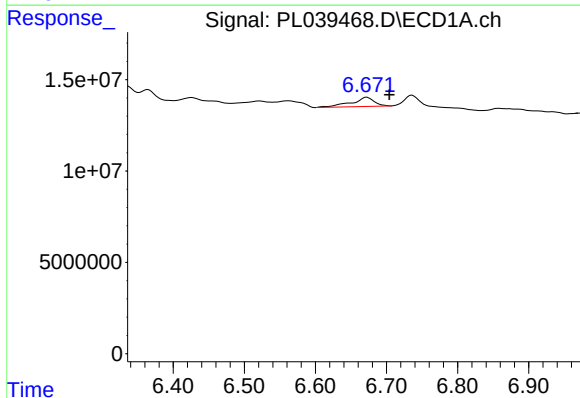


#20 Methoxychlor

R.T.: 6.673 min
Delta R.T.: -0.031 min
Response: 11205419
Conc: 2.74 ng/ml

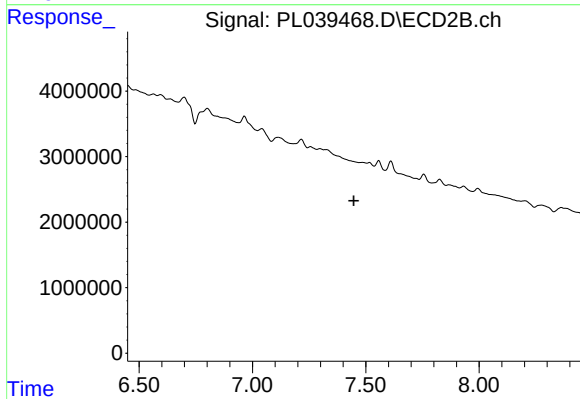

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.446 min
Response: 0
Conc: N.D.

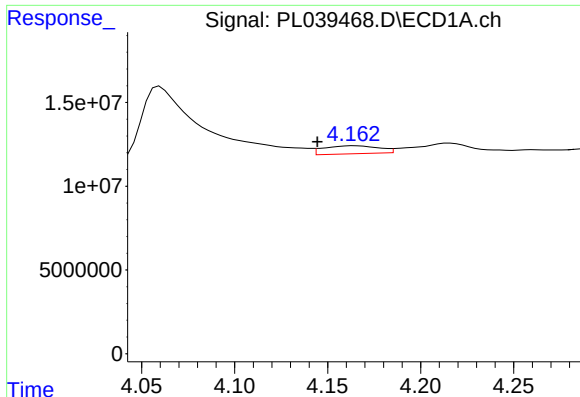

#23 Chlordane-1


R.T.: 4.165 min
Delta R.T.: 0.020 min
Response: 9915742
Conc: 31.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

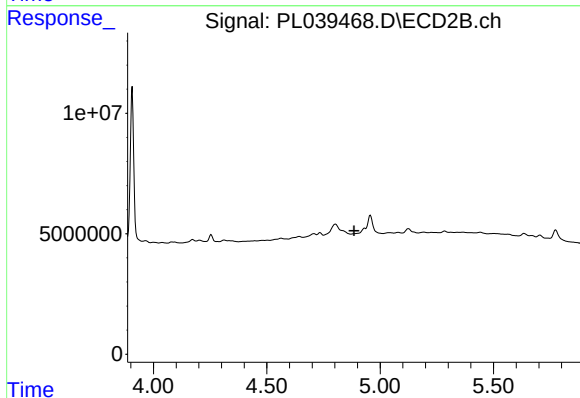


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.885 min
Response: 0
Conc: N.D.

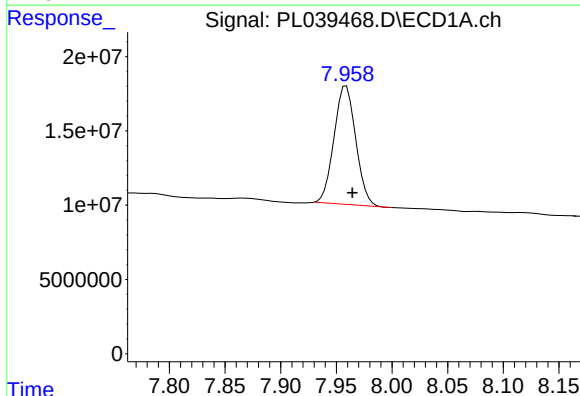

#28 Decachlorobiphenyl

R.T.: 7.959 min
Delta R.T.: -0.006 min
Response: 107795023
Conc: 15.35 ng/ml

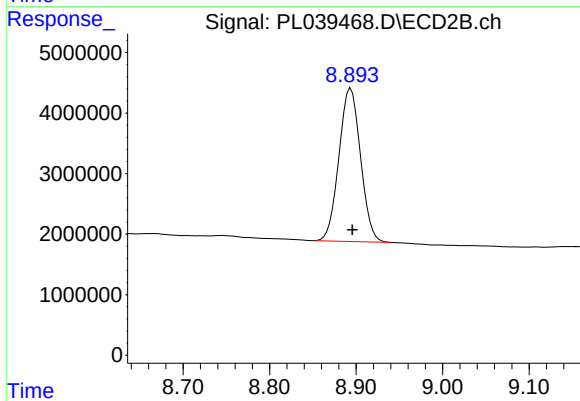

#28 Decachlorobiphenyl

R.T.: 8.894 min
Delta R.T.: -0.002 min
Response: 43702369
Conc: 18.83 ng/ml