

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082318\
 Data File : PL039469.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2018 15:59
 Operator : AJ\SJ
 Sample : J4612-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 24 03:40:21 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.304	3.906	62226493	24754644	8.902	9.234
28)	SA Decachlor...	7.959	8.893	90245724	36209154	12.849	15.603
Target Compounds							
2)	A alpha-BHC	3.687f	0.000	1504502	0	0.127	N.D. #
6)	B beta-BHC	4.216f	0.000	12455949	0	2.681	N.D. #
17)	MA 4,4'-DDT	6.148	0.000	2491610	0	0.329	N.D. #
20)	A Methoxychlor	6.672	0.000	2208045	0	0.540	N.D. #
23)	Chlordane-1	4.081	0.000	15534363	0	49.068	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082318\
Data File : PL039469.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2018 15:59
Operator : AJ\SJ
Sample : J4612-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 03:40:21 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

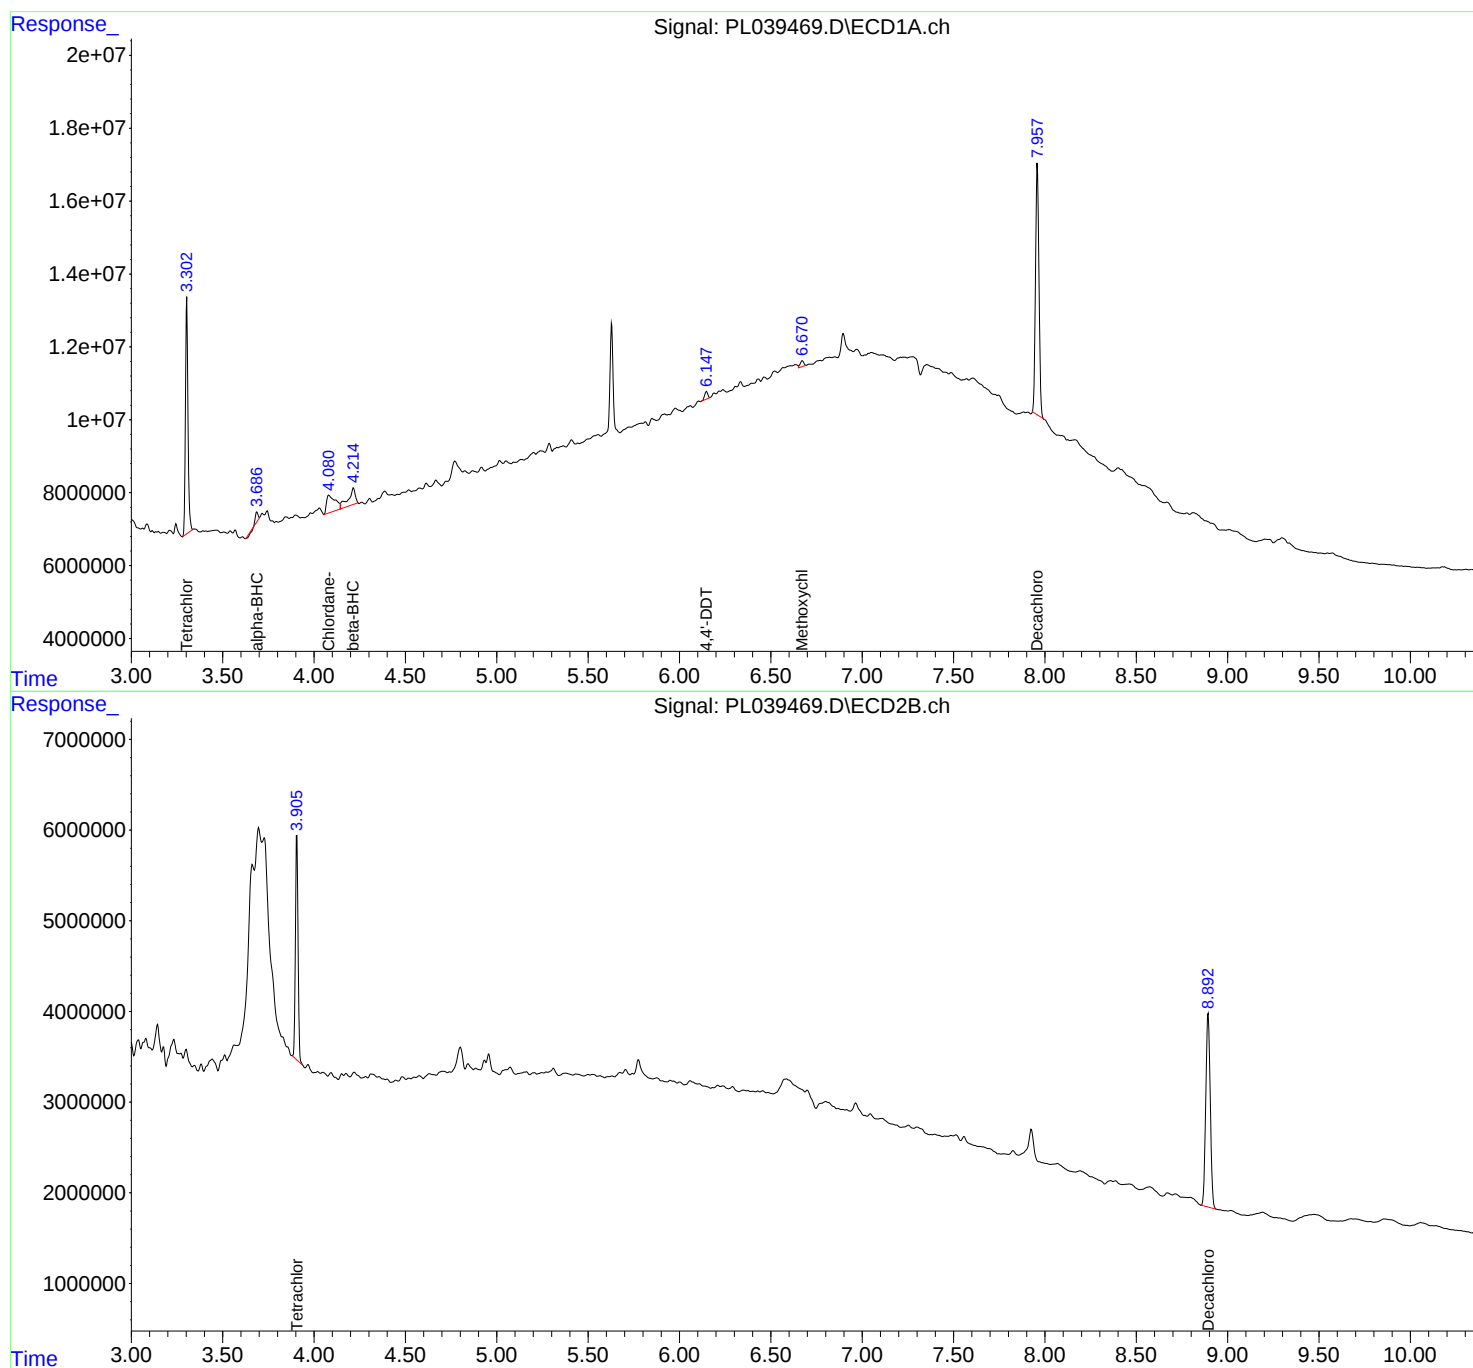


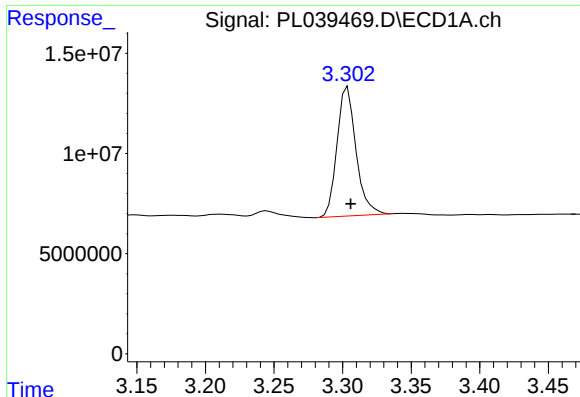

#1 Tetrachloro-m-xylene


R.T.: 3.304 min
Delta R.T.: -0.002 min
Response: 62226493
Conc: 8.90 ng/ml

Instrument :
ECD_L
ClientSampleId :

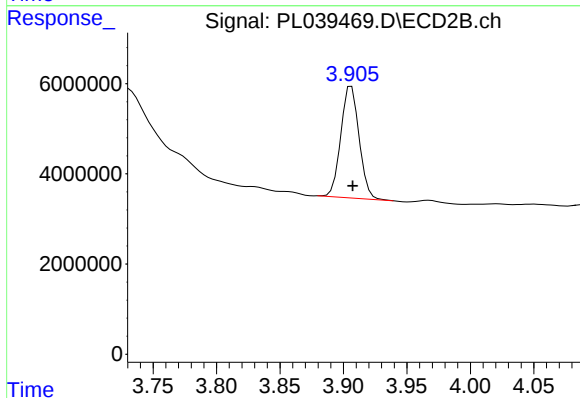


#1 Tetrachloro-m-xylene

R.T.: 3.906 min
Delta R.T.: 0.000 min
Response: 24754644
Conc: 9.23 ng/ml

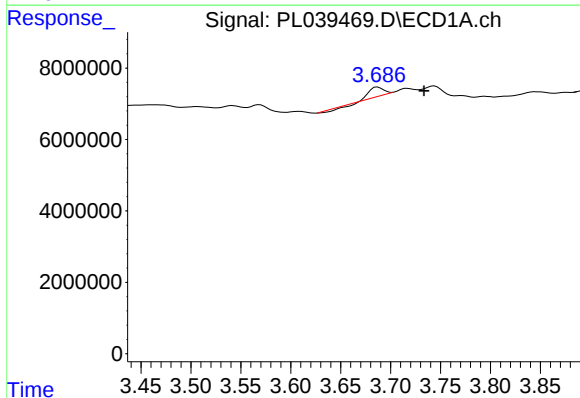


#2 alpha-BHC

R.T.: 3.687 min
Delta R.T.: -0.046 min
Response: 1504502
Conc: 0.13 ng/ml

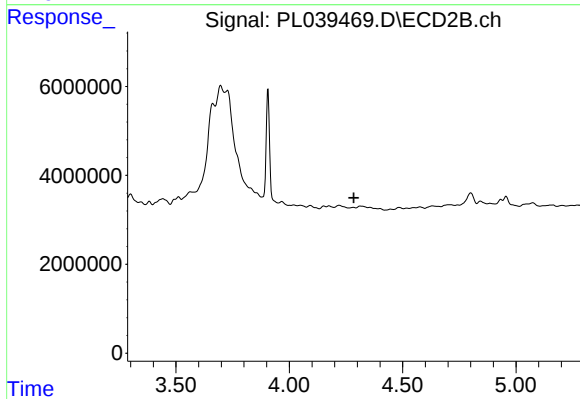

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.285 min
Response: 0
Conc: N.D.

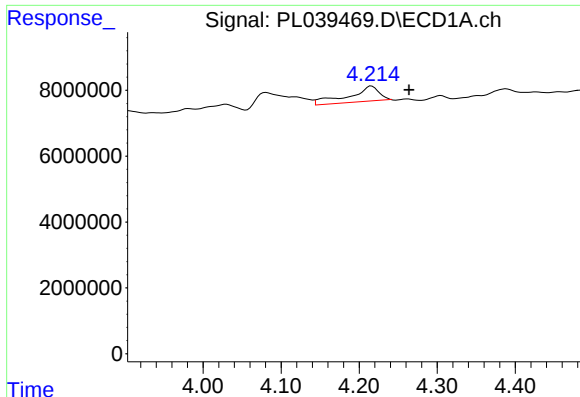

#6 beta-BHC


R.T.: 4.216 min
Delta R.T.: -0.048 min
Response: 12455949
Conc: 2.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

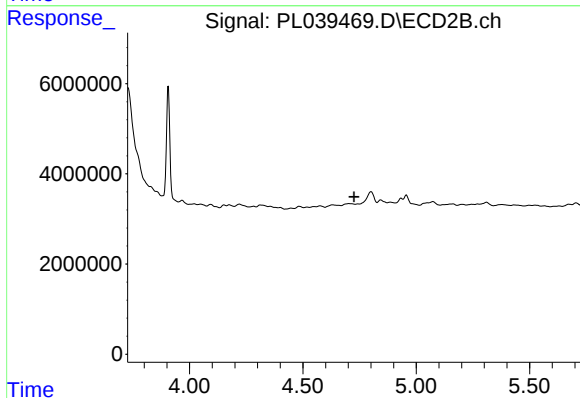


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

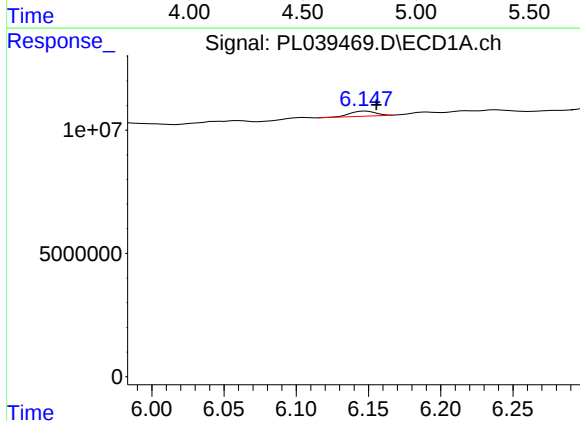


#17 4,4'-DDT

R.T.: 6.148 min
Delta R.T.: -0.007 min
Response: 2491610
Conc: 0.33 ng/ml

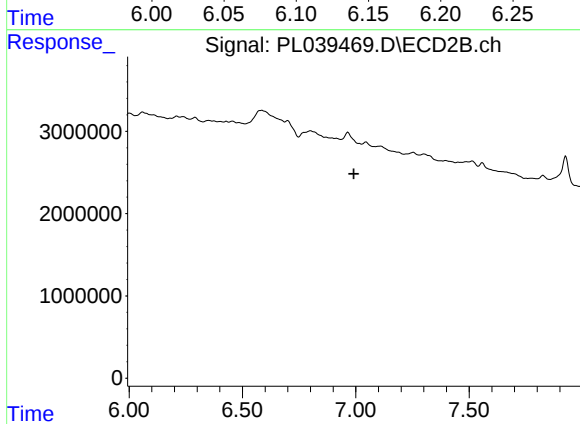

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 6.991 min
Response: 0
Conc: N.D.

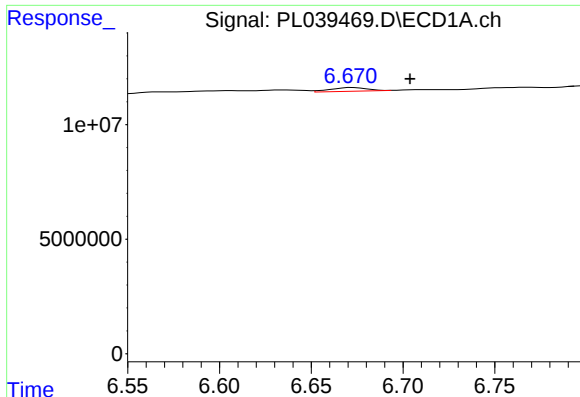

#20 Methoxychlor


R.T.: 6.672 min
Delta R.T.: -0.031 min
Response: 2208045
Conc: 0.54 ng/ml

Instrument :
ECD_L
ClientSampleId :

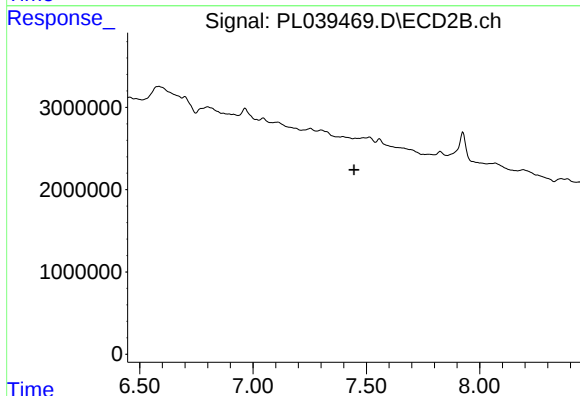


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.446 min
Response: 0
Conc: N.D.

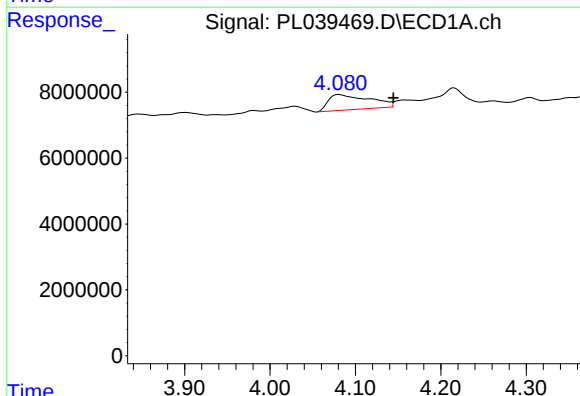


#23 Chlordane-1

R.T.: 4.081 min
Delta R.T.: -0.064 min
Response: 15534363
Conc: 49.07 ng/ml

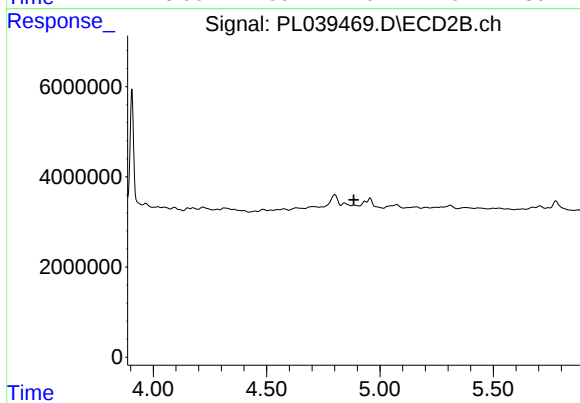

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.885 min
Response: 0
Conc: N.D.

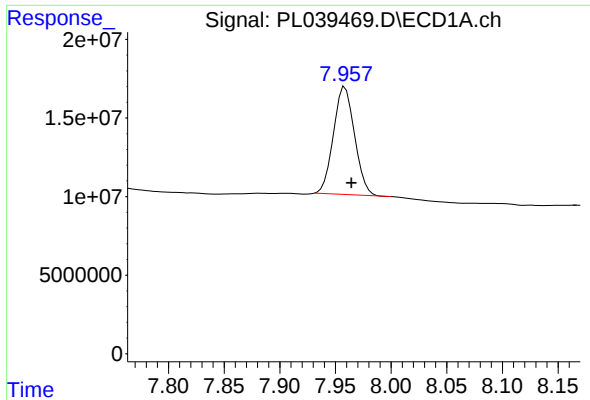

#28 Decachlorobiphenyl

R.T.: 7.959 min
Delta R.T.: -0.006 min
Response: 90245724
Conc: 12.85 ng/ml

Instrument :
ECD_L
ClientSampleId :

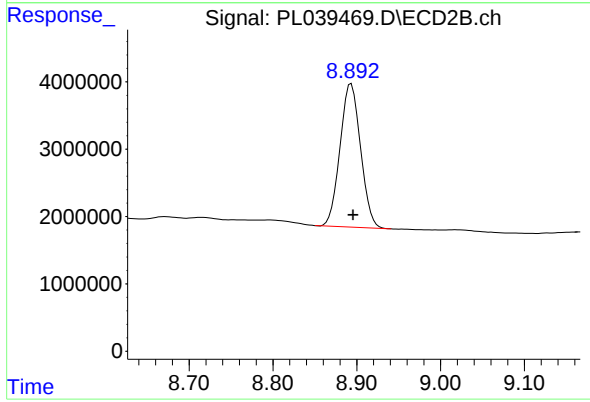

#28 Decachlorobiphenyl

R.T.: 8.893 min
Delta R.T.: -0.002 min
Response: 36209154
Conc: 15.60 ng/ml