

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082318\
 Data File : PL039481.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Aug 2018 09:10
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 24 10:15:49 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.305	3.905	167.3E6	69391632	23.939	25.884
28)	SA Decachlor...	7.960	8.891	164.6E6	60469230	23.439	26.057
Target Compounds							
6)	B beta-BHC	4.216f	0.000	5911891	0	1.273	N.D. #
8)	B Heptachlo...	4.919f	0.000	11499895	0	1.204	N.D. #
23)	Chlordane-1	4.174	0.000	3027073	0	9.562	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082318\
Data File : PL039481.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Aug 2018 09:10
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 10:15:49 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

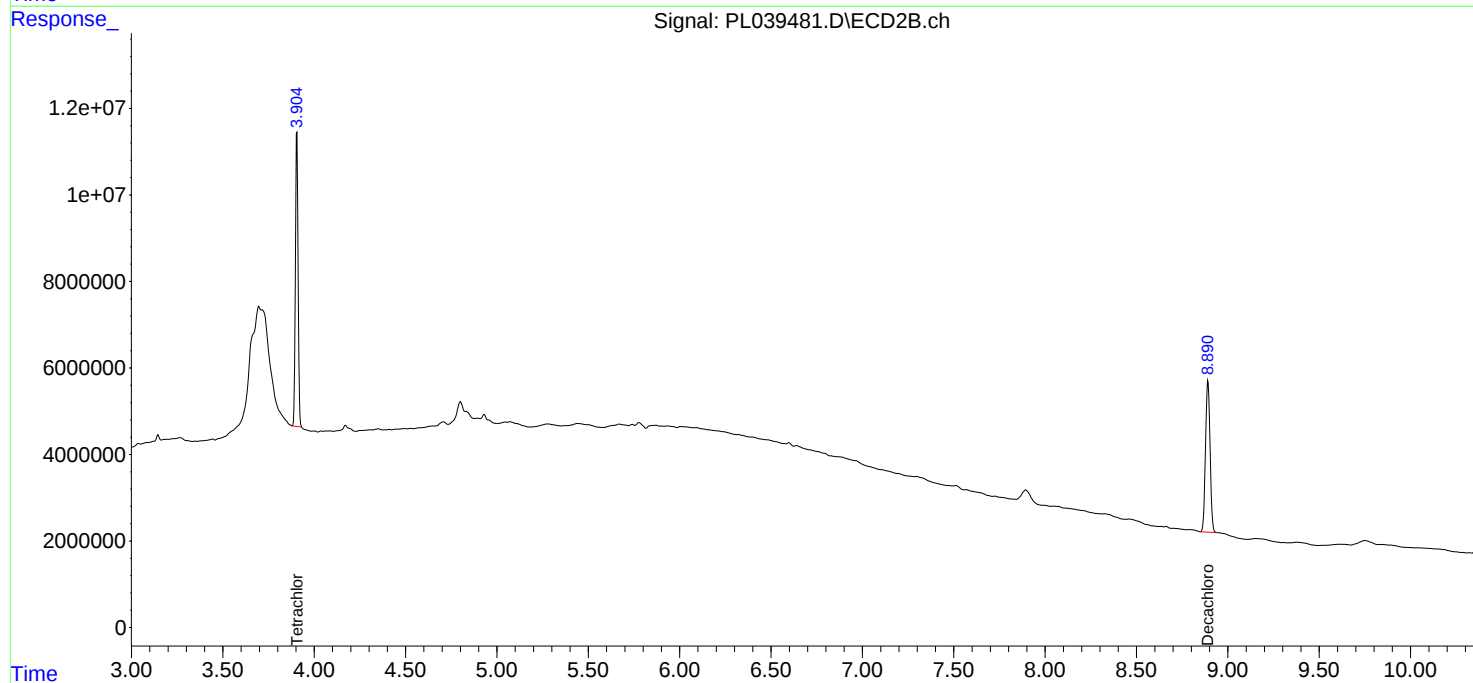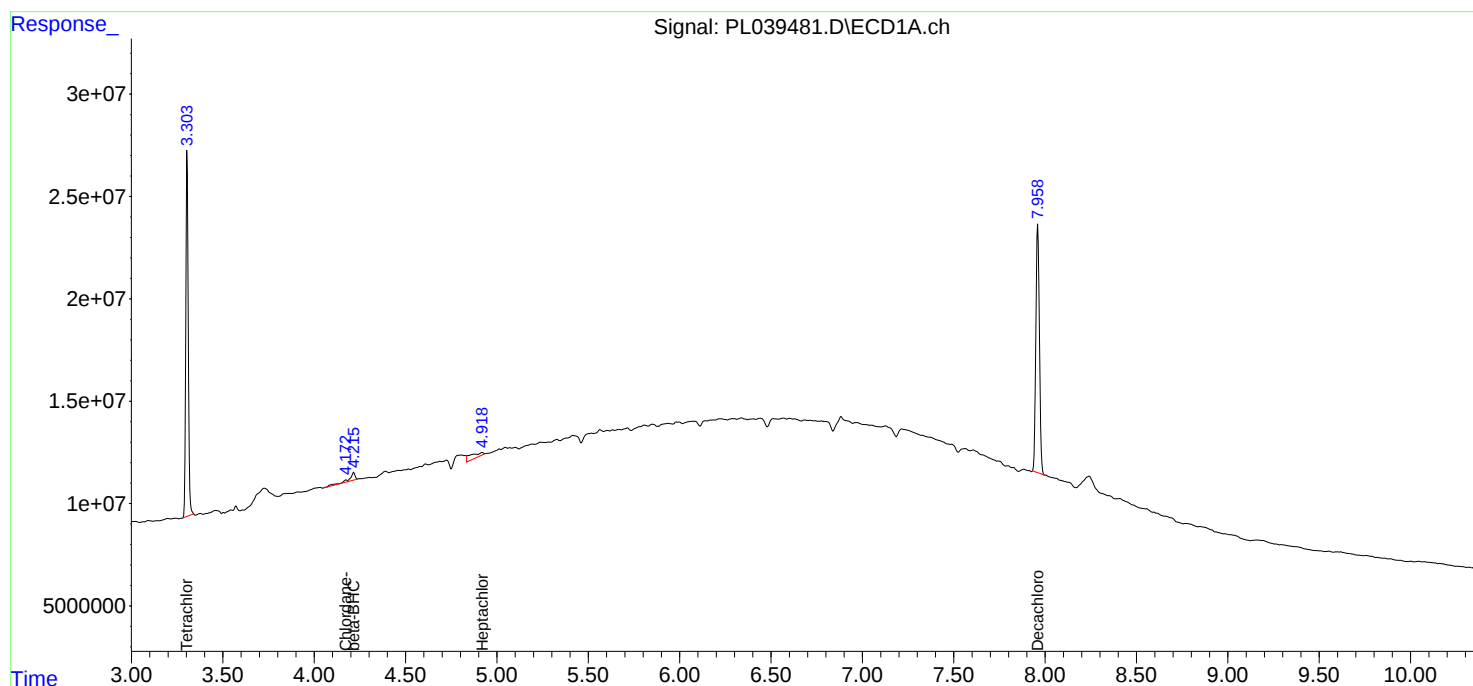


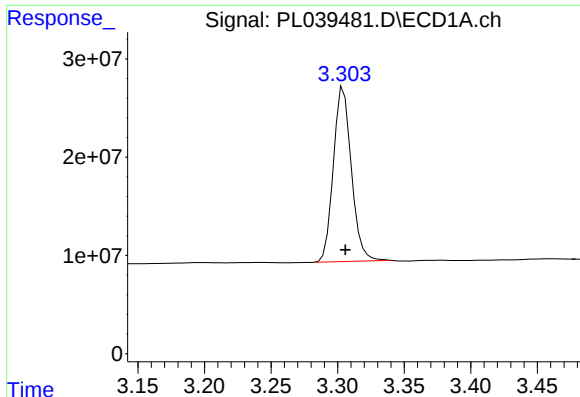

#1 Tetrachloro-m-xylene


R.T.: 3.305 min
Delta R.T.: -0.001 min
Response: 167344307
Conc: 23.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

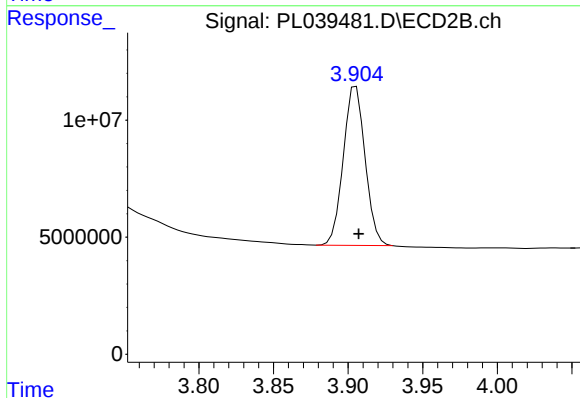


#1 Tetrachloro-m-xylene

R.T.: 3.905 min
Delta R.T.: -0.002 min
Response: 69391632
Conc: 25.88 ng/ml

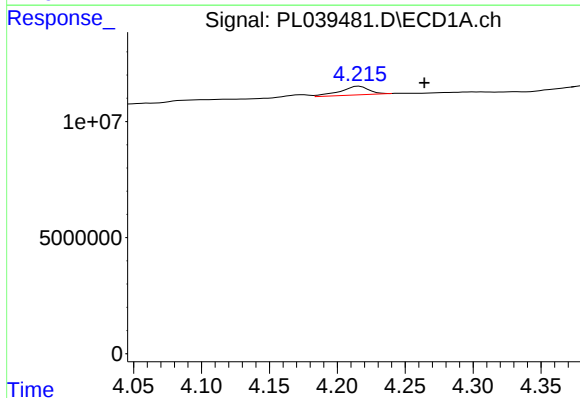


#6 beta-BHC

R.T.: 4.216 min
Delta R.T.: -0.048 min
Response: 5911891
Conc: 1.27 ng/ml

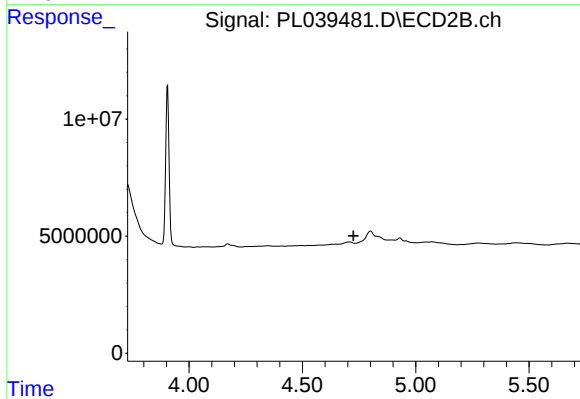

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.726 min
Response: 0
Conc: N.D.

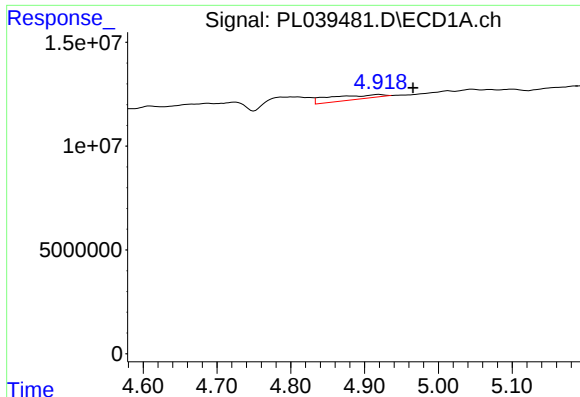

#8 Heptachlor epoxide


R.T.: 4.919 min
Delta R.T.: -0.047 min
Response: 11499895
Conc: 1.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

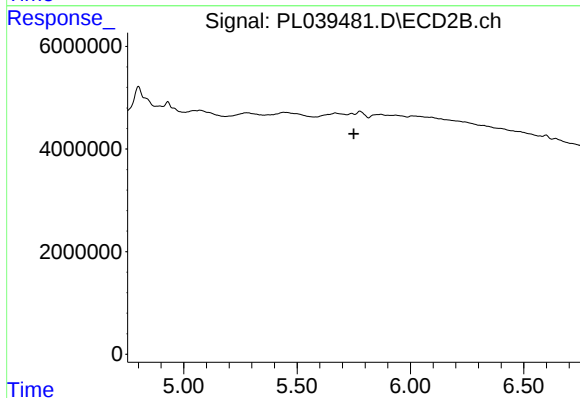


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.751 min
Response: 0
Conc: N.D.

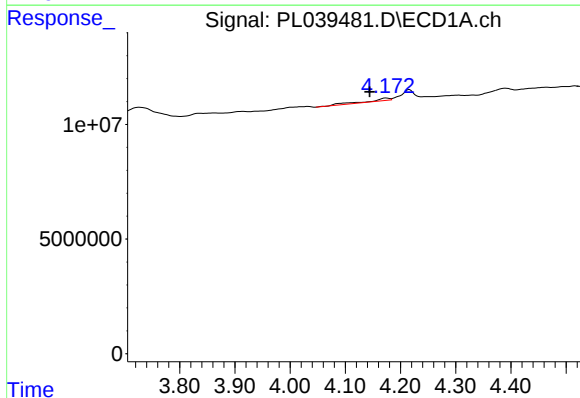


#23 Chlordane-1

R.T.: 4.174 min
Delta R.T.: 0.029 min
Response: 3027073
Conc: 9.56 ng/ml

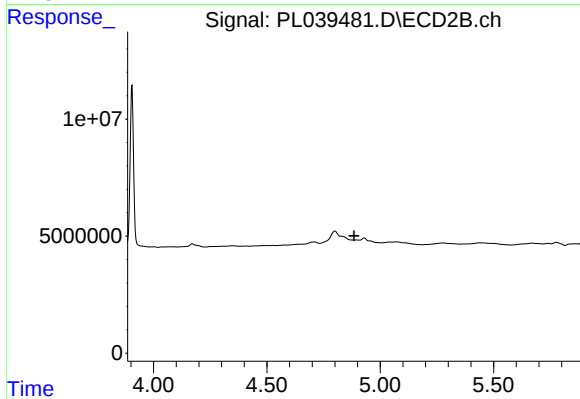

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.885 min
Response: 0
Conc: N.D.

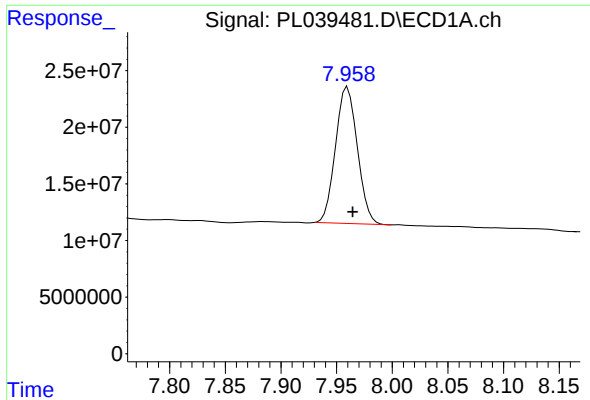

#28 Decachlorobiphenyl

R.T.: 7.960 min
Delta R.T.: -0.005 min
Response: 164624369
Conc: 23.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

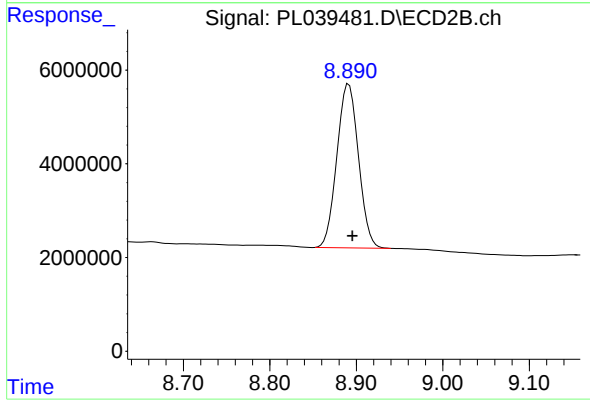

#28 Decachlorobiphenyl

R.T.: 8.891 min
Delta R.T.: -0.004 min
Response: 60469230
Conc: 26.06 ng/ml