

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082319\
 Data File : PL051790.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2019 22:50
 Operator : SG\AJ
 Sample : K4475-14
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 24 00:45:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.314	3.926	199.9E6	51030478	23.353	23.357
28)	SA Decachlor...	7.972	8.951	266.6E6	63797872	21.963	20.959
Target Compounds							
6)	B beta-BHC	0.000	4.805f	0	4341994	N.D.	2.979 #
15)	B Endosulfa...	0.000	6.845f	0	2971079	N.D.	0.901 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082319\
Data File : PL051790.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2019 22:50
Operator : SG\AJ
Sample : K4475-14
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 00:45:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

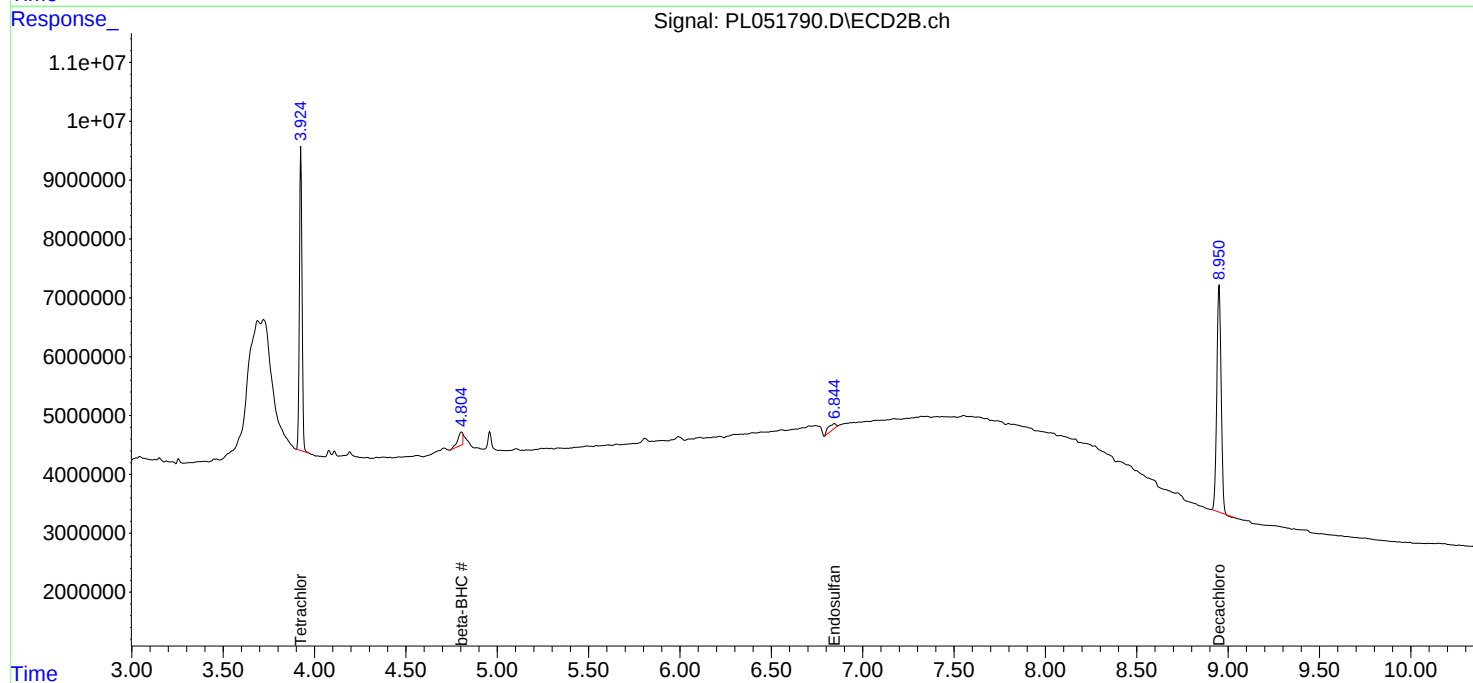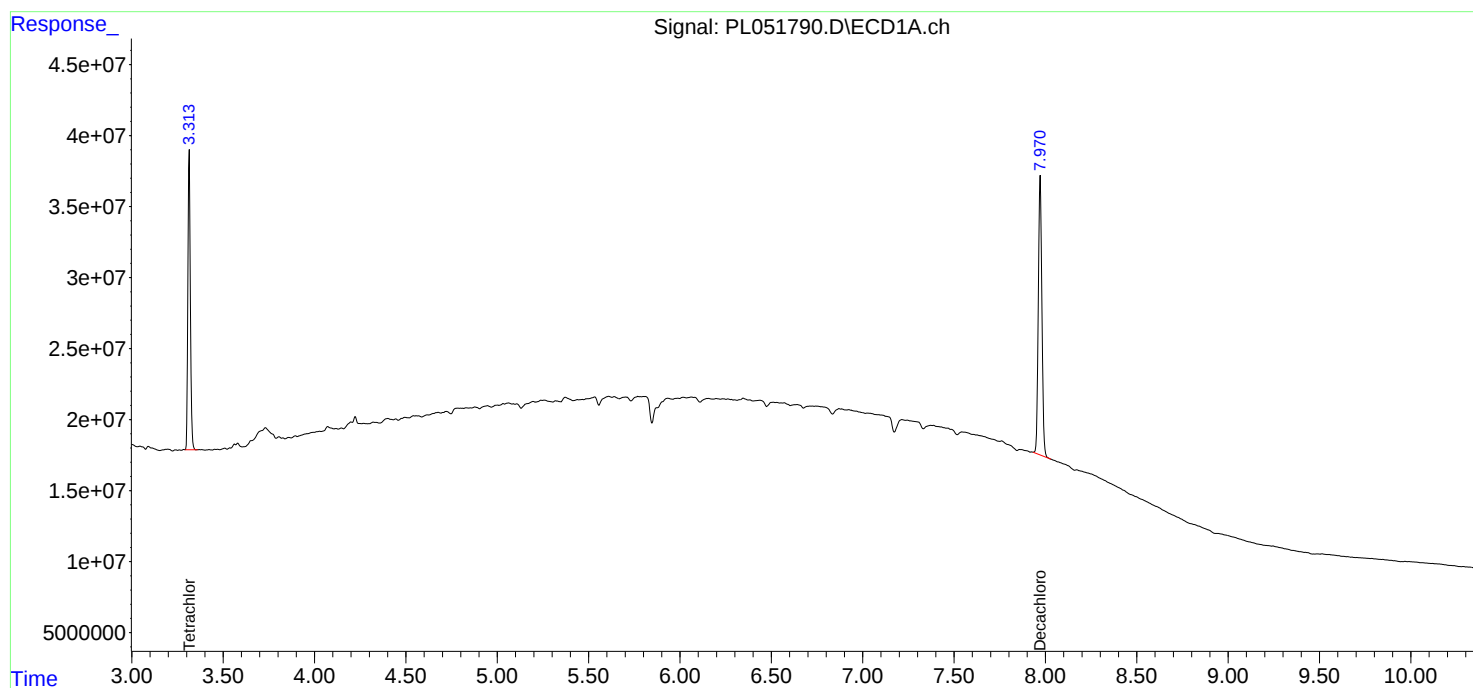


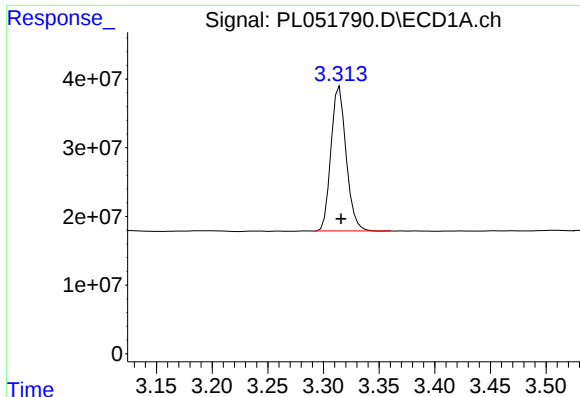

#1 Tetrachloro-m-xylene


R.T.: 3.314 min
Delta R.T.: -0.002 min
Response: 199867491
Conc: 23.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

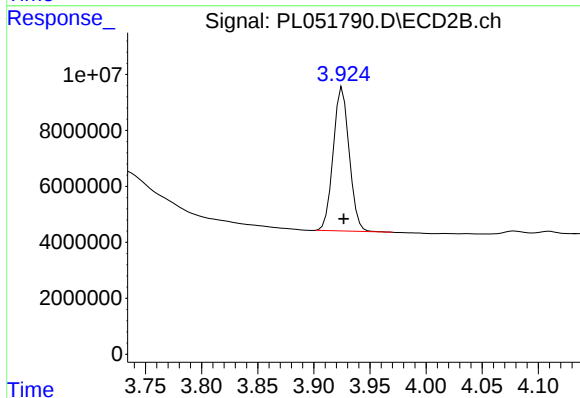


#1 Tetrachloro-m-xylene

R.T.: 3.926 min
Delta R.T.: -0.001 min
Response: 51030478
Conc: 23.36 ng/ml

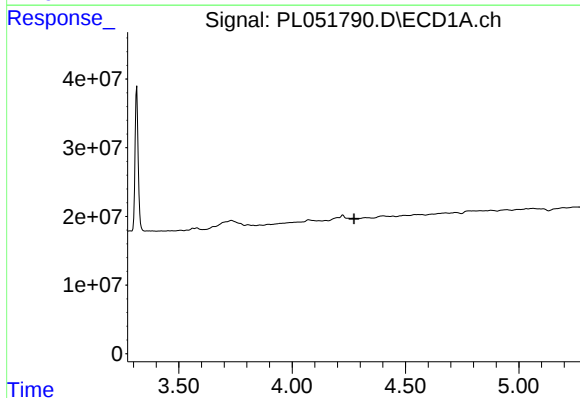


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.273 min
Response: 0
Conc: N.D.

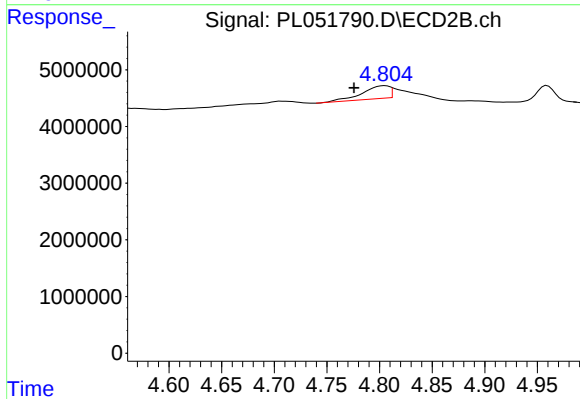

#6 beta-BHC


R.T.: 4.805 min
Delta R.T.: 0.029 min
Response: 4341994
Conc: 2.98 ng/ml

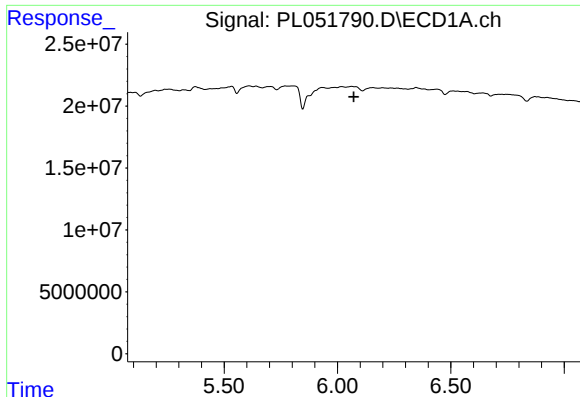

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.072 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

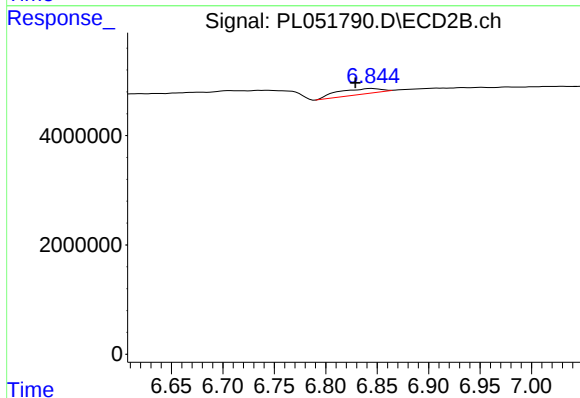


#15 Endosulfan II

R.T.: 6.845 min
Delta R.T.: 0.016 min
Response: 2971079
Conc: 0.90 ng/ml

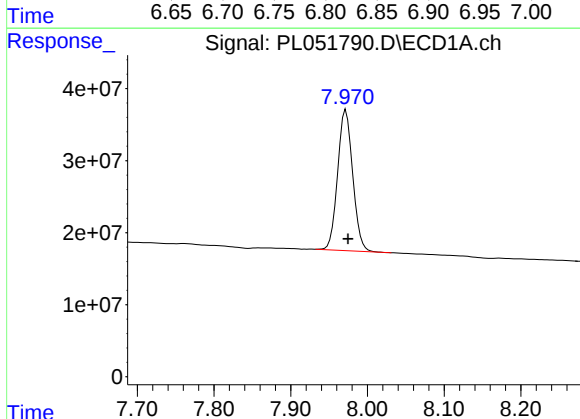

#28 Decachlorobiphenyl

R.T.: 7.972 min
Delta R.T.: -0.003 min
Response: 266578099
Conc: 21.96 ng/ml

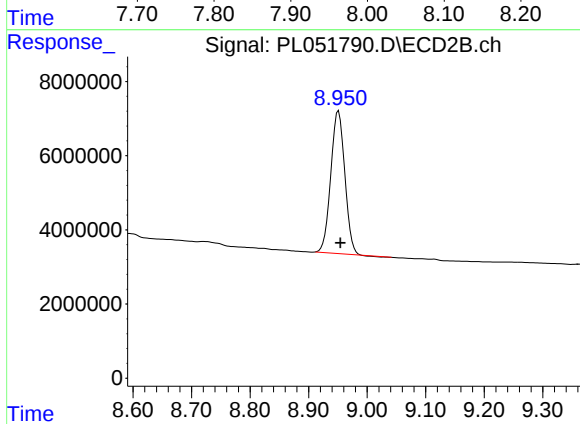

#28 Decachlorobiphenyl

R.T.: 8.951 min
Delta R.T.: -0.003 min
Response: 63797872
Conc: 20.96 ng/ml