

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082322\
 Data File : PL077284.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2022 12:29
 Operator : AR\AJ
 Sample : PB147197BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 23:46:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082222.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 23 05:36:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.424	2.631	21709150	46402317	15.955	15.099
28)	SA Decachlor...	8.918	7.739	20063513	41835703	17.121	14.993
Target Compounds							
7)	B delta-BHC	4.649f	0.000	228542	0	0.148	N.D. #
9)	A Endosulfan I	0.000	4.903f	0	313050	N.D.	0.101 #
11)	B alpha-Chl...	0.000	4.887f	0	265860	N.D.	0.081 #
12)	B 4,4'-DDE	0.000	5.088f	0	553951	N.D.	0.172 #
20)	A Methoxychlor	7.423f	0.000	199292	0	0.331	N.D. #
21)	B Endrin ke...	0.000	6.641	0	1102077	N.D.	0.383 #
22)	Mirex	8.023f	0.000	103043	0	0.112	N.D. #
26)	Chlordane-4	0.000	4.887f	0	265860	N.D.	0.840 #
27)	Chlordane-5	0.000	5.515	0	1631834	N.D.	18.638 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082322\
Data File : PL077284.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2022 12:29
Operator : AR\AJ
Sample : PB147197BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 23:46:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082222.M
Quant Title : GC Extractables
QLast Update : Tue Aug 23 05:36:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

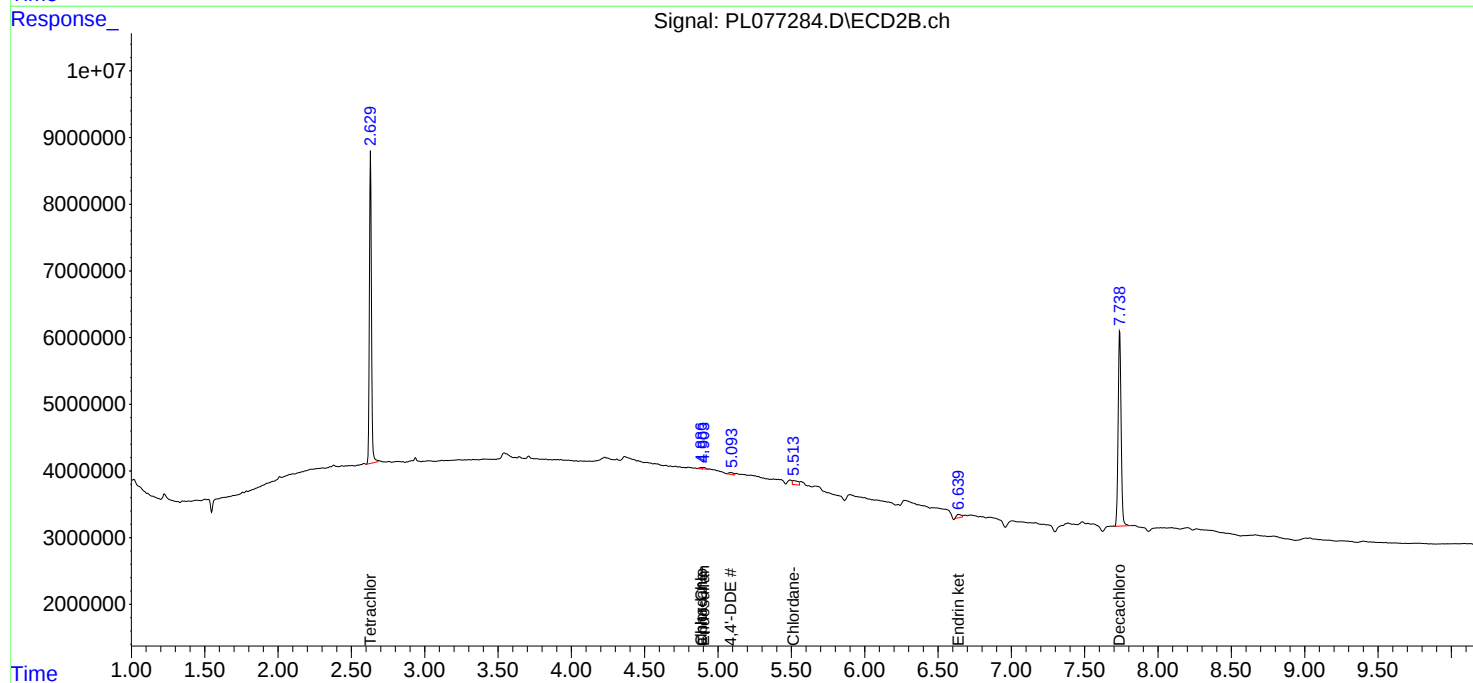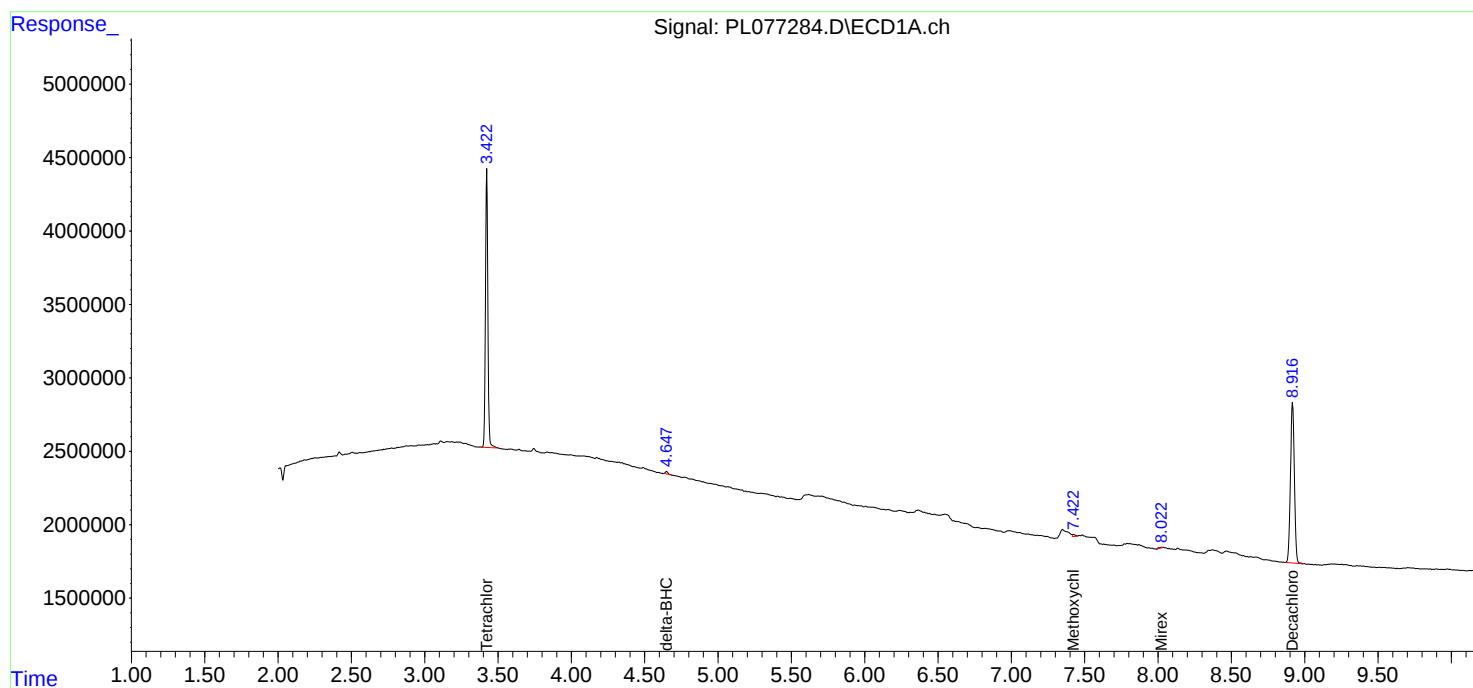


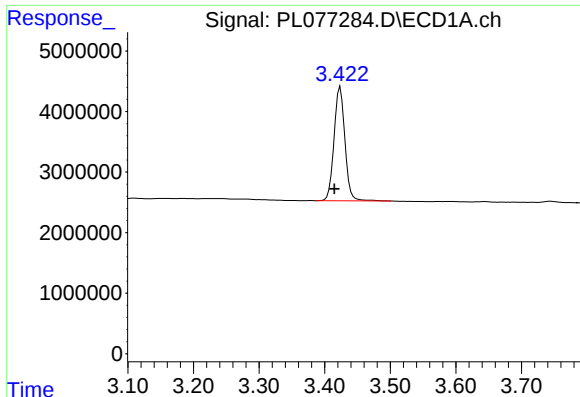

#1 Tetrachloro-m-xylene


R.T.: 3.424 min
Delta R.T.: 0.009 min
Response: 21709150
Conc: 15.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

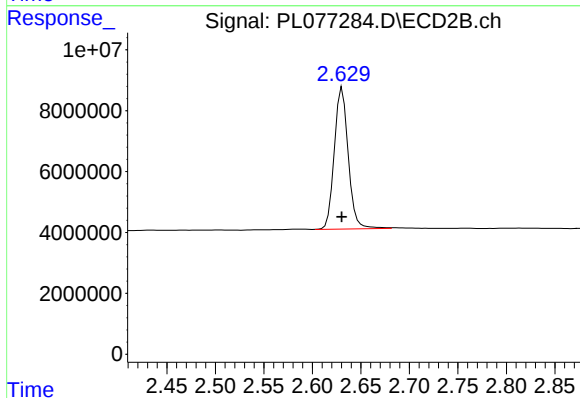


#1 Tetrachloro-m-xylene

R.T.: 2.631 min
Delta R.T.: 0.000 min
Response: 46402317
Conc: 15.10 ng/ml

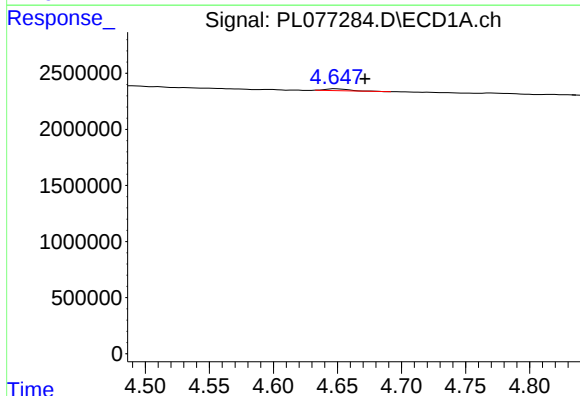


#7 delta-BHC

R.T.: 4.649 min
Delta R.T.: -0.023 min
Response: 228542
Conc: 0.15 ng/ml

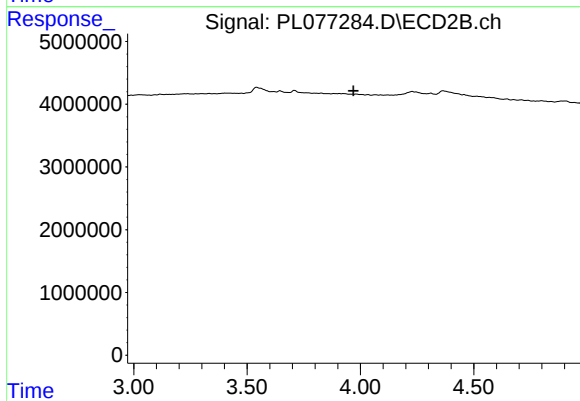

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 3.970 min
Response: 0
Conc: N.D.

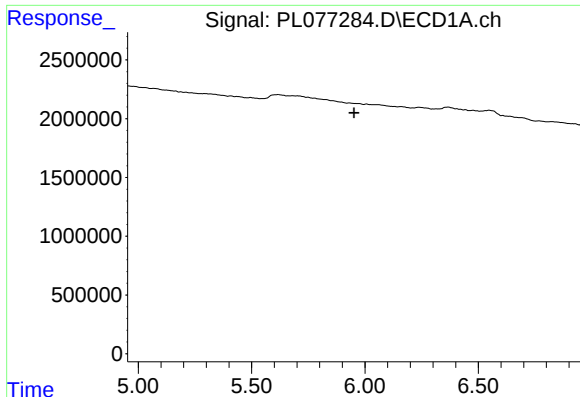

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.952 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

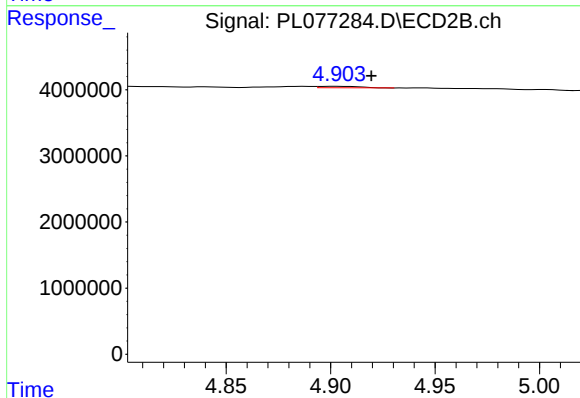


#9 Endosulfan I

R.T.: 4.903 min
Delta R.T.: -0.016 min
Response: 313050
Conc: 0.10 ng/ml

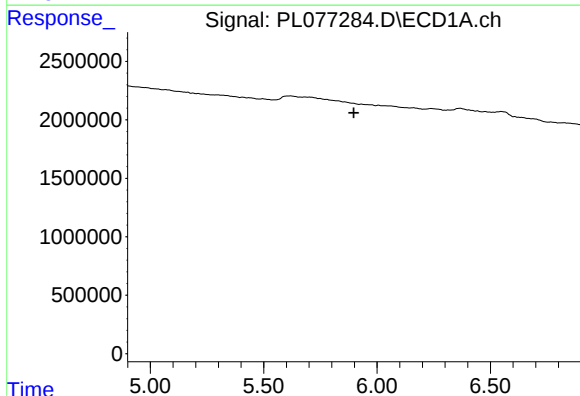


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.898 min
Response: 0
Conc: N.D.

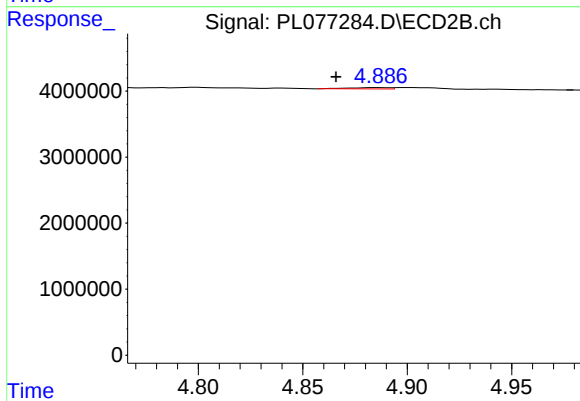

#11 alpha-Chlordane


R.T.: 4.887 min
Delta R.T.: 0.021 min
Response: 265860
Conc: 0.08 ng/ml

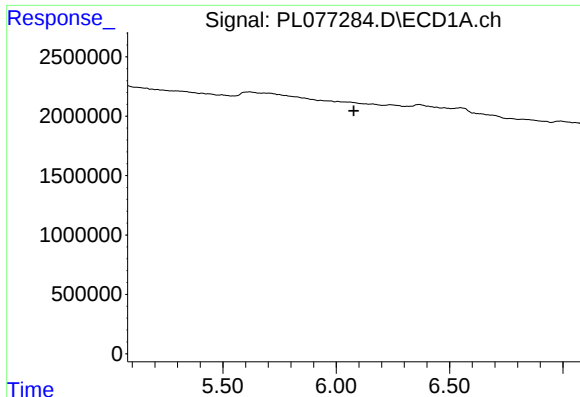

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 6.077 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

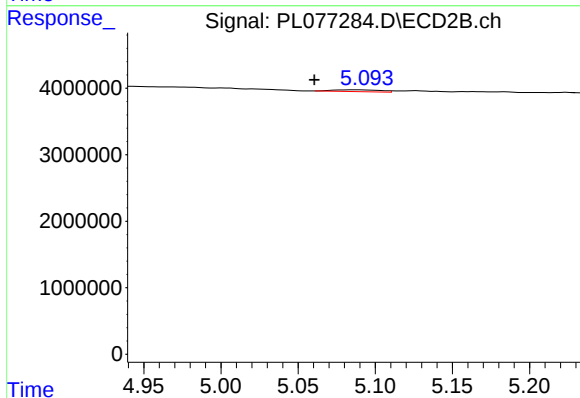


#12 4,4'-DDE

R.T.: 5.088 min
Delta R.T.: 0.027 min
Response: 553951
Conc: 0.17 ng/ml

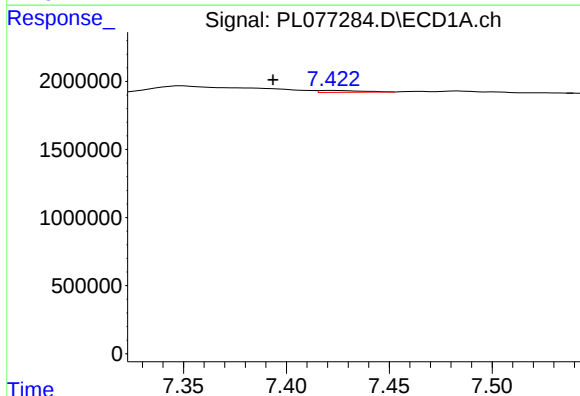


#20 Methoxychlor

R.T.: 7.423 min
Delta R.T.: 0.029 min
Response: 199292
Conc: 0.33 ng/ml

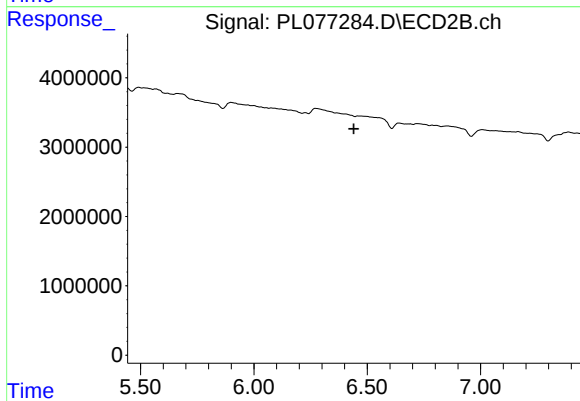

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.440 min
Response: 0
Conc: N.D.

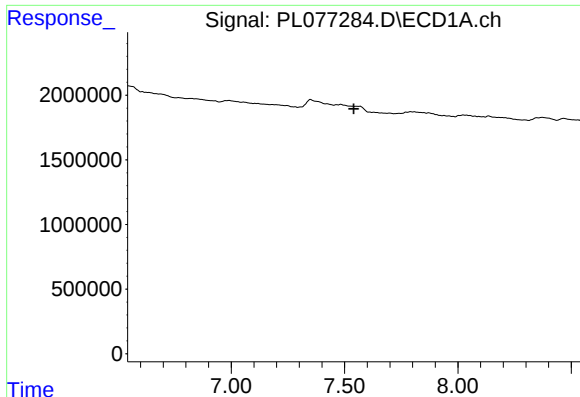

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.541 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

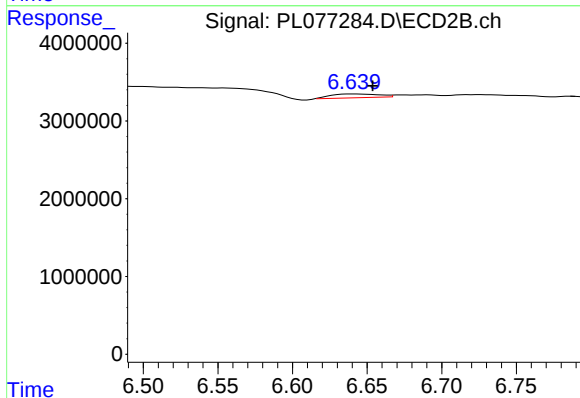


#21 Endrin ketone

R.T.: 6.641 min
Delta R.T.: -0.013 min
Response: 1102077
Conc: 0.38 ng/ml

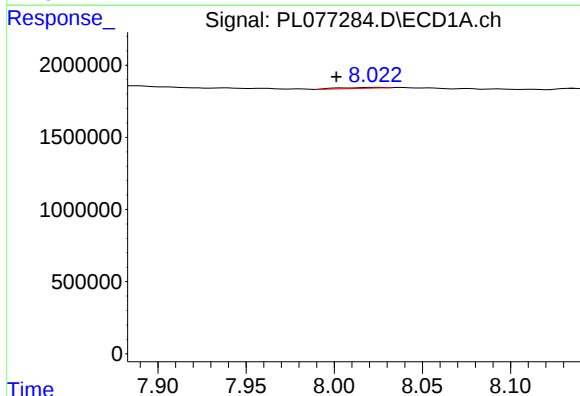


#22 Mirex

R.T.: 8.023 min
Delta R.T.: 0.022 min
Response: 103043
Conc: 0.11 ng/ml

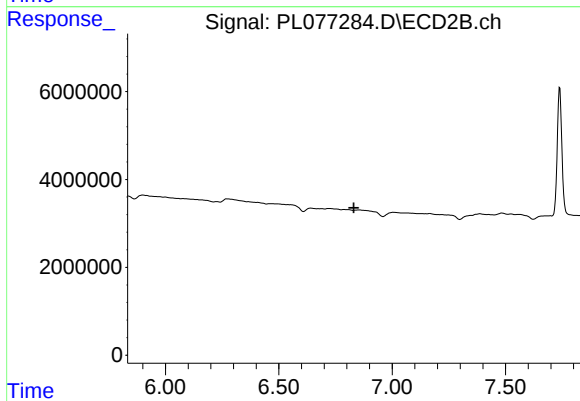

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 6.831 min
Response: 0
Conc: N.D.

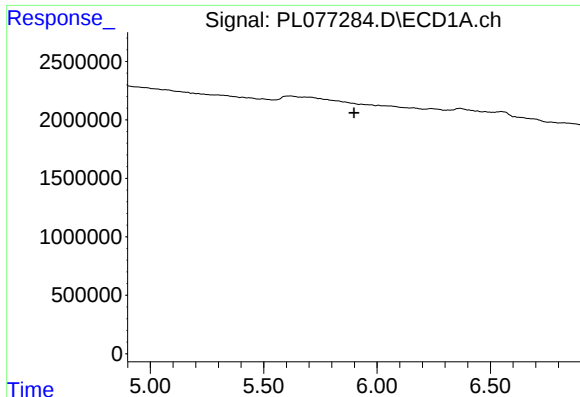

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.899 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

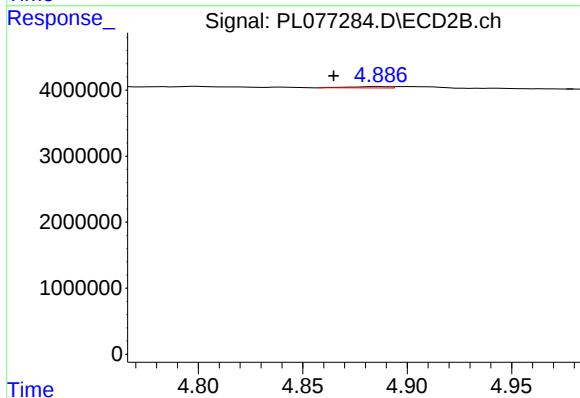


#26 Chlordane-4

R.T.: 4.887 min
Delta R.T.: 0.022 min
Response: 265860
Conc: 0.84 ng/ml

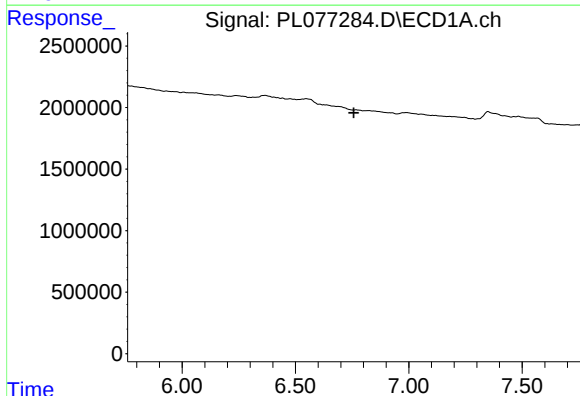


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.758 min
Response: 0
Conc: N.D.

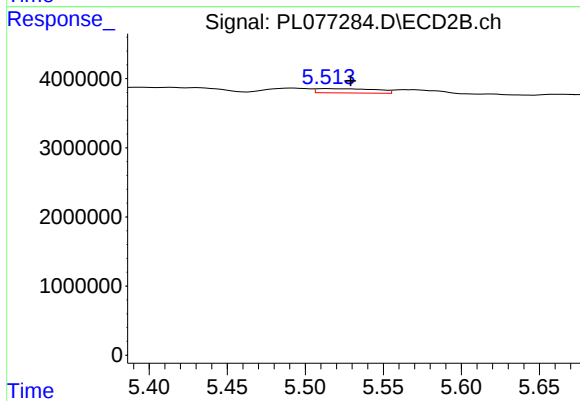

#27 Chlordane-5


R.T.: 5.515 min
Delta R.T.: -0.015 min
Response: 1631834
Conc: 18.64 ng/ml

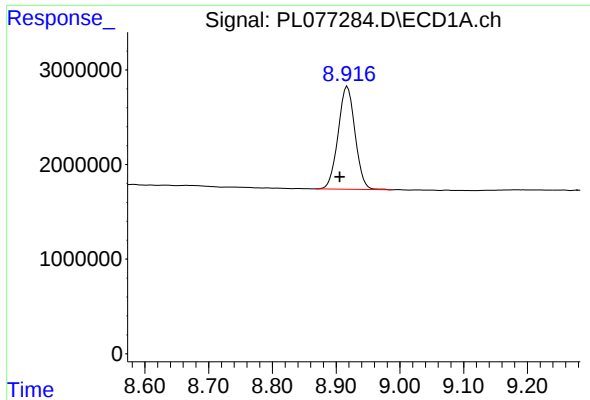

#28 Decachlorobiphenyl

R.T.: 8.918 min
Delta R.T.: 0.012 min
Response: 20063513
Conc: 17.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

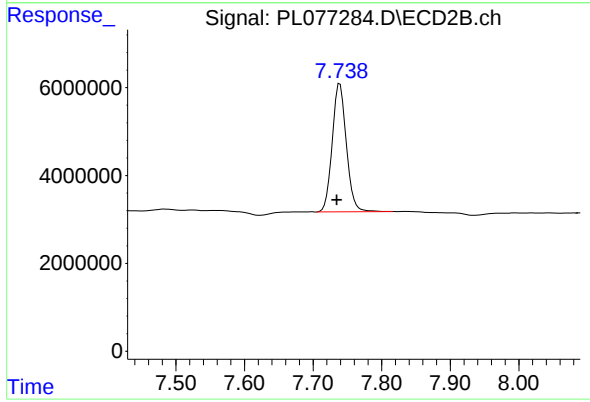

#28 Decachlorobiphenyl

R.T.: 7.739 min
Delta R.T.: 0.005 min
Response: 41835703
Conc: 14.99 ng/ml