

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082322\
 Data File : PL077289.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2022 13:44
 Operator : AR\AJ
 Sample : N4277-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 B-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 23:51:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082222.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 23 05:36:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.416	2.630	12958210	30399635	9.523	9.892
28)	SA Decachlor...	8.906	7.733	12833640	29029090	10.951	10.403
Target Compounds							
11)	B alpha-Chl...	5.900	4.863	3228115	6951405	2.295	2.123



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082322\
Data File : PL077289.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2022 13:44
Operator : AR\AJ
Sample : N4277-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
B-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 23:51:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082222.M
Quant Title : GC Extractables
QLast Update : Tue Aug 23 05:36:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

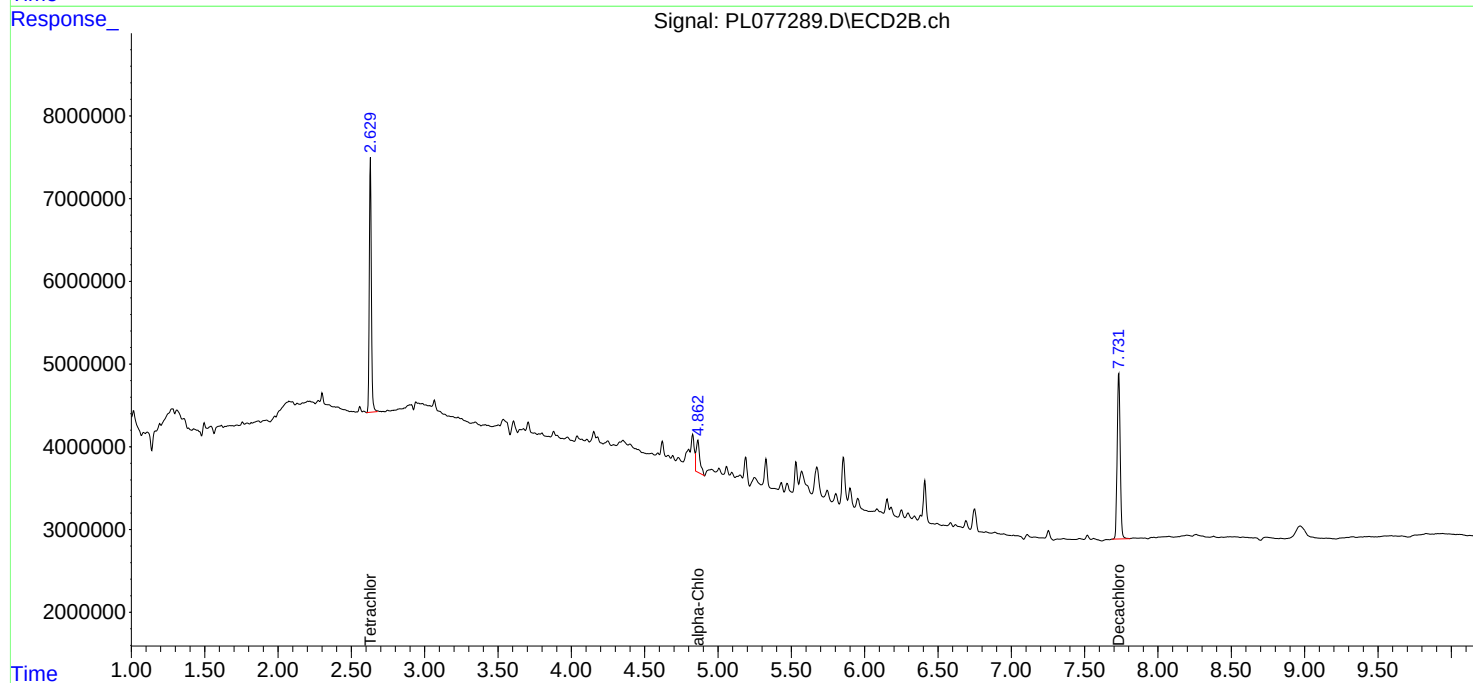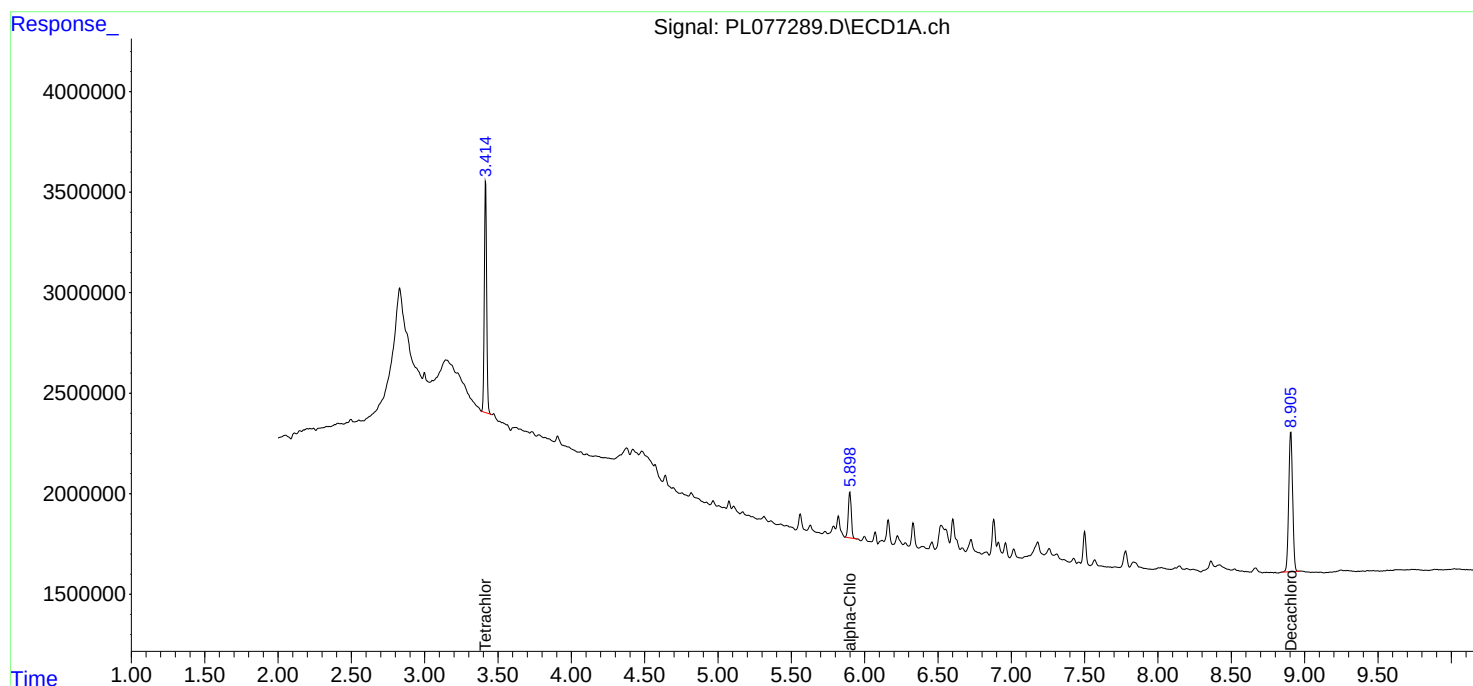


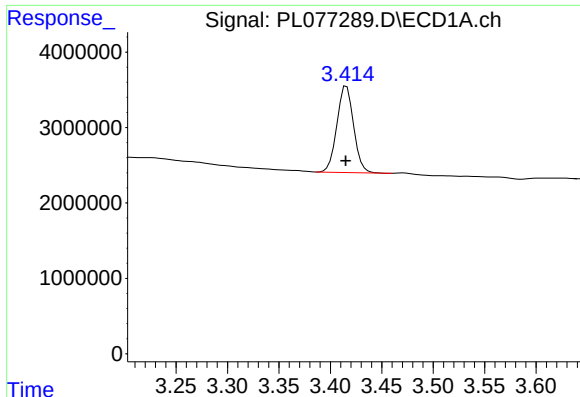

#1 Tetrachloro-m-xylene


R.T.: 3.416 min
Delta R.T.: 0.000 min
Response: 12958210
Conc: 9.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
B-2

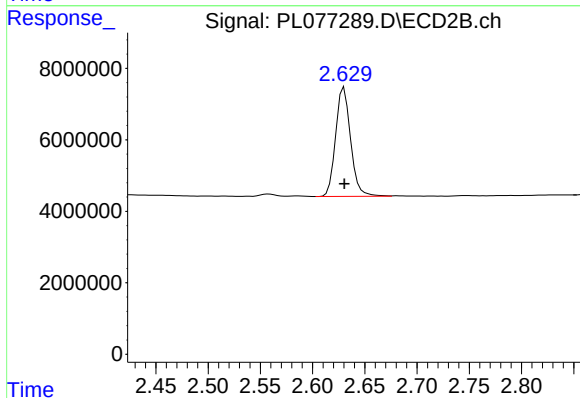


#1 Tetrachloro-m-xylene

R.T.: 2.630 min
Delta R.T.: 0.000 min
Response: 30399635
Conc: 9.89 ng/ml

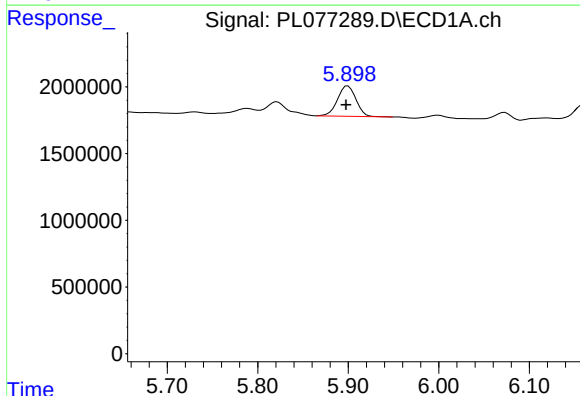


#11 alpha-Chlordane

R.T.: 5.900 min
Delta R.T.: 0.002 min
Response: 3228115
Conc: 2.29 ng/ml

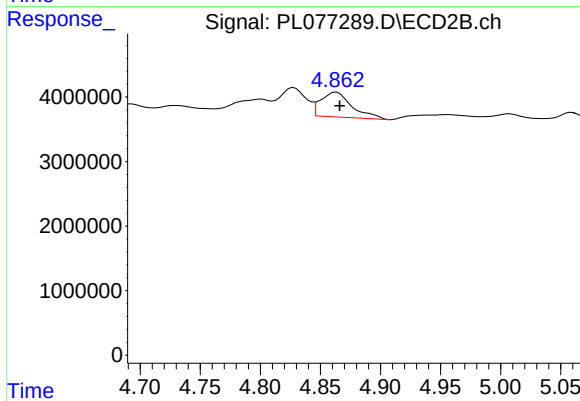

#11 alpha-Chlordane


R.T.: 4.863 min
Delta R.T.: -0.003 min
Response: 6951405
Conc: 2.12 ng/ml

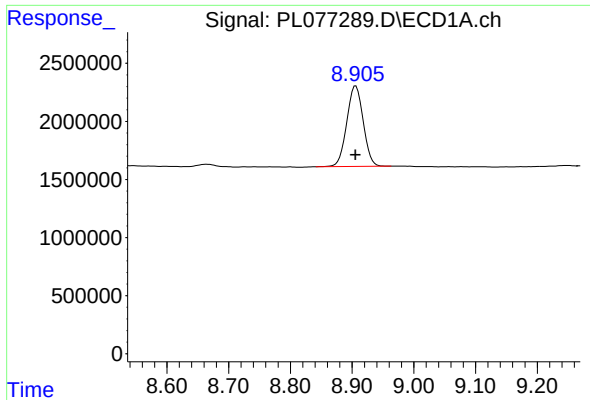

#28 Decachlorobiphenyl

R.T.: 8.906 min
Delta R.T.: 0.000 min
Response: 12833640
Conc: 10.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
B-2

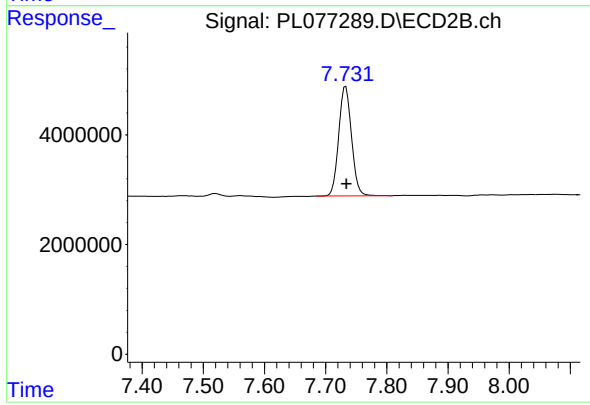

#28 Decachlorobiphenyl

R.T.: 7.733 min
Delta R.T.: -0.001 min
Response: 29029090
Conc: 10.40 ng/ml