

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082323\
 Data File : PL084924.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2023 10:44
 Operator : AR\AJ
 Sample : [PIBLK221
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 22:25:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 05:52:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.486	2.686	50399806	23006786	20.104	19.489
27)	SA Decachlor...	9.038	7.868	79401304	62502803	46.332	46.148
Target Compounds							
4)	MA Heptachlor	4.871	0.000	95436	0	<MDL	N.D. #
6)	B beta-BHC	4.423f	0.000	88338	0	<MDL	N.D. #
7)	B delta-BHC	4.724	0.000	2784485	0	0.763	N.D. #
9)	A Endosulfan I	5.955f	0.000	1946960	0	0.683	N.D. #
10)	B trans-Chl...	5.955f	0.000	1946960	0	0.617	N.D. #
11)	B cis-Chlor...	5.955	0.000	1946960	0	0.611	N.D. #
14)	MA Endrin	6.592f	0.000	470130	0	0.206	N.D. #
15)	B Endosulfa...	6.759	0.000	1423216	0	0.605	N.D. #
17)	MA 4,4'-DDT	6.962	0.000	458081	0	0.238	N.D. #
20)	A Methoxychlor	7.464	0.000	323508	0	0.333	N.D. #
23)	Toxaphene-2	6.962f	0.000	458081	0	6.892	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082323\
Data File : PL084924.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2023 10:44
Operator : AR\AJ
Sample : [PIBLK221
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 22:25:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

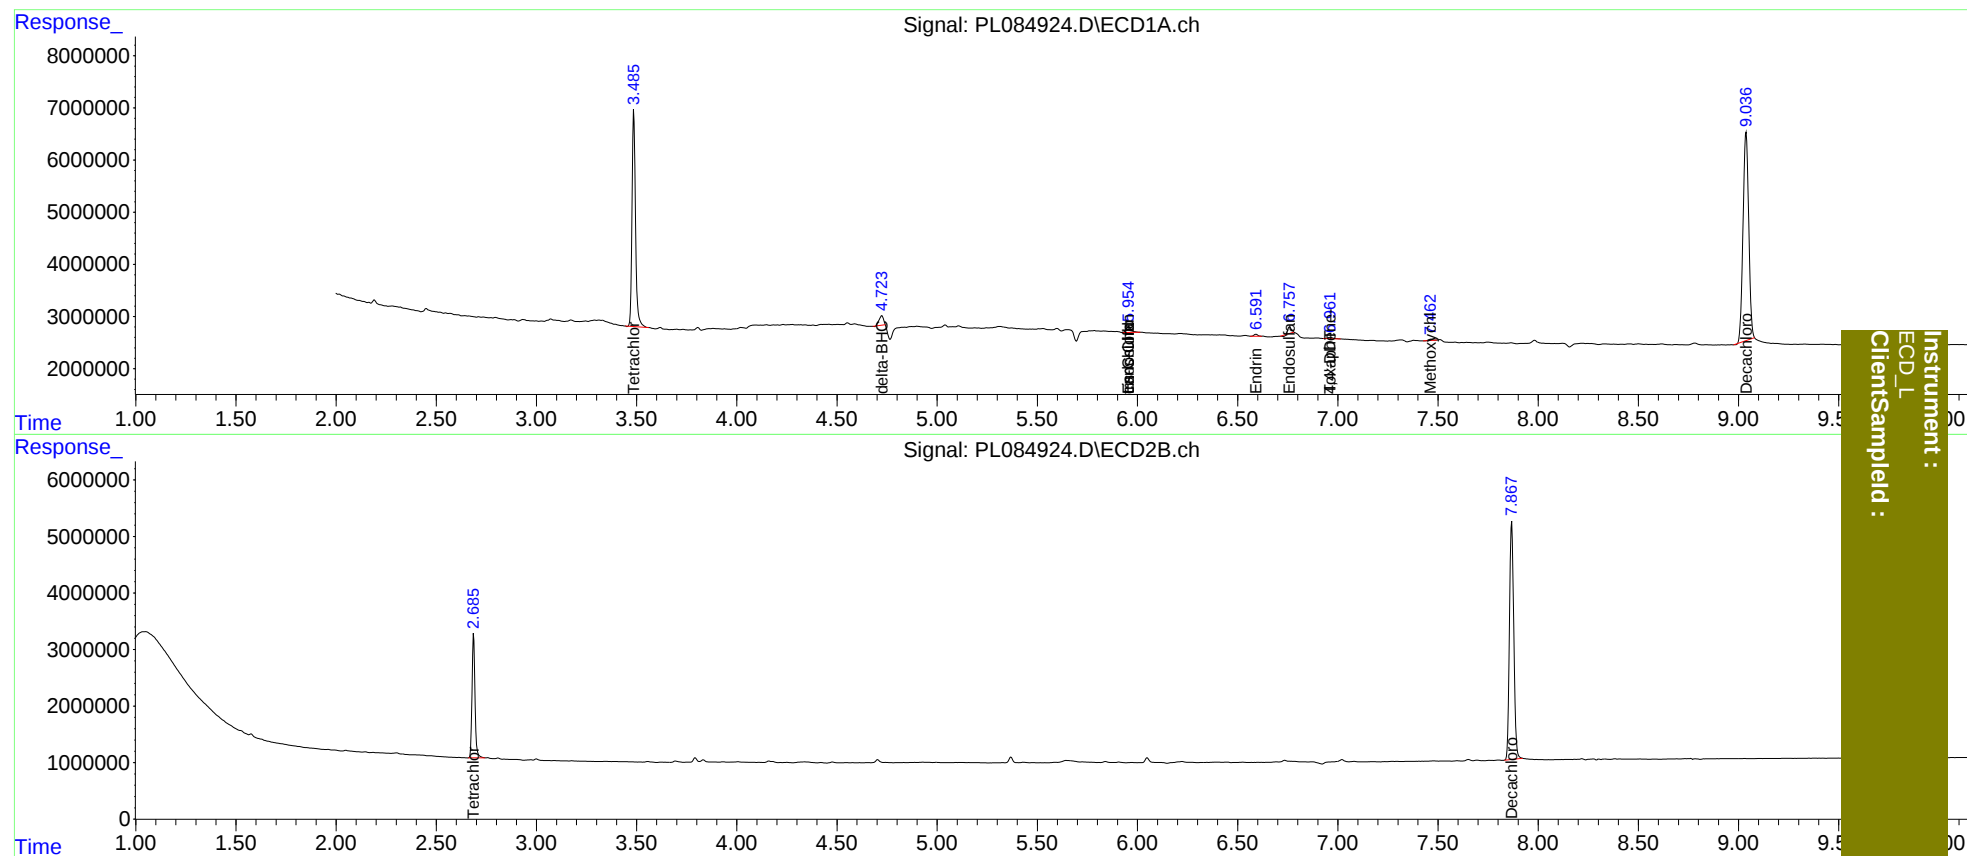


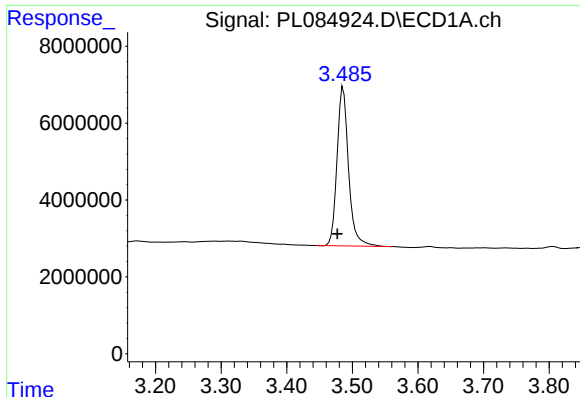

#1 Tetrachloro-m-xylene


R.T.: 3.486 min
Delta R.T.: 0.009 min
Response: 50399806
Conc: 20.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

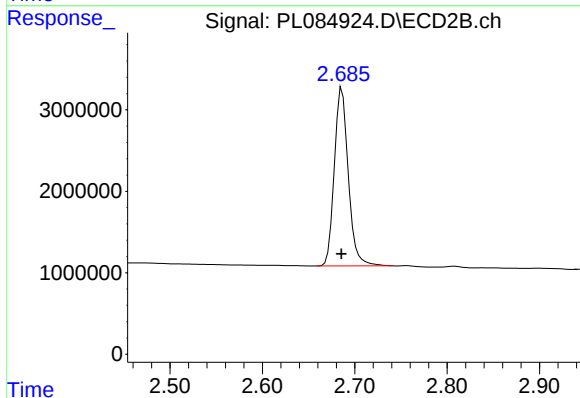


#1 Tetrachloro-m-xylene

R.T.: 2.686 min
Delta R.T.: 0.000 min
Response: 23006786
Conc: 19.49 ng/ml

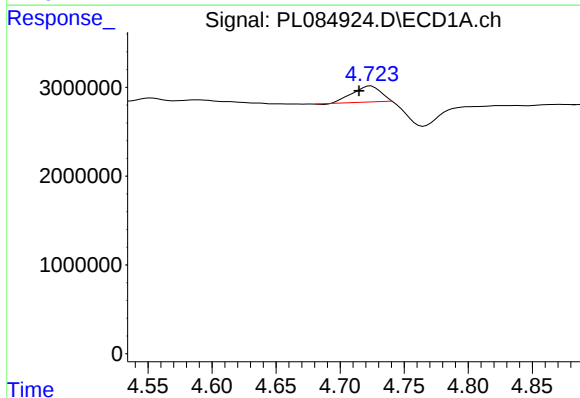


#7 delta-BHC

R.T.: 4.724 min
Delta R.T.: 0.009 min
Response: 2784485
Conc: 0.76 ng/ml

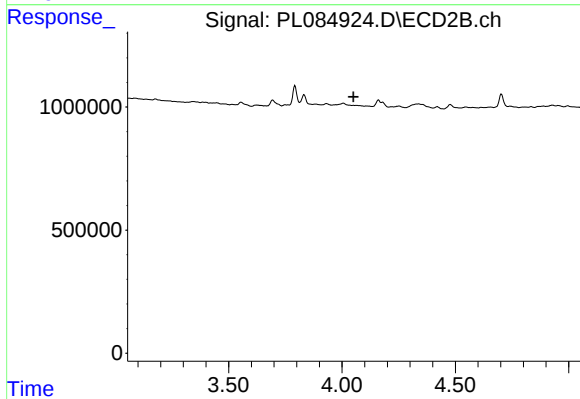

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.051 min
Response: 0
Conc: N.D.

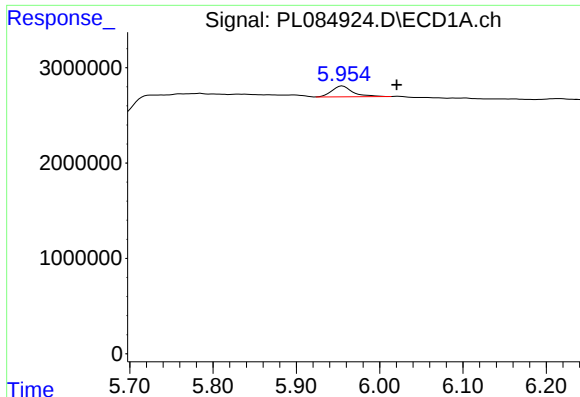

#9 Endosulfan I


R.T.: 5.955 min
Delta R.T.: -0.065 min
Response: 1946960
Conc: 0.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

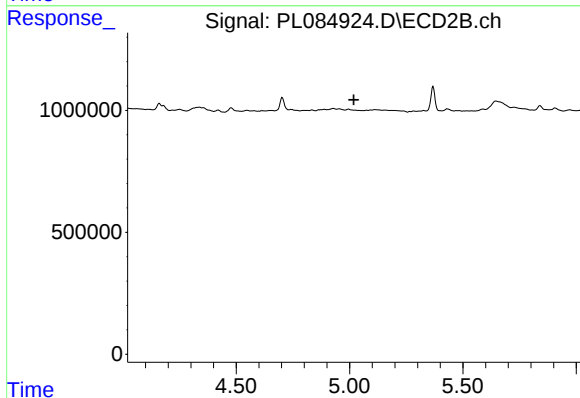


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.019 min
Response: 0
Conc: N.D.

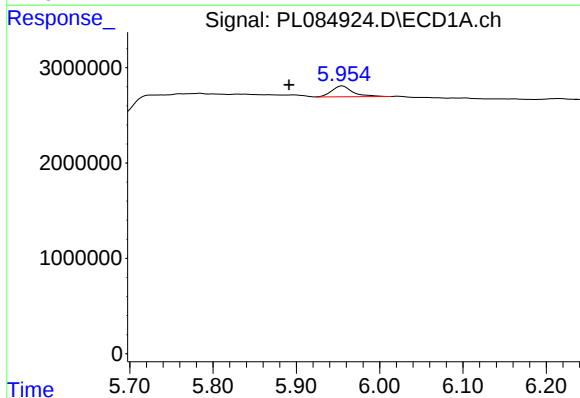


#10 trans-Chlordane

R.T.: 5.955 min
Delta R.T.: 0.064 min
Response: 1946960
Conc: 0.62 ng/ml

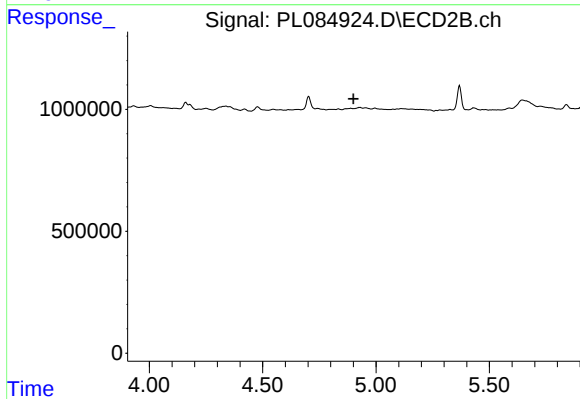

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T. : 4.901 min
Response: 0
Conc: N.D.

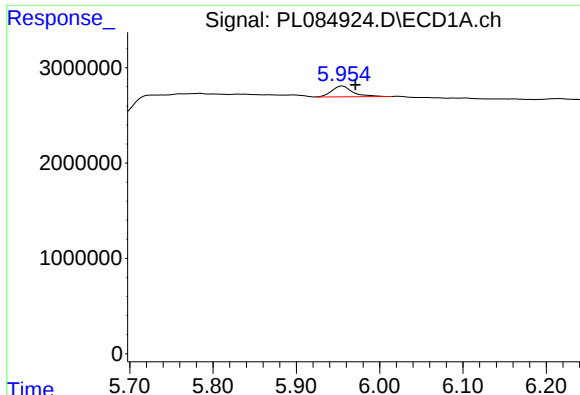

#11 cis-Chlordane


R.T.: 5.955 min
Delta R.T.: -0.016 min
Response: 1946960
Conc: 0.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

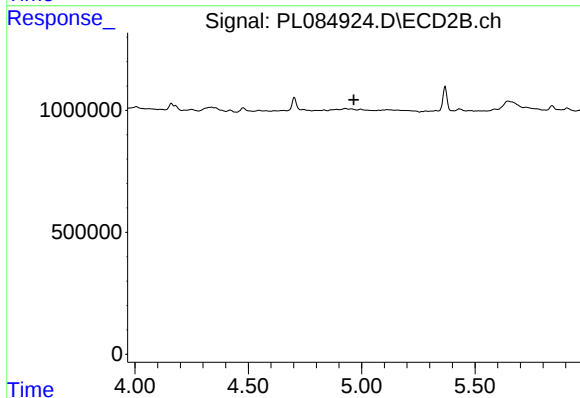


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.965 min
Response: 0
Conc: N.D.

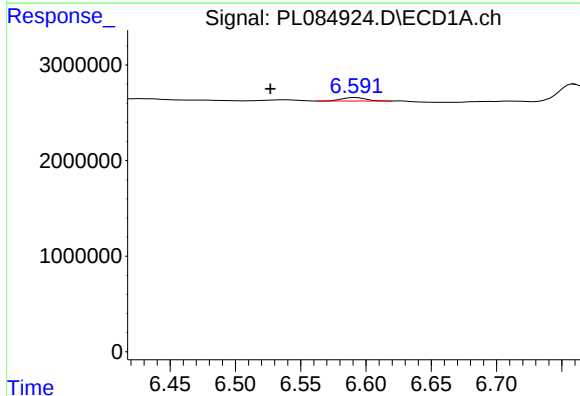


#14 Endrin

R.T.: 6.592 min
Delta R.T.: 0.065 min
Response: 470130
Conc: 0.21 ng/ml

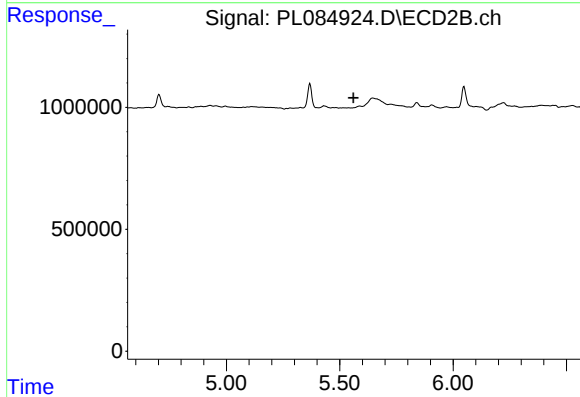

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 5.561 min
Response: 0
Conc: N.D.

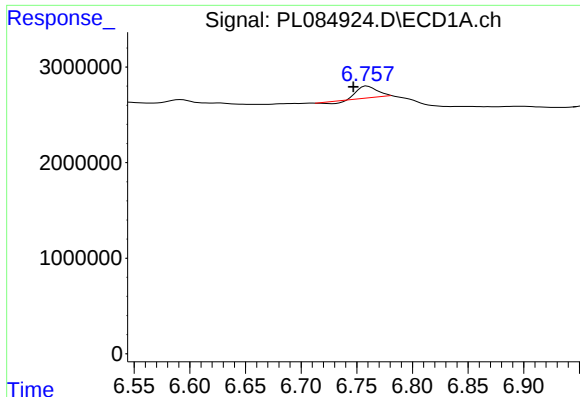

#15 Endosulfan II


R.T.: 6.759 min
Delta R.T.: 0.013 min
Response: 1423216
Conc: 0.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

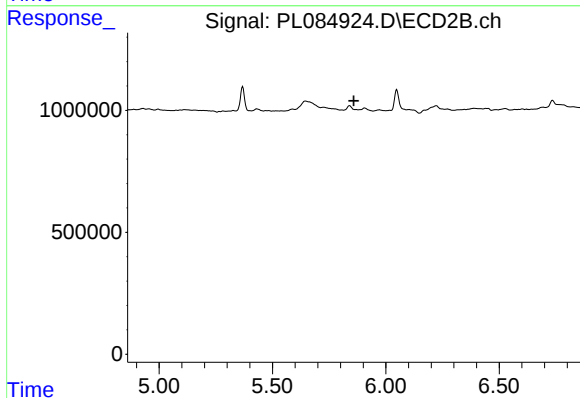


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.859 min
Response: 0
Conc: N.D.

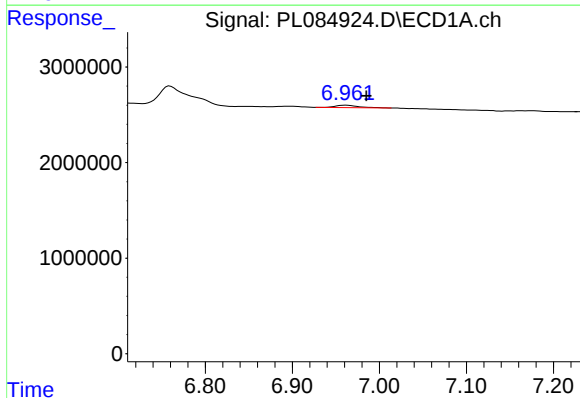


#17 4,4'-DDT

R.T.: 6.962 min
Delta R.T.: -0.024 min
Response: 458081
Conc: 0.24 ng/ml

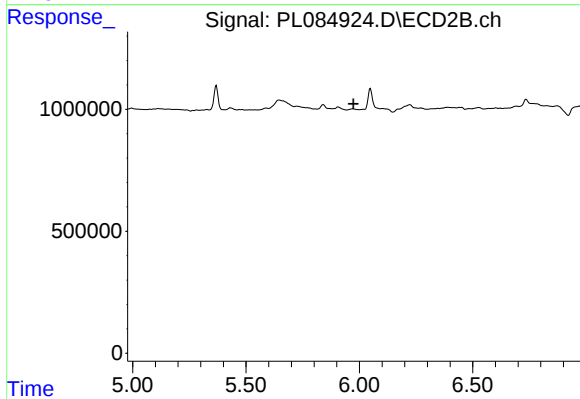

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 5.974 min
Response: 0
Conc: N.D.

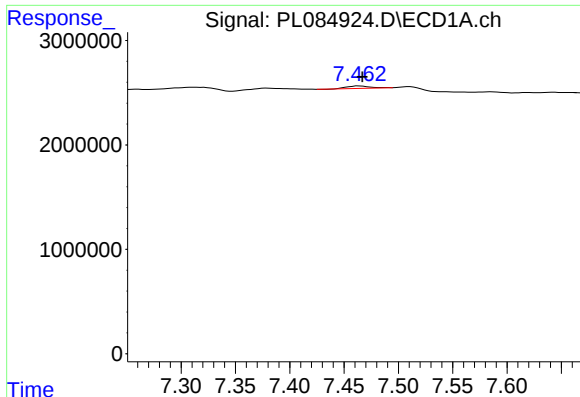

#20 Methoxychlor


R.T.: 7.464 min
Delta R.T.: -0.003 min
Response: 323508
Conc: 0.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

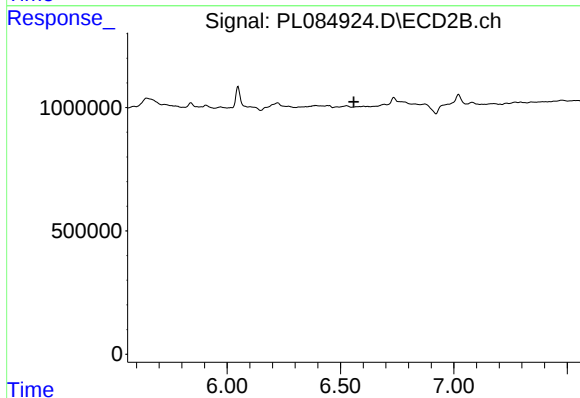


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.559 min
Response: 0
Conc: N.D.

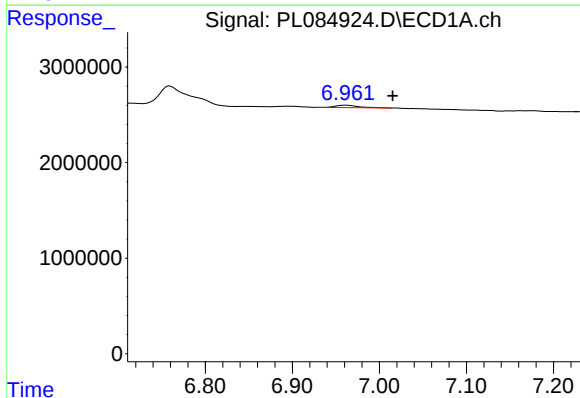


#23 Toxaphene-2

R.T.: 6.962 min
Delta R.T.: -0.054 min
Response: 458081
Conc: 6.89 ng/ml

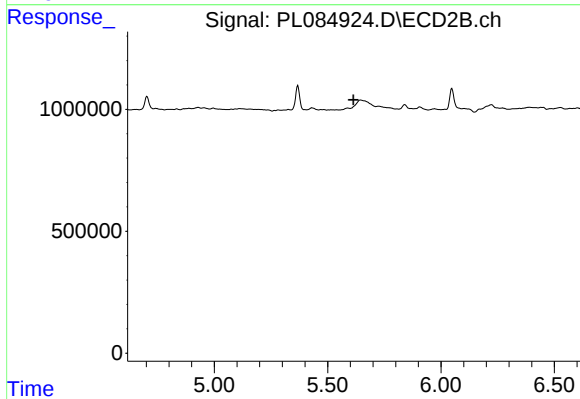

#23 Toxaphene-2


R.T.: 0.000 min
Exp R.T. : 5.615 min
Response: 0
Conc: N.D.

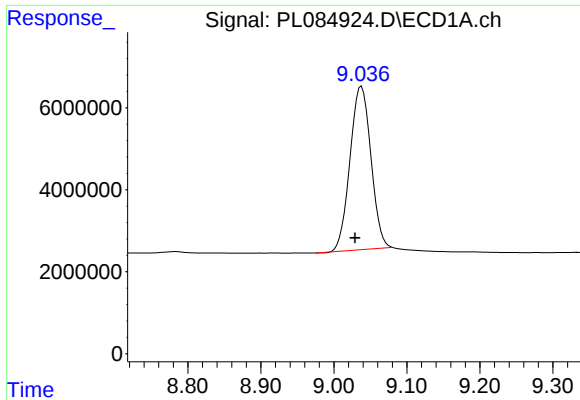

#27 Decachlorobiphenyl

R.T.: 9.038 min
Delta R.T.: 0.009 min
Response: 79401304
Conc: 46.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

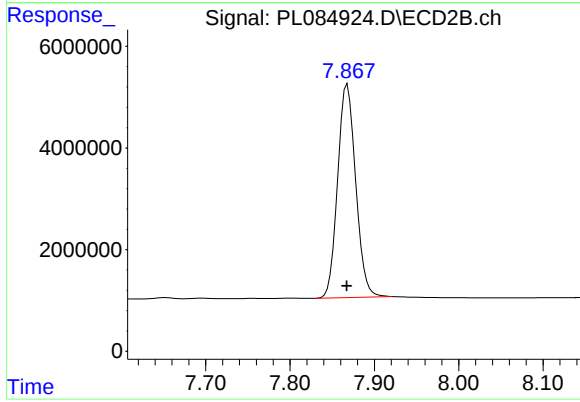

#27 Decachlorobiphenyl

R.T.: 7.868 min
Delta R.T.: 0.000 min
Response: 62502803
Conc: 46.15 ng/ml