

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082323\
 Data File : PL084929.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2023 12:55
 Operator : AR\AJ
 Sample : PIBLK222
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 22:26:59 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 05:52:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.486	2.687	48682034	23461973	19.419	19.875
27)	SA Decachlor...	9.038	7.869	78808212	63390818	45.986	46.804
Target Compounds							
2)	A alpha-BHC	3.897f	0.000	116389	0	<MDL	N.D. #
3)	MA gamma-BHC...	4.230f	0.000	64328	0	<MDL	N.D. #
6)	B beta-BHC	4.424f	0.000	166620	0	<MDL	N.D. #
7)	B delta-BHC	4.725	0.000	2668739	0	0.731	N.D. #
9)	A Endosulfan I	5.955f	0.000	1724514	0	0.605	N.D. #
10)	B trans-Chl...	5.955f	0.000	1724514	0	0.547	N.D. #
11)	B cis-Chlor...	5.955	0.000	1724514	0	0.541	N.D. #
12)	B 4,4'-DDE	6.213f	0.000	125874	0	<MDL	N.D. #
14)	MA Endrin	6.592f	0.000	386037	0	0.169	N.D. #
15)	B Endosulfa...	6.759	0.000	1134328	0	0.482	N.D. #
17)	MA 4,4'-DDT	6.962	0.000	404651	0	0.210	N.D. #
18)	B Endrin al...	6.897	0.000	71277	0	<MDL	N.D. #
20)	A Methoxychlor	7.465	0.000	150831	0	0.155	N.D. #
22)	Toxaphene-1	6.213	0.000	125874	0	6.121	N.D. #
23)	Toxaphene-2	6.962f	0.000	404651	0	6.089	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082323\
Data File : PL084929.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2023 12:55
Operator : AR\AJ
Sample : PIBLK222
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 22:26:59 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

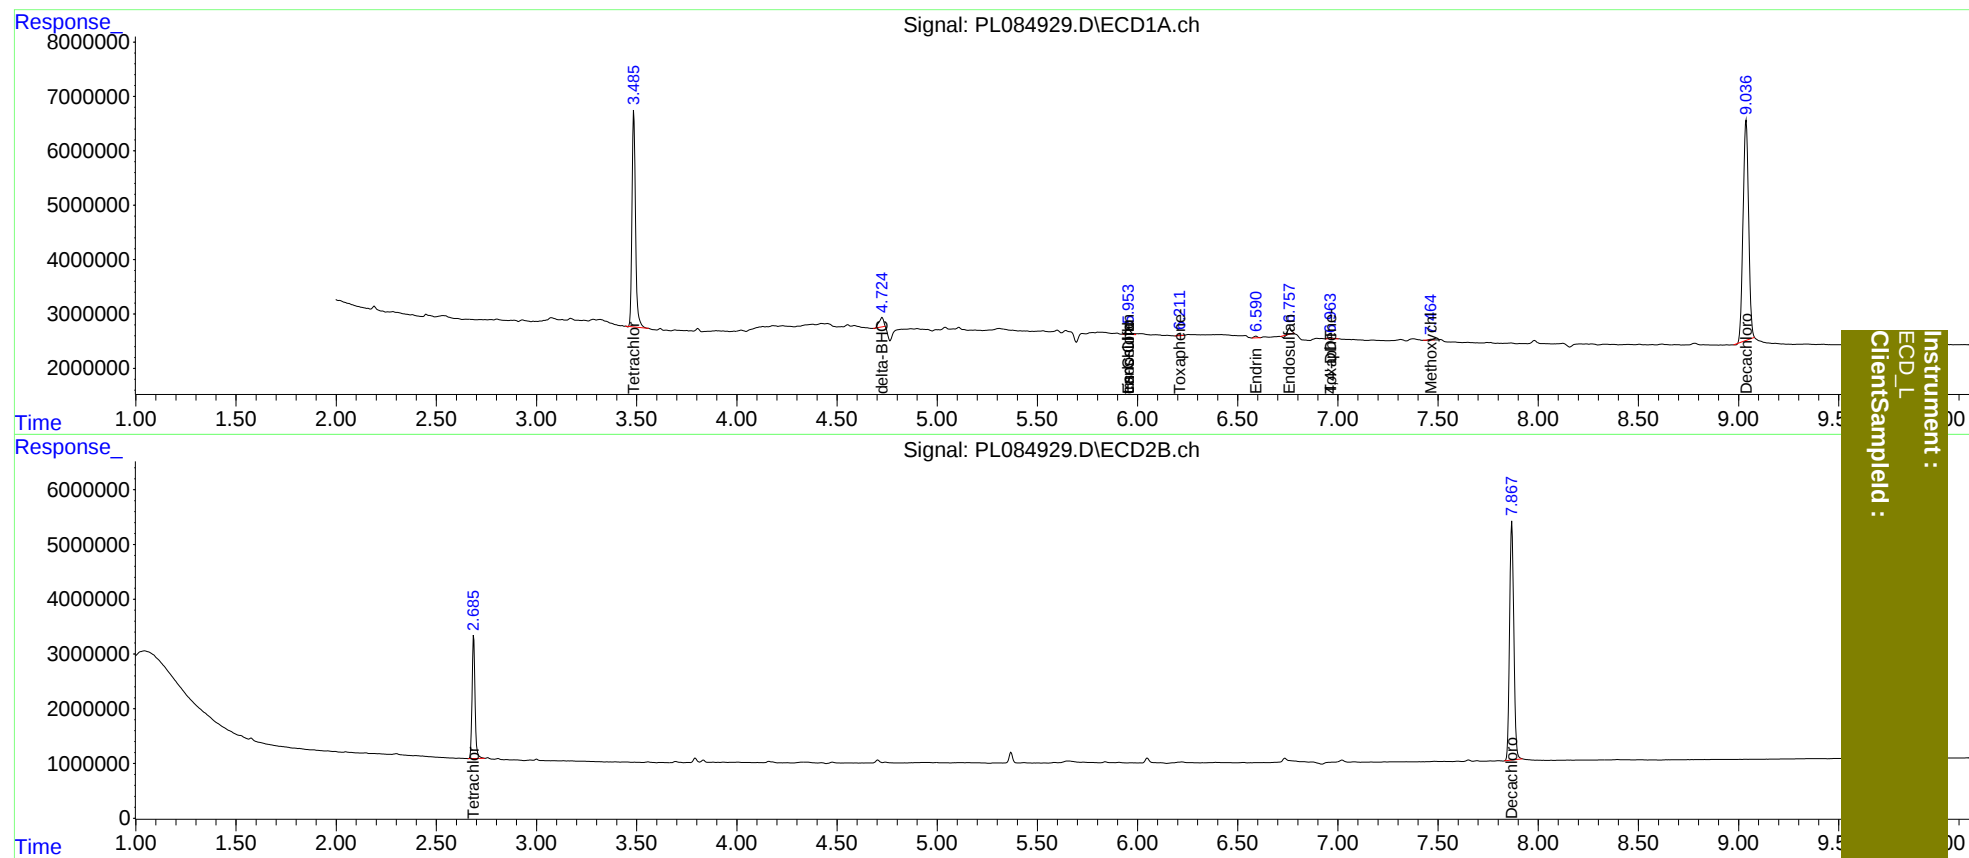


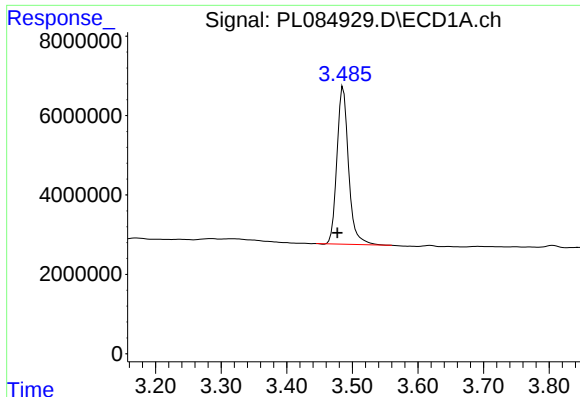

#1 Tetrachloro-m-xylene


R.T.: 3.486 min
Delta R.T.: 0.009 min
Response: 48682034
Conc: 19.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

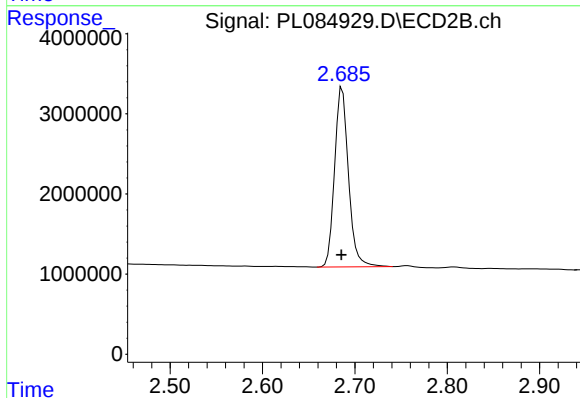


#1 Tetrachloro-m-xylene

R.T.: 2.687 min
Delta R.T.: 0.000 min
Response: 23461973
Conc: 19.87 ng/ml

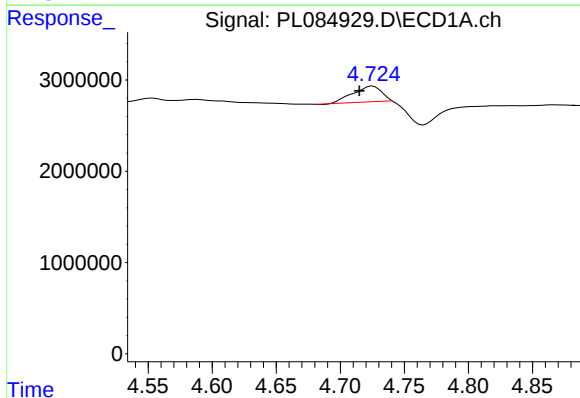


#7 delta-BHC

R.T.: 4.725 min
Delta R.T.: 0.010 min
Response: 2668739
Conc: 0.73 ng/ml

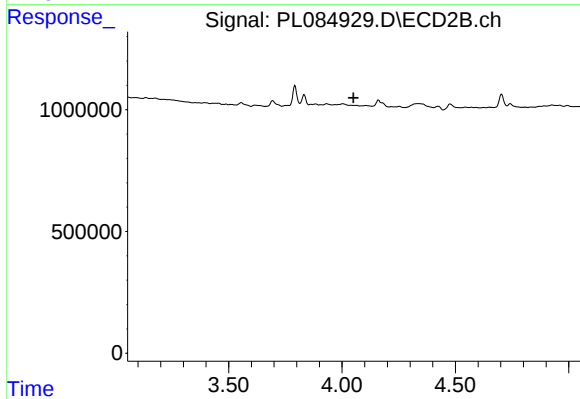

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.051 min
Response: 0
Conc: N.D.

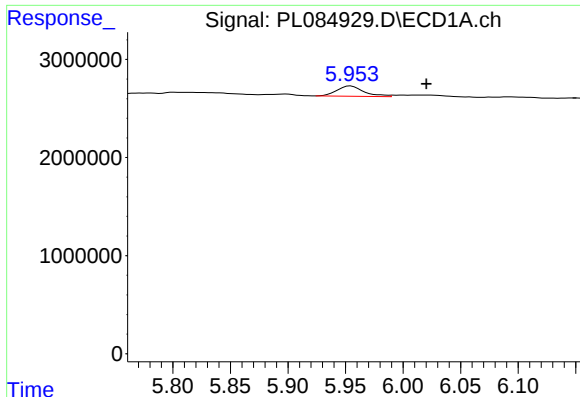

#9 Endosulfan I


R.T.: 5.955 min
Delta R.T.: -0.066 min
Response: 1724514
Conc: 0.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

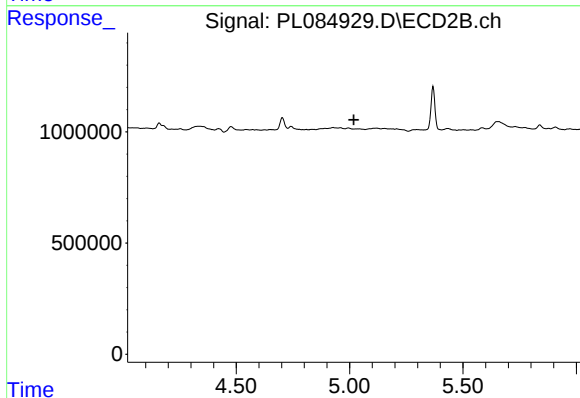


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.019 min
Response: 0
Conc: N.D.

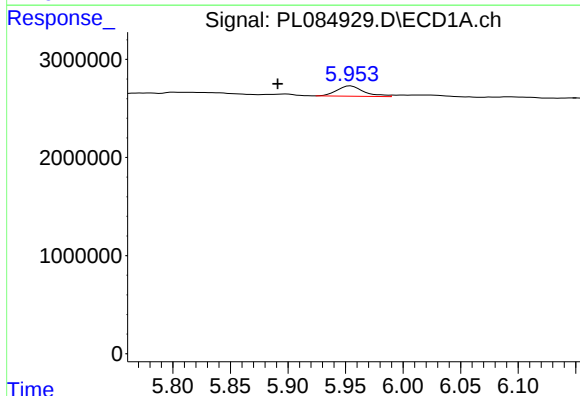


#10 trans-Chlordane

R.T.: 5.955 min
Delta R.T.: 0.063 min
Response: 1724514
Conc: 0.55 ng/ml

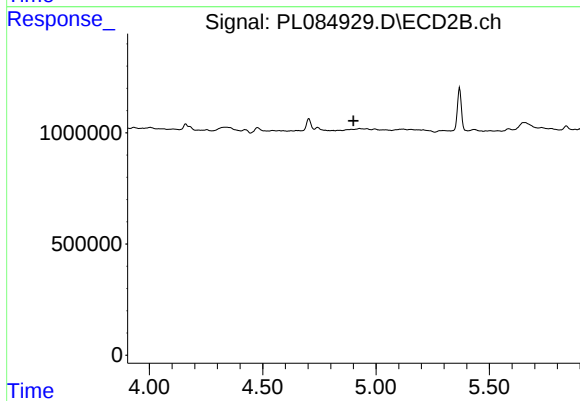

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T. : 4.901 min
Response: 0
Conc: N.D.

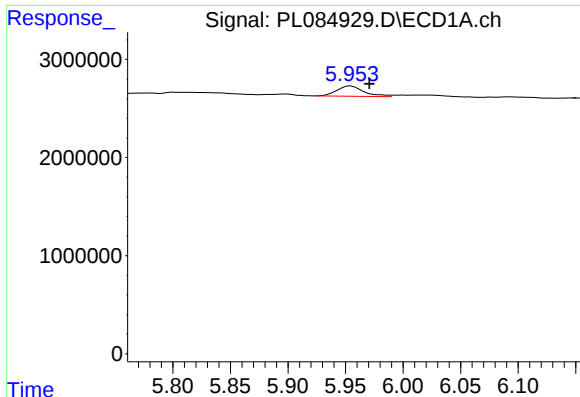

#11 cis-Chlordane


R.T.: 5.955 min
Delta R.T.: -0.016 min
Response: 1724514
Conc: 0.54 ng/ml

Instrument :
ECD_L
ClientSampleId :

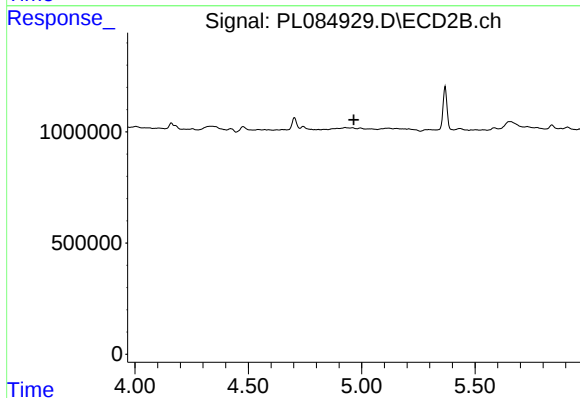


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.965 min
Response: 0
Conc: N.D.

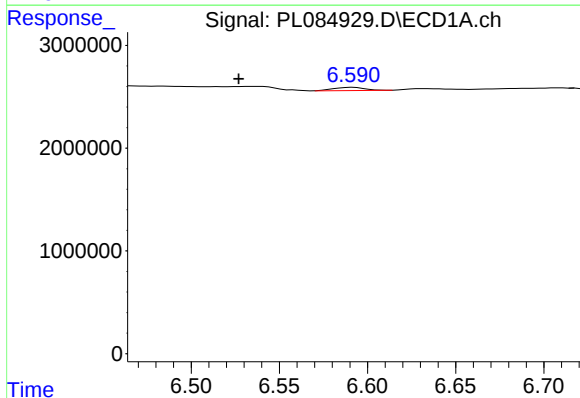


#14 Endrin

R.T.: 6.592 min
Delta R.T.: 0.065 min
Response: 386037
Conc: 0.17 ng/ml

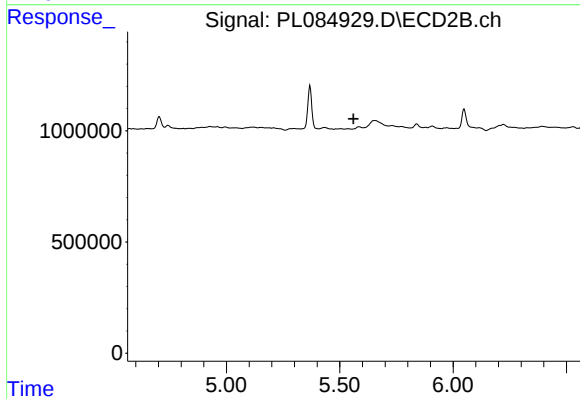

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 5.561 min
Response: 0
Conc: N.D.

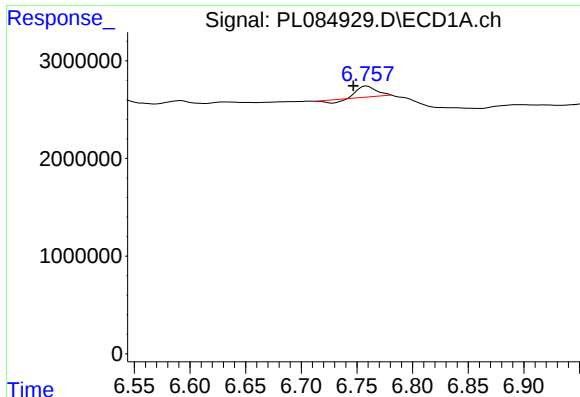

#15 Endosulfan II


R.T.: 6.759 min
Delta R.T.: 0.012 min
Response: 1134328
Conc: 0.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

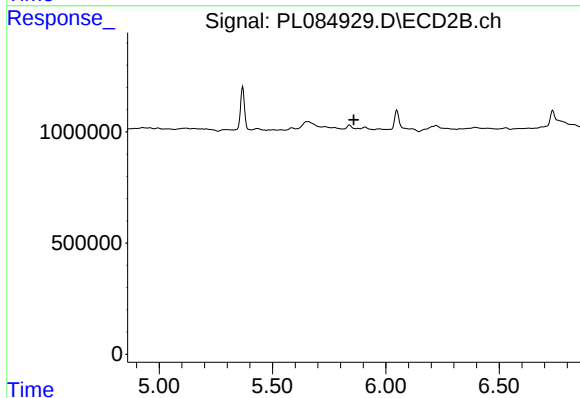


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.859 min
Response: 0
Conc: N.D.

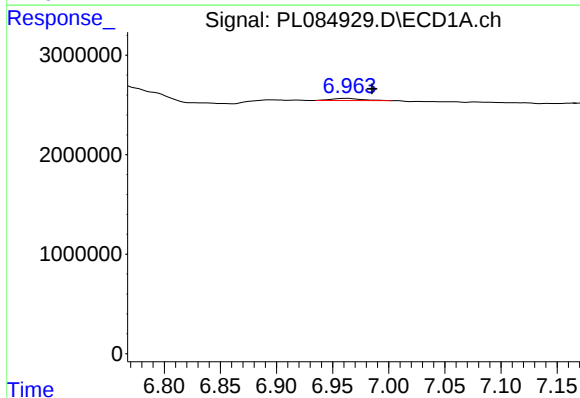


#17 4,4'-DDT

R.T.: 6.962 min
Delta R.T.: -0.024 min
Response: 404651
Conc: 0.21 ng/ml

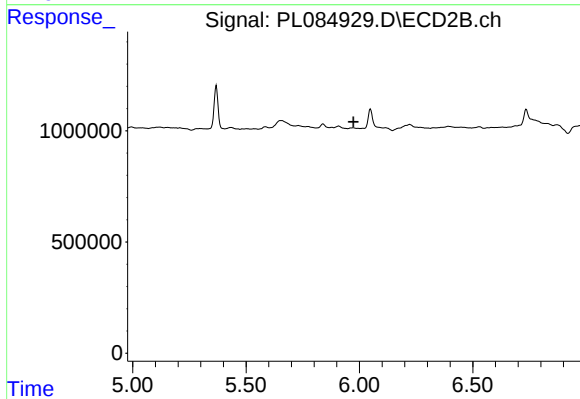

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 5.974 min
Response: 0
Conc: N.D.

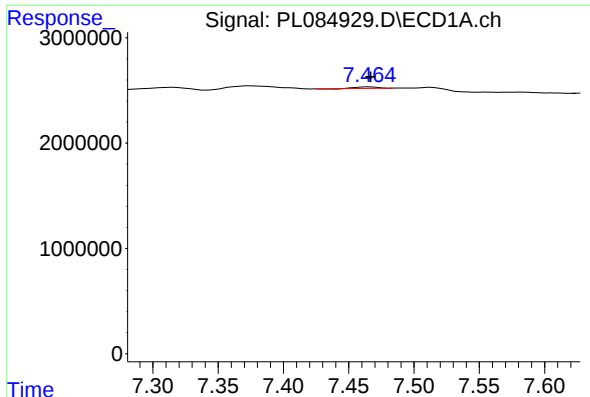

#20 Methoxychlor


R.T.: 7.465 min
Delta R.T.: -0.002 min
Response: 150831
Conc: 0.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

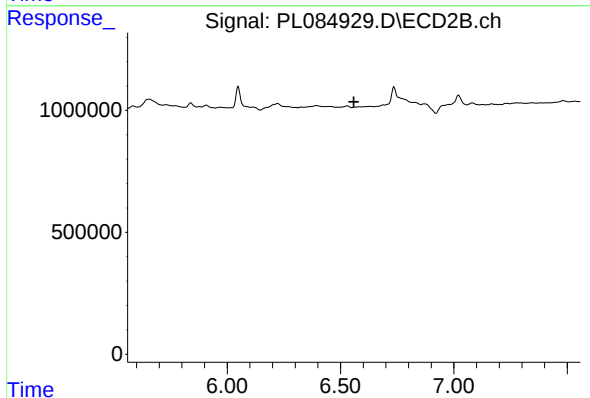


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.559 min
Response: 0
Conc: N.D.

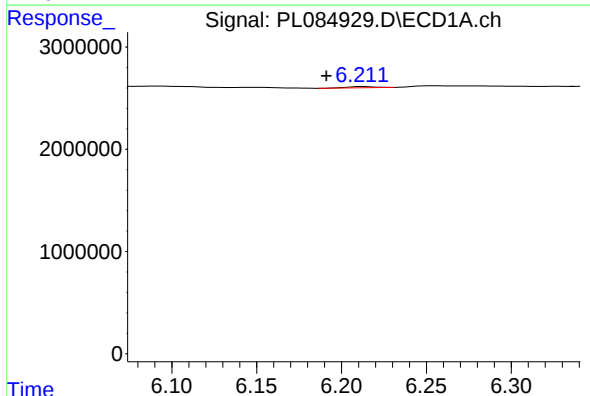


#22 Toxaphene-1

R.T.: 6.213 min
Delta R.T.: 0.021 min
Response: 125874
Conc: 6.12 ng/ml

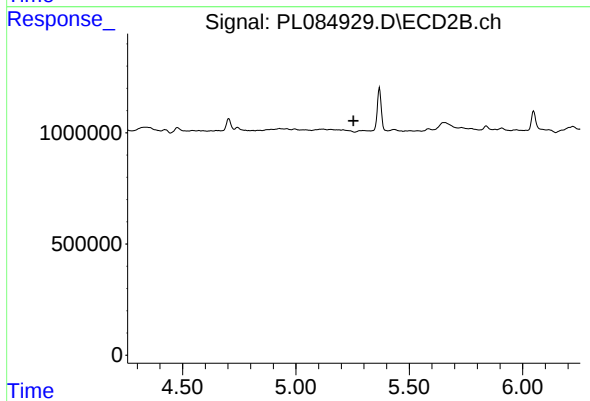

#22 Toxaphene-1


R.T.: 0.000 min
Exp R.T. : 5.254 min
Response: 0
Conc: N.D.

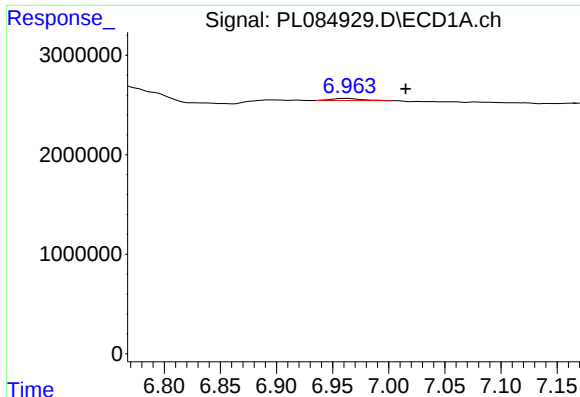

#23 Toxaphene-2


R.T.: 6.962 min
Delta R.T.: -0.054 min
Response: 404651
Conc: 6.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

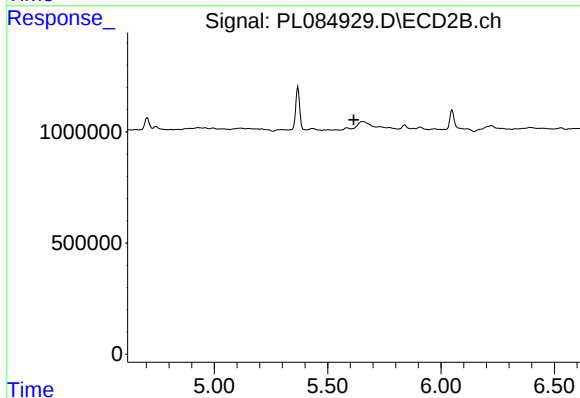


#23 Toxaphene-2

R.T.: 0.000 min
Exp R.T. : 5.615 min
Response: 0
Conc: N.D.

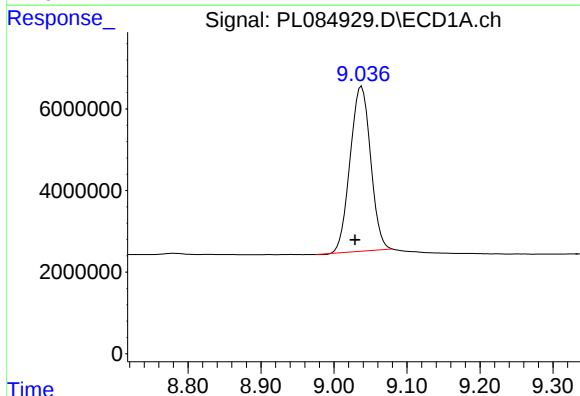

#27 Decachlorobiphenyl

R.T.: 9.038 min
Delta R.T.: 0.009 min
Response: 78808212
Conc: 45.99 ng/ml

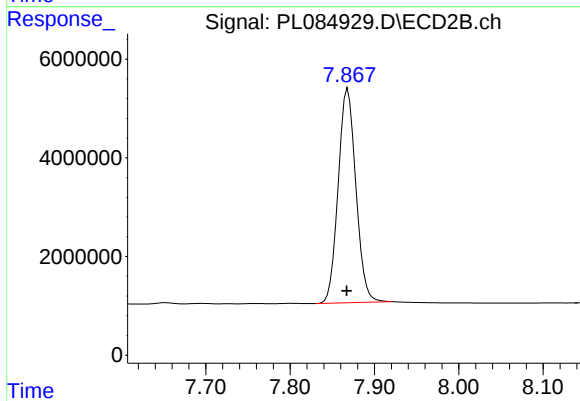

#27 Decachlorobiphenyl

R.T.: 7.869 min
Delta R.T.: 0.001 min
Response: 63390818
Conc: 46.80 ng/ml