

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082323\
 Data File : PL084945.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2023 19:12
 Operator : AR\AJ
 Sample : 04105-11
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 22:33:42 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 05:52:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.477	2.685	45151045	21215803	18.010	17.972
27)	SA Decachlor...	9.027	7.865	52751103	42026517	30.781	31.030
Target Compounds							
2)	A alpha-BHC	3.961f	0.000	279676	0	<MDL	N.D. #
6)	B beta-BHC	4.490	0.000	684681	0	0.388	N.D. #
9)	A Endosulfan I	6.036	0.000	242929	0	<MDL	N.D. #
10)	B trans-Chl...	5.869	0.000	331521	0	0.105	N.D. #
11)	B cis-Chlor...	6.036f	0.000	242929	0	<MDL	N.D. #
14)	MA Endrin	6.529	0.000	270080	0	0.119	N.D. #
15)	B Endosulfa...	6.796f	0.000	343620	0	0.146	N.D. #
17)	MA 4,4'-DDT	6.957	0.000	407481	0	0.211	N.D. #
20)	A Methoxychlor	7.508f	0.000	174536	0	0.180	N.D. #
23)	Toxaphene-2	6.957f	0.000	407481	0	6.131	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082323\
Data File : PL084945.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2023 19:12
Operator : AR\AJ
Sample : 04105-11
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 22:33:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

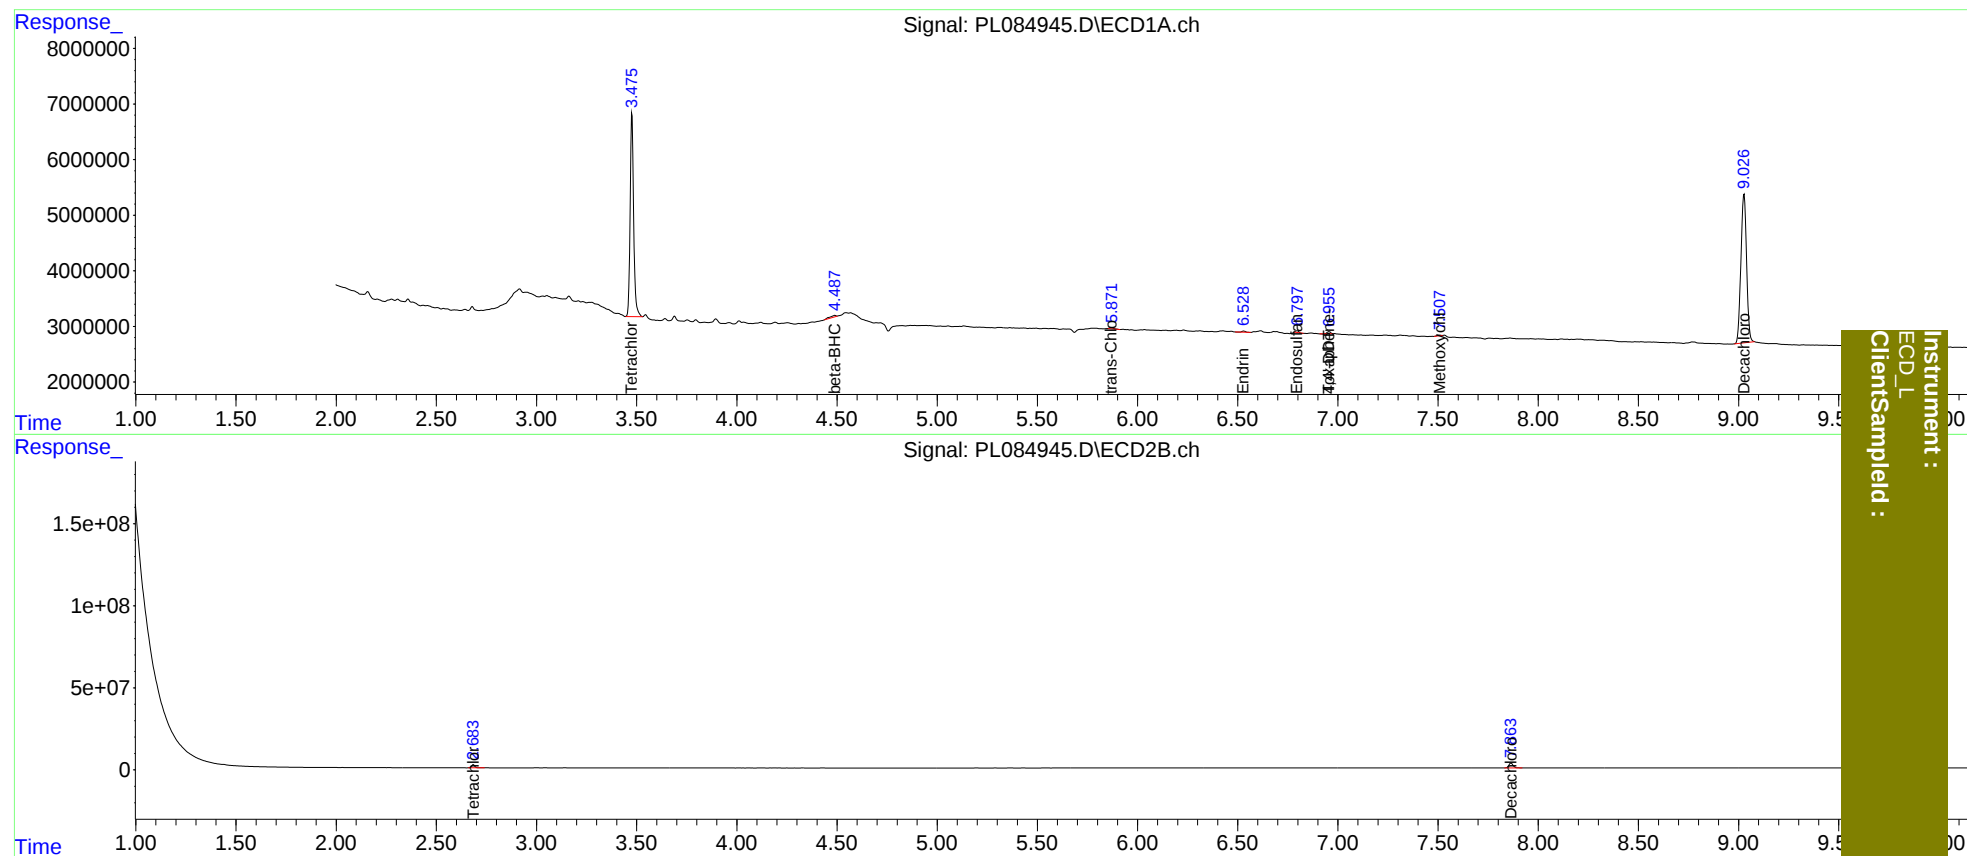


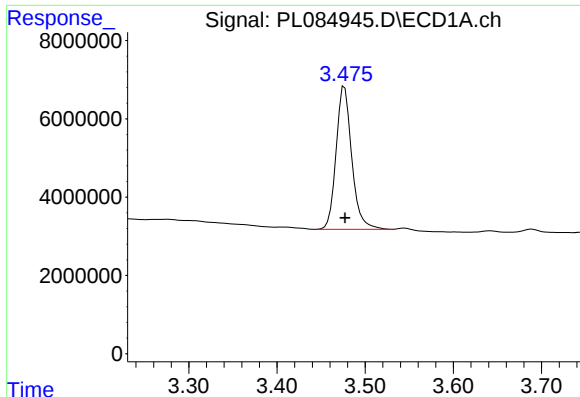

#1 Tetrachloro-m-xylene


R.T.: 3.477 min
Delta R.T.: 0.000 min
Response: 45151045
Conc: 18.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

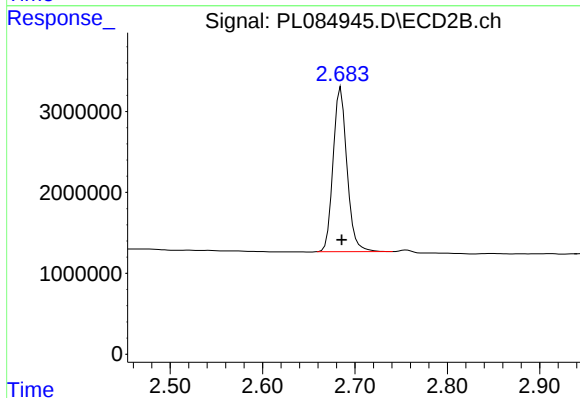


#1 Tetrachloro-m-xylene

R.T.: 2.685 min
Delta R.T.: 0.000 min
Response: 21215803
Conc: 17.97 ng/ml

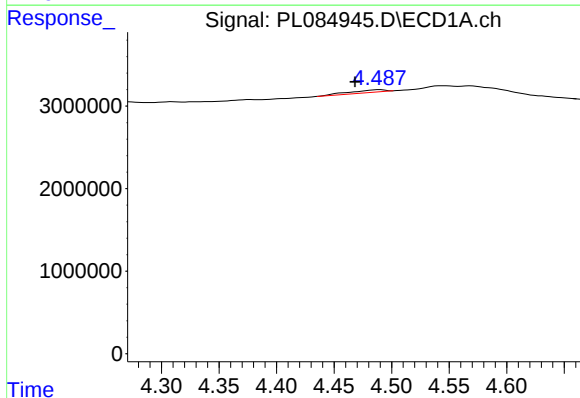


#6 beta-BHC

R.T.: 4.490 min
Delta R.T.: 0.021 min
Response: 684681
Conc: 0.39 ng/ml

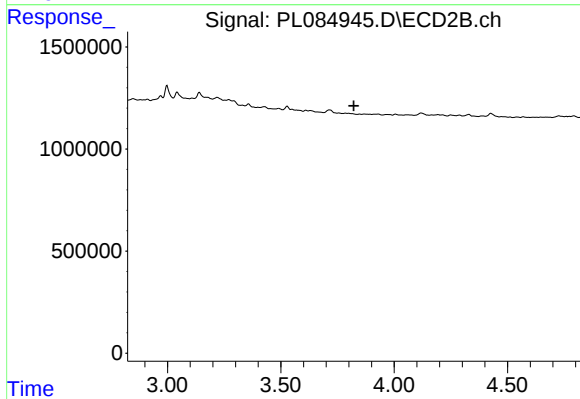

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 3.822 min
Response: 0
Conc: N.D.

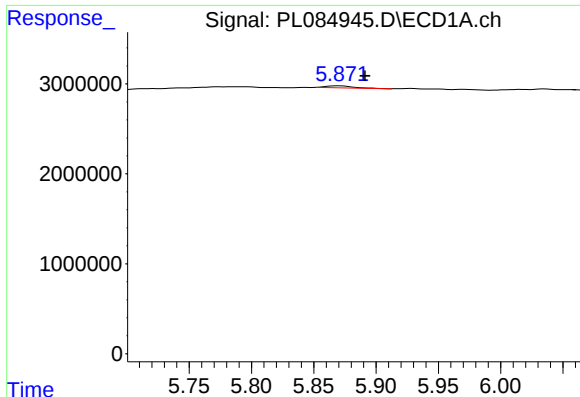

#10 trans-Chlordane


R.T.: 5.869 min
Delta R.T.: -0.022 min
Response: 331521
Conc: 0.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

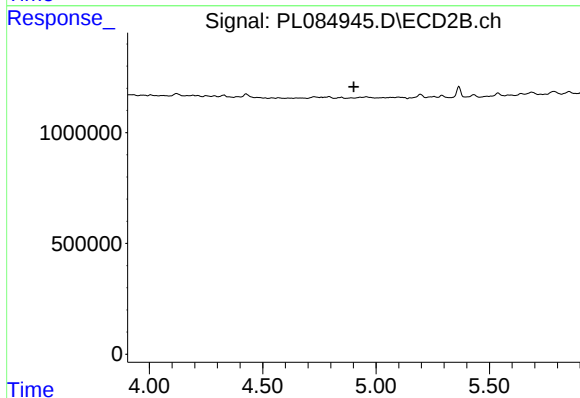


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.901 min
Response: 0
Conc: N.D.

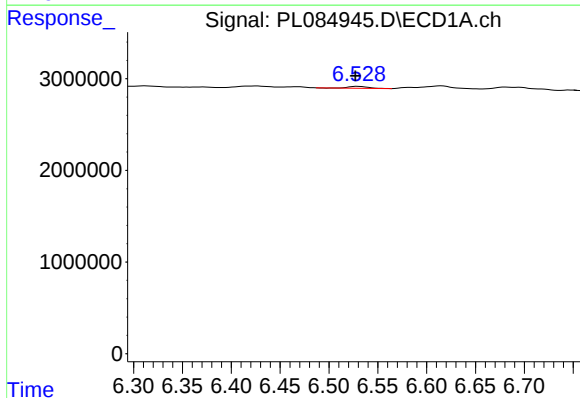


#14 Endrin

R.T.: 6.529 min
Delta R.T.: 0.002 min
Response: 270080
Conc: 0.12 ng/ml

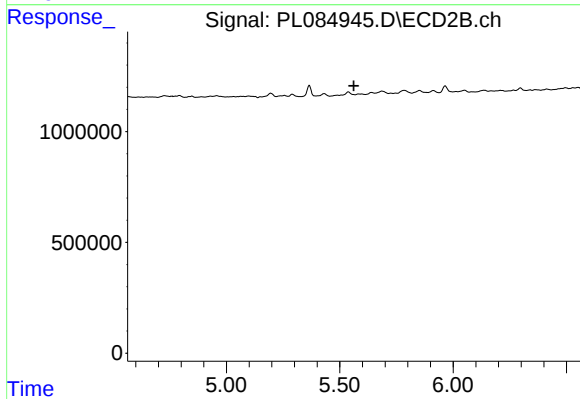

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 5.561 min
Response: 0
Conc: N.D.

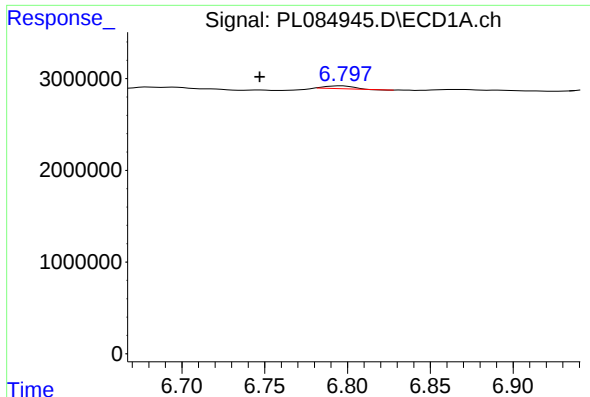

#15 Endosulfan II


R.T.: 6.796 min
Delta R.T.: 0.049 min
Response: 343620
Conc: 0.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

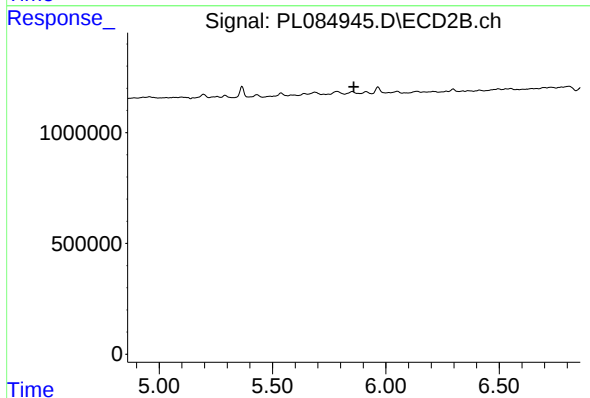


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.859 min
Response: 0
Conc: N.D.

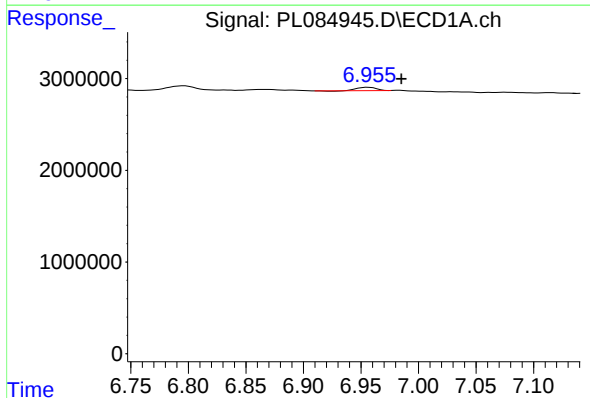


#17 4,4'-DDT

R.T.: 6.957 min
Delta R.T.: -0.029 min
Response: 407481
Conc: 0.21 ng/ml

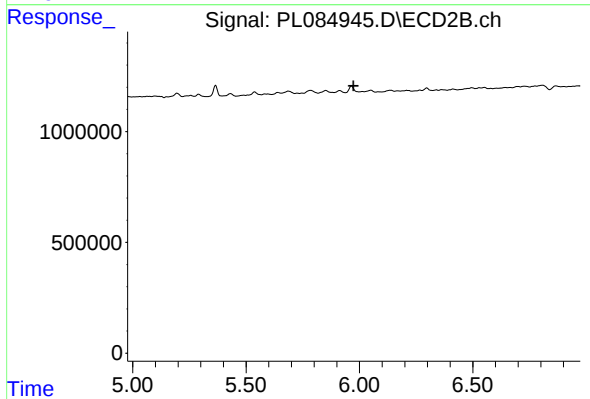

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 5.974 min
Response: 0
Conc: N.D.

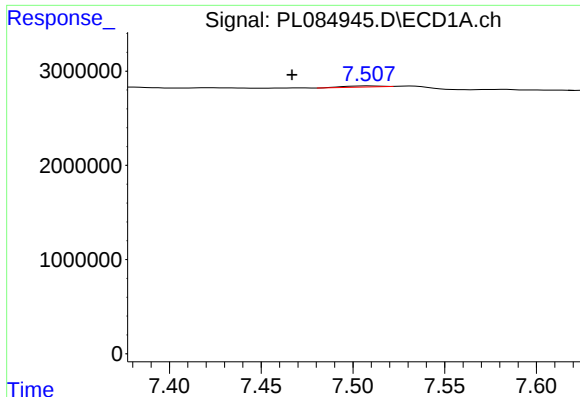

#20 Methoxychlor


R.T.: 7.508 min
Delta R.T.: 0.042 min
Response: 174536
Conc: 0.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

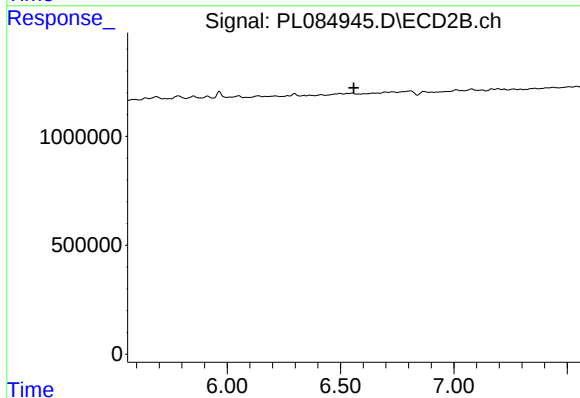


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.559 min
Response: 0
Conc: N.D.

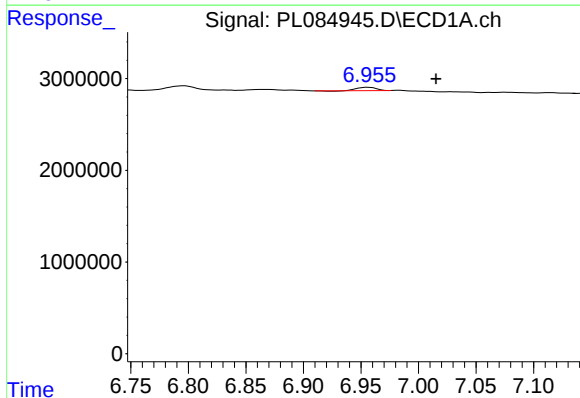


#23 Toxaphene-2

R.T.: 6.957 min
Delta R.T.: -0.059 min
Response: 407481
Conc: 6.13 ng/ml

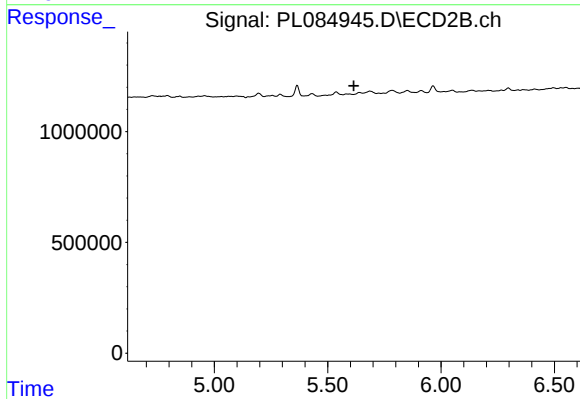

#23 Toxaphene-2


R.T.: 0.000 min
Exp R.T. : 5.615 min
Response: 0
Conc: N.D.

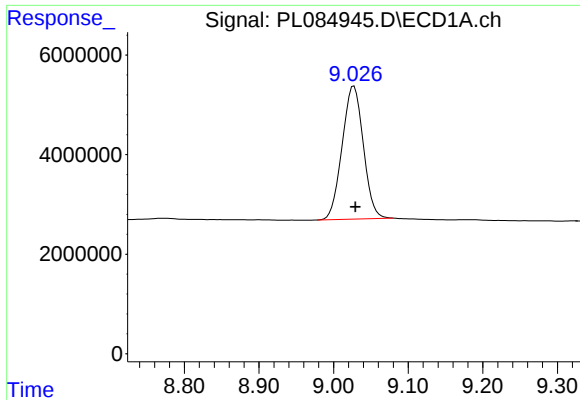

#27 Decachlorobiphenyl

R.T.: 9.027 min
Delta R.T.: -0.002 min
Response: 52751103
Conc: 30.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

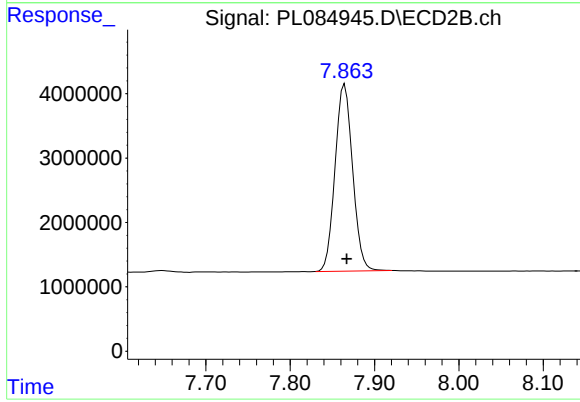

#27 Decachlorobiphenyl

R.T.: 7.865 min
Delta R.T.: -0.002 min
Response: 42026517
Conc: 31.03 ng/ml