

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082323\
 Data File : PL084950.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2023 20:22
 Operator : AR\AJ
 Sample : PIBLK223
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 22:35:32 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 05:52:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.477	2.685	50590090	23842624	20.180	20.197
27)	SA Decachlor...	9.024	7.864	78677921	63681455	45.910	47.018
Target Compounds							
7)	B delta-BHC	4.715	0.000	4106384	0	1.125	N.D. #
9)	A Endosulfan I	6.022	0.000	128369	0	<MDL	N.D. #
10)	B trans-Chl...	5.944f	0.000	1765262	0	0.560	N.D. #
11)	B cis-Chlor...	5.944	0.000	1765262	0	0.554	N.D. #
14)	MA Endrin	6.582f	0.000	629200	0	0.276	N.D. #
15)	B Endosulfa...	6.748	0.000	2059449	0	0.876	N.D. #
17)	MA 4,4'-DDT	6.952	0.000	378651	0	0.196	N.D. #
20)	A Methoxychlor	7.454	0.000	320429	0	0.330	N.D. #
23)	Toxaphene-2	6.952f	0.000	378651	0	5.697	N.D. #
26)	Toxaphene-5	7.917	0.000	176323	0	5.363	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082323\
Data File : PL084950.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2023 20:22
Operator : AR\AJ
Sample : PIBLK223
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 22:35:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

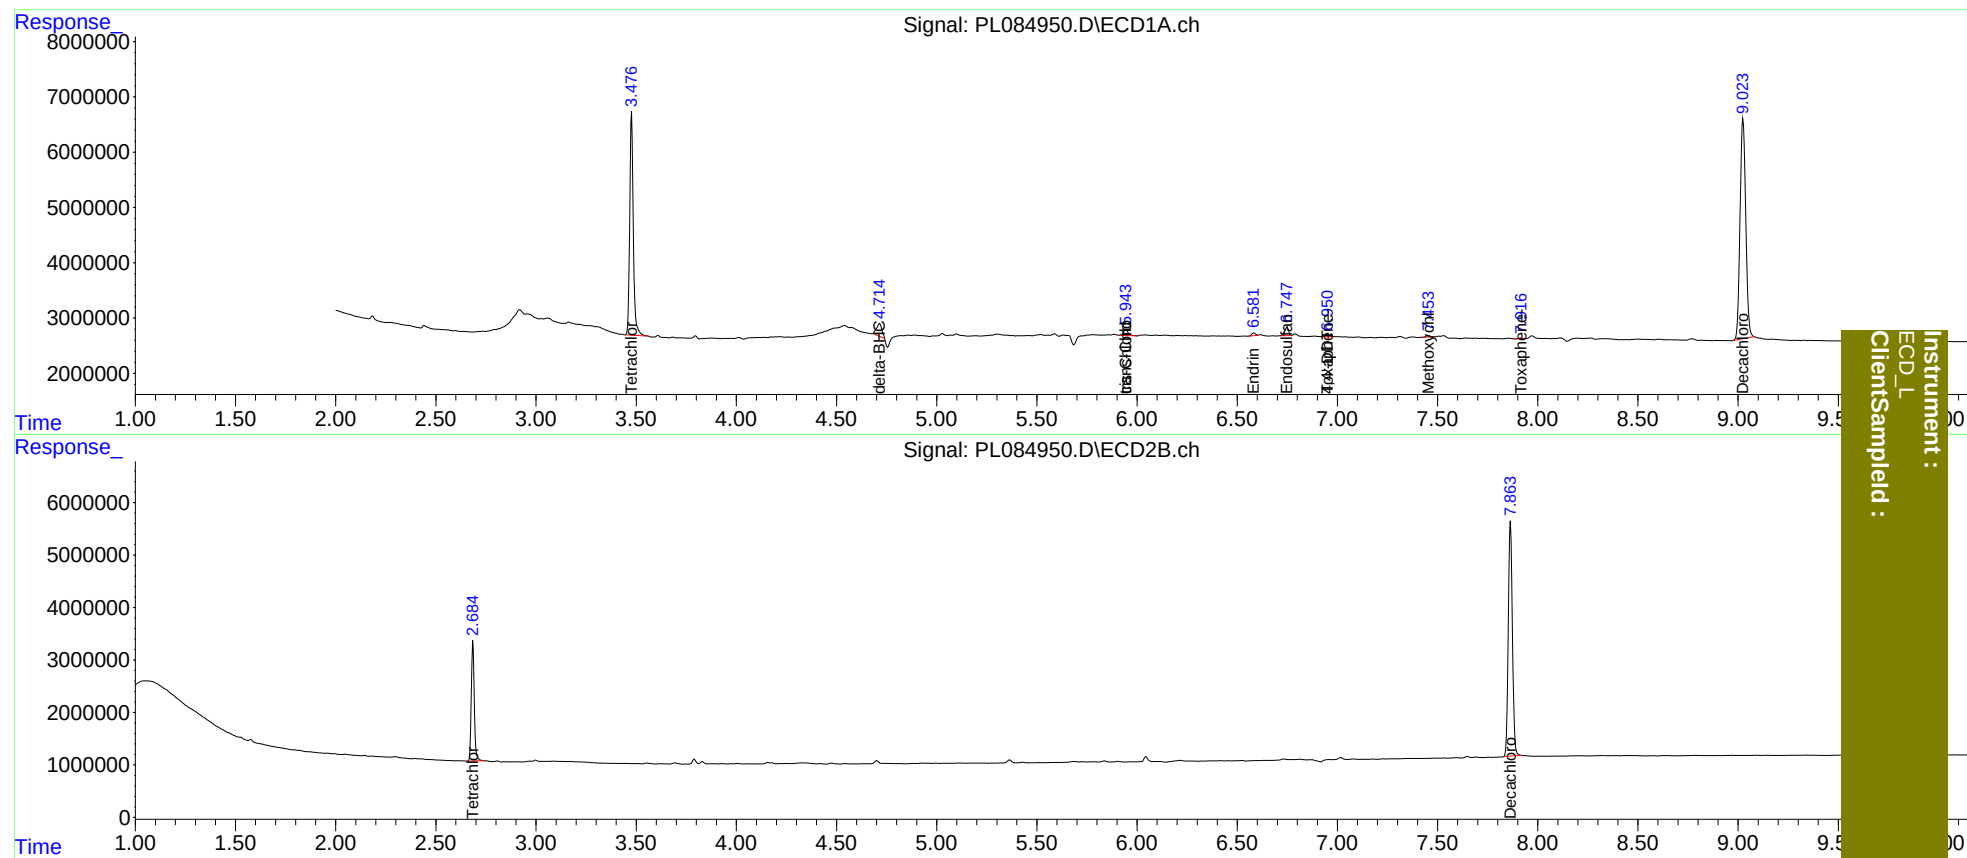


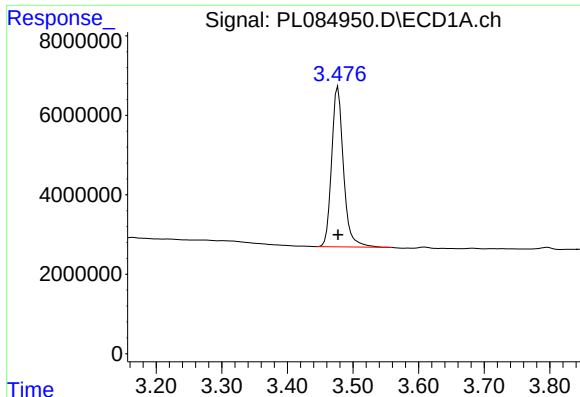

#1 Tetrachloro-m-xylene


R.T.: 3.477 min
Delta R.T.: 0.000 min
Response: 50590090
Conc: 20.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

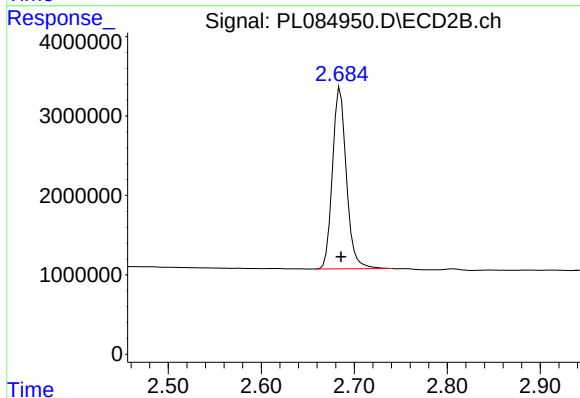


#1 Tetrachloro-m-xylene

R.T.: 2.685 min
Delta R.T.: 0.000 min
Response: 23842624
Conc: 20.20 ng/ml

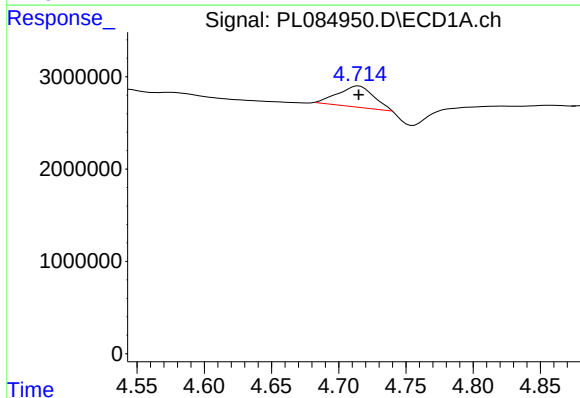


#7 delta-BHC

R.T.: 4.715 min
Delta R.T.: 0.000 min
Response: 4106384
Conc: 1.13 ng/ml

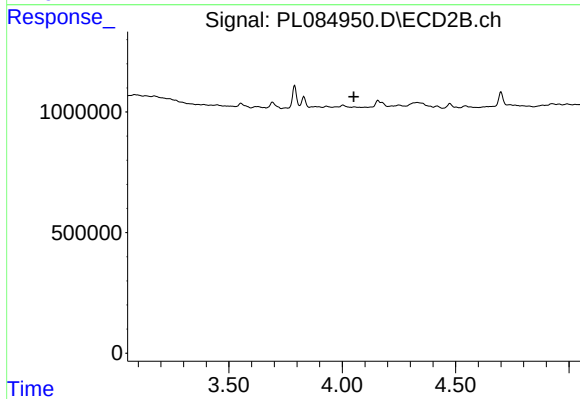

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.051 min
Response: 0
Conc: N.D.

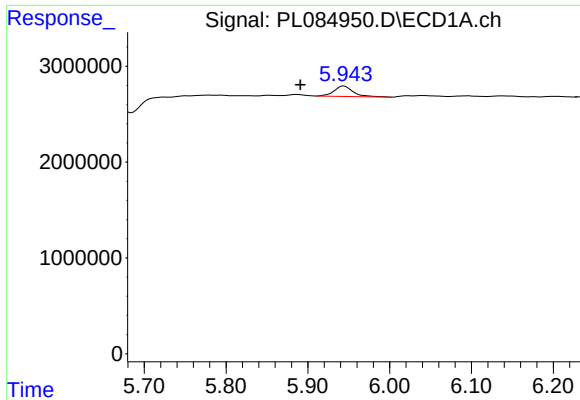

#10 trans-Chlordane


R.T.: 5.944 min
Delta R.T.: 0.053 min
Response: 1765262
Conc: 0.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

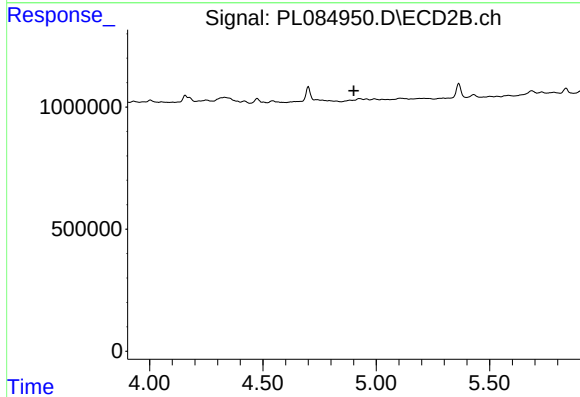


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.901 min
Response: 0
Conc: N.D.

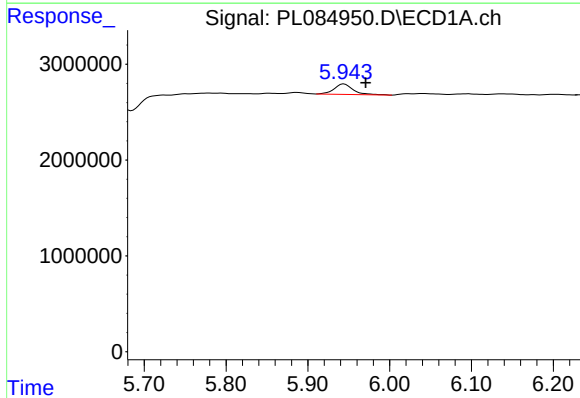


#11 cis-Chlordane

R.T.: 5.944 min
Delta R.T.: -0.027 min
Response: 1765262
Conc: 0.55 ng/ml

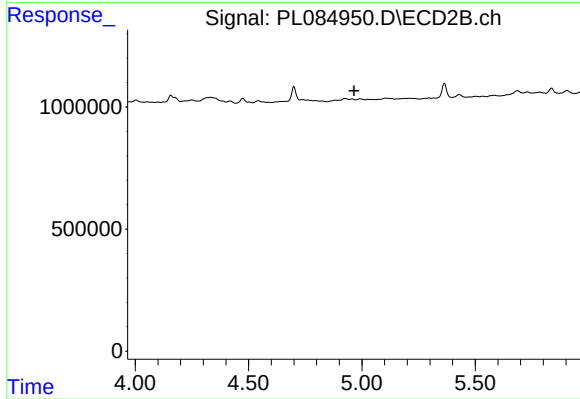

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T. : 4.965 min
Response: 0
Conc: N.D.

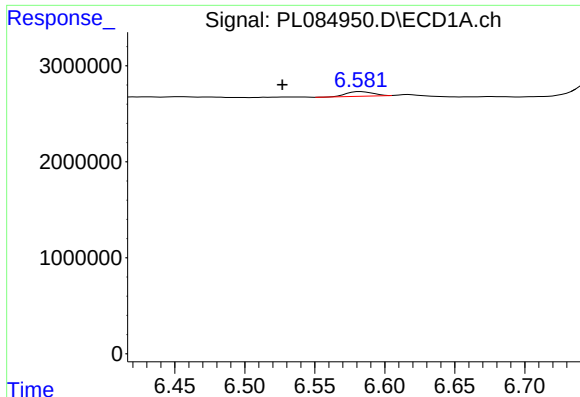

#14 Endrin


R.T.: 6.582 min
Delta R.T.: 0.055 min
Response: 629200
Conc: 0.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

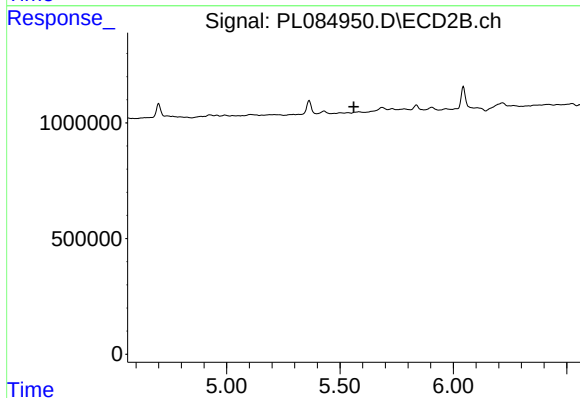


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 5.561 min
Response: 0
Conc: N.D.

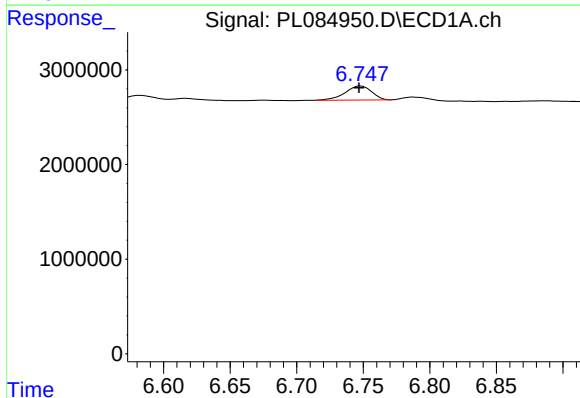


#15 Endosulfan II

R.T.: 6.748 min
Delta R.T.: 0.002 min
Response: 2059449
Conc: 0.88 ng/ml

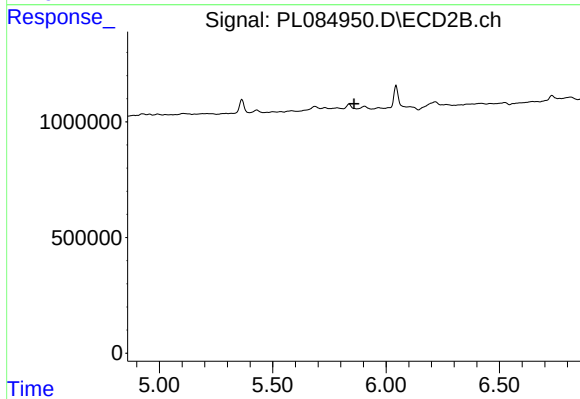

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 5.859 min
Response: 0
Conc: N.D.

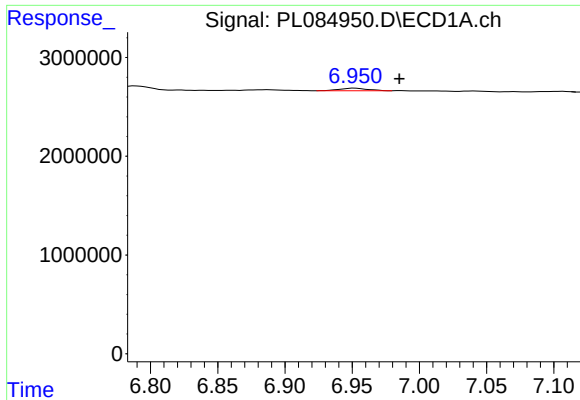

#17 4,4'-DDT


R.T.: 6.952 min
Delta R.T.: -0.033 min
Response: 378651
Conc: 0.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

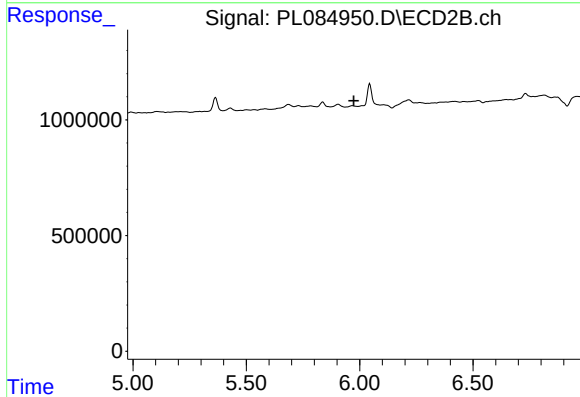


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 5.974 min
Response: 0
Conc: N.D.

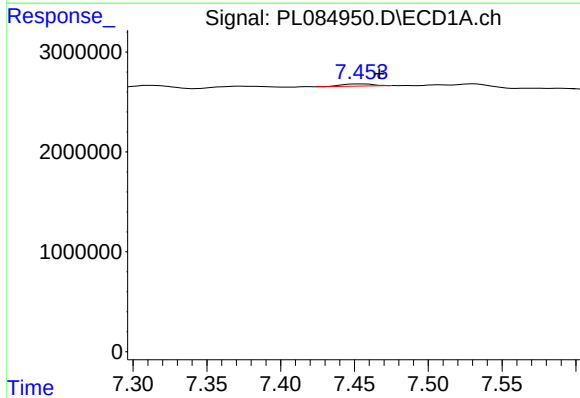


#20 Methoxychlor

R.T.: 7.454 min
Delta R.T.: -0.013 min
Response: 320429
Conc: 0.33 ng/ml

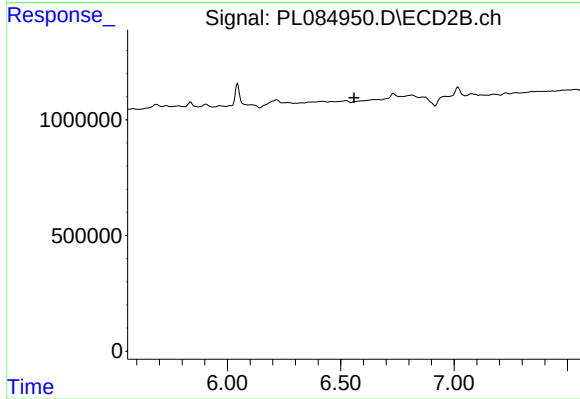

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 6.559 min
Response: 0
Conc: N.D.

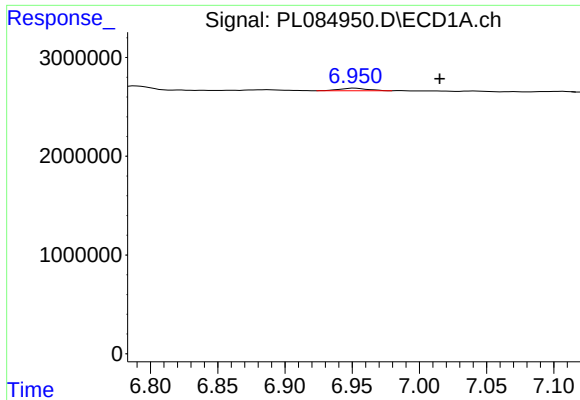

#23 Toxaphene-2


R.T.: 6.952 min
Delta R.T.: -0.063 min
Response: 378651
Conc: 5.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

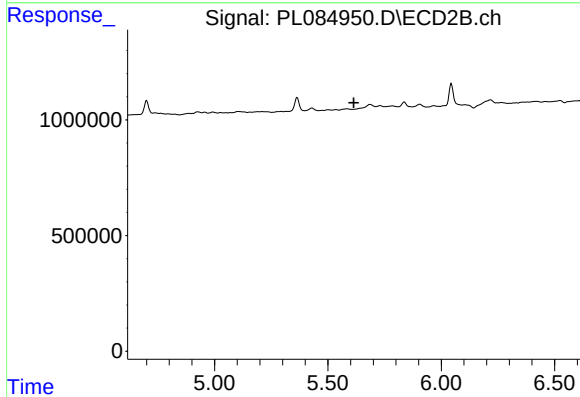


#23 Toxaphene-2

R.T.: 0.000 min
Exp R.T. : 5.615 min
Response: 0
Conc: N.D.

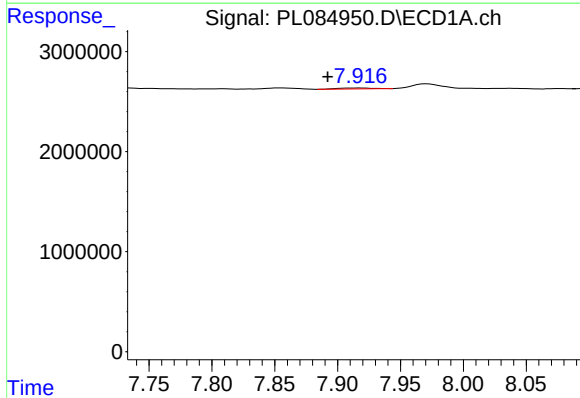


#26 Toxaphene-5

R.T.: 7.917 min
Delta R.T.: 0.025 min
Response: 176323
Conc: 5.36 ng/ml

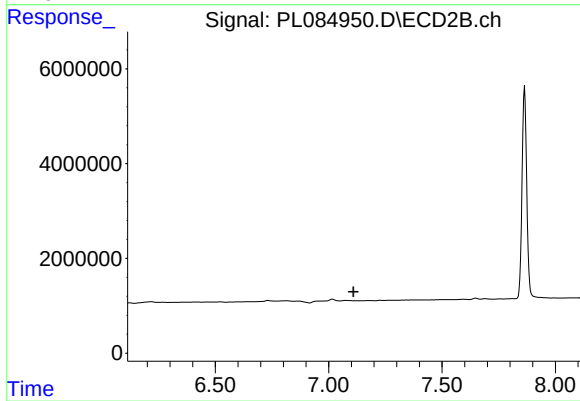

#26 Toxaphene-5


R.T.: 0.000 min
Exp R.T. : 7.110 min
Response: 0
Conc: N.D.

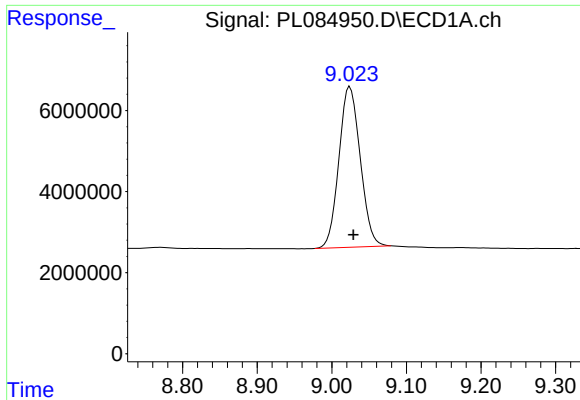

#27 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: -0.005 min
Response: 78677921
Conc: 45.91 ng/ml

Instrument :
ECD_L
ClientSampleId :

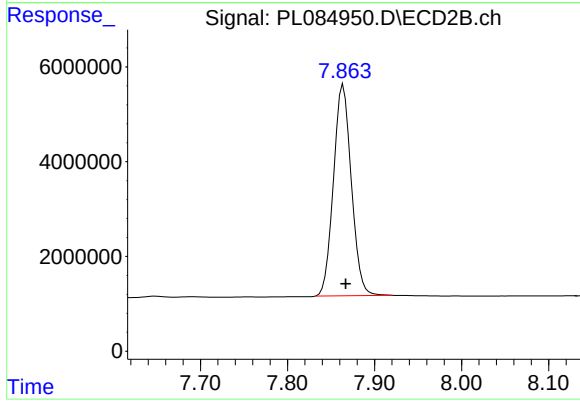

#27 Decachlorobiphenyl

R.T.: 7.864 min
Delta R.T.: -0.003 min
Response: 63681455
Conc: 47.02 ng/ml