

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082323\
 Data File : PL084956.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2023 21:45
 Operator : AR\AJ
 Sample : 04105-20MS
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BH924MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 08/25/2023
 Supervised By : mohammad ahmed 08/25/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 22:38:02 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 05:52:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.475	2.685	47673272	22490214	19.017m	19.051
27)	SA Decachlor...	9.025	7.865	59348981	47847885	34.631	35.328
Target Compounds							
2)	A alpha-BHC	3.935	3.189	203.5E6	99045516	56.273	58.391
3)	MA gamma-BHC...	4.268	3.520	188.8E6	90743758	54.519	55.960
4)	MA Heptachlor	4.861	3.861	194.2E6	88285598	50.155	54.488
5)	MB Aldrin	5.203	4.141	183.4E6	85927112	50.764	54.780
6)	B beta-BHC	4.468	3.822	82895535	40228976	46.939	48.970
7)	B delta-BHC	4.715	4.050	188.2E6	94291581	51.576	54.360
8)	B Heptachlo...	5.633	4.647	165.7E6	80234084	49.646	53.054
9)	A Endosulfan I	6.019	5.017	148.8E6	73851557	52.218	54.774
10)	B trans-Chl...	5.890	4.900	159.9E6	82087794	50.695	54.481
11)	B cis-Chlor...	5.970	4.964	157.7E6	80600612	49.475	52.103
12)	B 4,4'-DDE	6.149	5.162	279.7E6	163.2E6	105.729	111.408
13)	MA Dieldrin	6.296	5.284	308.8E6	176.3E6	107.986	113.758
14)	MA Endrin	6.526	5.560	255.6E6	160.4E6	112.204	116.497
15)	B Endosulfa...	6.747	5.857	235.7E6	150.3E6	100.224	108.230
16)	A 4,4'-DDD	6.669	5.720	198.6E6	136.4E6	104.962	114.109
17)	MA 4,4'-DDT	6.984	5.972	223.5E6	152.5E6	115.929	117.645
18)	B Endrin al...	6.877	6.039	175.3E6	114.3E6	94.205	100.533
19)	B Endosulfa...	7.114	6.263	220.7E6	146.4E6	99.795	107.150
20)	A Methoxychlor	7.466	6.557	503.3E6	379.0E6	518.708	535.499
21)	B Endrin ke...	7.597	6.768	221.6E6	175.9E6	100.946	109.036

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082323\
Data File : PL084956.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2023 21:45
Operator : AR\AJ
Sample : 04105-20MS
Misc :
ALS Vial : 30 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 22:38:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

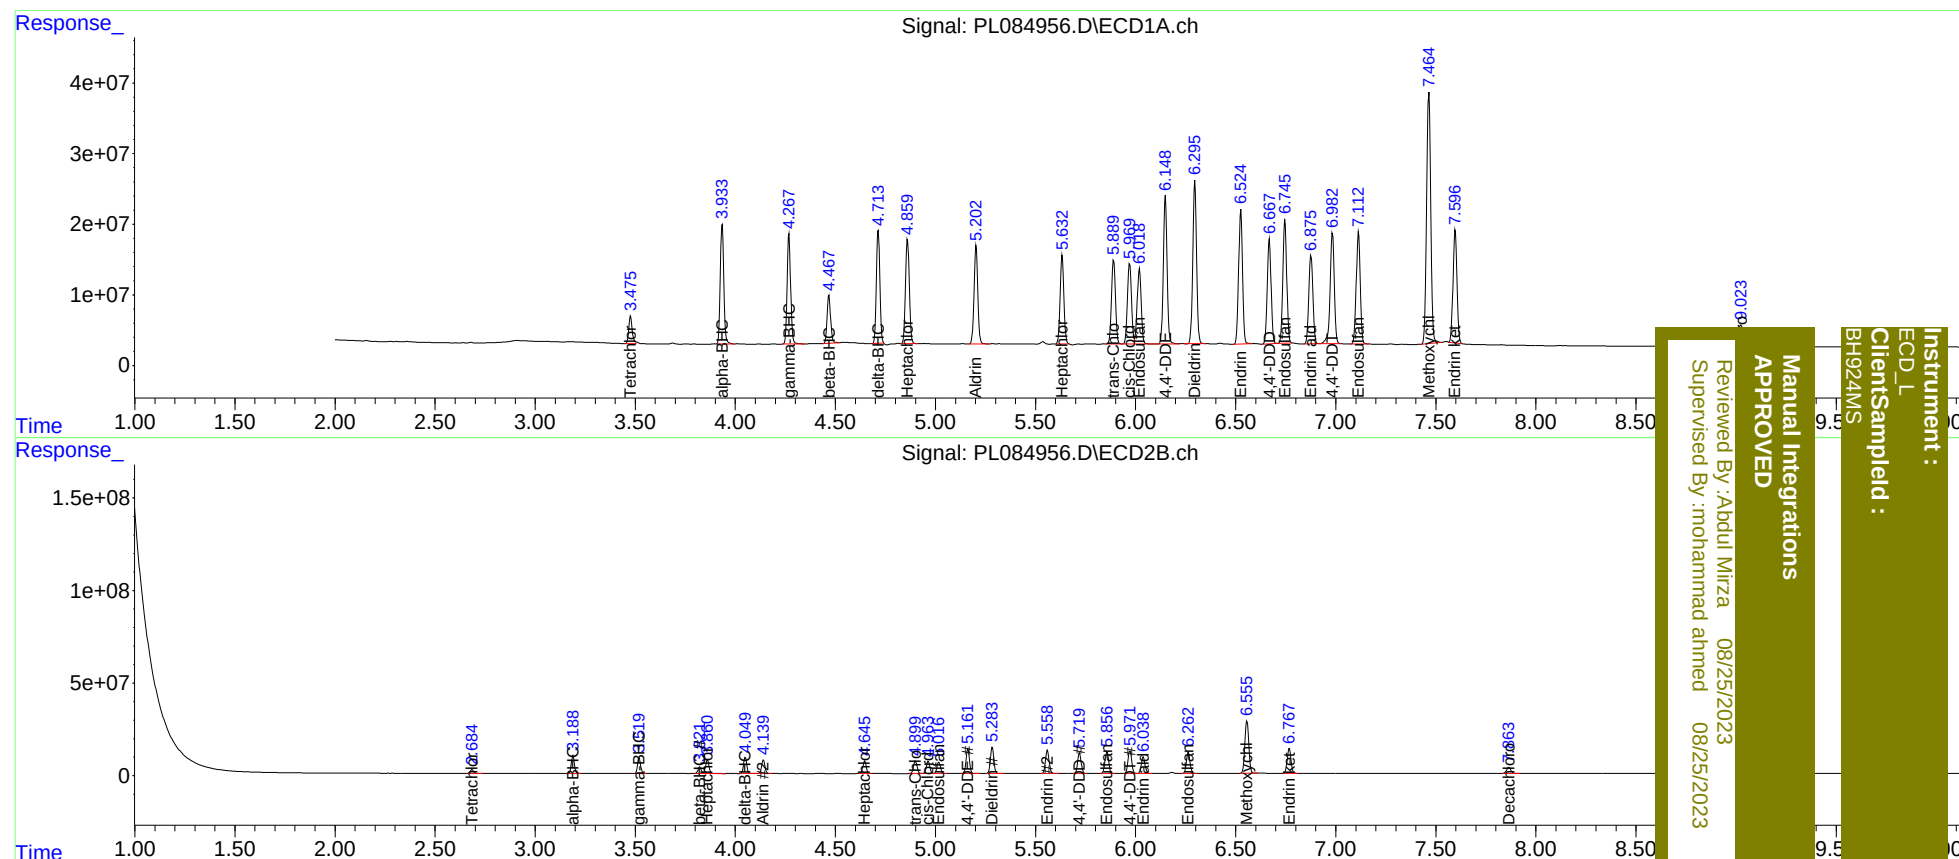

Reviewed By: Abdul Mirza 08/25/2023
Supervised By: mohammad ahmed 08/25/2023

Manual Integrations
APPROVED

Instrument :
ECD_L
Client Sampled :
BH924MS