

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082324\
 Data File : PL091272.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Aug 2024 16:01
 Operator : AR\AJ
 Sample : PB162918BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB162918BL

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/23/2024
 Supervised By :Ankita Jodhani 08/23/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 01:28:27 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081324.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 14 13:09:19 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.545	2.784	42211958	46987198	19.659	24.071m
28) SA Decachlor...	9.055	7.924	34906410	44542799	22.896	23.516

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082324\
Data File : PL091272.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2024 16:01
Operator : AR\AJ
Sample : PB162918BL
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PB162918BL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 08/23/2024
Supervised By : Ankita Jodhani 08/23/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 01:28:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081324.M
Quant Title : GC Extractables
QLast Update : Wed Aug 14 13:09:19 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

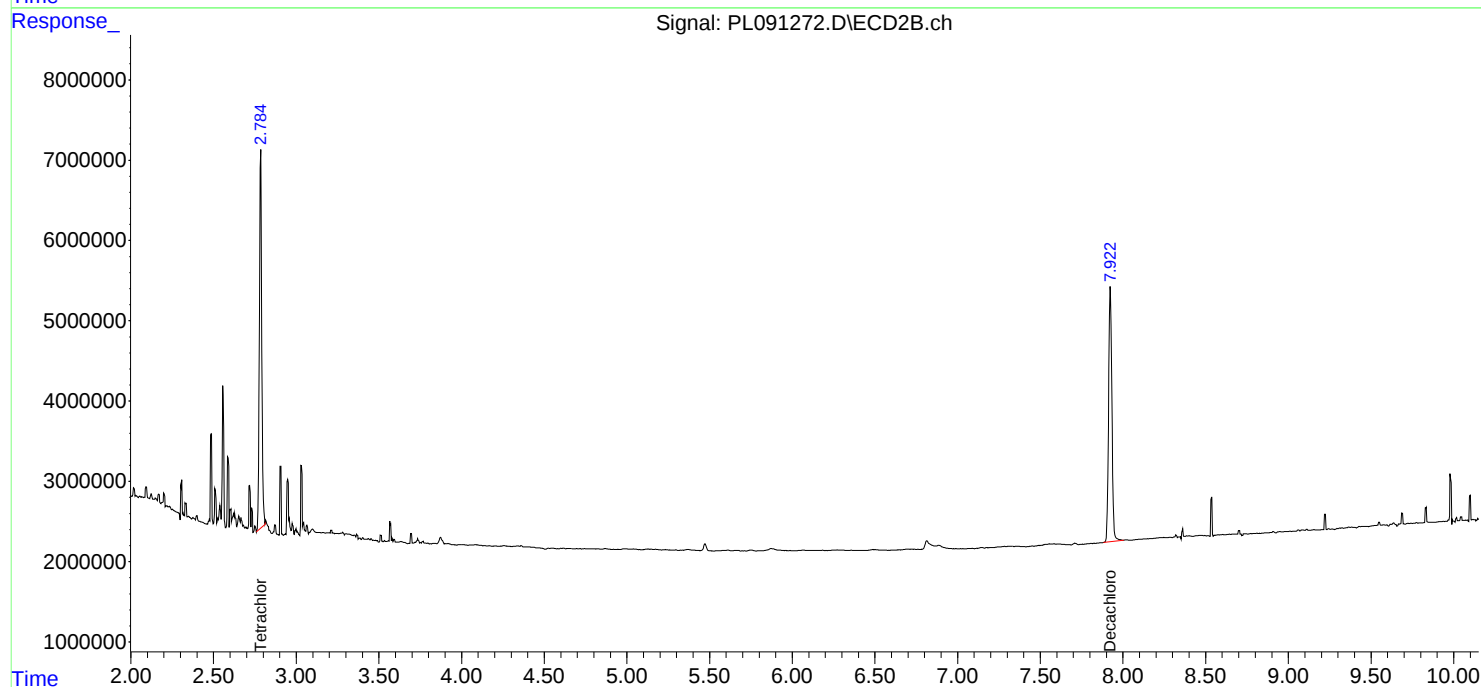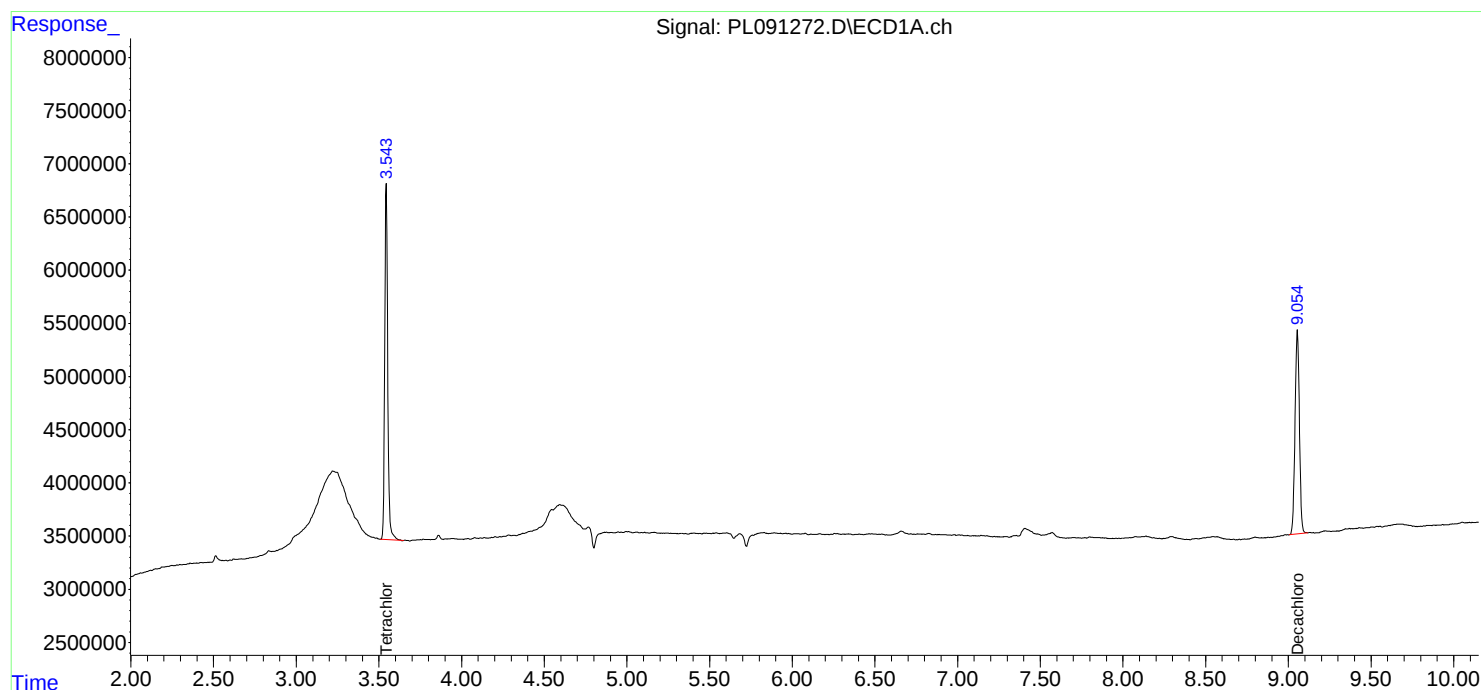

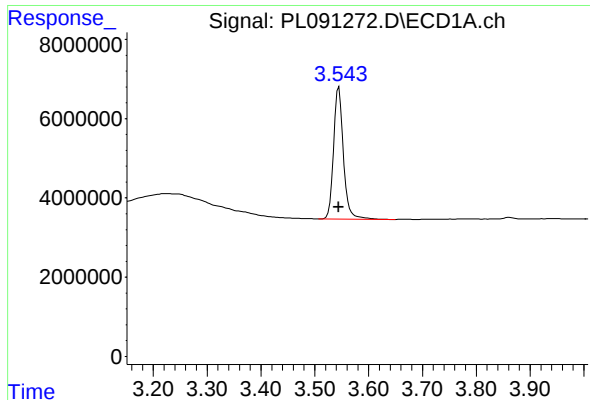


#1 Tetrachloro-m-xylene

R.T.: 3.545 min
Delta R.T.: 0.000 min
Response: 42211958
Conc: 19.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB162918BL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/23/2024
Supervised By :Ankita Jodhani 08/23/2024

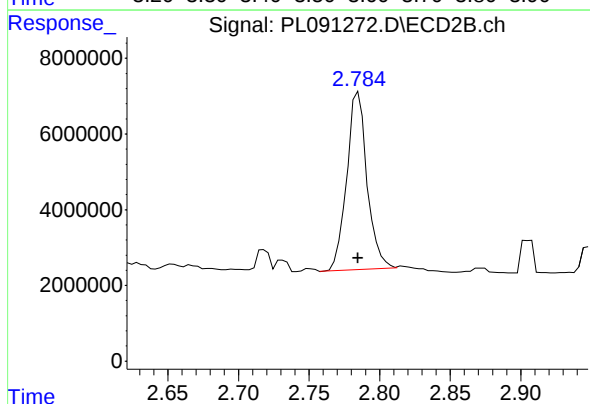


#1 Tetrachloro-m-xylene

R.T.: 2.784 min
Delta R.T.: -0.001 min
Response: 46987198
Conc: 24.07 ng/ml

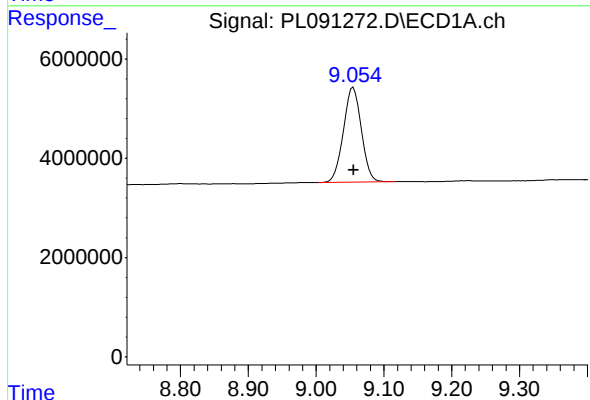

#28 Decachlorobiphenyl

R.T.: 9.055 min
Delta R.T.: 0.000 min
Response: 34906410
Conc: 22.90 ng/ml

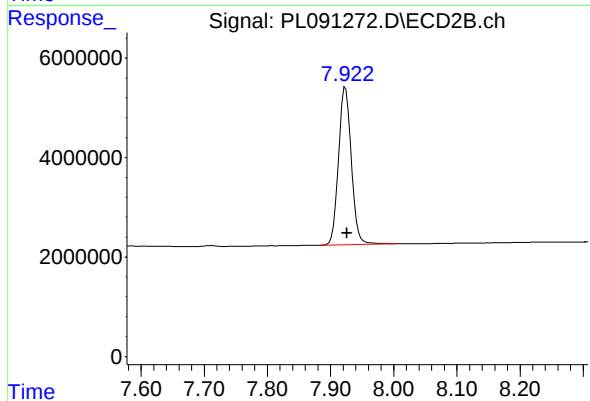

#28 Decachlorobiphenyl

R.T.: 7.924 min
Delta R.T.: -0.002 min
Response: 44542799
Conc: 23.52 ng/ml