

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082324\
 Data File : PL091289.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Aug 2024 20:36
 Operator : AR\AJ
 Sample : P3698-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HD-01-8-21-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 01:35:10 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081324.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 14 13:09:19 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.544	2.785	26072686	25838118	12.143	13.237
28) SA Decachlor...	9.053	7.923	19803712	23094554	12.990	12.193

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082324\
Data File : PL091289.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2024 20:36
Operator : AR\AJ
Sample : P3698-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HD-01-8-21-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 01:35:10 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081324.M
Quant Title : GC Extractables
QLast Update : Wed Aug 14 13:09:19 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

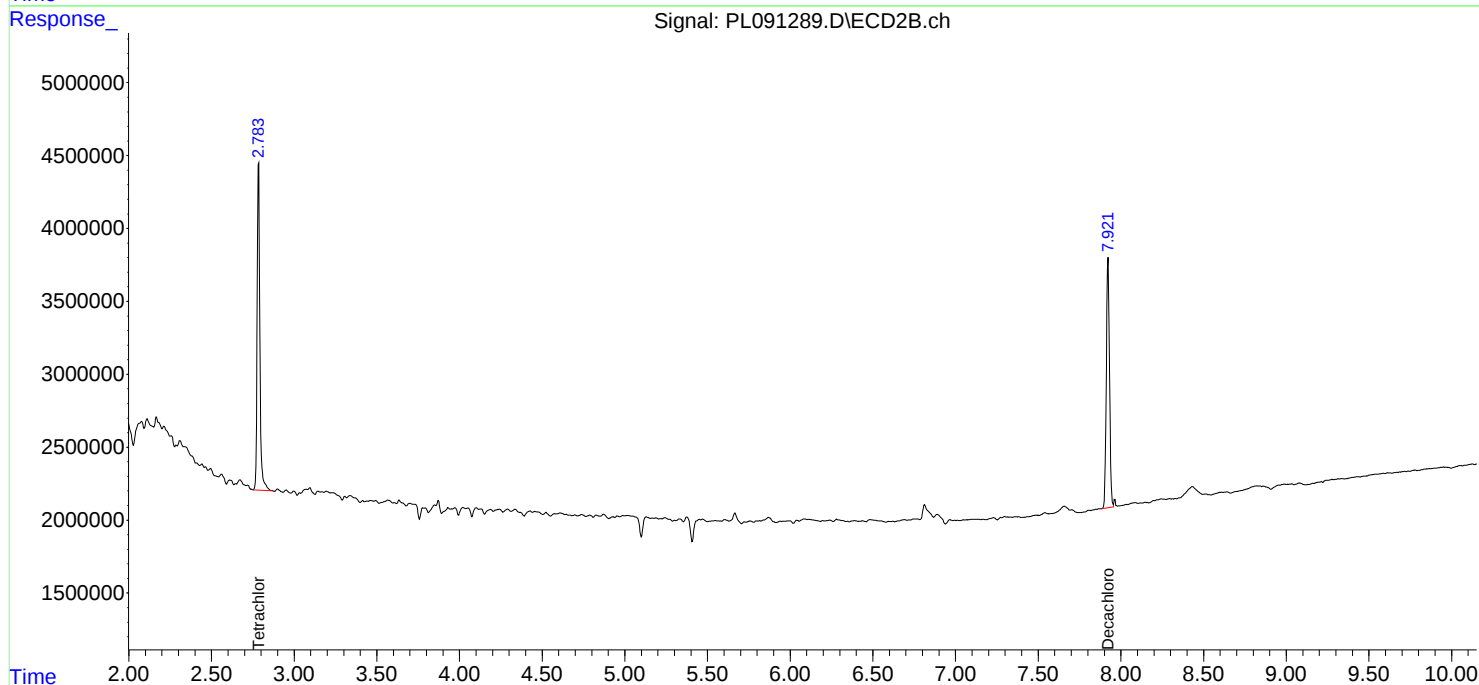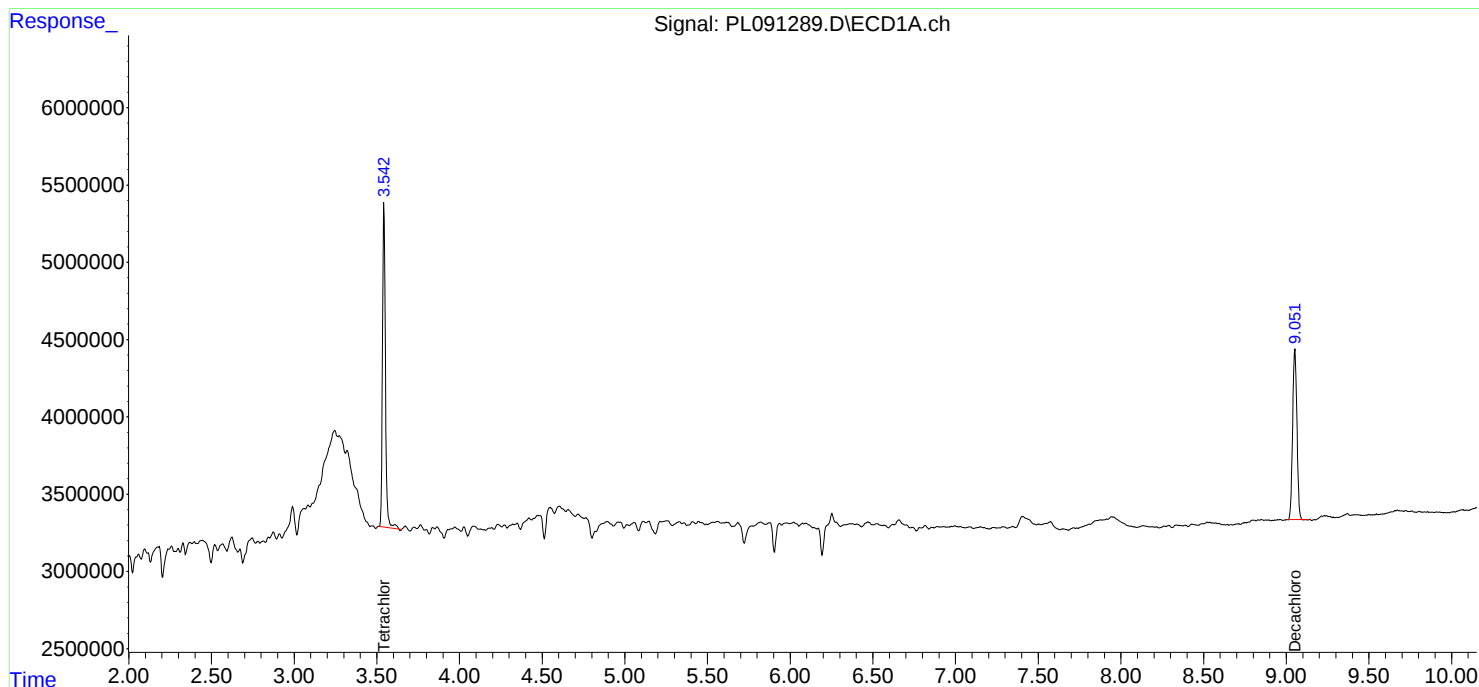


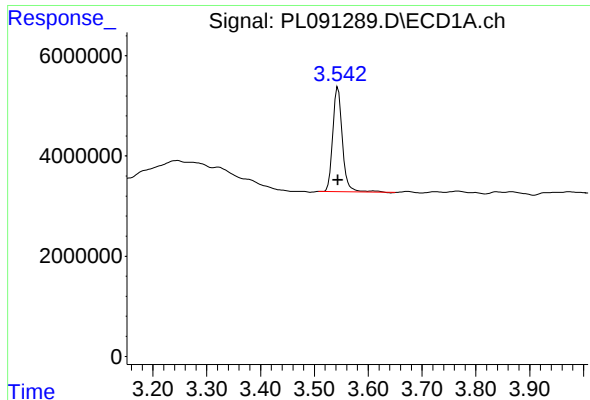

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.000 min
Response: 26072686
Conc: 12.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
HD-01-8-21-2024

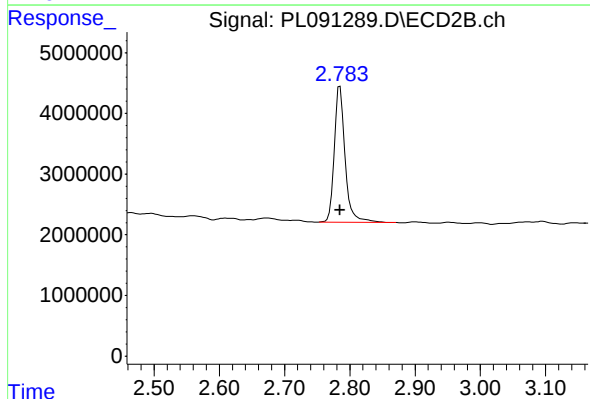


#1 Tetrachloro-m-xylene

R.T.: 2.785 min
Delta R.T.: 0.000 min
Response: 25838118
Conc: 13.24 ng/ml

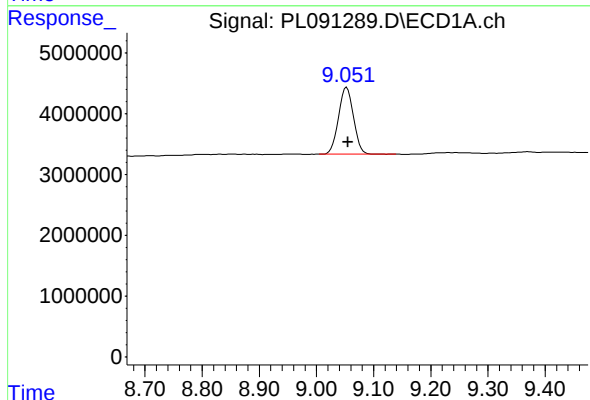

#28 Decachlorobiphenyl

R.T.: 9.053 min
Delta R.T.: -0.003 min
Response: 19803712
Conc: 12.99 ng/ml

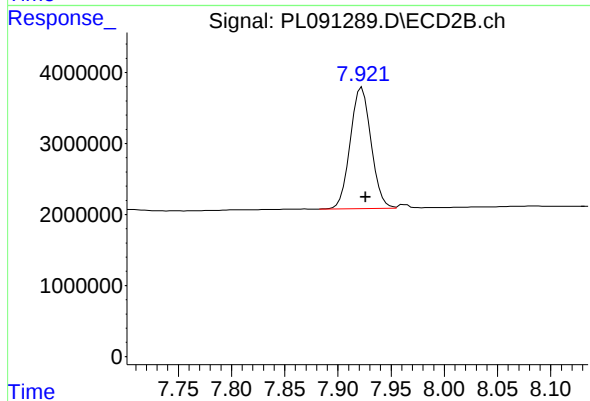

#28 Decachlorobiphenyl

R.T.: 7.923 min
Delta R.T.: -0.003 min
Response: 23094554
Conc: 12.19 ng/ml