

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082420\
 Data File : PL060935.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Aug 2020 14:44
 Operator : DD\AJ
 Sample : L3773-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 24 18:04:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081820.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 19 06:13:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.461	4.009	26047960	32531510	15.603	11.695 #
28)	SA Decachlor...	8.216	9.097	29536231	41333012	20.677	20.450
Target Compounds							
4)	MA Heptachlor	4.488	0.000	6346834	0	3.197	N.D. #
6)	B beta-BHC	4.456f	0.000	5998441	0	6.677	N.D. #
8)	B Heptachlo...	0.000	5.887	0	37462335	N.D.	13.402 #
11)	B alpha-Chl...	5.466	0.000	5666216	0	3.440	N.D. #
13)	MA Dieldrin	5.756	0.000	5504221	0	3.424	N.D. #
14)	MA Endrin	0.000	6.703f	0	8757852	N.D.	3.371 #
15)	B Endosulfa...	0.000	6.957f	0	3661596	N.D.	1.404 #
23)	Chlordane-1	0.000	4.996	0	1314249	N.D.	12.328 #
24)	Chlordane-2	4.839	0.000	4702341	0	85.567	N.D. #
26)	Chlordane-4	5.466	0.000	5666216	0	49.482	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082420\
Data File : PL060935.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Aug 2020 14:44
Operator : DD\AJ
Sample : L3773-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 18:04:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081820.M
Quant Title : GC Extractables
QLast Update : Wed Aug 19 06:13:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

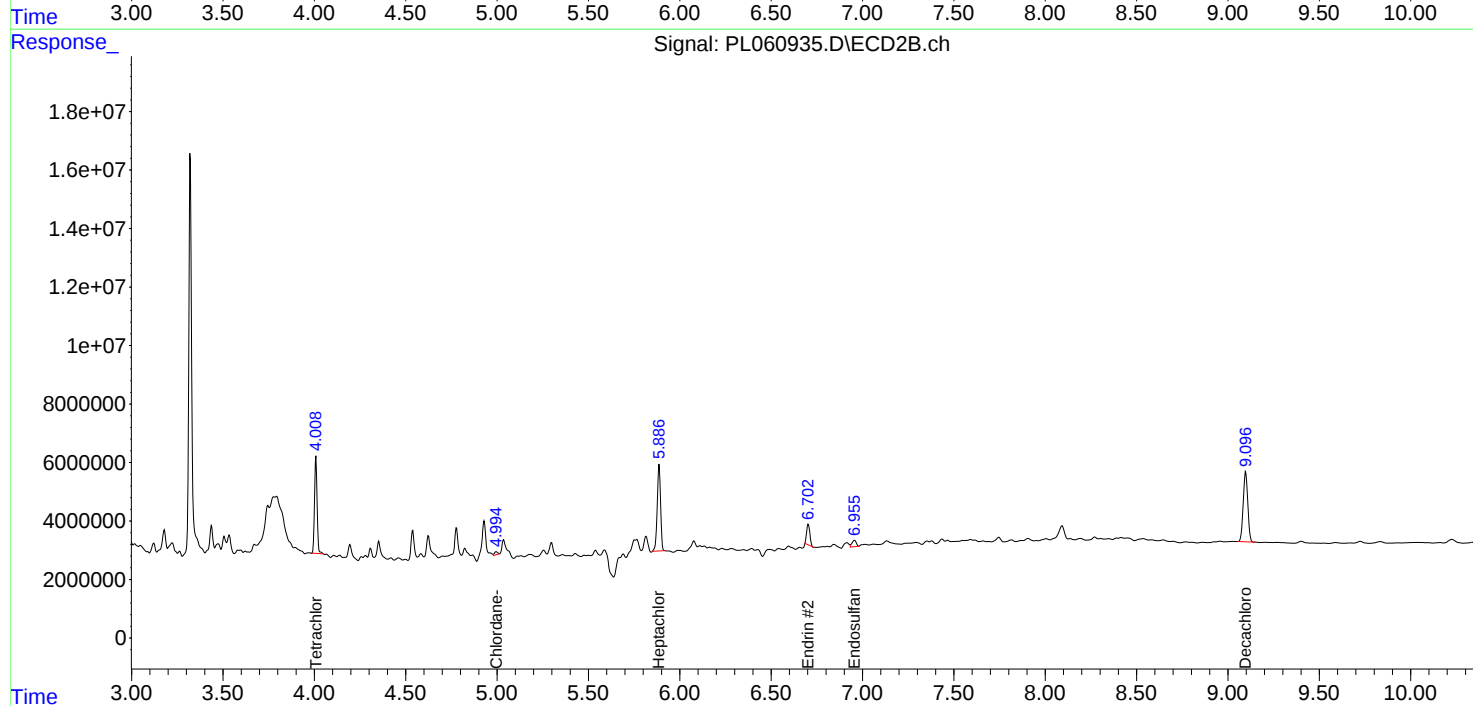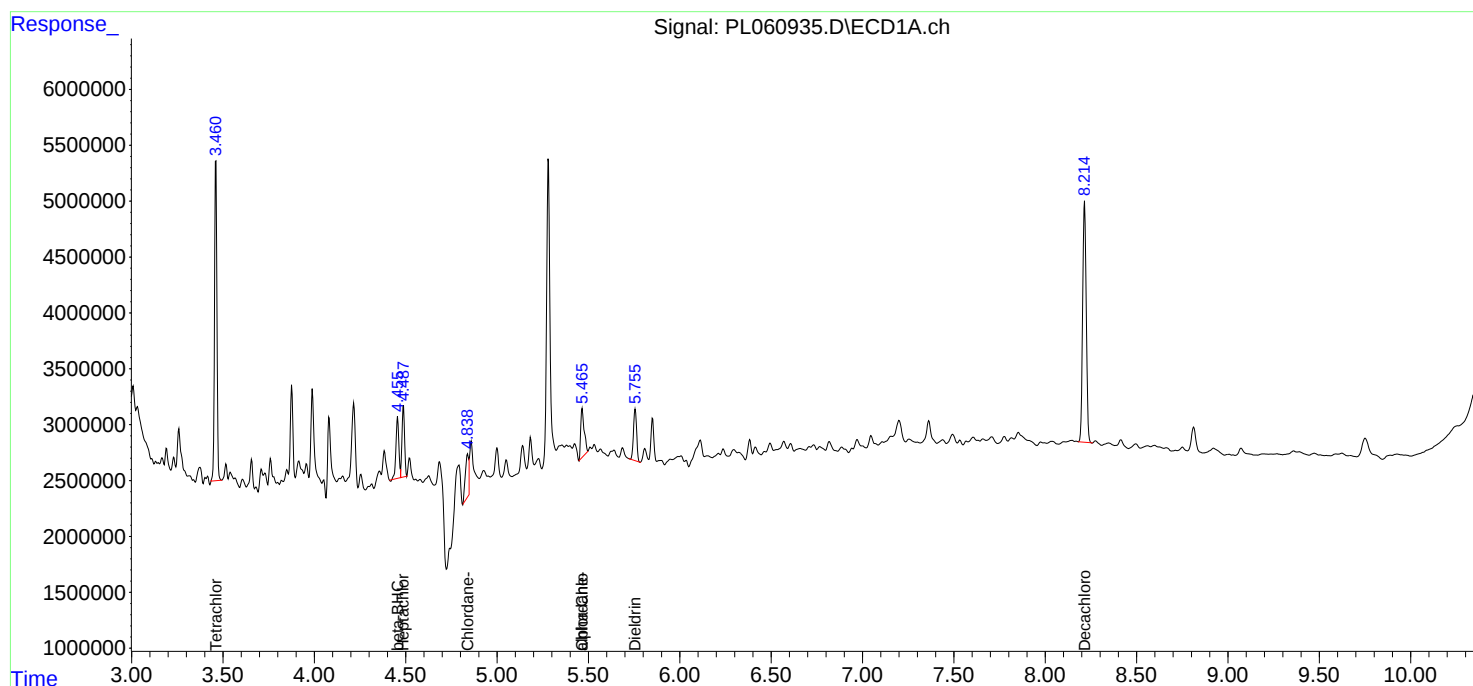


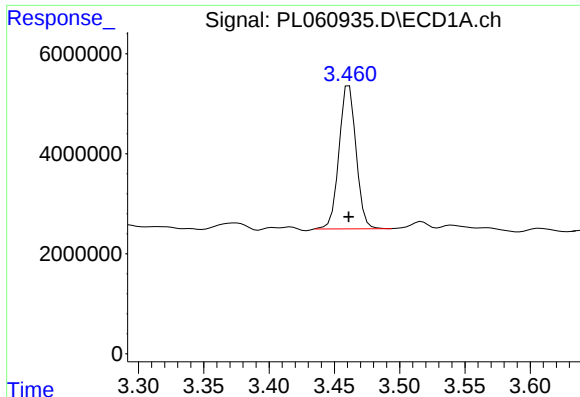

#1 Tetrachloro-m-xylene


R.T.: 3.461 min
Delta R.T.: 0.000 min
Response: 26047960
Conc: 15.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

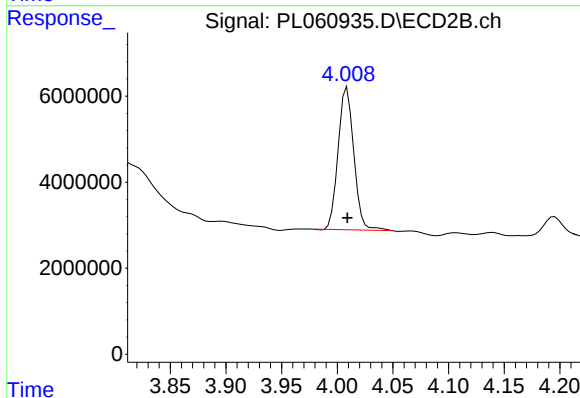


#1 Tetrachloro-m-xylene

R.T.: 4.009 min
Delta R.T.: 0.000 min
Response: 32531510
Conc: 11.69 ng/ml

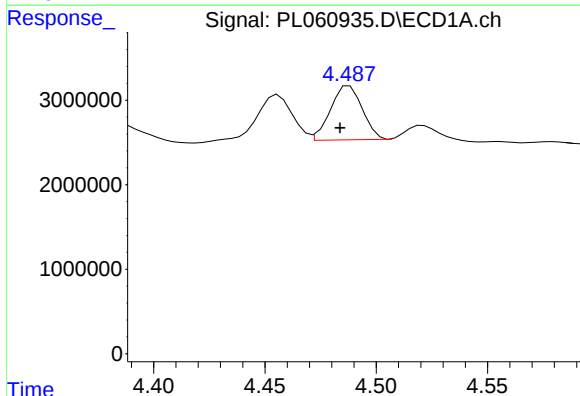


#4 Heptachlor

R.T.: 4.488 min
Delta R.T.: 0.004 min
Response: 6346834
Conc: 3.20 ng/ml

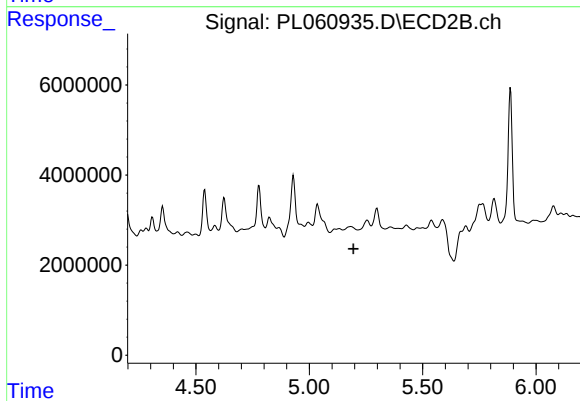

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 5.195 min
Response: 0
Conc: N.D.

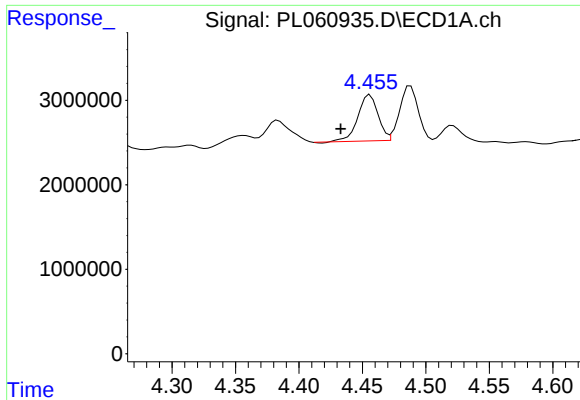

#6 beta-BHC


R.T.: 4.456 min
Delta R.T.: 0.023 min
Response: 5998441
Conc: 6.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

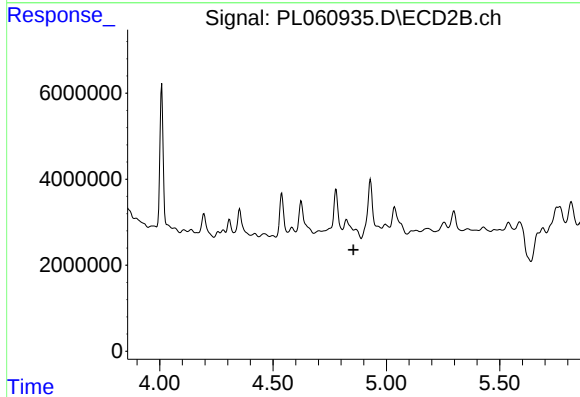


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.855 min
Response: 0
Conc: N.D.

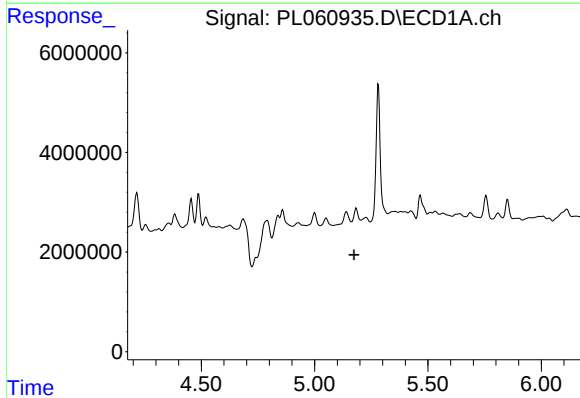


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.175 min
Response: 0
Conc: N.D.

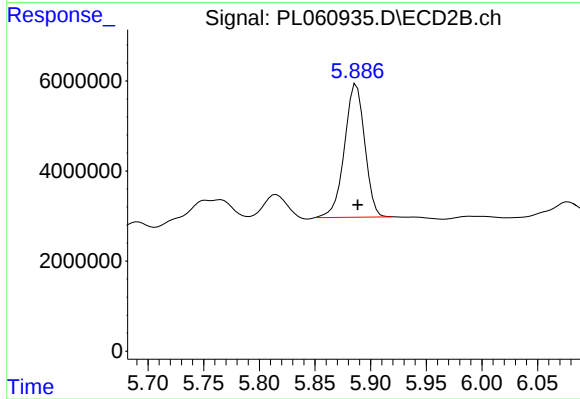

#8 Heptachlor epoxide


R.T.: 5.887 min
Delta R.T.: -0.001 min
Response: 37462335
Conc: 13.40 ng/ml

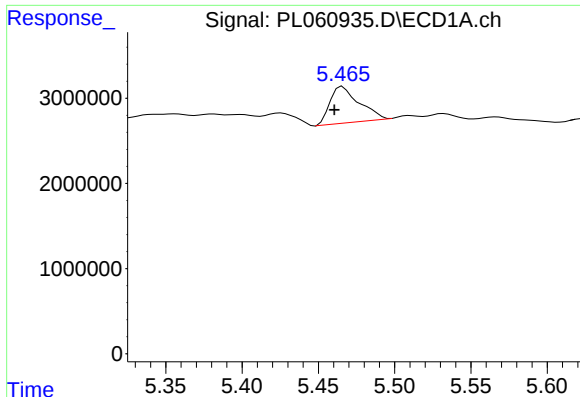

#11 alpha-Chlordane


R.T.: 5.466 min
Delta R.T.: 0.005 min
Response: 5666216
Conc: 3.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

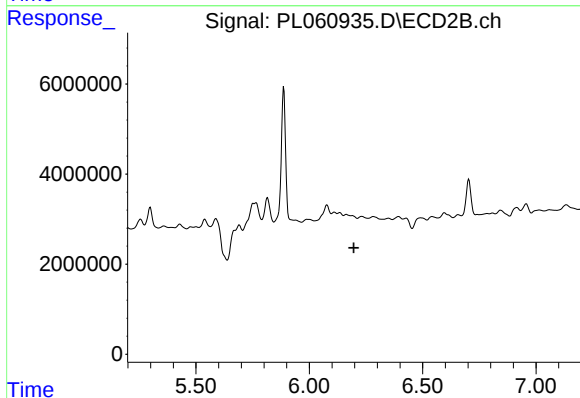


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.197 min
Response: 0
Conc: N.D.

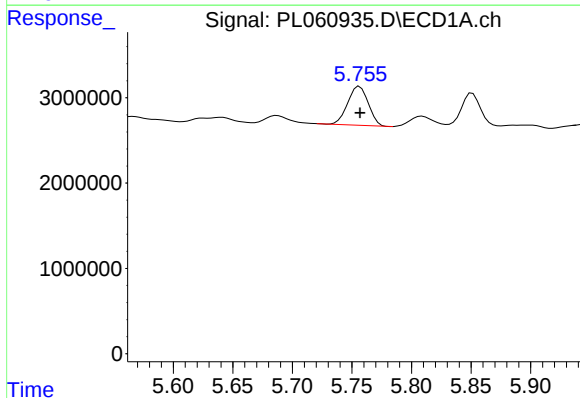


#13 Dieldrin

R.T.: 5.756 min
Delta R.T.: 0.000 min
Response: 5504221
Conc: 3.42 ng/ml

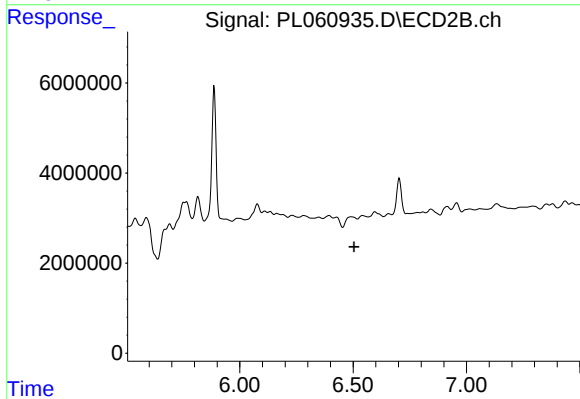

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.505 min
Response: 0
Conc: N.D.

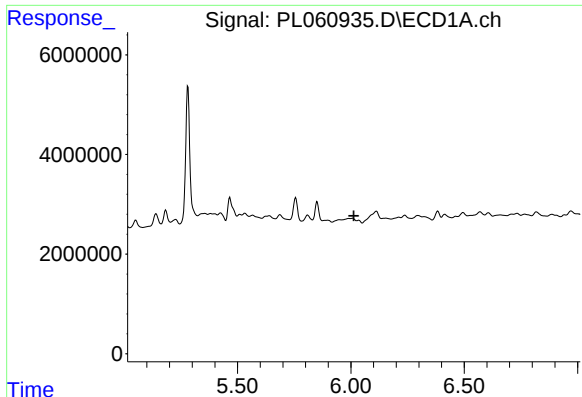

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.013 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

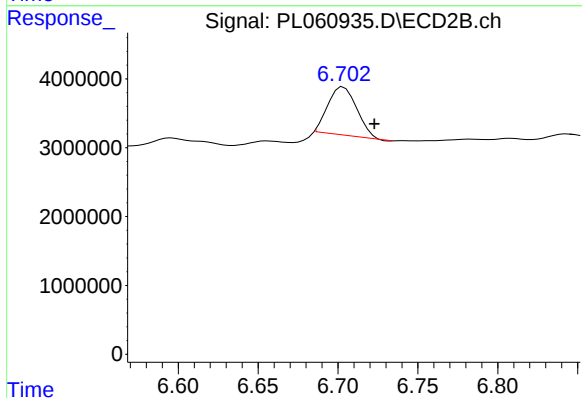


#14 Endrin

R.T.: 6.703 min
Delta R.T.: -0.019 min
Response: 8757852
Conc: 3.37 ng/ml

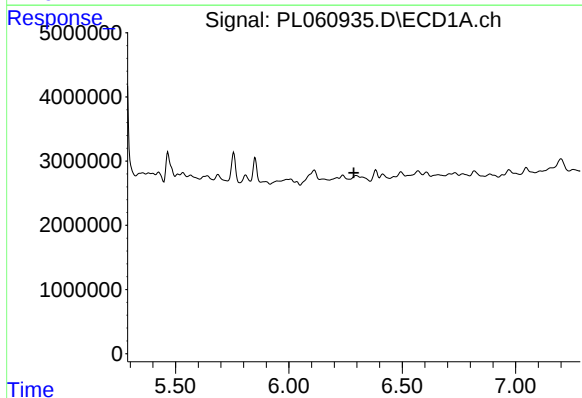


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.287 min
Response: 0
Conc: N.D.

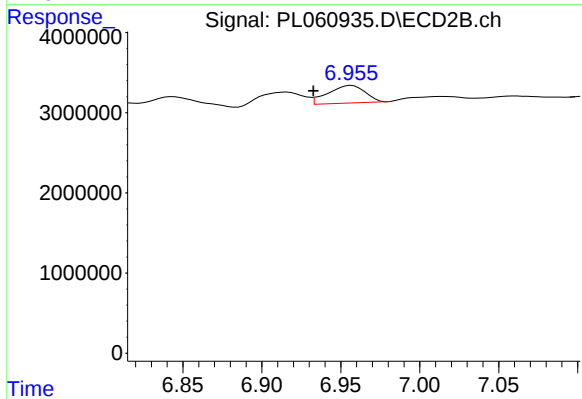

#15 Endosulfan II


R.T.: 6.957 min
Delta R.T.: 0.024 min
Response: 3661596
Conc: 1.40 ng/ml

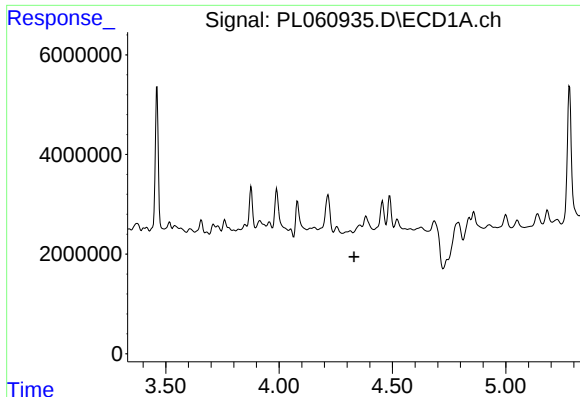

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.331 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

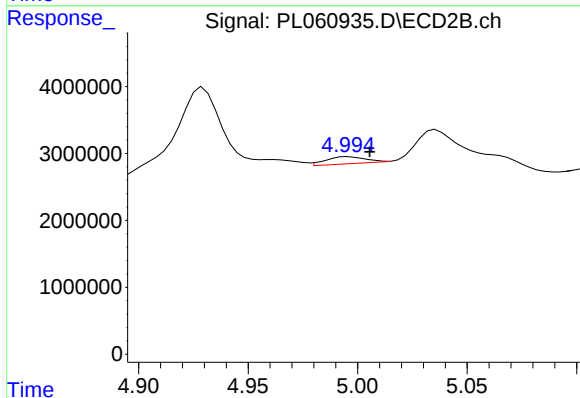


#23 Chlordane-1

R.T.: 4.996 min
Delta R.T.: -0.010 min
Response: 1314249
Conc: 12.33 ng/ml

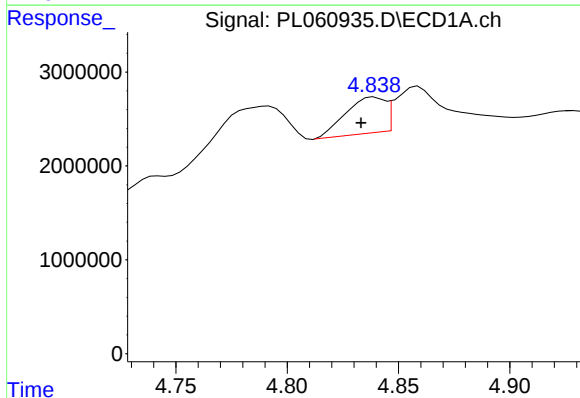


#24 Chlordane-2

R.T.: 4.839 min
Delta R.T.: 0.006 min
Response: 4702341
Conc: 85.57 ng/ml

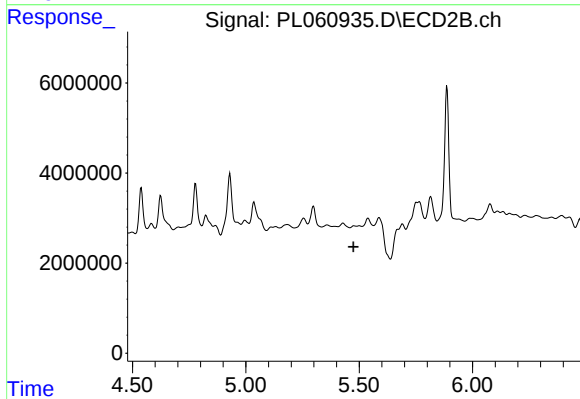

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.475 min
Response: 0
Conc: N.D.

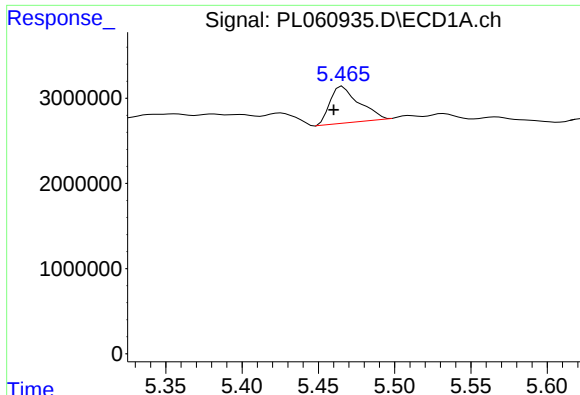

#26 Chlordane-4


R.T.: 5.466 min
Delta R.T.: 0.006 min
Response: 5666216
Conc: 49.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

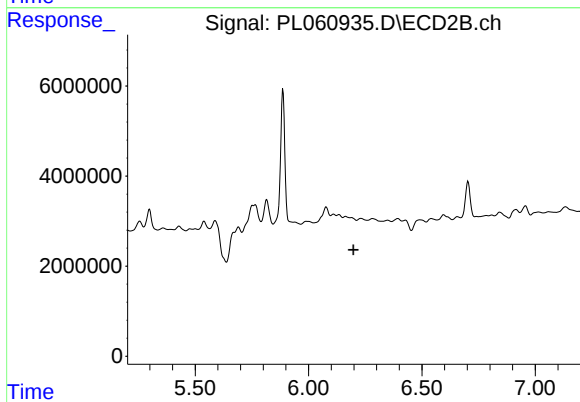


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.199 min
Response: 0
Conc: N.D.

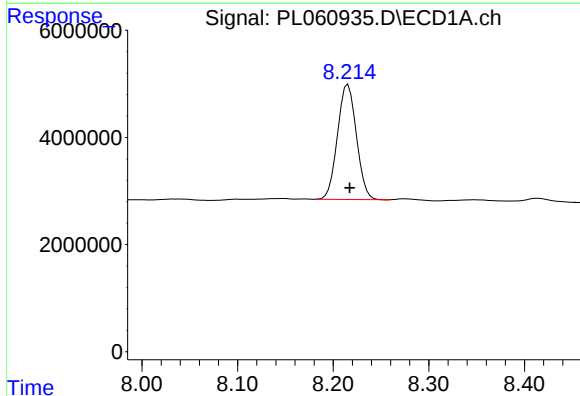

#28 Decachlorobiphenyl

R.T.: 8.216 min
Delta R.T.: -0.002 min
Response: 29536231
Conc: 20.68 ng/ml

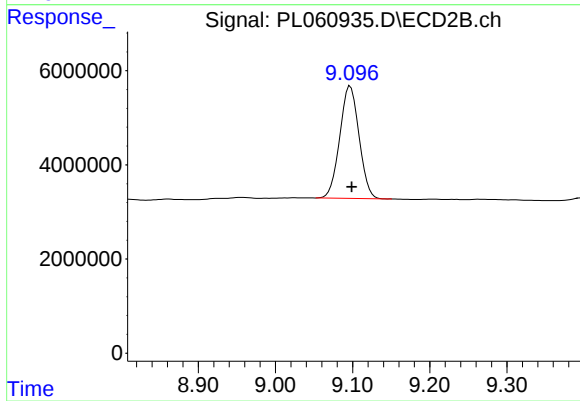

#28 Decachlorobiphenyl

R.T.: 9.097 min
Delta R.T.: -0.002 min
Response: 41333012
Conc: 20.45 ng/ml