

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082420\
 Data File : PL060942.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Aug 2020 16:23
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 24 18:06:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081820.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 19 06:13:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.461	4.009	35265719	48098628	21.125	17.291
28)	SA Decachlor...	8.215	9.097	36758285	36119958	25.733	17.871 #
Target Compounds							
9)	A Endosulfan I	0.000	6.273f	0	25062066	N.D.	8.471 #
13)	MA Dieldrin	0.000	6.529f	0	37568386	N.D.	12.207 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082420\
Data File : PL060942.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Aug 2020 16:23
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 18:06:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081820.M
Quant Title : GC Extractables
QLast Update : Wed Aug 19 06:13:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

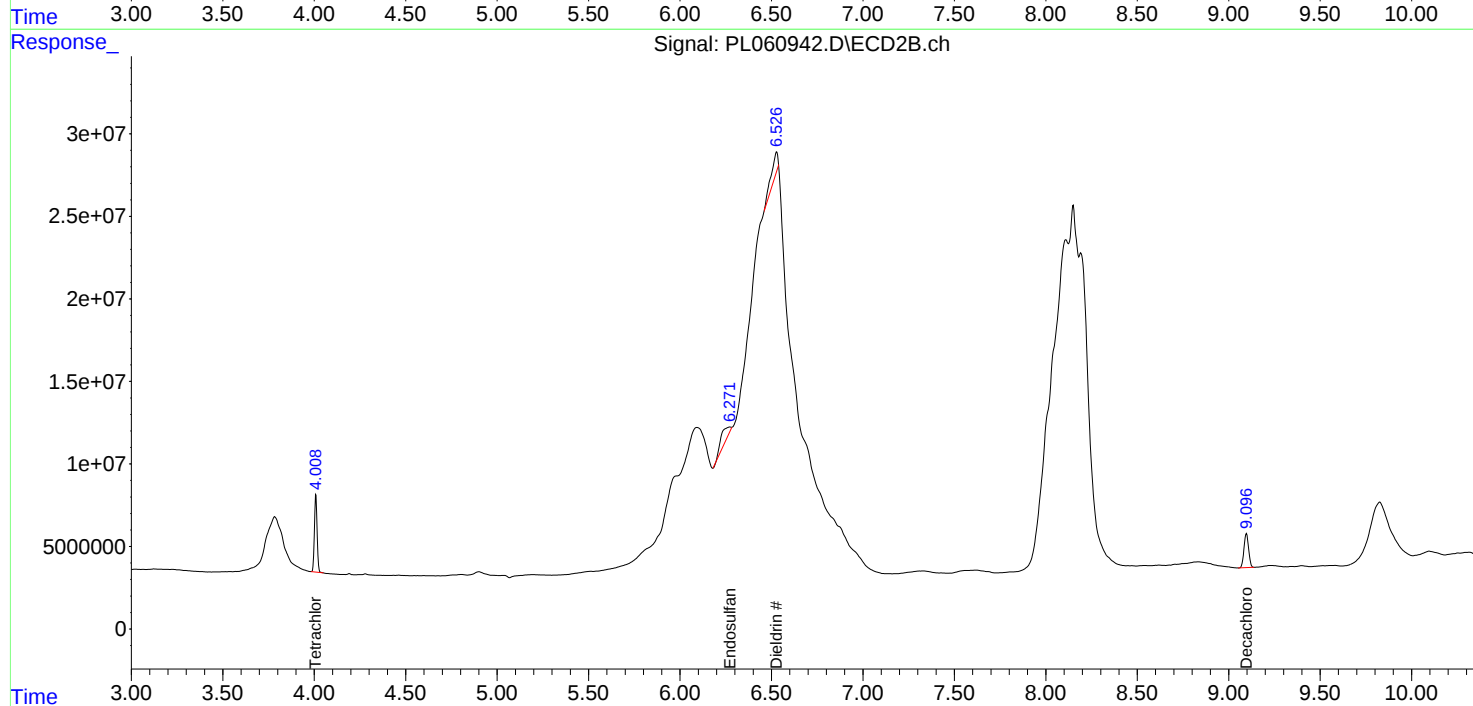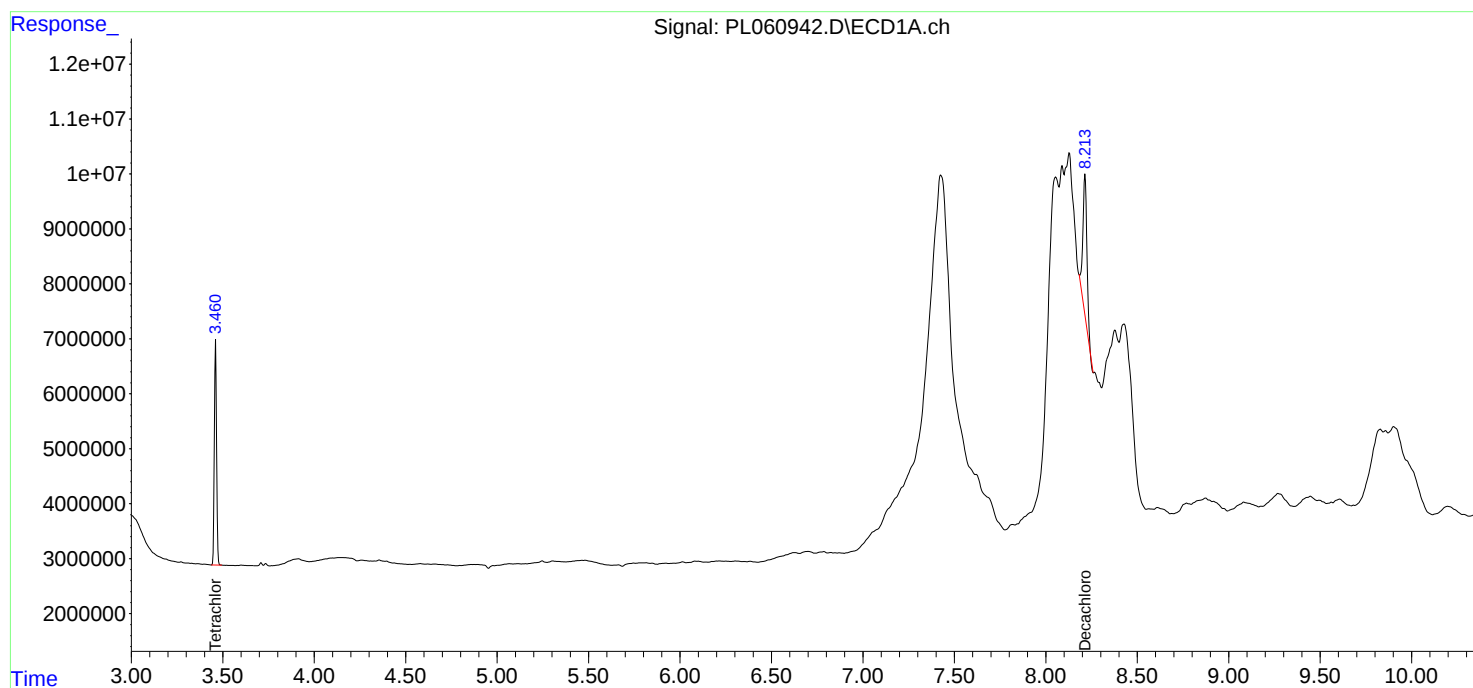


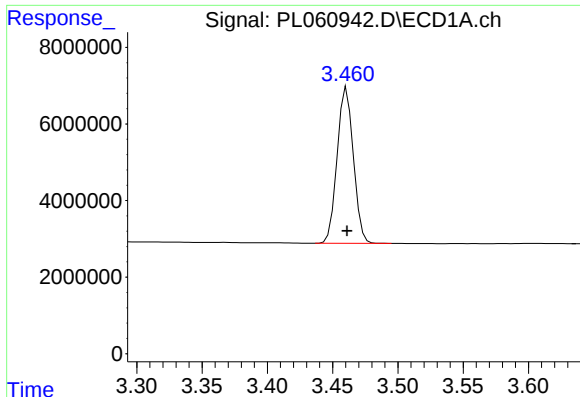

#1 Tetrachloro-m-xylene


R.T.: 3.461 min
Delta R.T.: 0.000 min
Response: 35265719
Conc: 21.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

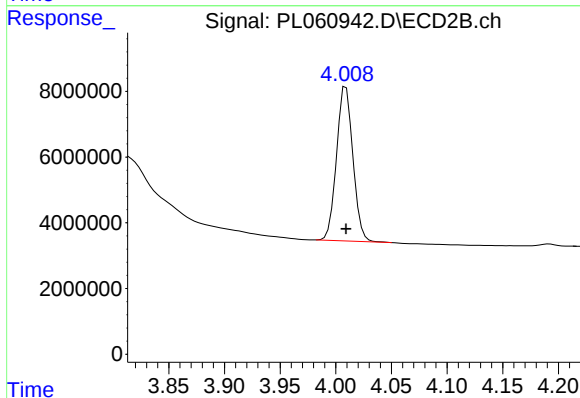


#1 Tetrachloro-m-xylene

R.T.: 4.009 min
Delta R.T.: 0.000 min
Response: 48098628
Conc: 17.29 ng/ml

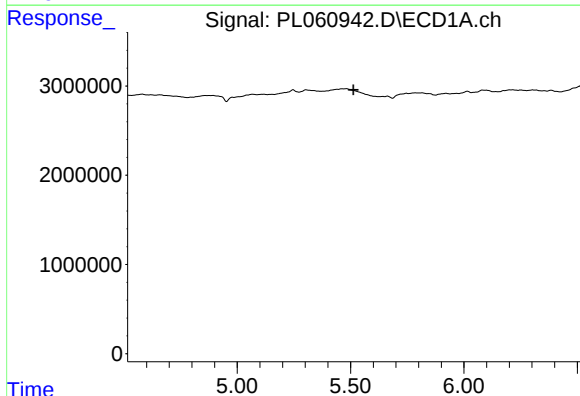


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.514 min
Response: 0
Conc: N.D.

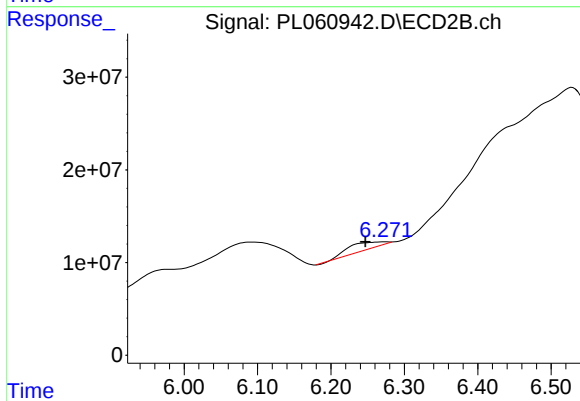

#9 Endosulfan I


R.T.: 6.273 min
Delta R.T.: 0.026 min
Response: 25062066
Conc: 8.47 ng/ml

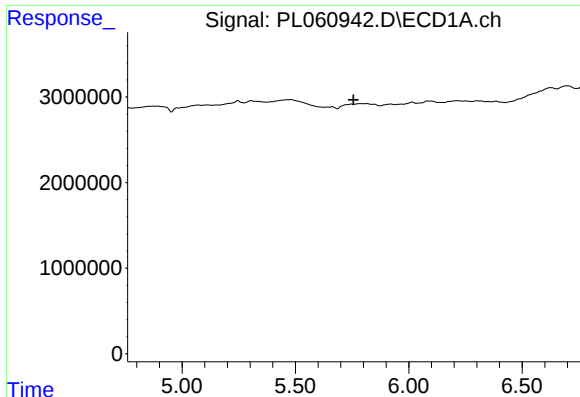

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.757 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

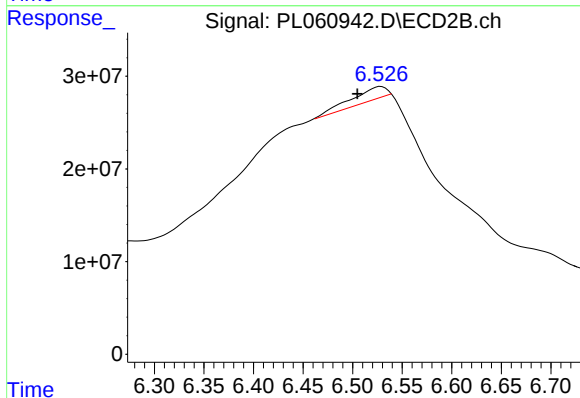


#13 Dieldrin

R.T.: 6.529 min
Delta R.T.: 0.024 min
Response: 37568386
Conc: 12.21 ng/ml

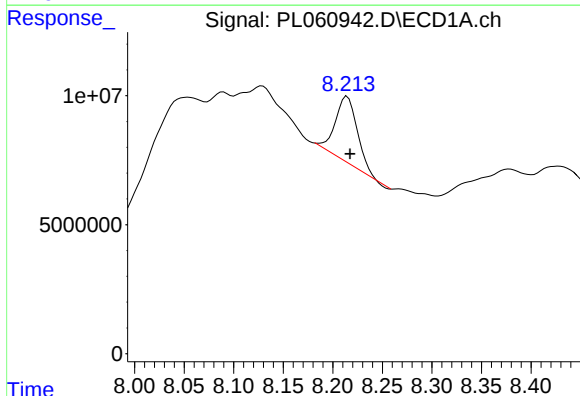

#28 Decachlorobiphenyl

R.T.: 8.215 min
Delta R.T.: -0.003 min
Response: 36758285
Conc: 25.73 ng/ml

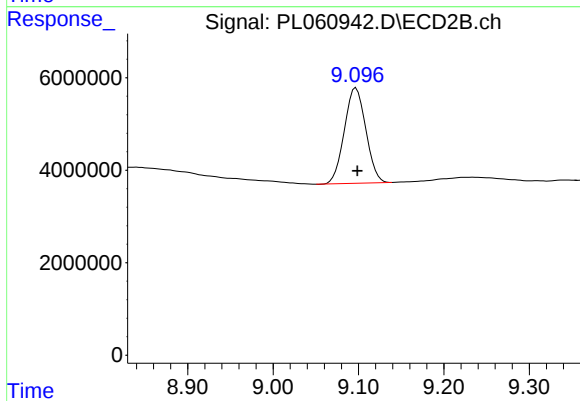

#28 Decachlorobiphenyl

R.T.: 9.097 min
Delta R.T.: -0.002 min
Response: 36119958
Conc: 17.87 ng/ml