

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082421\
 Data File : PL0693412.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Aug 2021 10:53
 Operator : AR\AJ
 Sample : M3466-01 10XRE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 25 00:49:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 21 02:23:37 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.643	5.569	871809	2093920	1.890	1.462
28)	SA Decachlor...	10.410	11.499	1158353	1970825	1.716	1.608
Target Compounds							
8)	B Heptachlo...	0.000	8.041	0	4955284	N.D.	3.294 #
9)	A Endosulfan I	0.000	8.446	0	480834	N.D.	0.348 #
10)	B gamma-Chl...	0.000	8.304	0	2468513	N.D.	1.605 #
11)	B alpha-Chl...	0.000	8.387	0	2507609	N.D.	1.678 #
16)	A 4,4'-DDD	0.000	9.111	0	2064045	N.D.	1.683 #
17)	MA 4,4'-DDT	8.489	9.430	672691	2173920	1.169	1.774 #
25)	Chlordane-3	0.000	8.304	0	2468513	N.D.	11.527 #
26)	Chlordane-4	0.000	8.387	0	2507609	N.D.	9.743 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082421\
Data File : PL0693412.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Aug 2021 10:53
Operator : AR\AJ
Sample : M3466-01 10XRE
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 25 00:49:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
Quant Title : GC Extractables
QLast Update : Sat Aug 21 02:23:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

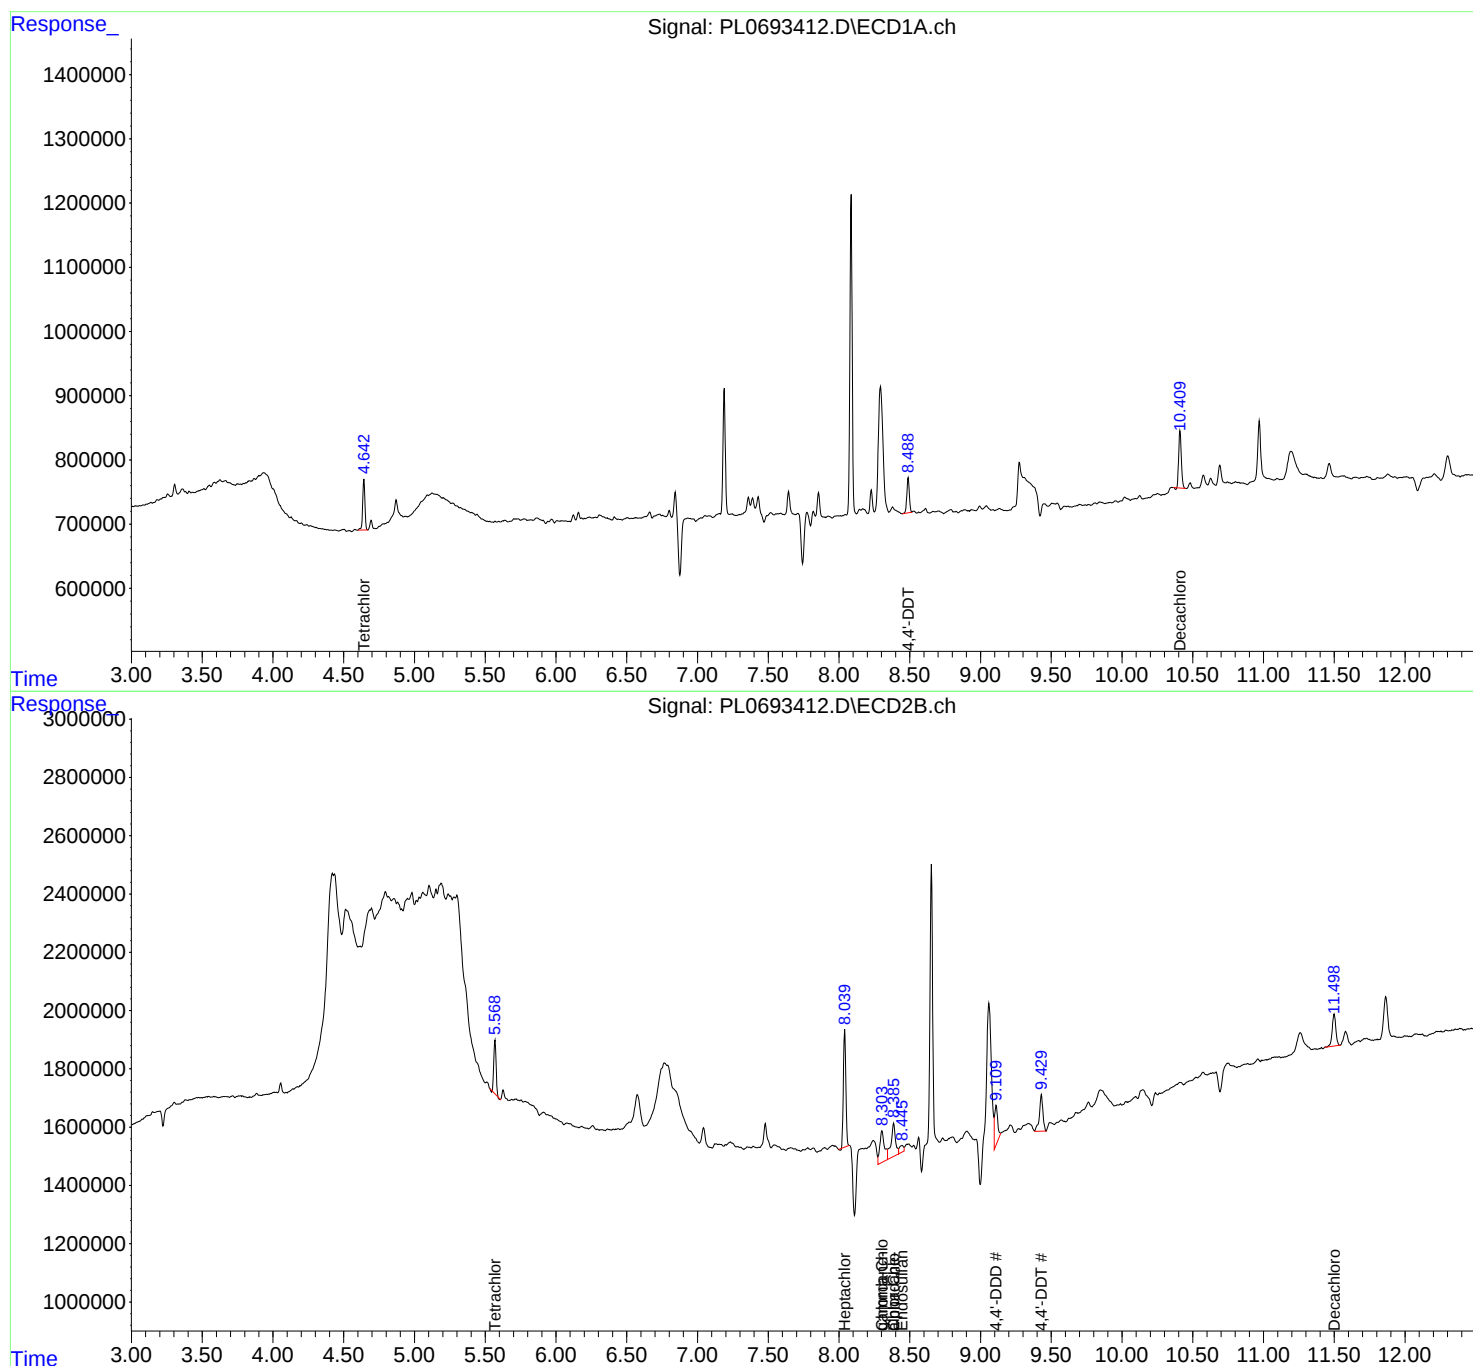


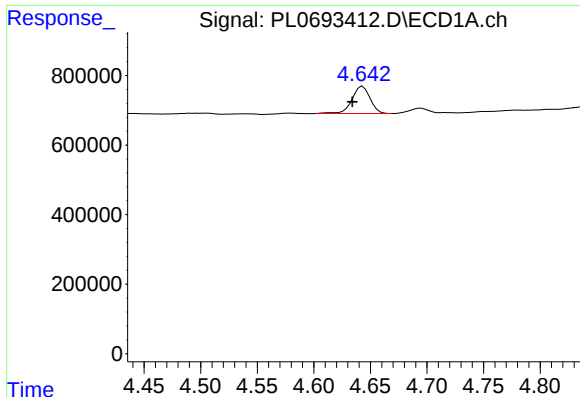

#1 Tetrachloro-m-xylene


R.T.: 4.643 min
Delta R.T.: 0.009 min
Response: 871809
Conc: 1.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

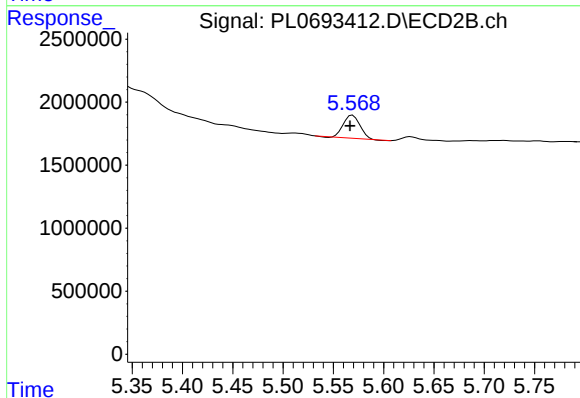


#1 Tetrachloro-m-xylene

R.T.: 5.569 min
Delta R.T.: 0.002 min
Response: 2093920
Conc: 1.46 ng/ml

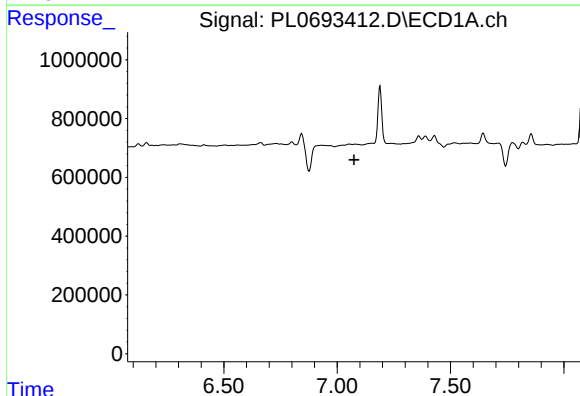


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.075 min
Response: 0
Conc: N.D.

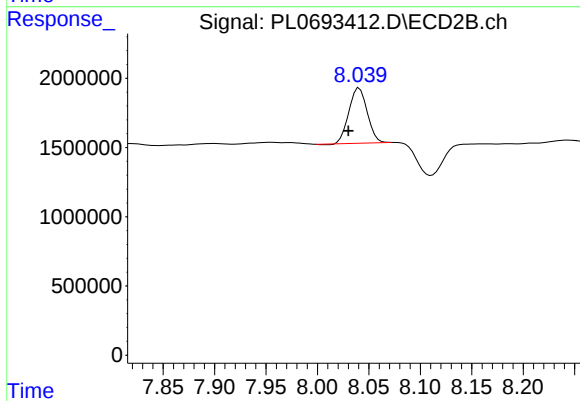

#8 Heptachlor epoxide


R.T.: 8.041 min
Delta R.T.: 0.011 min
Response: 4955284
Conc: 3.29 ng/ml

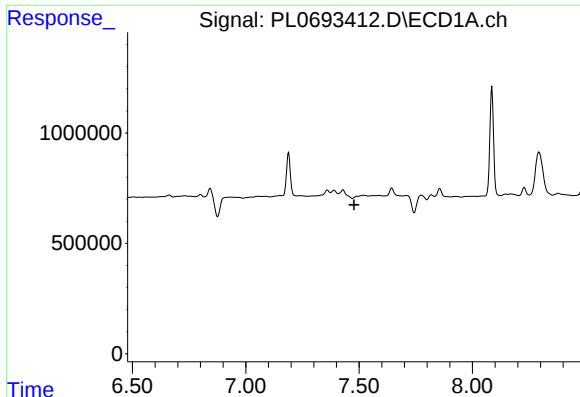

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.478 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

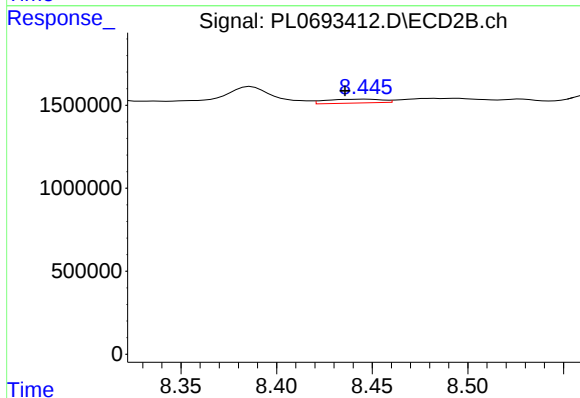


#9 Endosulfan I

R.T.: 8.446 min
Delta R.T.: 0.011 min
Response: 480834
Conc: 0.35 ng/ml

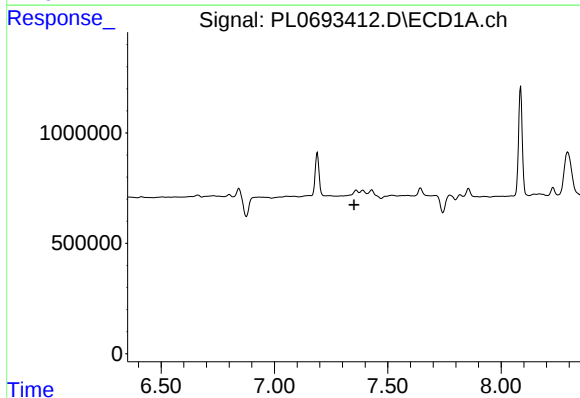


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.352 min
Response: 0
Conc: N.D.

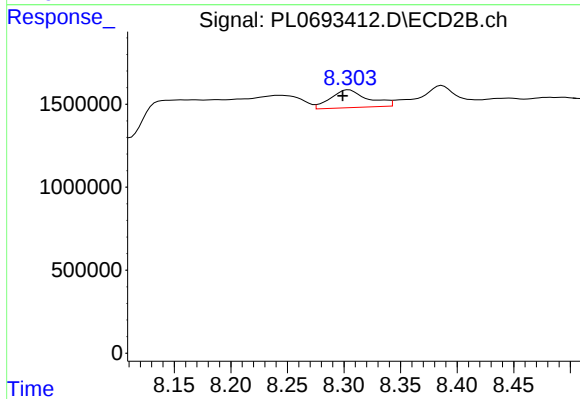

#10 gamma-Chlordane


R.T.: 8.304 min
Delta R.T.: 0.005 min
Response: 2468513
Conc: 1.60 ng/ml

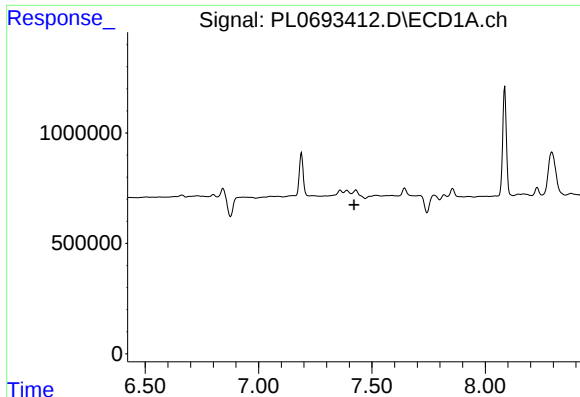

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.422 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

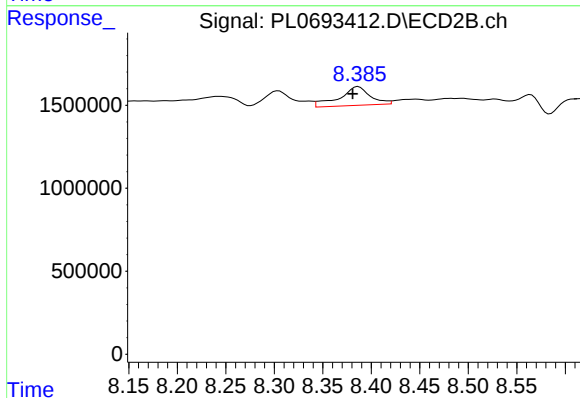


#11 alpha-Chlordane

R.T.: 8.387 min
Delta R.T.: 0.006 min
Response: 2507609
Conc: 1.68 ng/ml

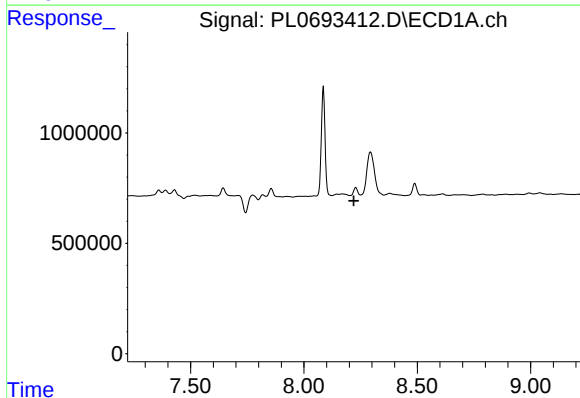


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.220 min
Response: 0
Conc: N.D.

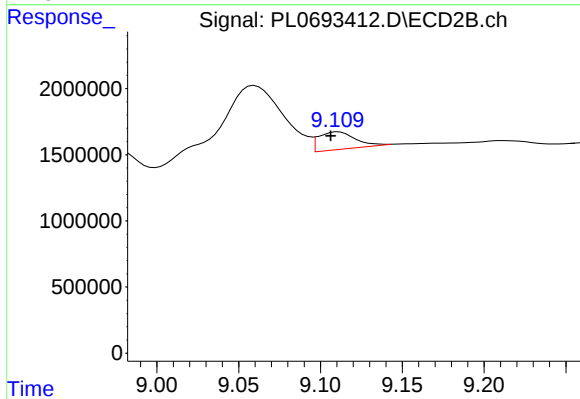

#16 4,4'-DDD


R.T.: 9.111 min
Delta R.T.: 0.005 min
Response: 2064045
Conc: 1.68 ng/ml

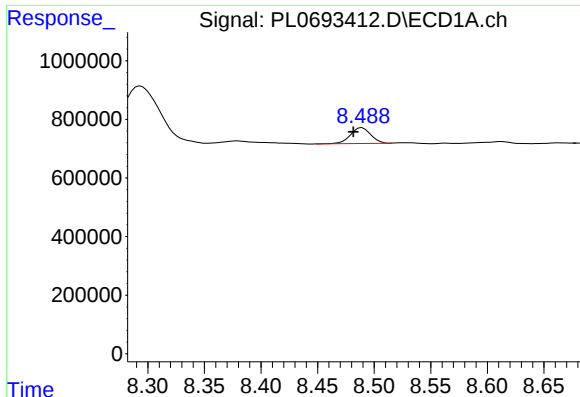

#17 4,4'-DDT


R.T.: 8.489 min
Delta R.T.: 0.008 min
Response: 672691
Conc: 1.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

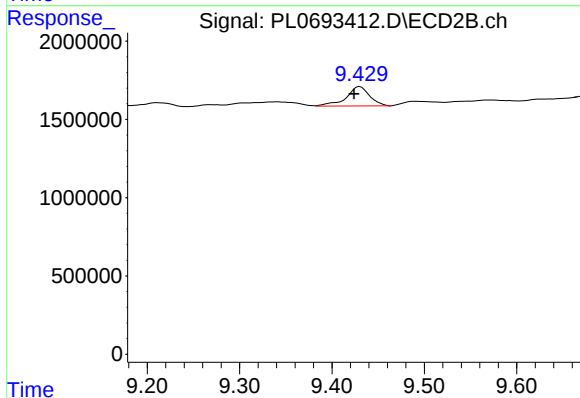


#17 4,4'-DDT

R.T.: 9.430 min
Delta R.T.: 0.006 min
Response: 2173920
Conc: 1.77 ng/ml

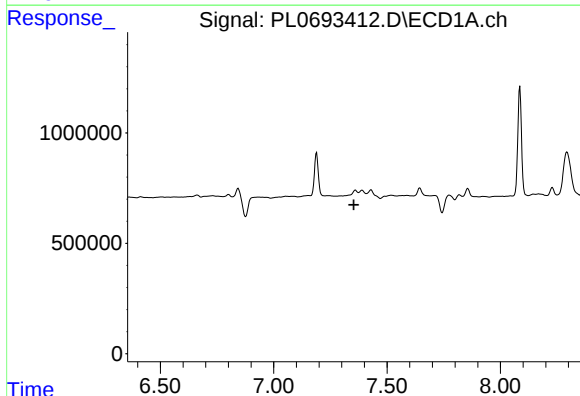


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 7.354 min
Response: 0
Conc: N.D.

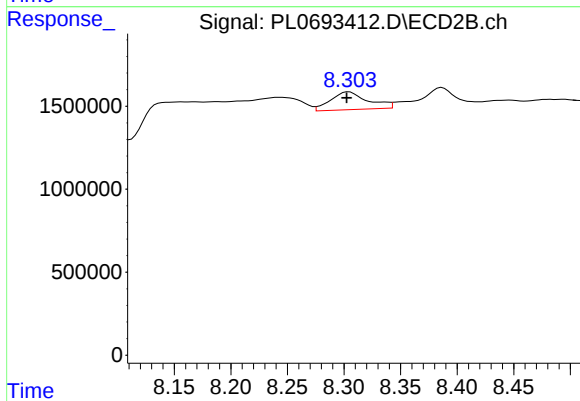

#25 Chlordane-3


R.T.: 8.304 min
Delta R.T.: 0.002 min
Response: 2468513
Conc: 11.53 ng/ml

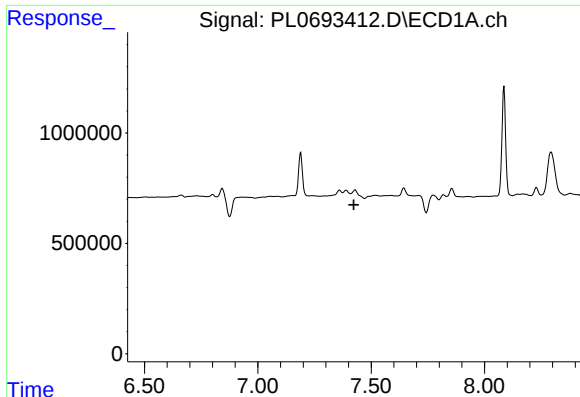

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.423 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

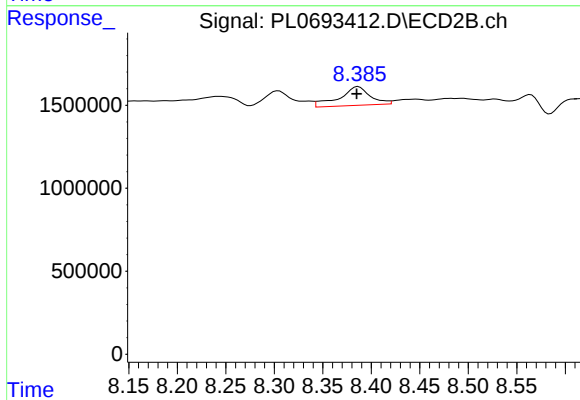


#26 Chlordane-4

R.T.: 8.387 min
Delta R.T.: 0.002 min
Response: 2507609
Conc: 9.74 ng/ml

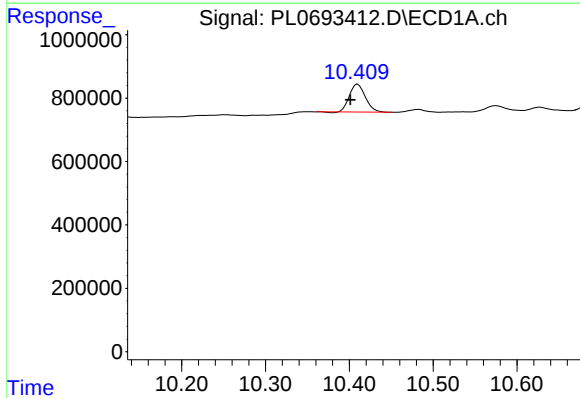

#28 Decachlorobiphenyl

R.T.: 10.410 min
Delta R.T.: 0.009 min
Response: 1158353
Conc: 1.72 ng/ml

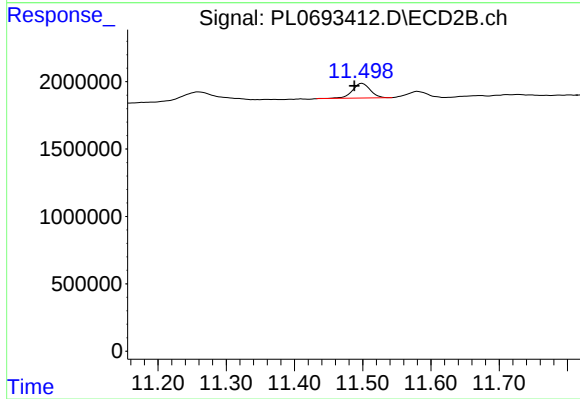

#28 Decachlorobiphenyl

R.T.: 11.499 min
Delta R.T.: 0.011 min
Response: 1970825
Conc: 1.61 ng/ml