

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082421\
 Data File : PL0693416.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Aug 2021 13:18
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 25 00:50:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 21 02:23:37 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.635	5.569	9853672	27042628	21.357	18.878
28)	SA Decachlor...	10.405	11.496	10620437	20999123	15.735	17.134
Target Compounds							
4)	MA Heptachlor	6.152f	0.000	812980	0	1.174	N.D. #
7)	B delta-BHC	0.000	7.036f	0	3330065	N.D.	1.803 #
8)	B Heptachlo...	0.000	8.039	0	1511680	N.D.	1.005 #
14)	MA Endrin	8.081f	0.000	290906	0	0.504	N.D. #
22)	Mirex	0.000	10.557f	0	1613157	N.D.	1.721 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082421\
Data File : PL0693416.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Aug 2021 13:18
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 25 00:50:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
Quant Title : GC Extractables
QLast Update : Sat Aug 21 02:23:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

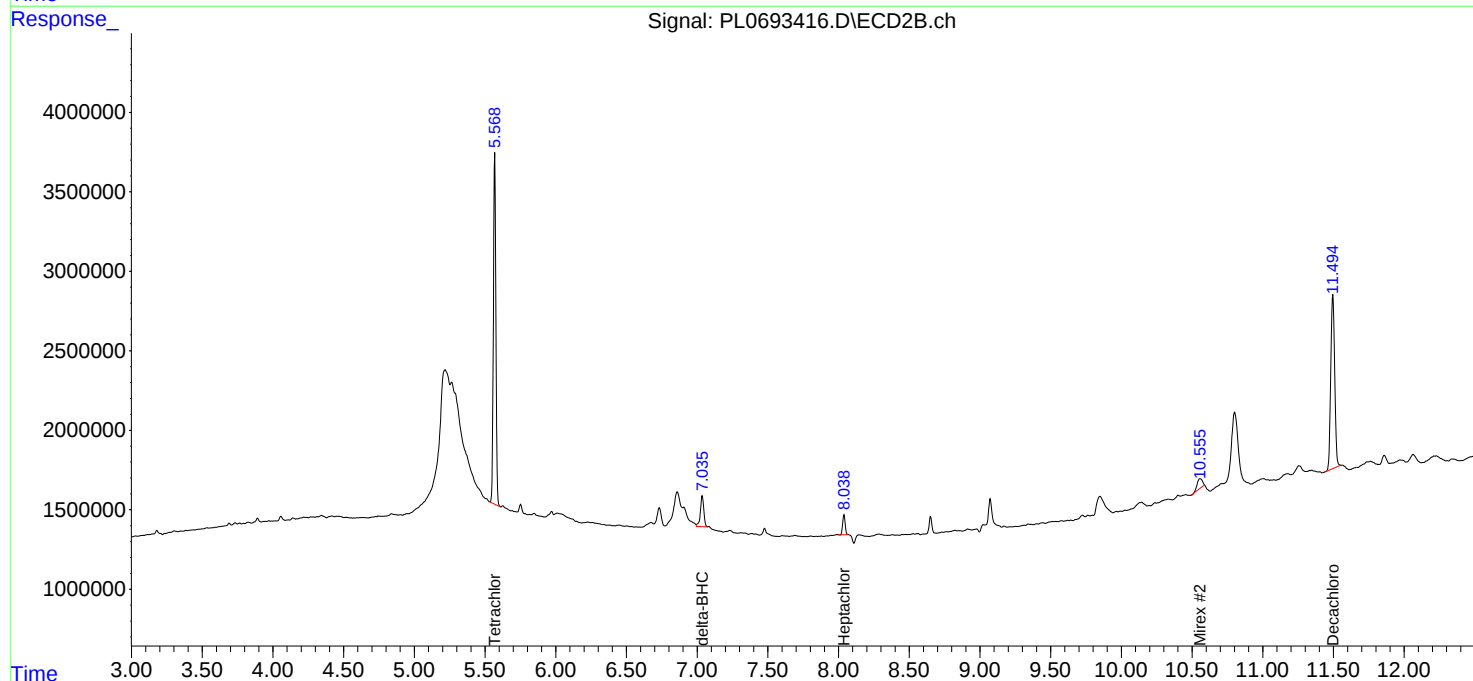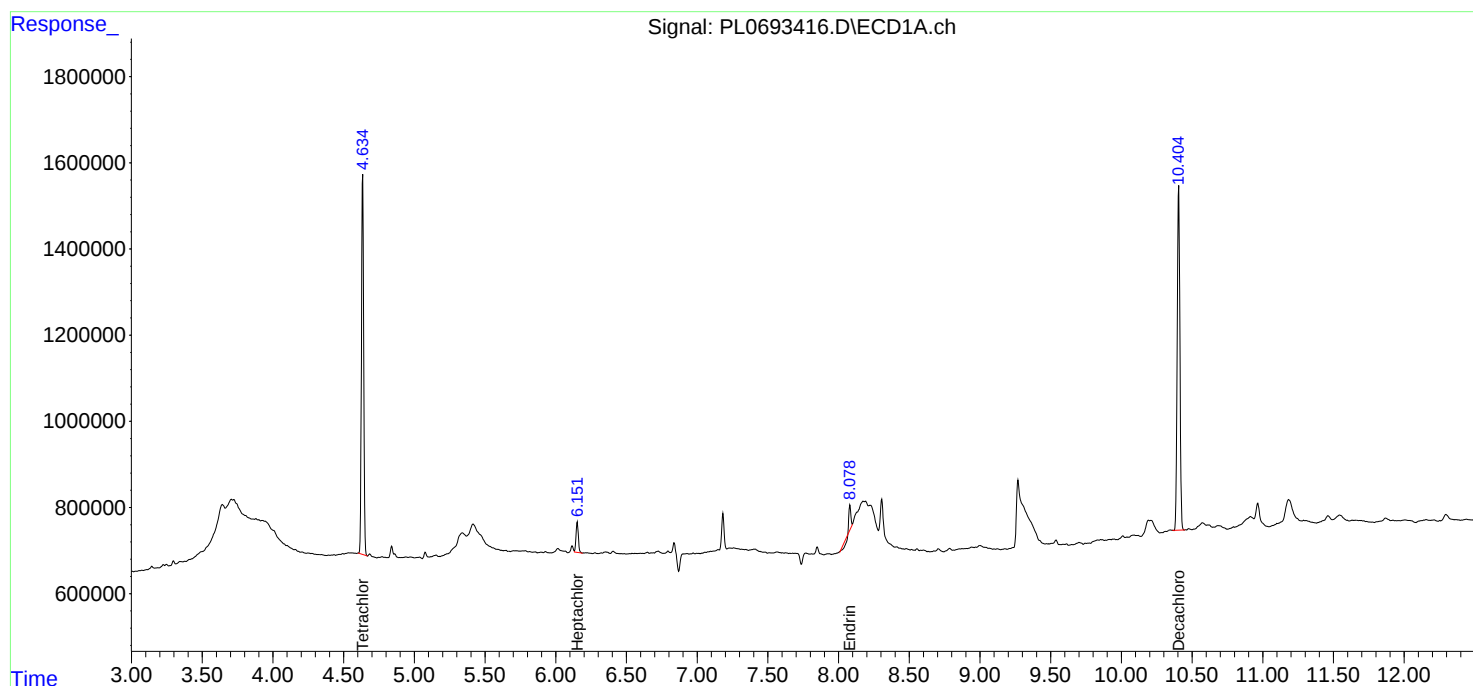


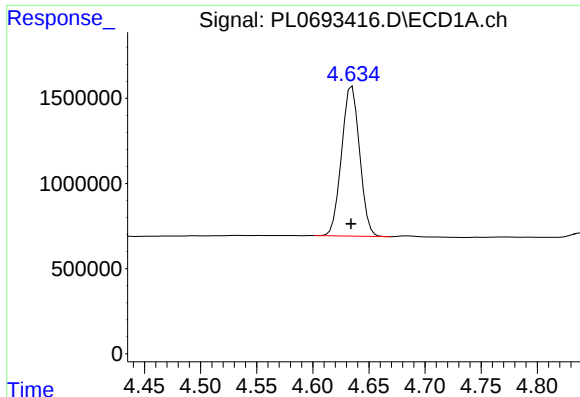

#1 Tetrachloro-m-xylene


R.T.: 4.635 min
Delta R.T.: 0.001 min
Response: 9853672
Conc: 21.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

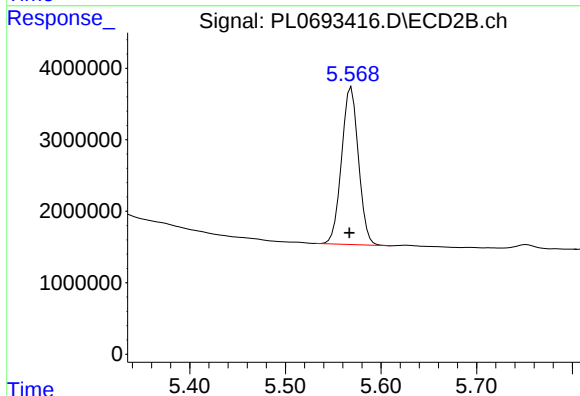


#1 Tetrachloro-m-xylene

R.T.: 5.569 min
Delta R.T.: 0.002 min
Response: 27042628
Conc: 18.88 ng/ml

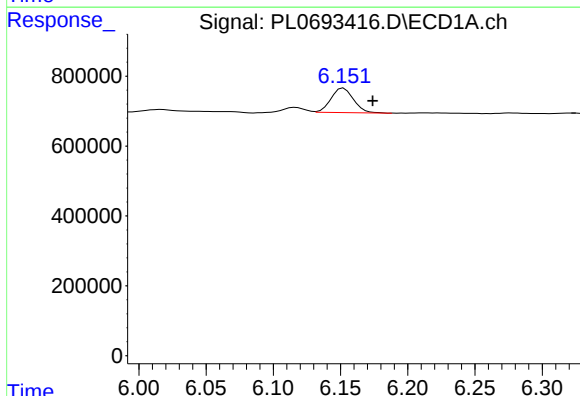


#4 Heptachlor

R.T.: 6.152 min
Delta R.T.: -0.022 min
Response: 812980
Conc: 1.17 ng/ml

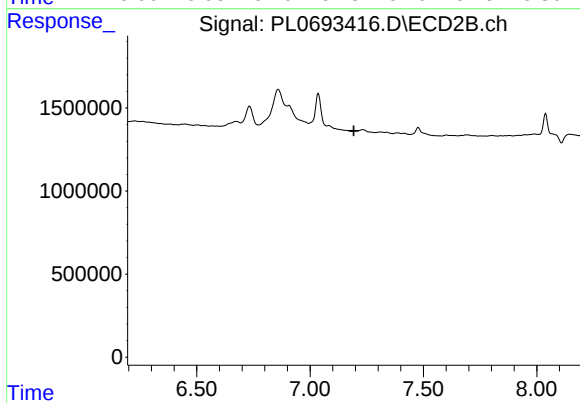

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 7.193 min
Response: 0
Conc: N.D.

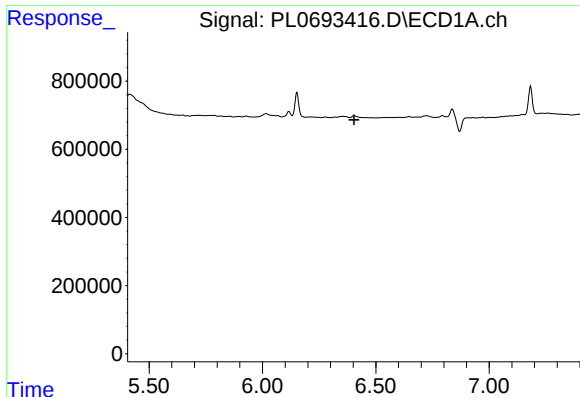

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.404 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

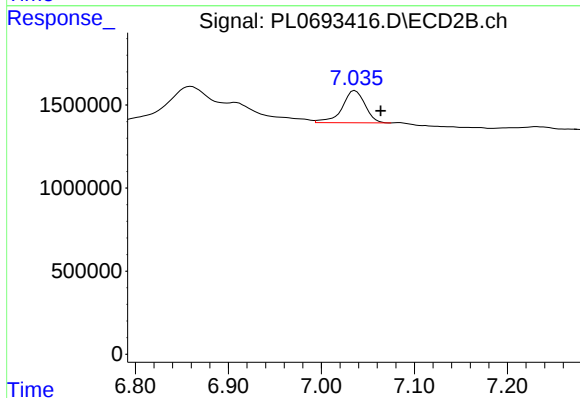


#7 delta-BHC

R.T.: 7.036 min
Delta R.T.: -0.028 min
Response: 3330065
Conc: 1.80 ng/ml

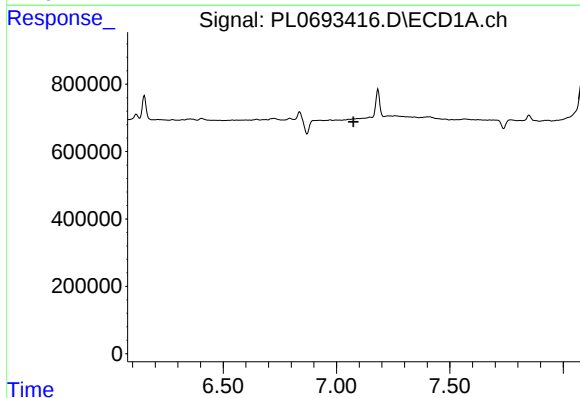


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 7.075 min
Response: 0
Conc: N.D.

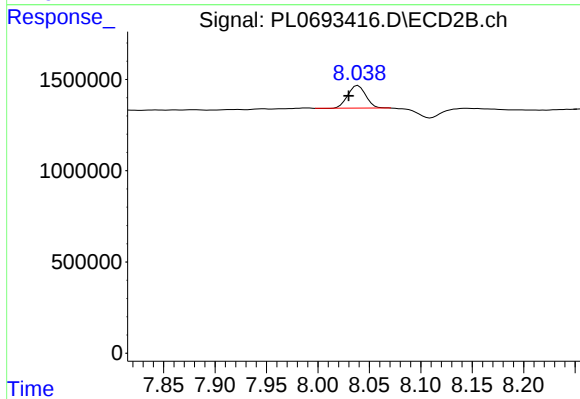

#8 Heptachlor epoxide


R.T.: 8.039 min
Delta R.T.: 0.009 min
Response: 1511680
Conc: 1.00 ng/ml

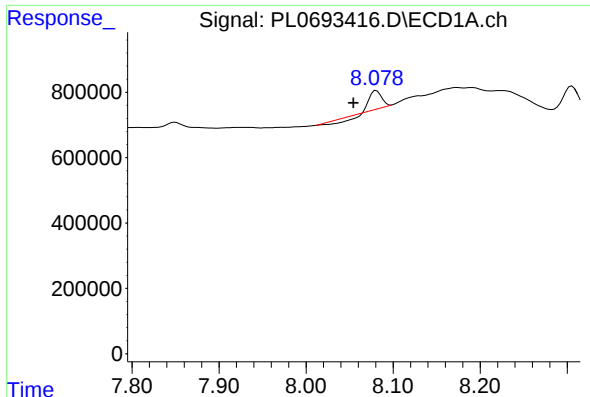

#14 Endrin


R.T.: 8.081 min
Delta R.T.: 0.027 min
Response: 290906
Conc: 0.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

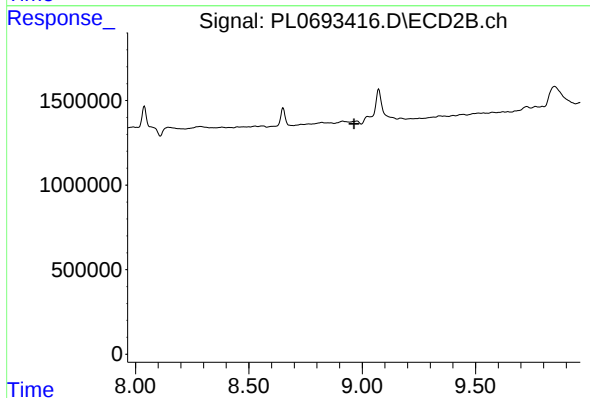


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.964 min
Response: 0
Conc: N.D.

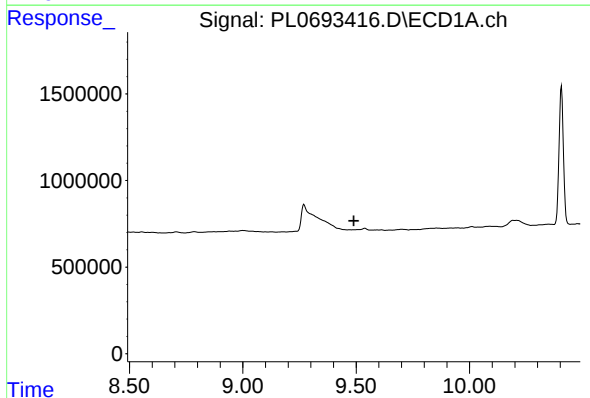


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 9.490 min
Response: 0
Conc: N.D.

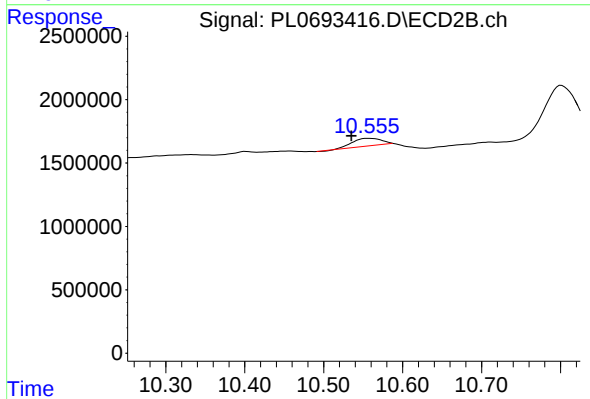

#22 Mirex


R.T.: 10.557 min
Delta R.T.: 0.022 min
Response: 1613157
Conc: 1.72 ng/ml

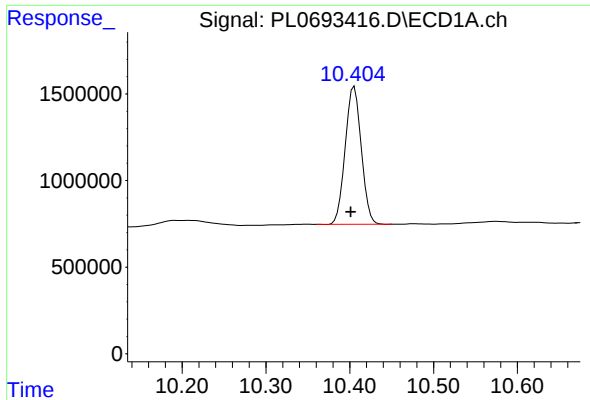

#28 Decachlorobiphenyl

R.T.: 10.405 min
Delta R.T.: 0.004 min
Response: 10620437
Conc: 15.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

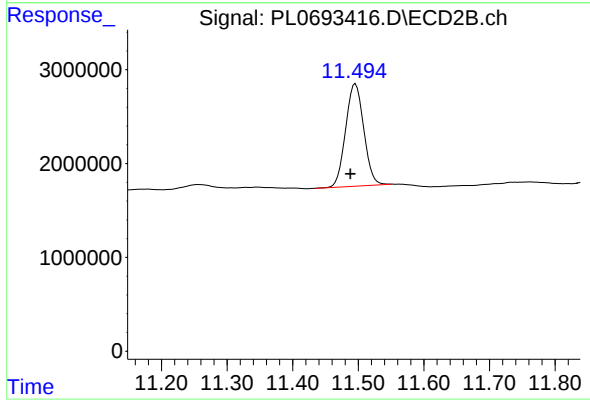

#28 Decachlorobiphenyl

R.T.: 11.496 min
Delta R.T.: 0.008 min
Response: 20999123
Conc: 17.13 ng/ml