

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082421\
 Data File : PL0693423.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Aug 2021 18:18
 Operator : AR\AJ
 Sample : M3521-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 25 00:51:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 21 02:23:37 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.632	5.565	7747828	52441844	16.793	36.609 #
28)	SA Decachlor...	10.400	11.488	9494716	21140530	14.067	17.250
Target Compounds							
9)	A Endosulfan I	7.500f	8.442	6319298	1180264	10.674	0.853 #
10)	B gamma-Chl...	0.000	8.292	0	7036448	N.D.	4.574 #
11)	B alpha-Chl...	0.000	8.383	0	1561357	N.D.	1.045 #
16)	A 4,4'-DDD	0.000	9.100	0	1259434	N.D.	1.027 #
20)	A Methoxychlor	9.098f	9.900	1021395	692143	2.727	1.078 #
23)	Chlordane-1	0.000	6.980f	0	945568	N.D.	16.703 #
25)	Chlordane-3	0.000	8.292	0	7036448	N.D.	32.858 #
26)	Chlordane-4	0.000	8.383	0	1561357	N.D.	6.066 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082421\
Data File : PL0693423.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Aug 2021 18:18
Operator : AR\AJ
Sample : M3521-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 25 00:51:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
Quant Title : GC Extractables
QLast Update : Sat Aug 21 02:23:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

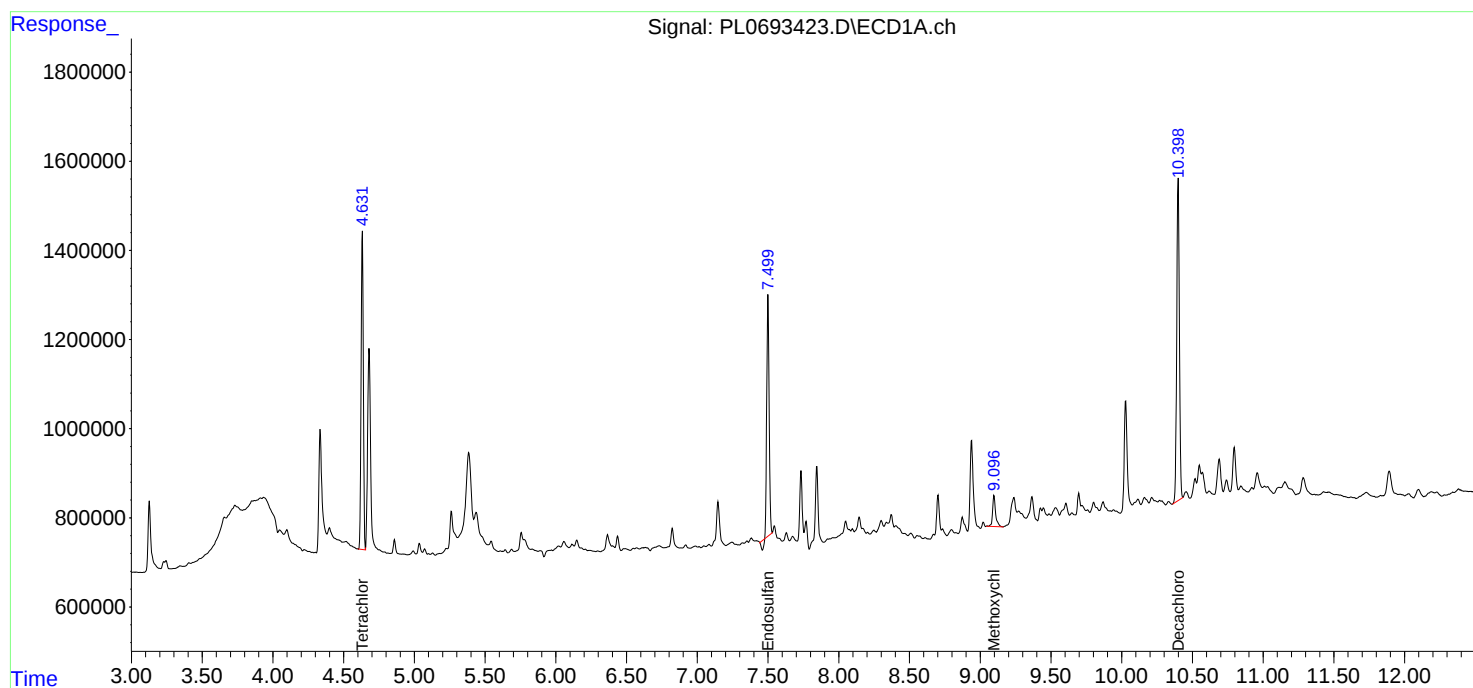


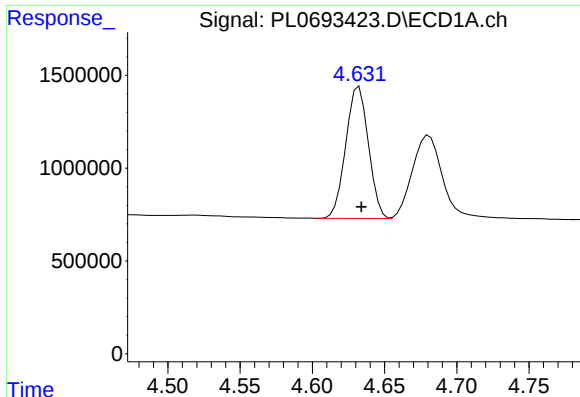

#1 Tetrachloro-m-xylene


R.T.: 4.632 min
Delta R.T.: -0.002 min
Response: 7747828
Conc: 16.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

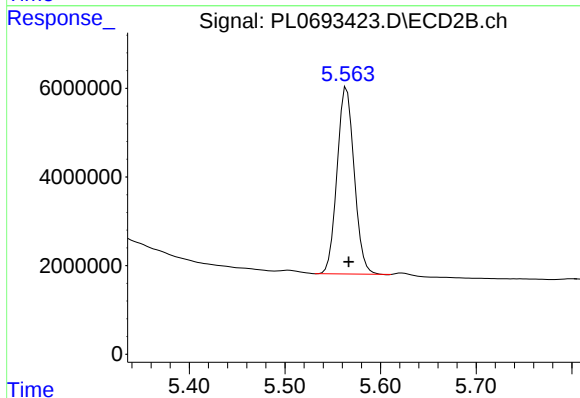


#1 Tetrachloro-m-xylene

R.T.: 5.565 min
Delta R.T.: -0.002 min
Response: 52441844
Conc: 36.61 ng/ml

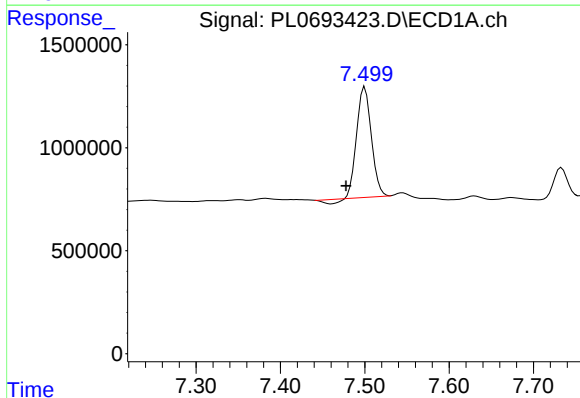


#9 Endosulfan I

R.T.: 7.500 min
Delta R.T.: 0.022 min
Response: 6319298
Conc: 10.67 ng/ml

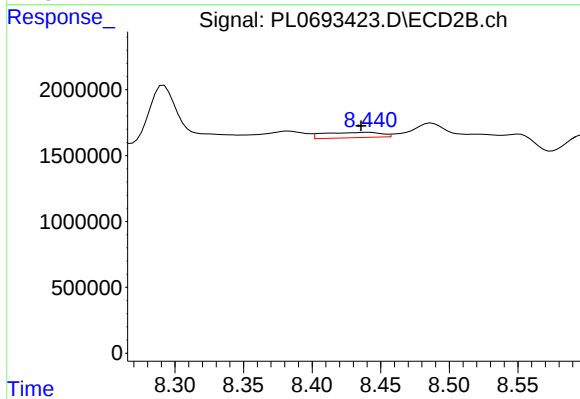

#9 Endosulfan I


R.T.: 8.442 min
Delta R.T.: 0.006 min
Response: 1180264
Conc: 0.85 ng/ml

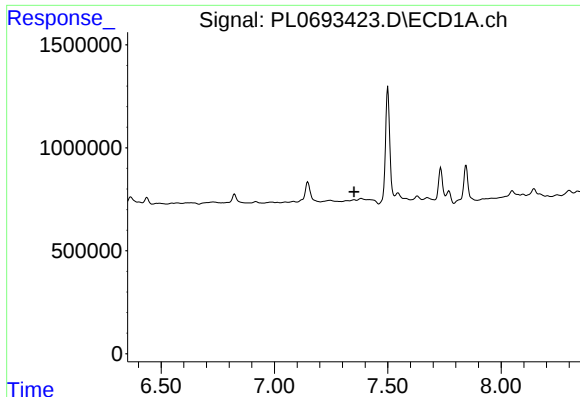

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.352 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

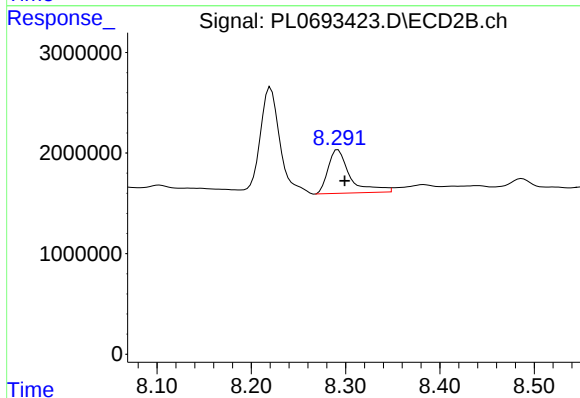


#10 gamma-Chlordane

R.T.: 8.292 min
Delta R.T.: -0.007 min
Response: 7036448
Conc: 4.57 ng/ml

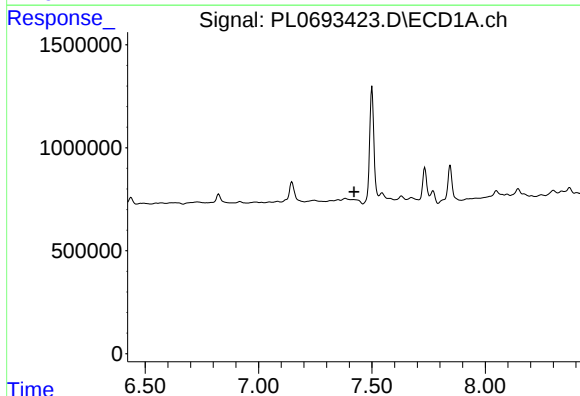


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.422 min
Response: 0
Conc: N.D.

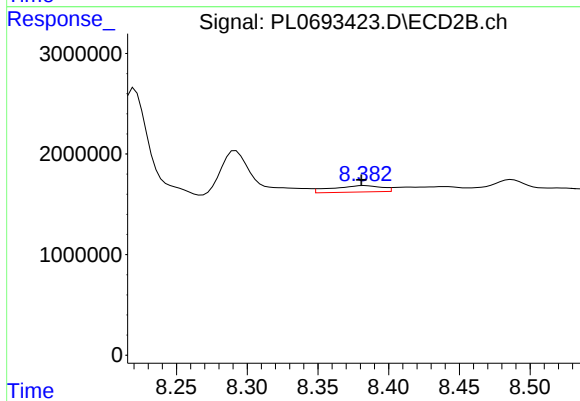

#11 alpha-Chlordane


R.T.: 8.383 min
Delta R.T.: 0.003 min
Response: 1561357
Conc: 1.04 ng/ml

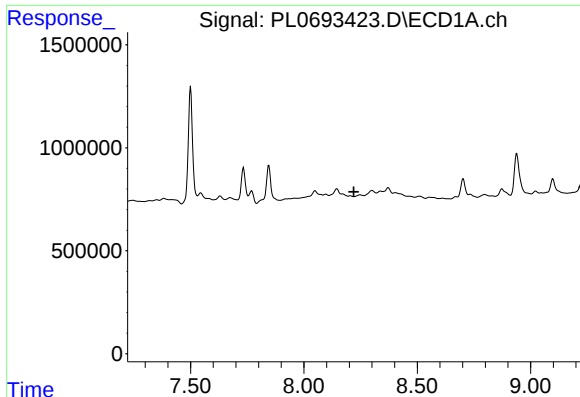

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.220 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

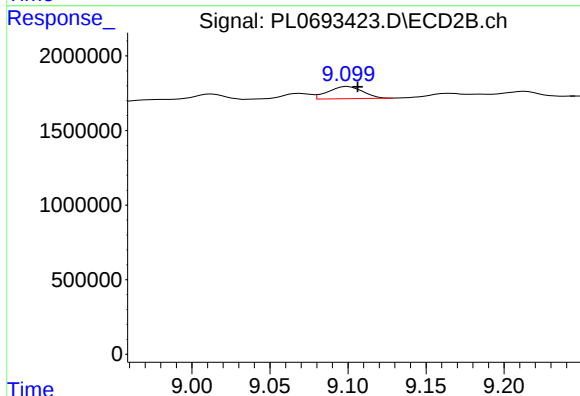


#16 4,4'-DDD

R.T.: 9.100 min
Delta R.T.: -0.006 min
Response: 1259434
Conc: 1.03 ng/ml

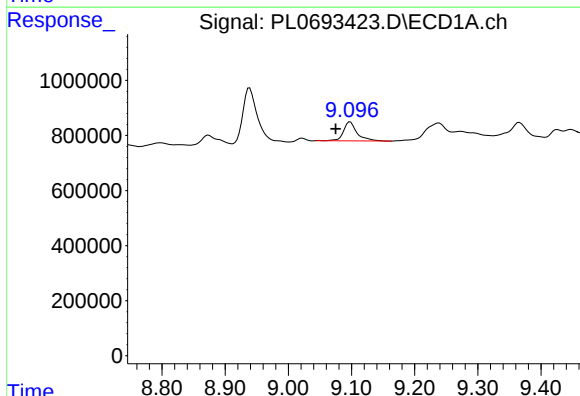


#20 Methoxychlor

R.T.: 9.098 min
Delta R.T.: 0.023 min
Response: 1021395
Conc: 2.73 ng/ml

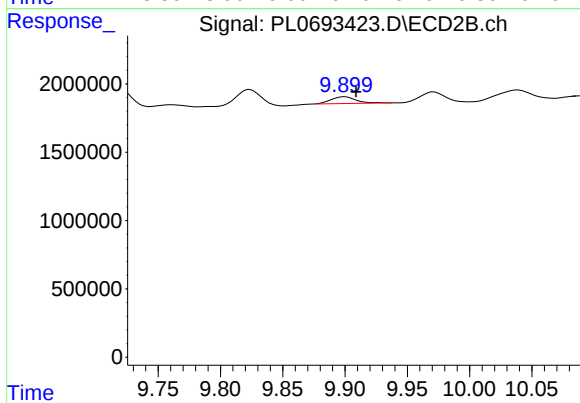

#20 Methoxychlor


R.T.: 9.900 min
Delta R.T.: -0.009 min
Response: 692143
Conc: 1.08 ng/ml

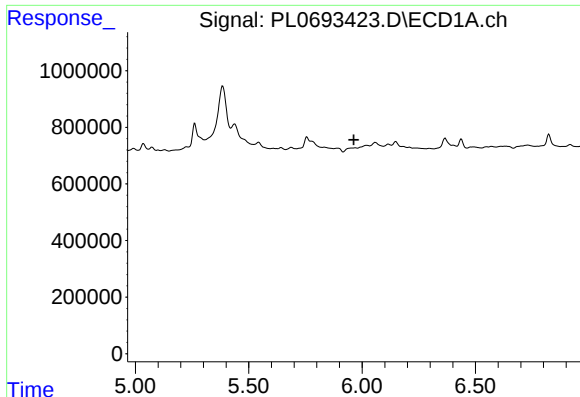

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.964 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

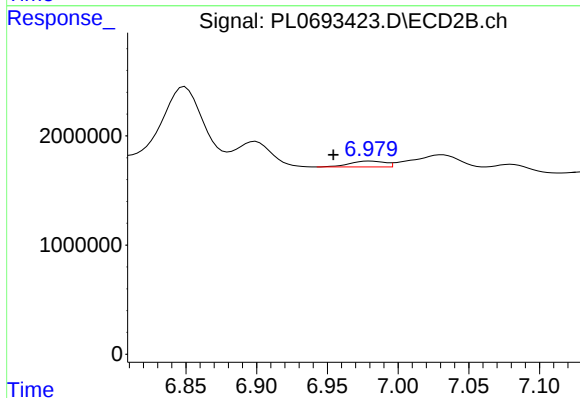


#23 Chlordane-1

R.T.: 6.980 min
Delta R.T.: 0.026 min
Response: 945568
Conc: 16.70 ng/ml

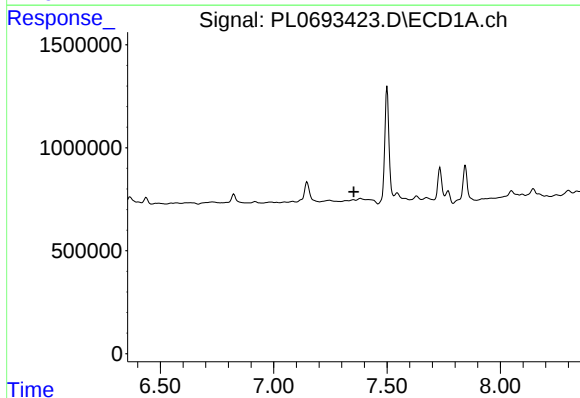


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.354 min
Response: 0
Conc: N.D.

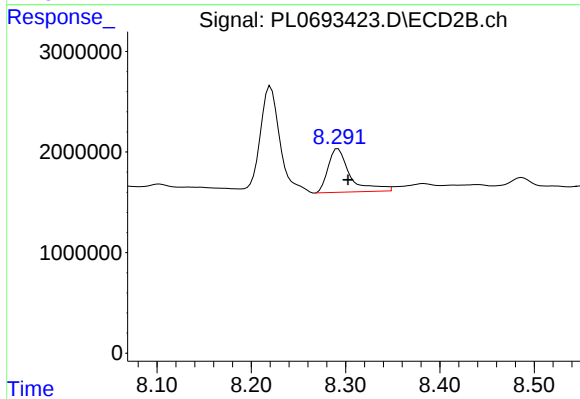

#25 Chlordane-3


R.T.: 8.292 min
Delta R.T.: -0.011 min
Response: 7036448
Conc: 32.86 ng/ml

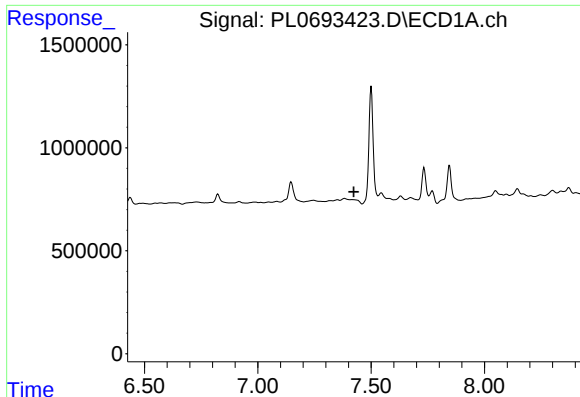

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.423 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

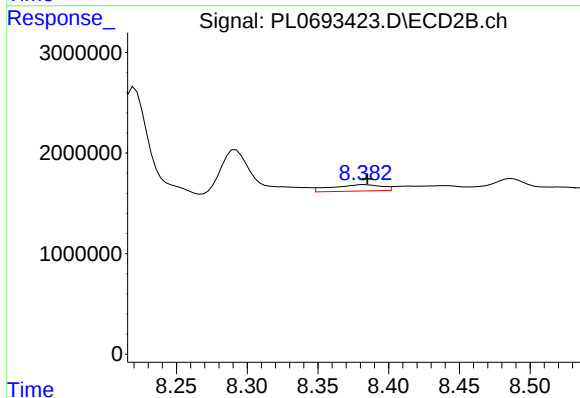


#26 Chlordane-4

R.T.: 8.383 min
Delta R.T.: -0.002 min
Response: 1561357
Conc: 6.07 ng/ml

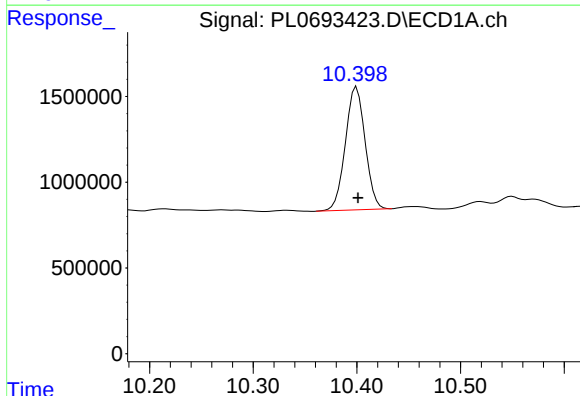

#28 Decachlorobiphenyl

R.T.: 10.400 min
Delta R.T.: -0.002 min
Response: 9494716
Conc: 14.07 ng/ml

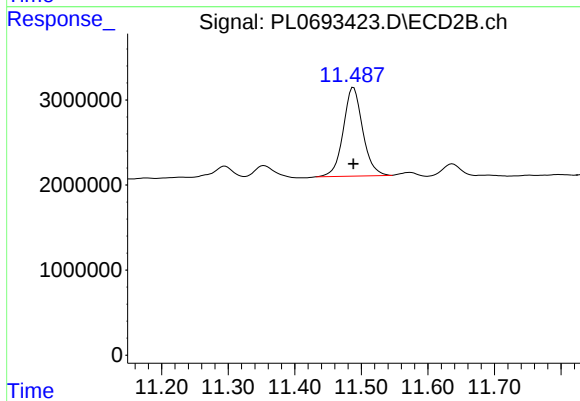

#28 Decachlorobiphenyl

R.T.: 11.488 min
Delta R.T.: 0.000 min
Response: 21140530
Conc: 17.25 ng/ml