

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082422\
 Data File : PL077306.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Aug 2022 14:47
 Operator : AR\AJ
 Sample : N4310-01 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EO-02-082322

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/25/2022
 Supervised By :Ankita Jodhani 08/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 24 23:57:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082222.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 23 05:36:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.415	2.630	2321512	7260349	1.706	2.362 #
28) SA Decachlor...	8.906	7.731	3583075	5996105	3.058	2.149m#
Target Compounds						
17) MA 4,4'-DDT	6.913	5.861	5284182	10669966	4.730	4.051

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082422\
Data File : PL077306.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Aug 2022 14:47
Operator : AR\AJ
Sample : N4310-01 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
EO-02-082322


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 08/25/2022
Supervised By : Ankita Jodhani 08/25/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 23:57:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082222.M
Quant Title : GC Extractables
QLast Update : Tue Aug 23 05:36:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

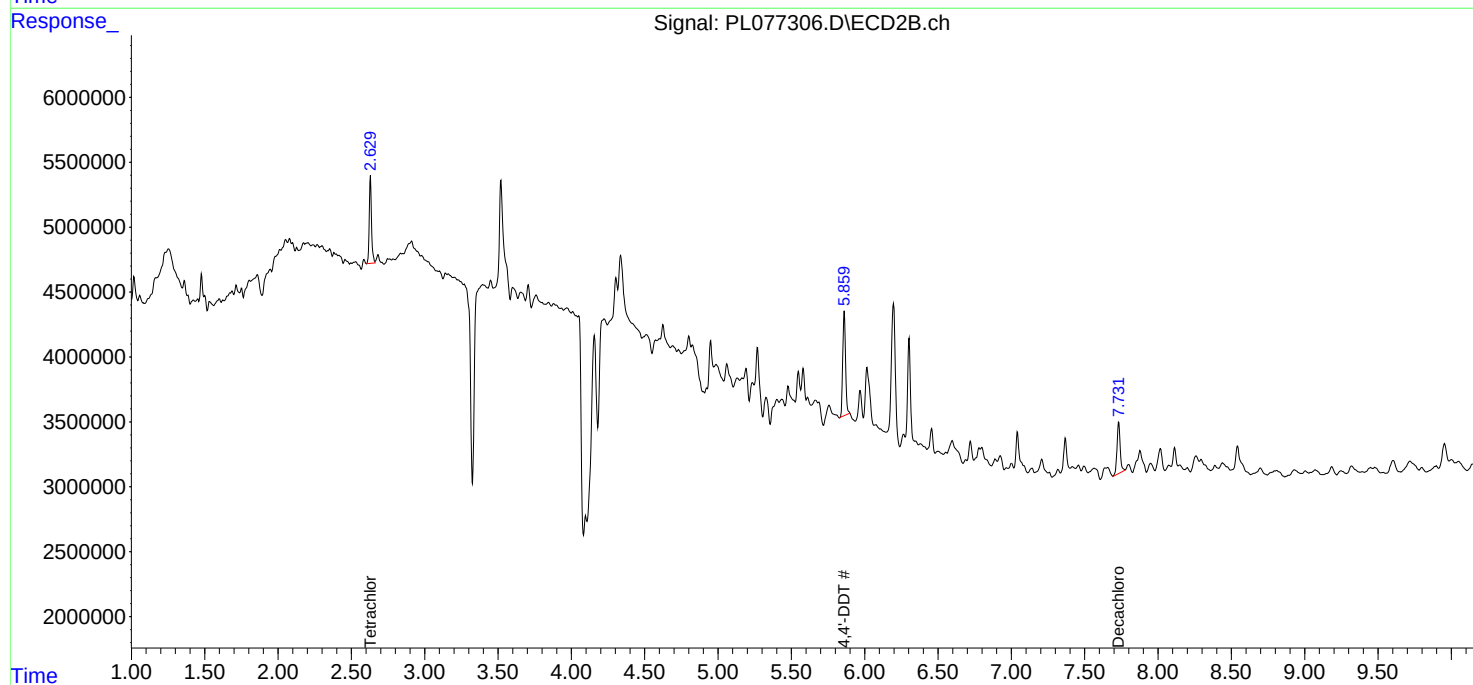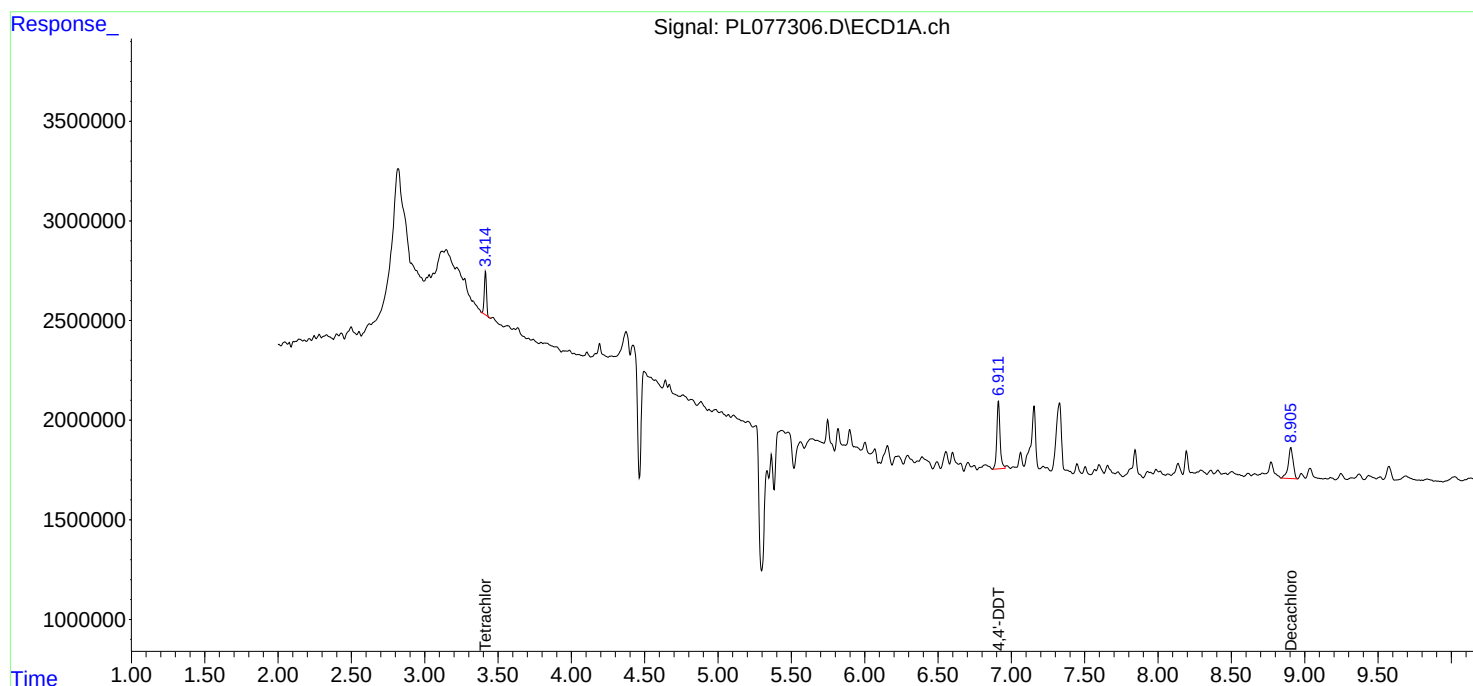

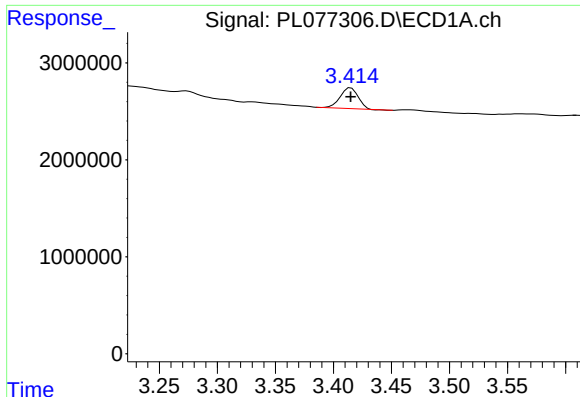


#1 Tetrachloro-m-xylene

R.T.: 3.415 min
Delta R.T.: 0.000 min
Response: 2321512
Conc: 1.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-02-082322


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/25/2022
Supervised By :Ankita Jodhani 08/25/2022

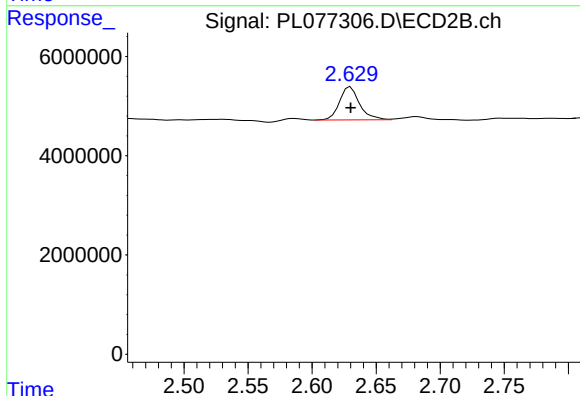


#1 Tetrachloro-m-xylene

R.T.: 2.630 min
Delta R.T.: 0.000 min
Response: 7260349
Conc: 2.36 ng/ml

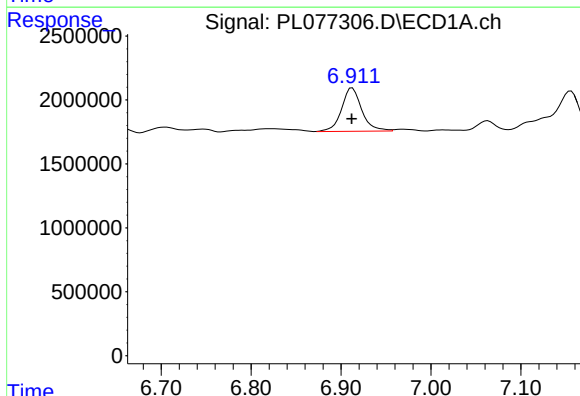


#17 4,4'-DDT

R.T.: 6.913 min
Delta R.T.: 0.000 min
Response: 5284182
Conc: 4.73 ng/ml

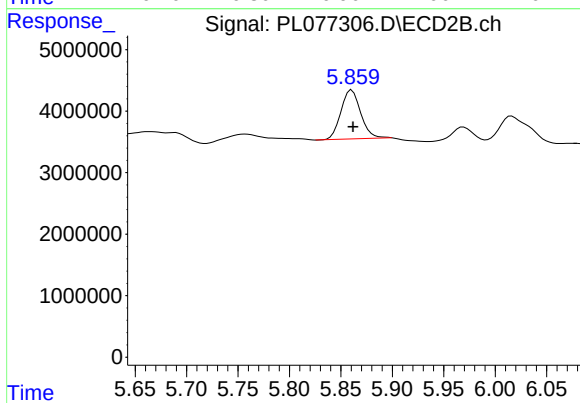

#17 4,4'-DDT

R.T.: 5.861 min
Delta R.T.: -0.001 min
Response: 10669966
Conc: 4.05 ng/ml

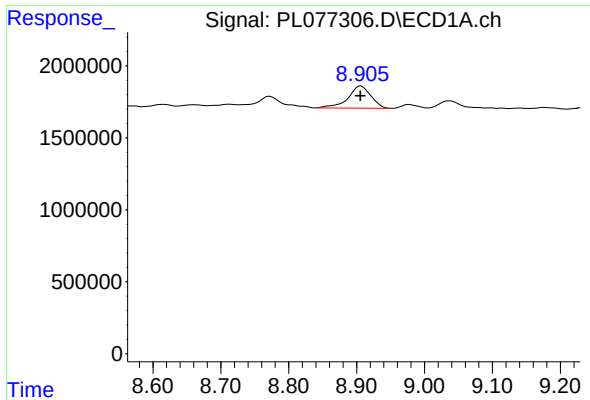


#28 Decachlorobiphenyl

R.T.: 8.906 min
Delta R.T.: 0.000 min
Response: 3583075
Conc: 3.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-02-082322

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/25/2022
Supervised By :Ankita Jodhani 08/25/2022

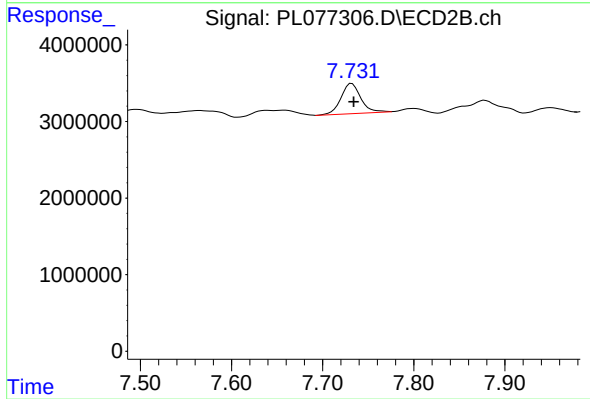

#28 Decachlorobiphenyl

R.T.: 7.731 min
Delta R.T.: -0.004 min
Response: 5996105
Conc: 2.15 ng/ml m