

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082520\
 Data File : PL060970.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Aug 2020 19:48
 Operator : DD\AJ
 Sample : L3784-10
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 26 02:27:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 25 16:59:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.462	4.011	23124952	33990079	12.531	13.078
28)	SA Decachlor...	8.217	9.100	21353775	28904461	12.676	13.699
Target Compounds							
2)	A alpha-BHC	0.000	4.426f	0	1703947	N.D.	0.419 #
10)	B gamma-Chl...	0.000	6.130	0	1679095	N.D.	0.541 #
11)	B alpha-Chl...	0.000	6.200	0	2314115	N.D.	0.744 #
12)	B 4,4'-DDE	5.625	6.354	2866217	5065256	1.558	1.753
15)	B Endosulfa...	0.000	6.907f	0	813337	N.D.	0.316 #
17)	MA 4,4'-DDT	6.381	7.148	3137053	5012682	2.075	2.177
25)	Chlordane-3	0.000	6.130	0	1679095	N.D.	4.201 #
26)	Chlordane-4	0.000	6.200	0	2314115	N.D.	4.814 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082520\
Data File : PL060970.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Aug 2020 19:48
Operator : DD\AJ
Sample : L3784-10
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 26 02:27:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
Quant Title : GC Extractables
QLast Update : Tue Aug 25 16:59:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

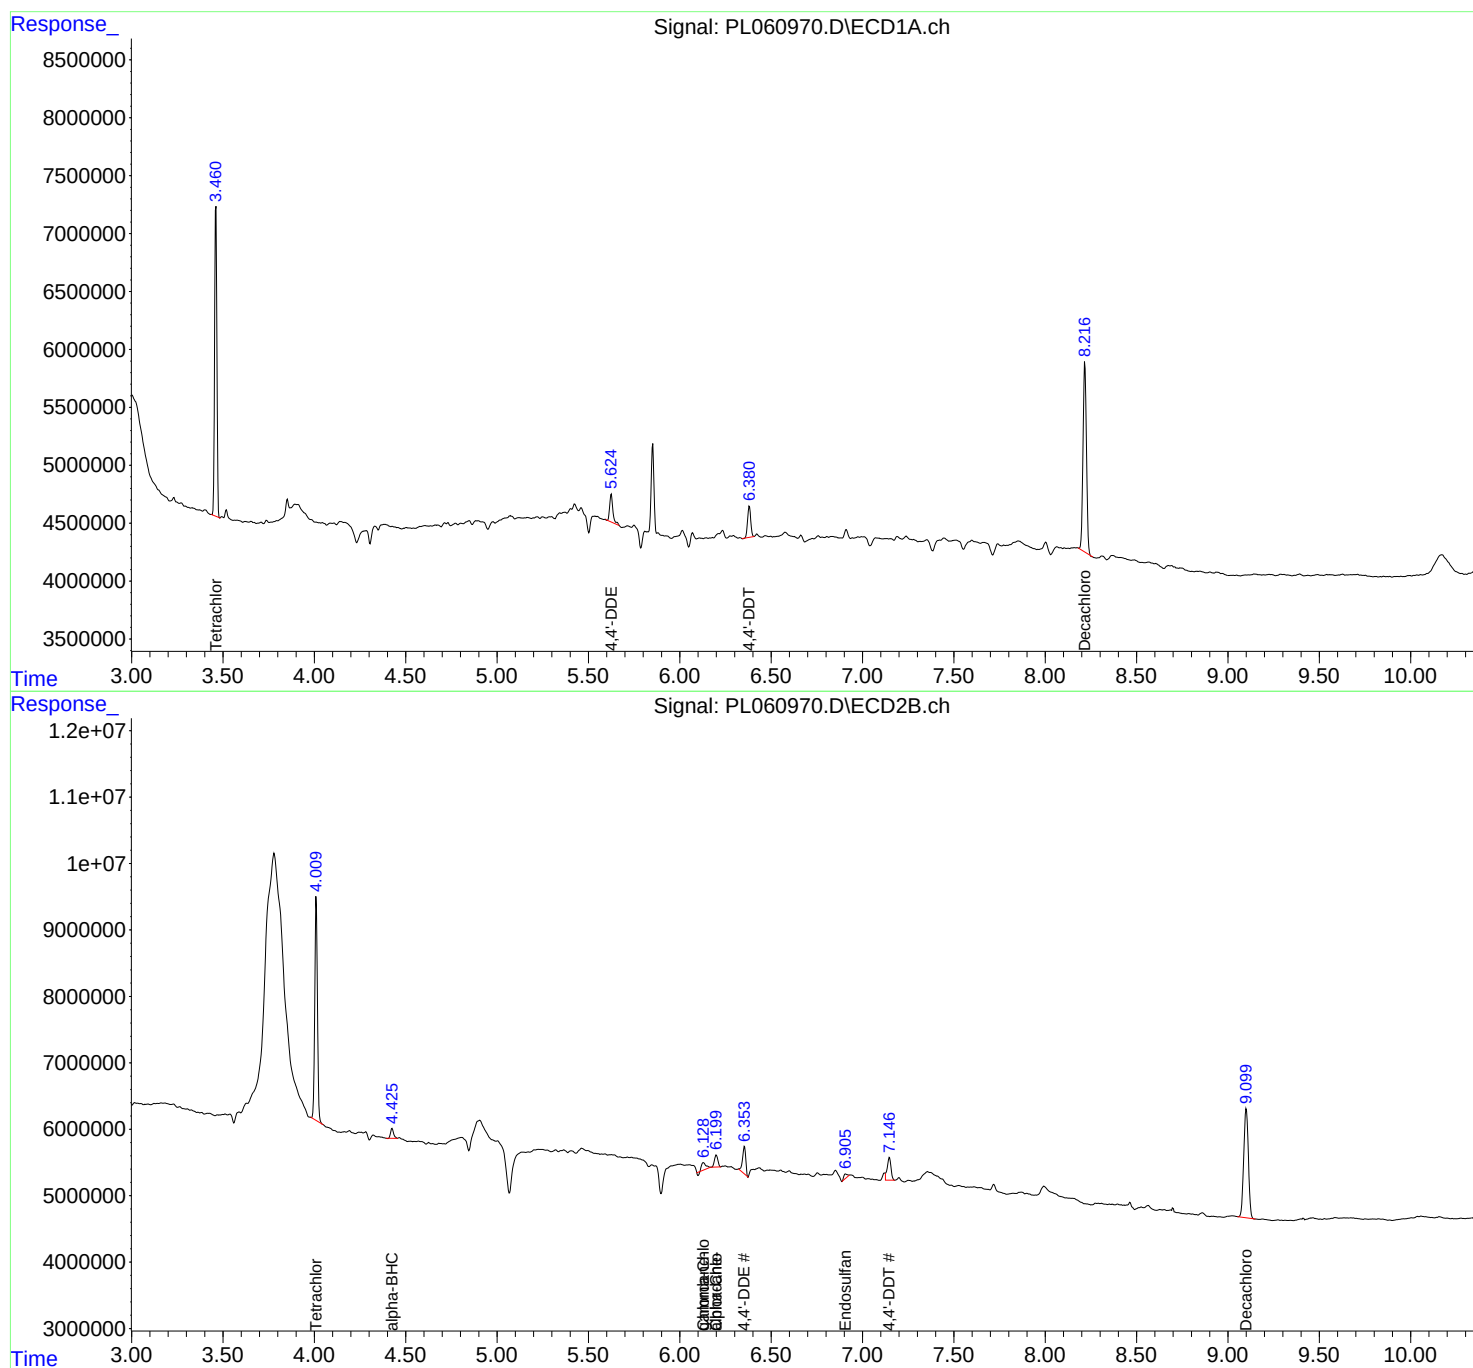


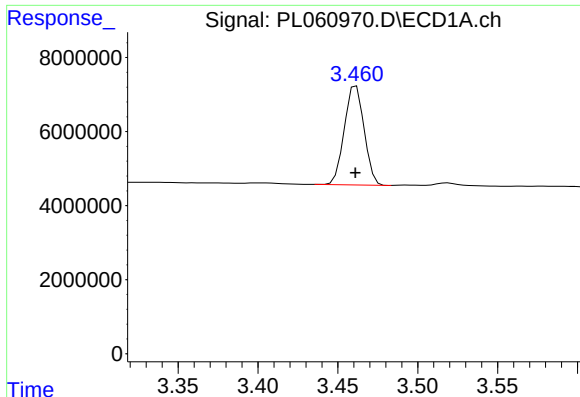

#1 Tetrachloro-m-xylene


R.T.: 3.462 min
Delta R.T.: 0.000 min
Response: 23124952
Conc: 12.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

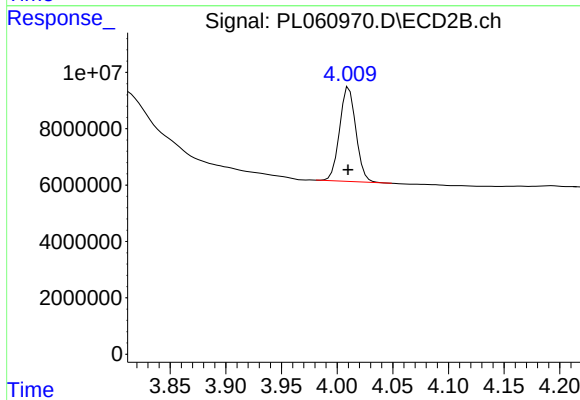


#1 Tetrachloro-m-xylene

R.T.: 4.011 min
Delta R.T.: 0.000 min
Response: 33990079
Conc: 13.08 ng/ml

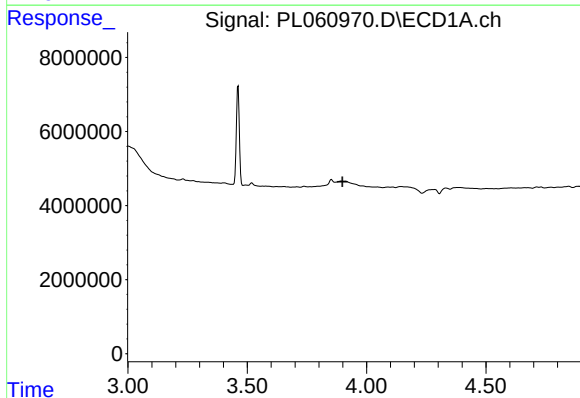


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.898 min
Response: 0
Conc: N.D.

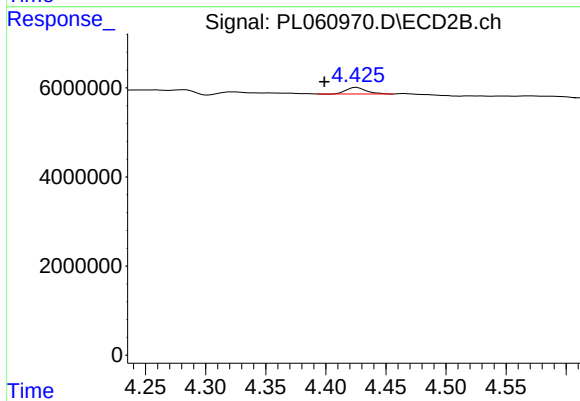

#2 alpha-BHC


R.T.: 4.426 min
Delta R.T.: 0.027 min
Response: 1703947
Conc: 0.42 ng/ml

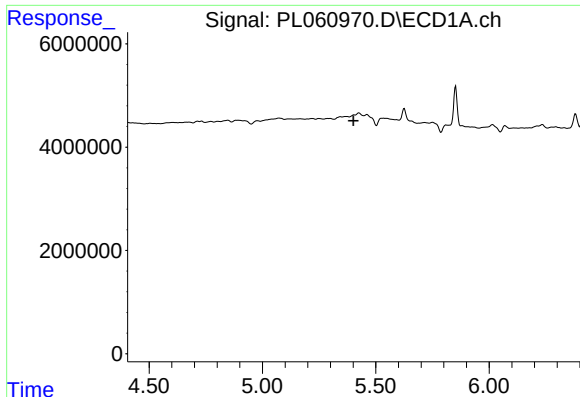

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.402 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

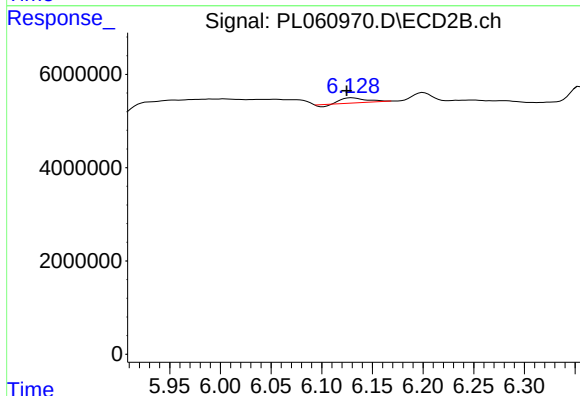


#10 gamma-Chlordane

R.T.: 6.130 min
Delta R.T.: 0.005 min
Response: 1679095
Conc: 0.54 ng/ml

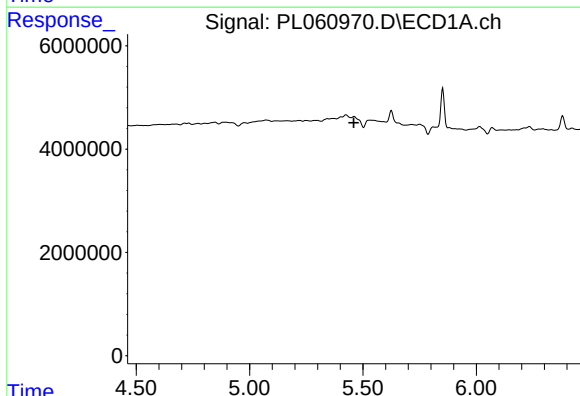


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.460 min
Response: 0
Conc: N.D.

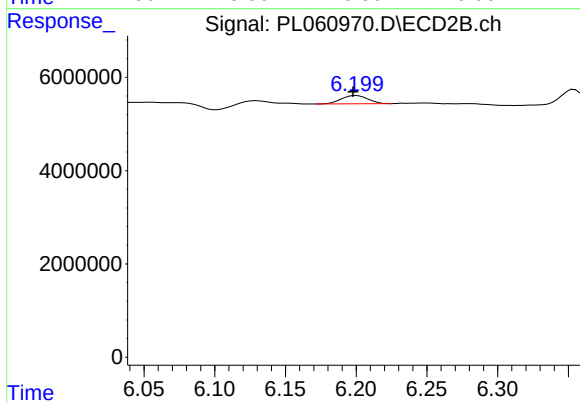

#11 alpha-Chlordane


R.T.: 6.200 min
Delta R.T.: 0.002 min
Response: 2314115
Conc: 0.74 ng/ml

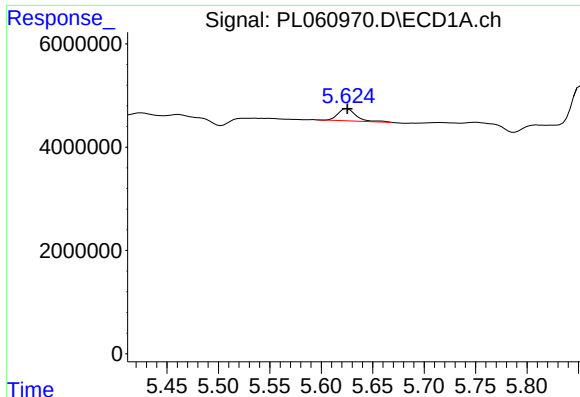

#12 4,4'-DDE


R.T.: 5.625 min
Delta R.T.: 0.000 min
Response: 2866217
Conc: 1.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

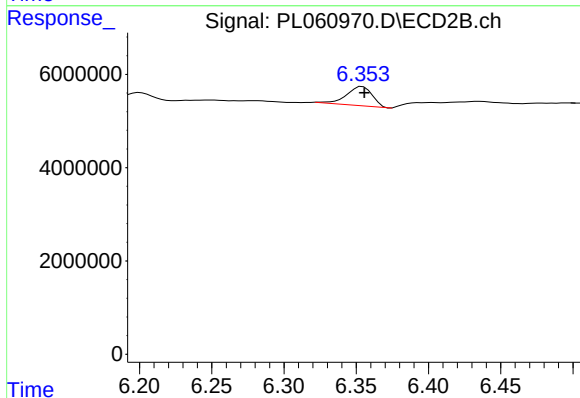


#12 4,4'-DDE

R.T.: 6.354 min
Delta R.T.: -0.001 min
Response: 5065256
Conc: 1.75 ng/ml

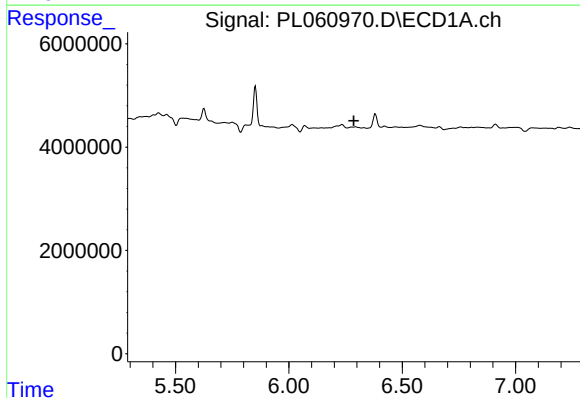


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.286 min
Response: 0
Conc: N.D.

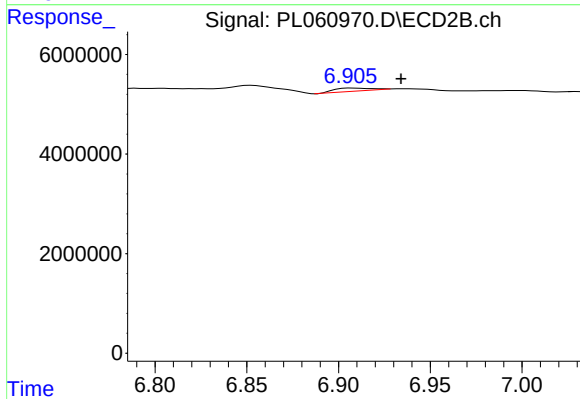

#15 Endosulfan II


R.T.: 6.907 min
Delta R.T.: -0.027 min
Response: 813337
Conc: 0.32 ng/ml

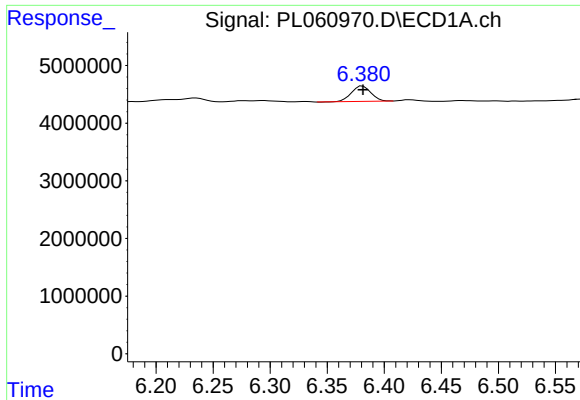

#17 4,4'-DDT


R.T.: 6.381 min
Delta R.T.: 0.000 min
Response: 3137053
Conc: 2.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

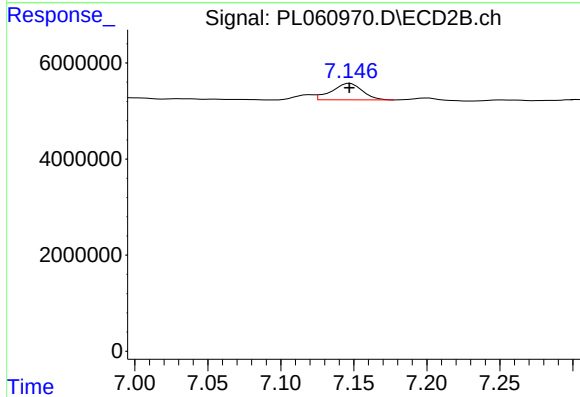


#17 4,4'-DDT

R.T.: 7.148 min
Delta R.T.: 0.000 min
Response: 5012682
Conc: 2.18 ng/ml

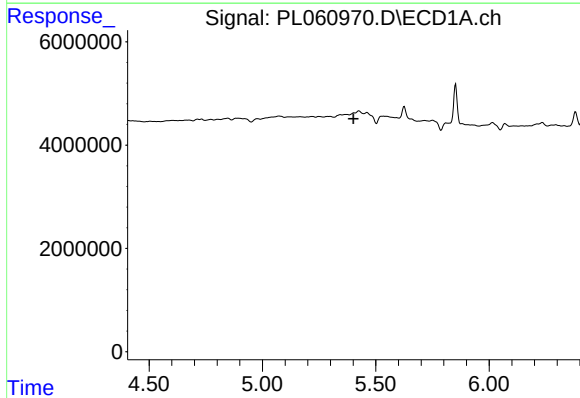


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.402 min
Response: 0
Conc: N.D.

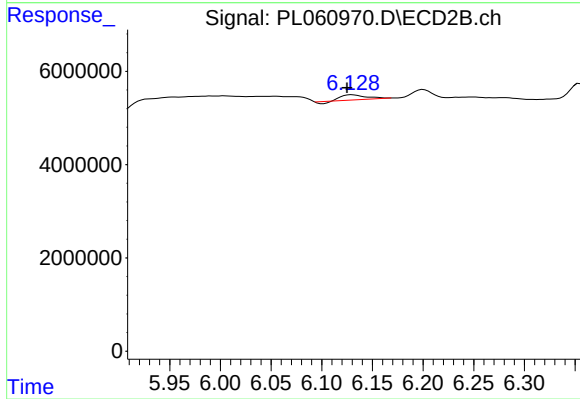

#25 Chlordane-3


R.T.: 6.130 min
Delta R.T.: 0.005 min
Response: 1679095
Conc: 4.20 ng/ml

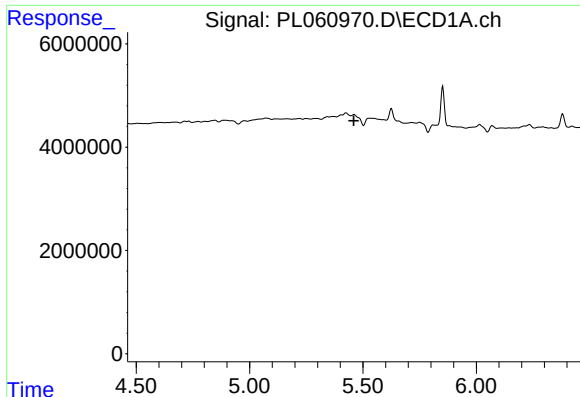

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.460 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

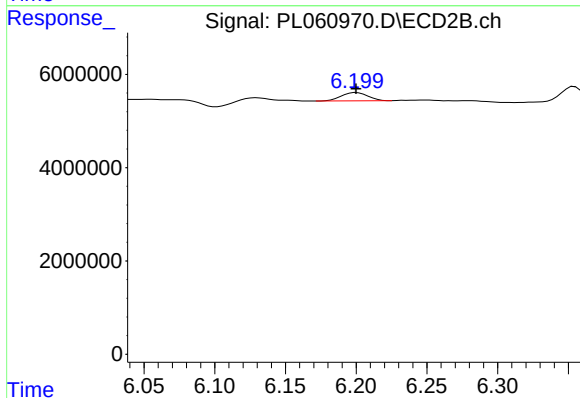


#26 Chlordane-4

R.T.: 6.200 min
Delta R.T.: 0.000 min
Response: 2314115
Conc: 4.81 ng/ml

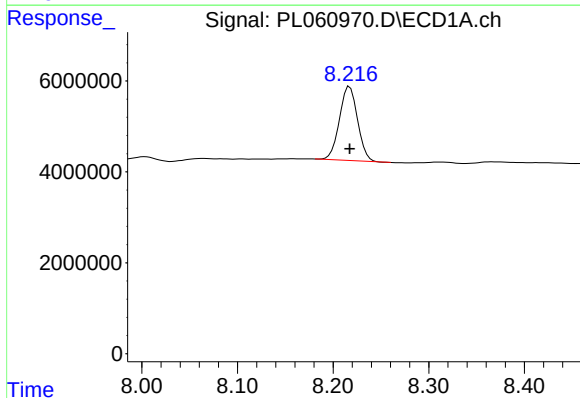

#28 Decachlorobiphenyl

R.T.: 8.217 min
Delta R.T.: 0.000 min
Response: 21353775
Conc: 12.68 ng/ml

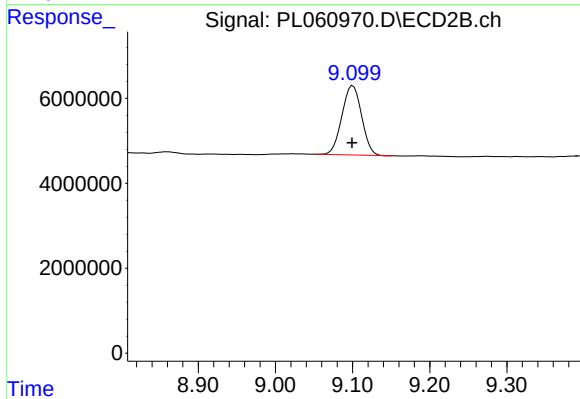

#28 Decachlorobiphenyl

R.T.: 9.100 min
Delta R.T.: 0.001 min
Response: 28904461
Conc: 13.70 ng/ml