

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082521\
 Data File : PL0693461.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Aug 2021 19:41
 Operator : AR\AJ
 Sample : M3528-01MS 10X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 26 03:53:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 21 02:23:37 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.632	5.565	880879	2733306	1.909	1.908
28)	SA Decachlor...	10.398	11.485	1931304	3862128	2.861	3.151
Target Compounds							
4)	MA Heptachlor	6.148f	0.000	1164603	0	1.682	N.D. #
7)	B delta-BHC	0.000	7.081f	0	967909	N.D.	0.524 #
9)	A Endosulfan I	7.499f	0.000	755305	0	1.276	N.D. #
16)	A 4,4'-DDD	0.000	9.101	0	683270	N.D.	0.557 #
23)	Chlordane-1	0.000	6.969	0	1608402	N.D.	28.411 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082521\
Data File : PL0693461.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Aug 2021 19:41
Operator : AR\AJ
Sample : M3528-01MS 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 26 03:53:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
Quant Title : GC Extractables
QLast Update : Sat Aug 21 02:23:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

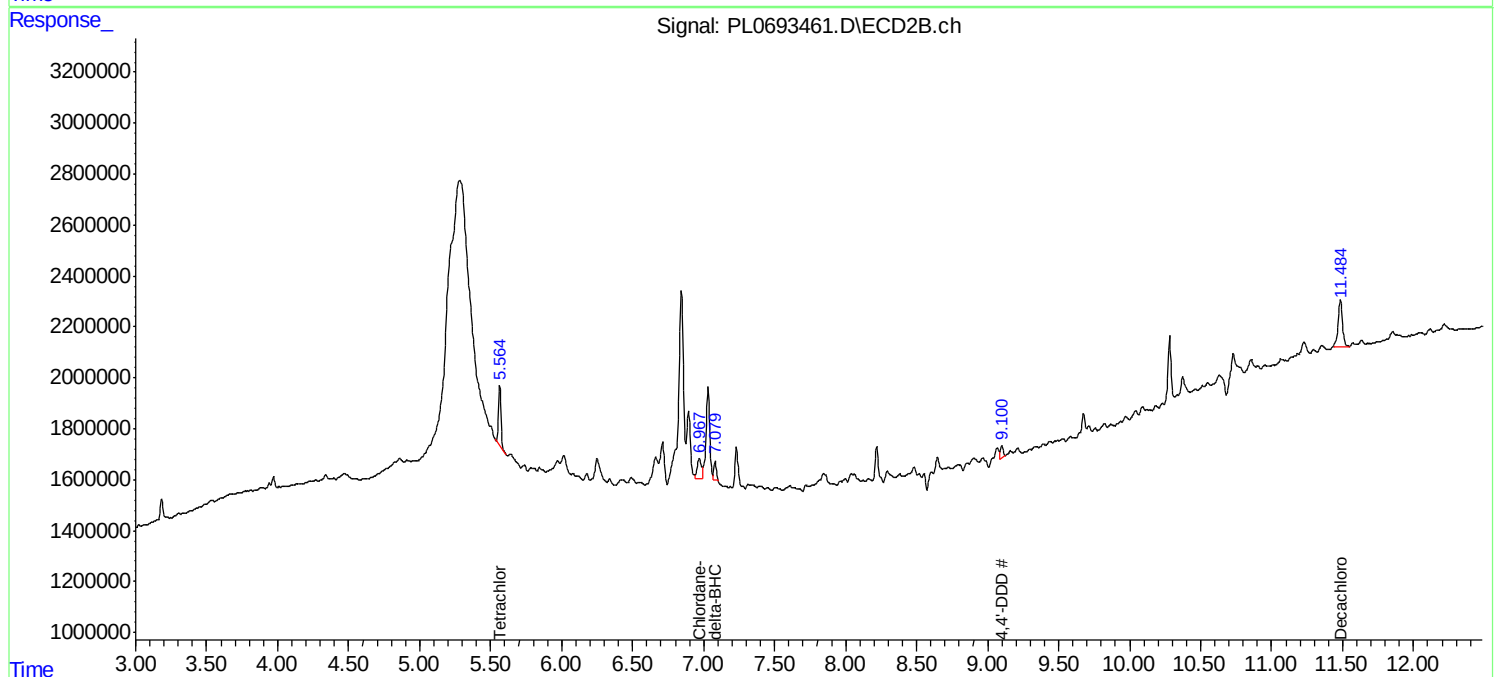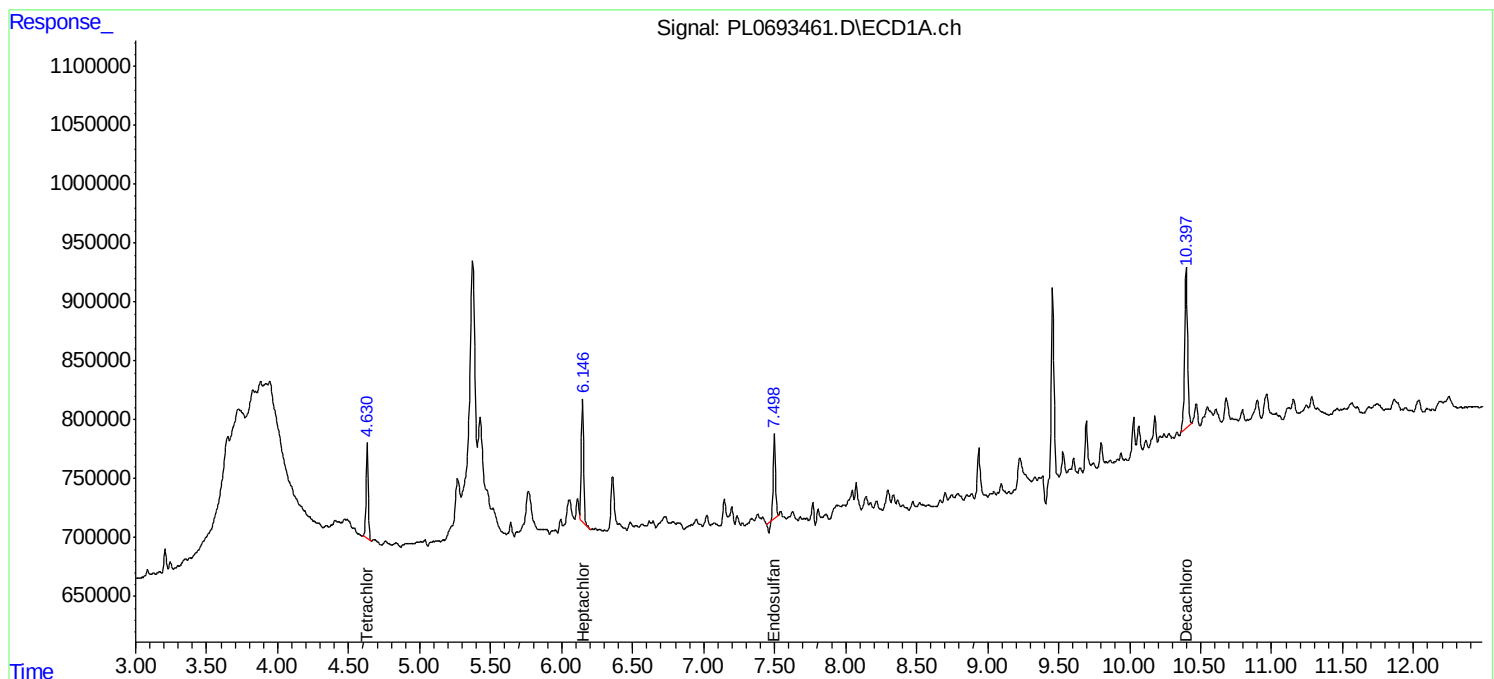


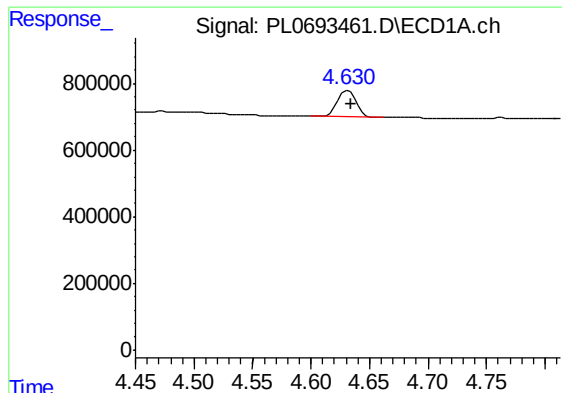

#1 Tetrachloro-m-xylene


R.T.: 4.632 min
Delta R.T.: -0.002 min
Response: 880879
Conc: 1.91 ng/ml

Instrument :
ECD_L
ClientSampleId :

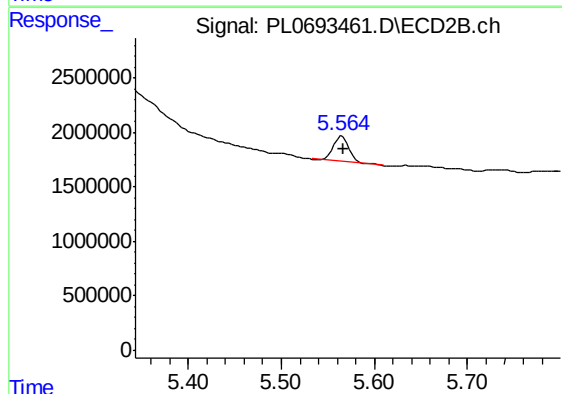


#1 Tetrachloro-m-xylene

R.T.: 5.565 min
Delta R.T.: -0.002 min
Response: 2733306
Conc: 1.91 ng/ml

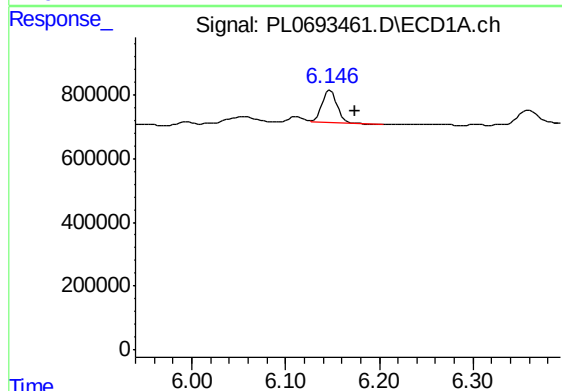


#4 Heptachlor

R.T.: 6.148 min
Delta R.T.: -0.026 min
Response: 1164603
Conc: 1.68 ng/ml

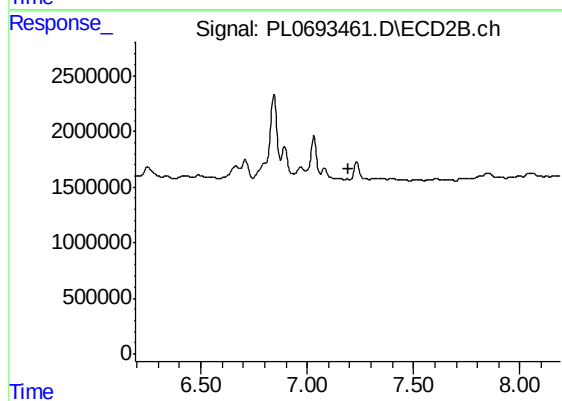

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 7.193 min
Response: 0
Conc: N.D.

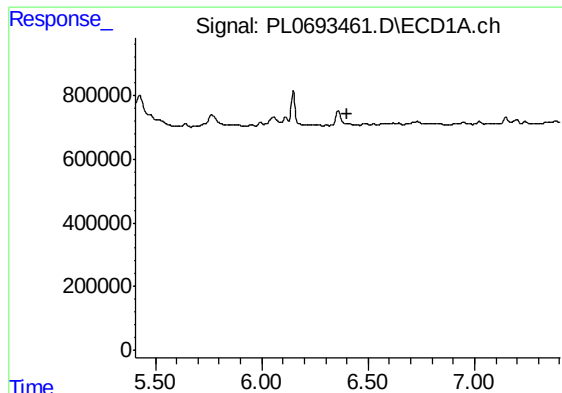

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.404 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

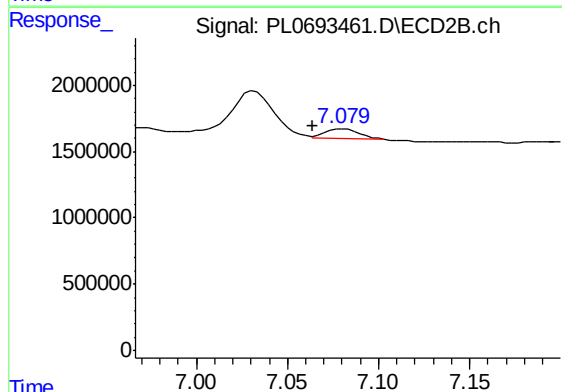


#7 delta-BHC

R.T.: 7.081 min
Delta R.T.: 0.017 min
Response: 967909
Conc: 0.52 ng/ml

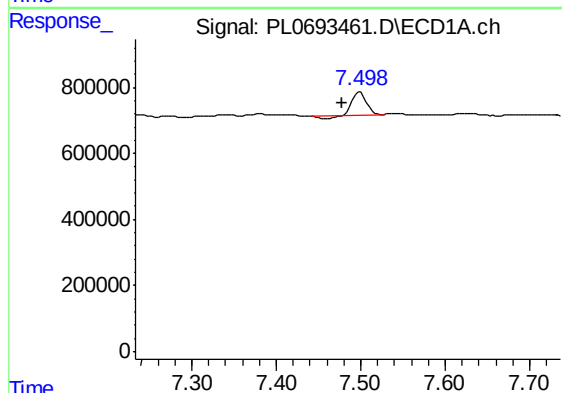


#9 Endosulfan I

R.T.: 7.499 min
Delta R.T.: 0.021 min
Response: 755305
Conc: 1.28 ng/ml

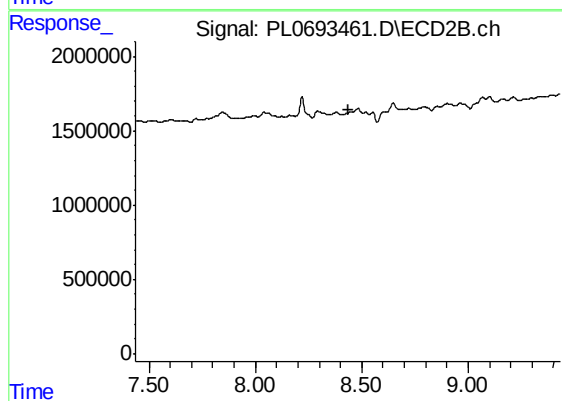

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 8.436 min
Response: 0
Conc: N.D.

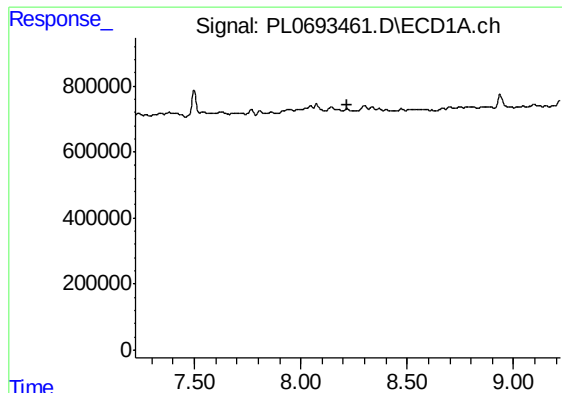

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.220 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

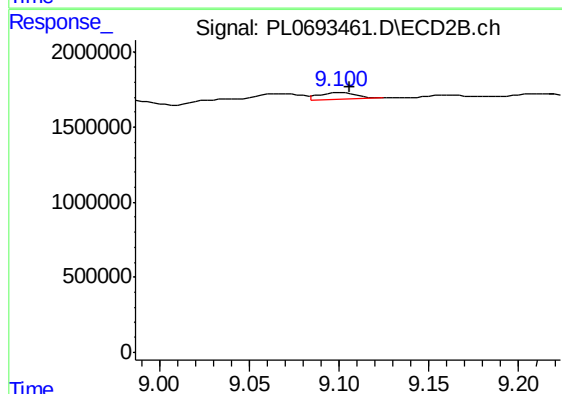


#16 4,4'-DDD

R.T.: 9.101 min
Delta R.T.: -0.005 min
Response: 683270
Conc: 0.56 ng/ml

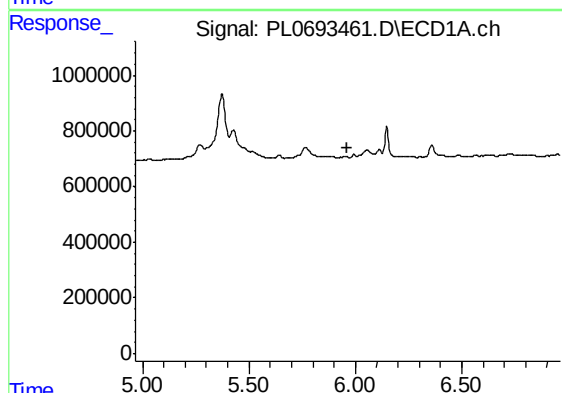


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.964 min
Response: 0
Conc: N.D.

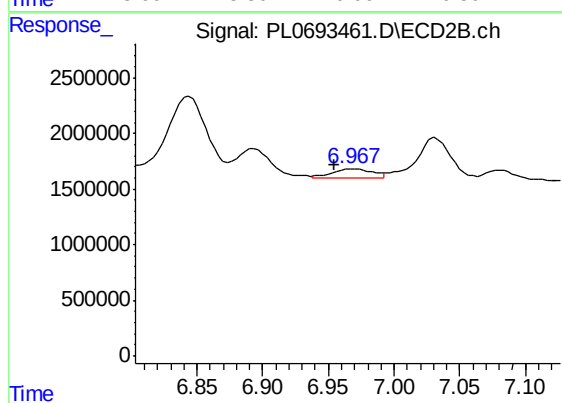

#23 Chlordane-1


R.T.: 6.969 min
Delta R.T.: 0.015 min
Response: 1608402
Conc: 28.41 ng/ml

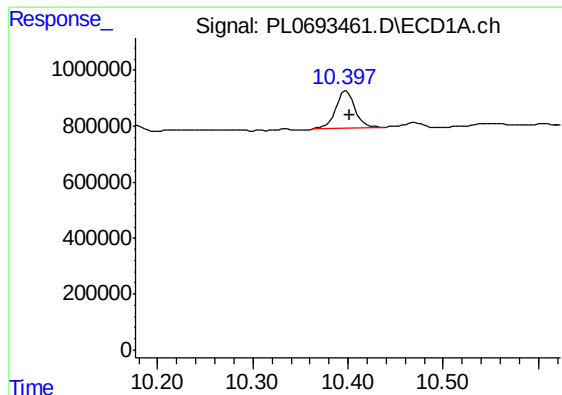

#28 Decachlorobiphenyl

R.T.: 10.398 min
Delta R.T.: -0.003 min
Response: 1931304
Conc: 2.86 ng/ml

Instrument :
ECD_L
ClientSampleId :

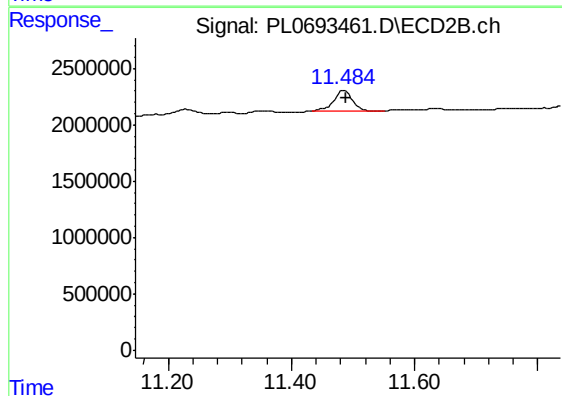

#28 Decachlorobiphenyl

R.T.: 11.485 min
Delta R.T.: -0.003 min
Response: 3862128
Conc: 3.15 ng/ml