

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082521\
 Data File : PL069445.D
 Signal(s): Signal#1: ECD1A.ch Signal#2: ECD2B.ch
 Acq On : 25 Aug 2021 14:38
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 26 03:48:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 21 02:23:37 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.634	5.569	8774531	28188401	19.018	19.678
28) SA Decachlor...	10.402	11.493	12732428	25091632	18.864	20.473
Target Compounds						
4) MA Heptachlor	6.151f	0.000	905475	0	1.307	N.D. #
7) B delta-BHC	0.000	7.035f	0	5099452	N.D.	2.761 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082521\
Data File : PL0693445.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Aug 2021 14:38
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 26 03:48:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
Quant Title : GC Extractables
QLast Update : Sat Aug 21 02:23:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

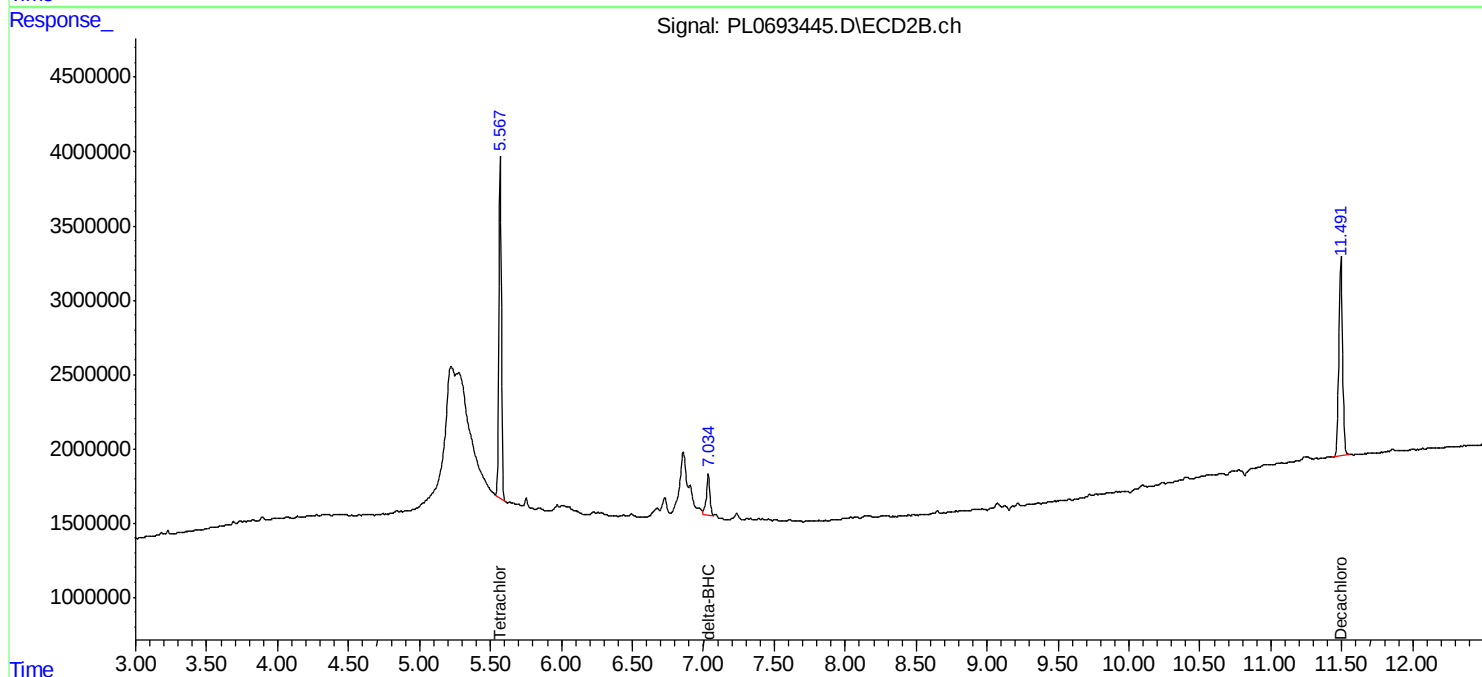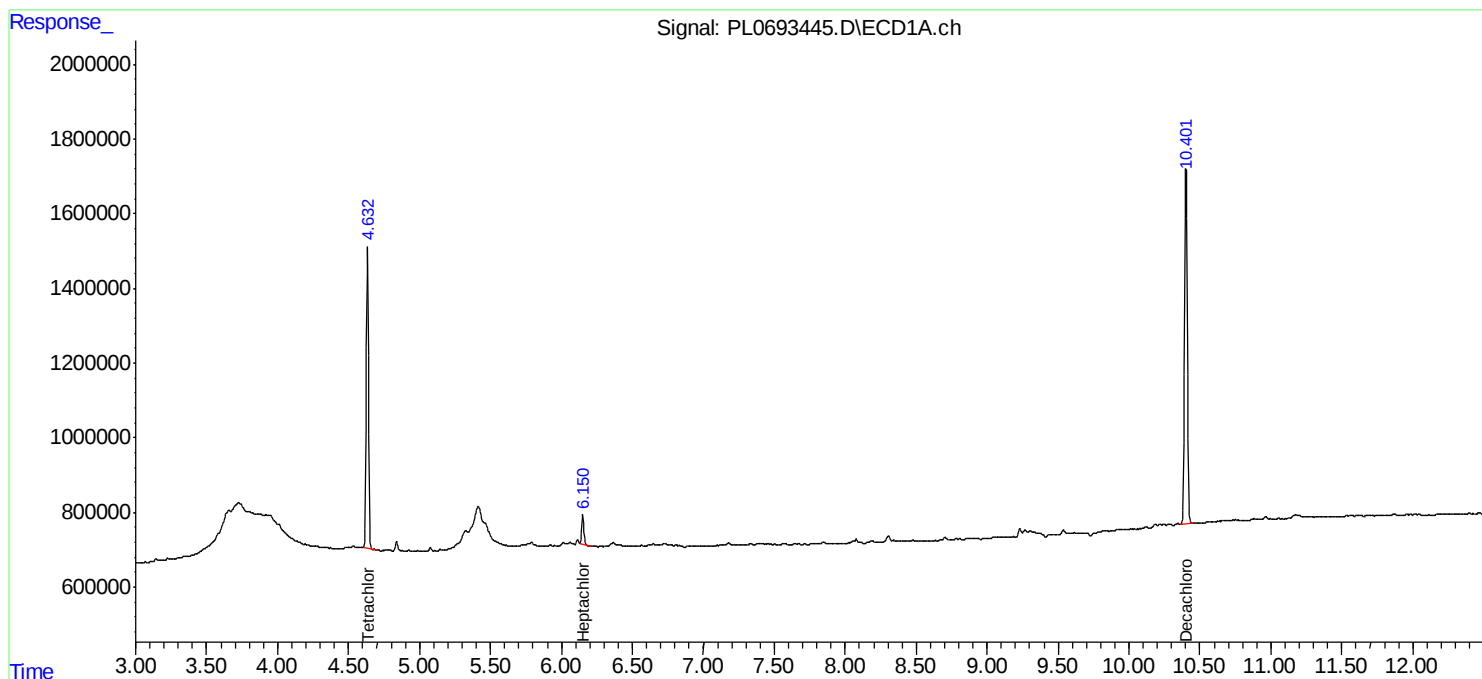


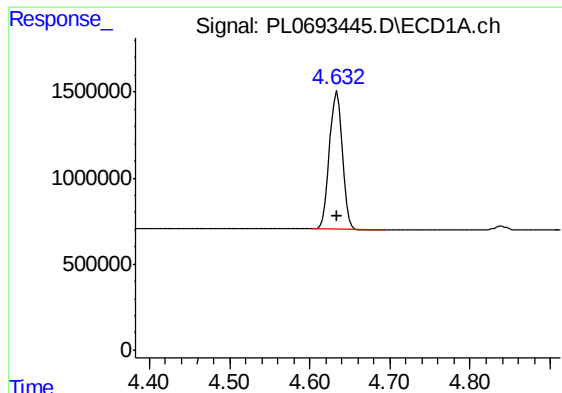

#1 Tetrachloro-m-xylene


R.T.: 4.634 min
Delta R.T.: 0.000 min
Response: 8774531
Conc: 19.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

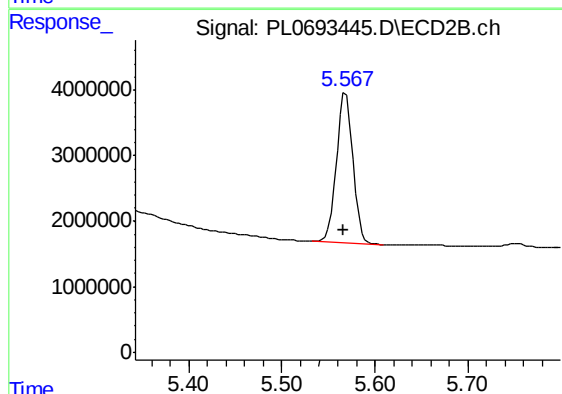


#1 Tetrachloro-m-xylene

R.T.: 5.569 min
Delta R.T.: 0.002 min
Response: 28188401
Conc: 19.68 ng/ml

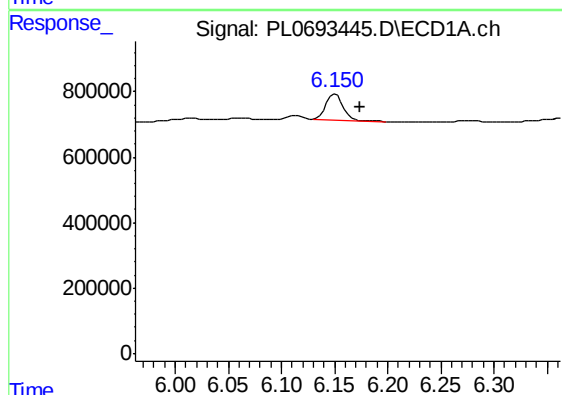


#4 Heptachlor

R.T.: 6.151 min
Delta R.T.: -0.023 min
Response: 905475
Conc: 1.31 ng/ml

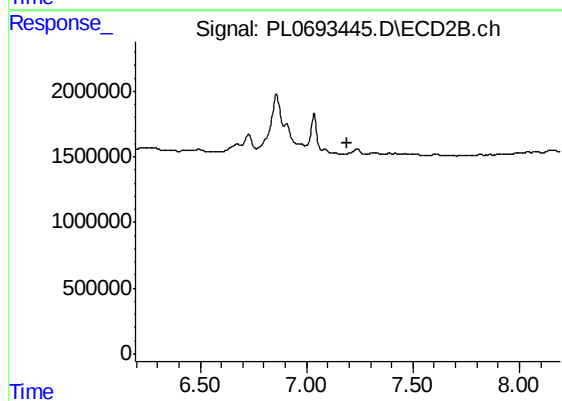

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 7.193 min
Response: 0
Conc: N.D.

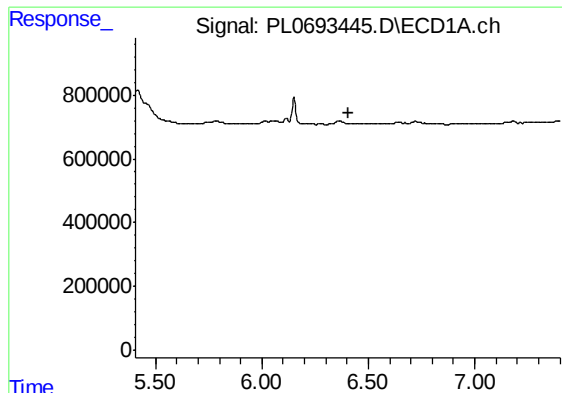

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.404 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

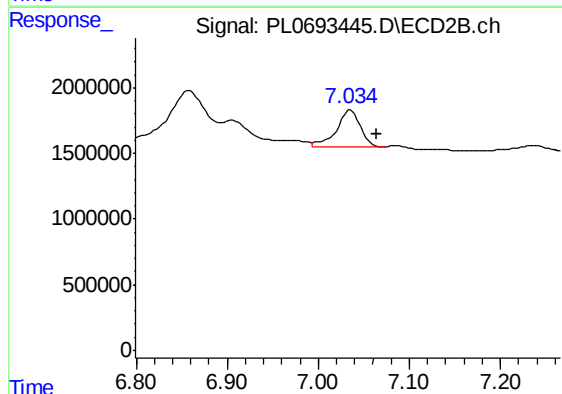


#7 delta-BHC

R.T.: 7.035 min
Delta R.T.: -0.028 min
Response: 5099452
Conc: 2.76 ng/ml

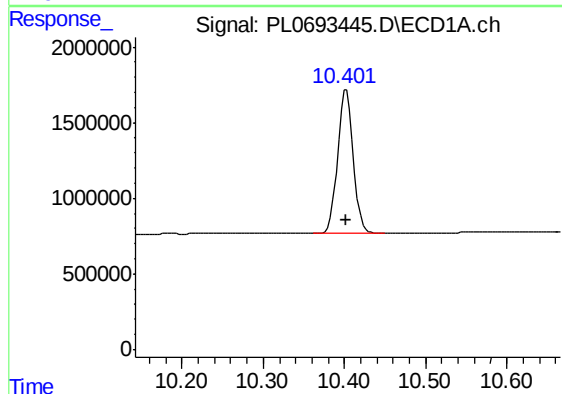

#28 Decachlorobiphenyl

R.T.: 10.402 min
Delta R.T.: 0.000 min
Response: 12732428
Conc: 18.86 ng/ml

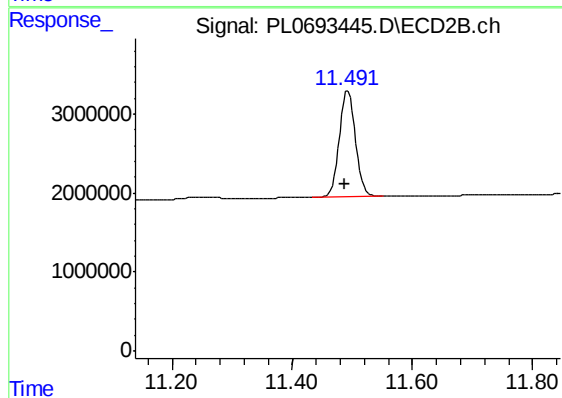

#28 Decachlorobiphenyl

R.T.: 11.493 min
Delta R.T.: 0.005 min
Response: 25091632
Conc: 20.47 ng/ml