

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082521\
 Data File : PL0693455.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Aug 2021 18:01
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 26 03:52:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 21 02:23:37 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.632	5.566	9009584	30288436	19.528	21.144
28)	SA Decachlor...	10.398	11.485	12863889	25939002	19.059	21.165
Target Compounds							
4)	MA Heptachlor	6.148f	0.000	954481	0	1.378	N.D. #
15)	B Endosulfa...	0.000	9.213f	0	743754	N.D.	0.629 #
23)	Chlordane-1	0.000	6.973f	0	1728281	N.D.	30.529 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082521\
Data File : PL0693455.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Aug 2021 18:01
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 26 03:52:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
Quant Title : GC Extractables
QLast Update : Sat Aug 21 02:23:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

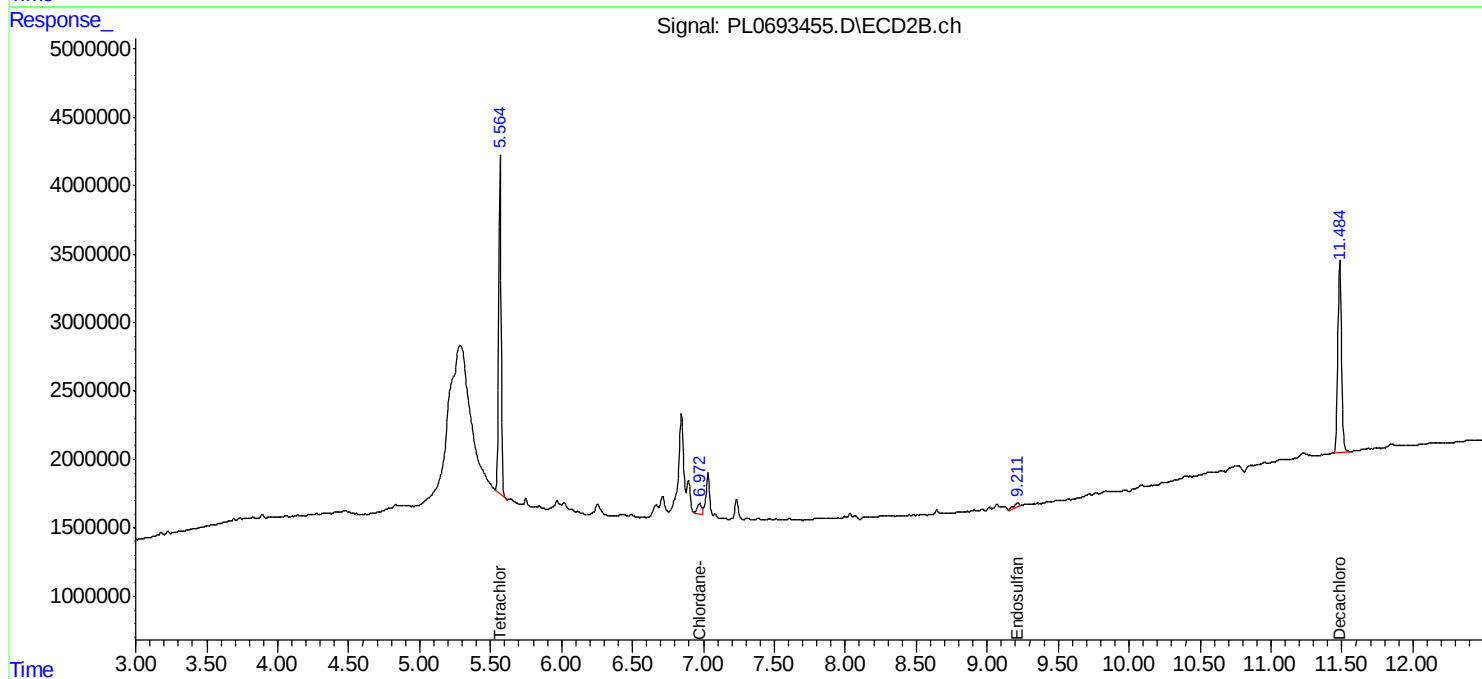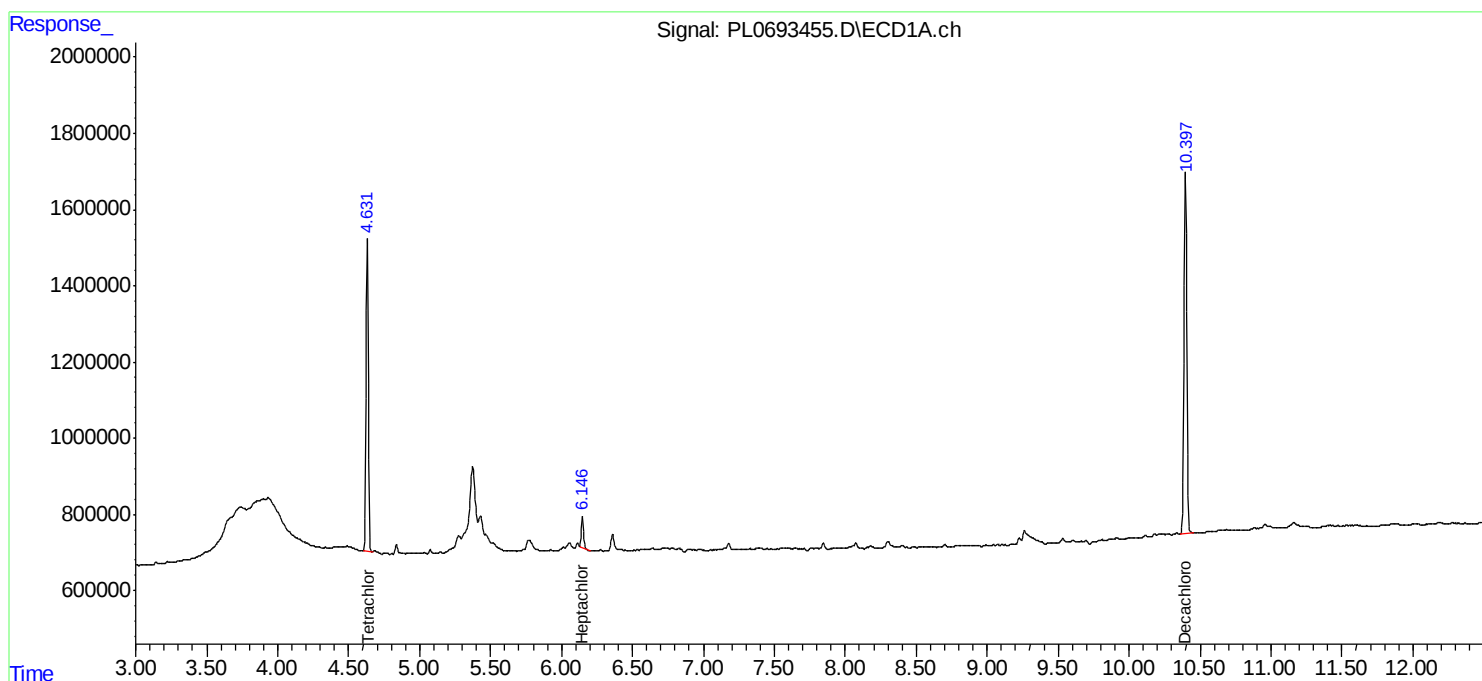


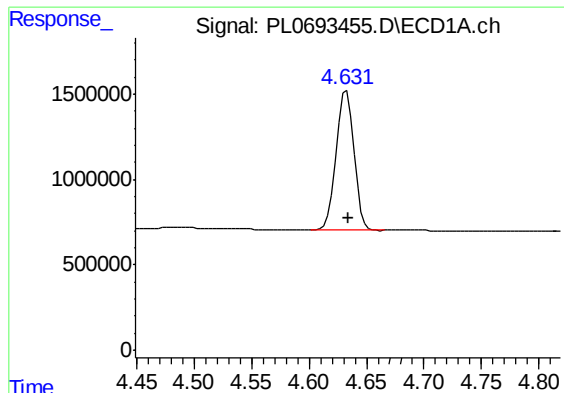

#1 Tetrachloro-m-xylene


R.T.: 4.632 min
Delta R.T.: -0.002 min
Response: 9009584
Conc: 19.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

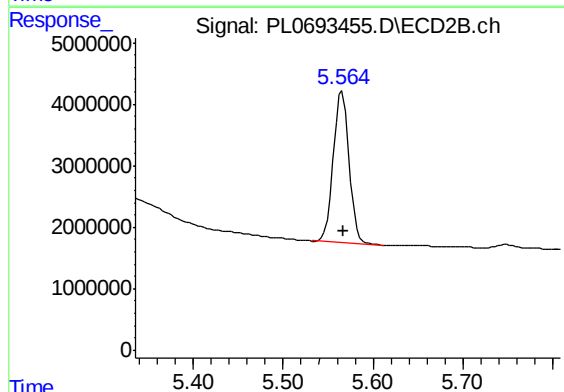


#1 Tetrachloro-m-xylene

R.T.: 5.566 min
Delta R.T.: -0.001 min
Response: 30288436
Conc: 21.14 ng/ml

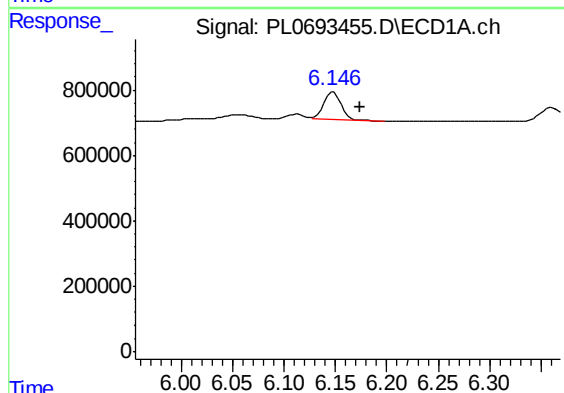


#4 Heptachlor

R.T.: 6.148 min
Delta R.T.: -0.026 min
Response: 954481
Conc: 1.38 ng/ml

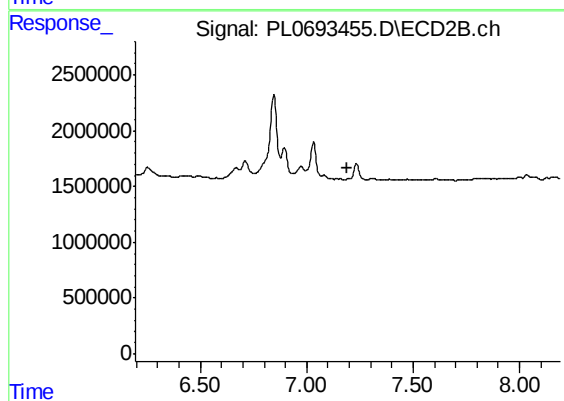

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 7.193 min
Response: 0
Conc: N.D.

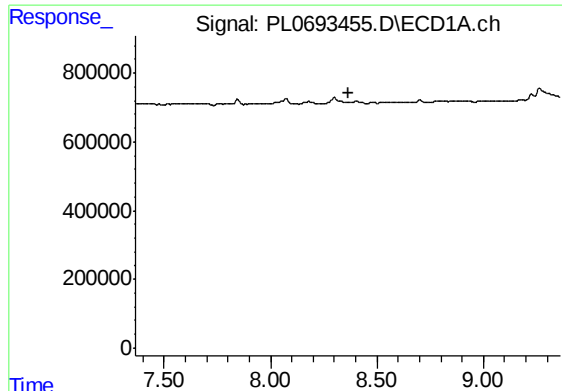

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 8.365 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

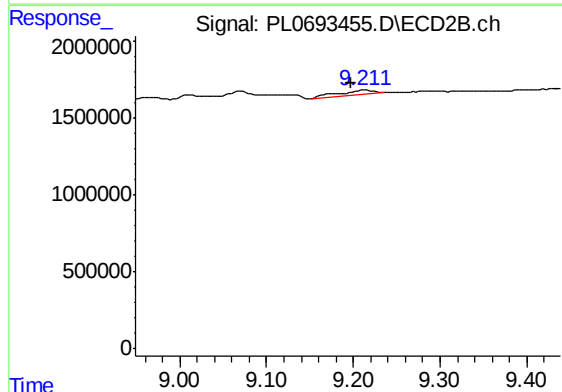


#15 Endosulfan II

R.T.: 9.213 min
Delta R.T.: 0.016 min
Response: 743754
Conc: 0.63 ng/ml

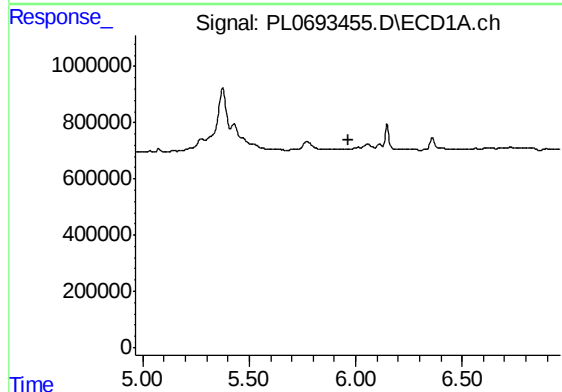


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.964 min
Response: 0
Conc: N.D.

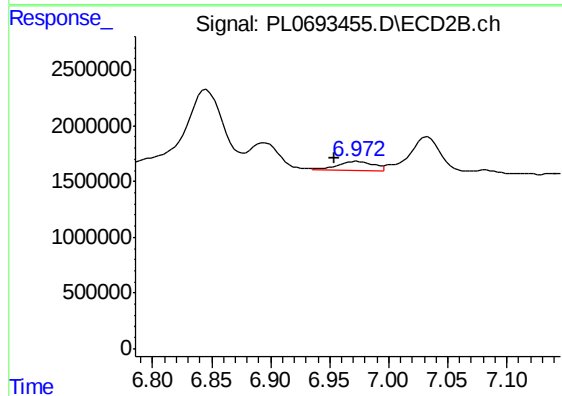

#23 Chlordane-1


R.T.: 6.973 min
Delta R.T.: 0.019 min
Response: 1728281
Conc: 30.53 ng/ml

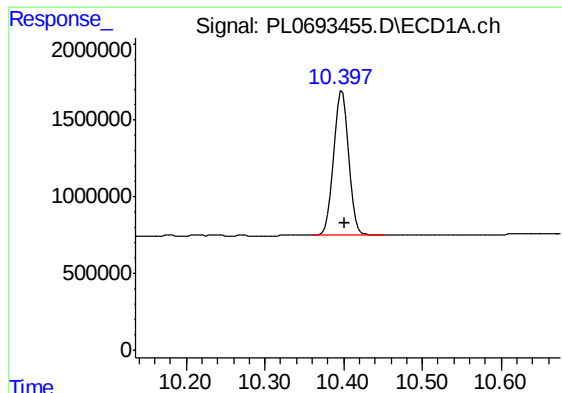

#28 Decachlorobiphenyl

R.T.: 10.398 min
Delta R.T.: -0.003 min
Response: 12863889
Conc: 19.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

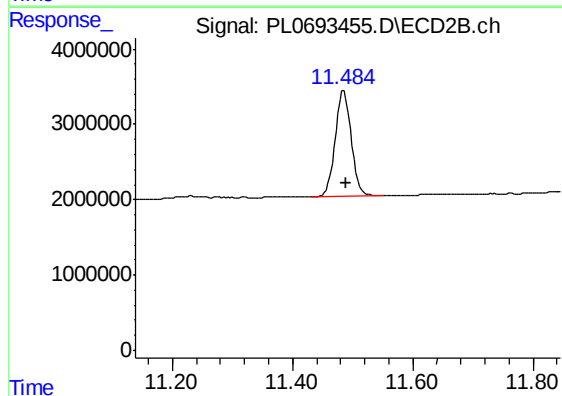

#28 Decachlorobiphenyl

R.T.: 11.485 min
Delta R.T.: -0.003 min
Response: 25939002
Conc: 21.16 ng/ml