

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082521\
 Data File : PL0693463.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Aug 2021 20:14
 Operator : AR\AJ
 Sample : M3528-01 10X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PT-3-082421RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 26 03:54:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 21 02:23:37 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.631	5.565	883087	2823861	1.914	1.971
28)	SA Decachlor...	10.398	11.485	1860888	3712987	2.757	3.030
Target Compounds							
4)	MA Heptachlor	6.147f	0.000	1180529	0	1.705	N.D. #
7)	B delta-BHC	0.000	7.080f	0	1062414	N.D.	0.575 #
9)	A Endosulfan I	7.498f	0.000	753676	0	1.273	N.D. #
10)	B gamma-Chl...	0.000	8.292	0	724389	N.D.	0.471 #
16)	A 4,4'-DDD	0.000	9.102	0	751423	N.D.	0.613 #
25)	Chlordane-3	0.000	8.292	0	724389	N.D.	3.383 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082521\
Data File : PL0693463.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Aug 2021 20:14
Operator : AR\AJ
Sample : M3528-01 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
PT-3-082421RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 26 03:54:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
Quant Title : GC Extractables
QLast Update : Sat Aug 21 02:23:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

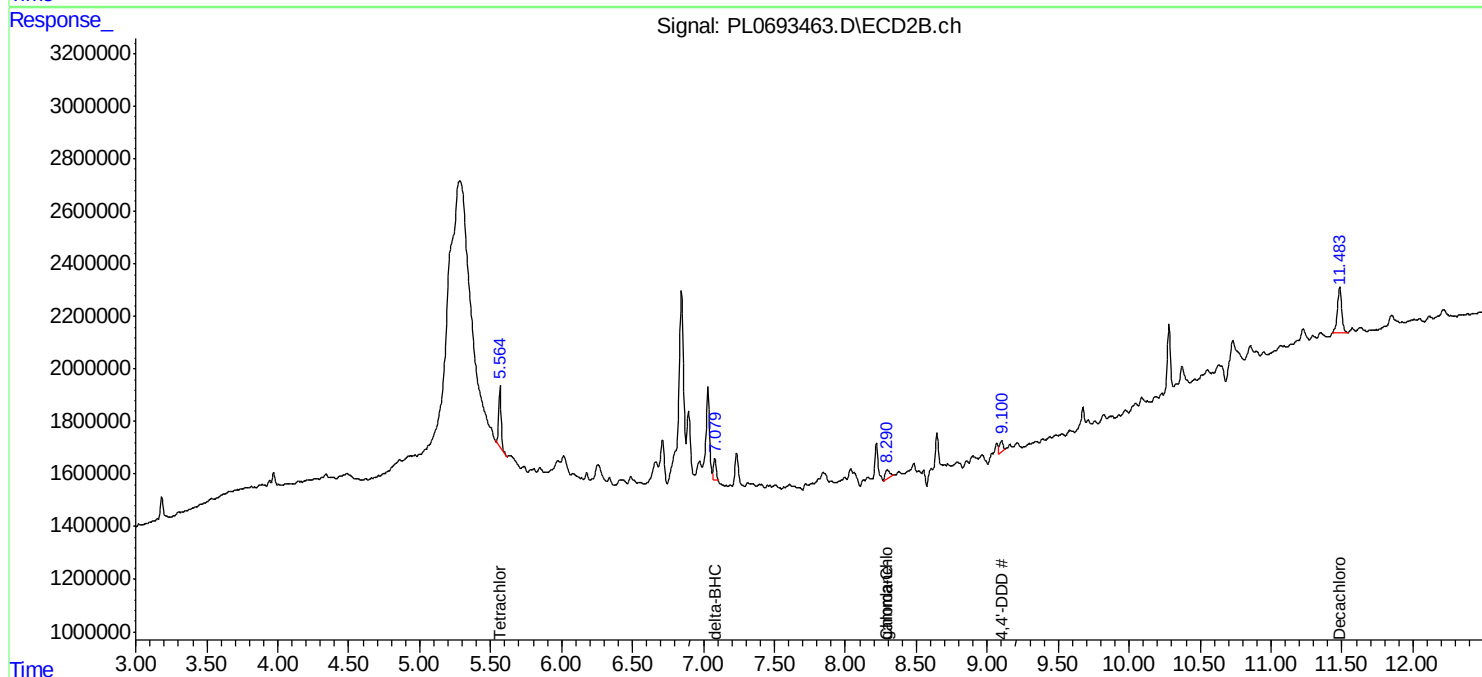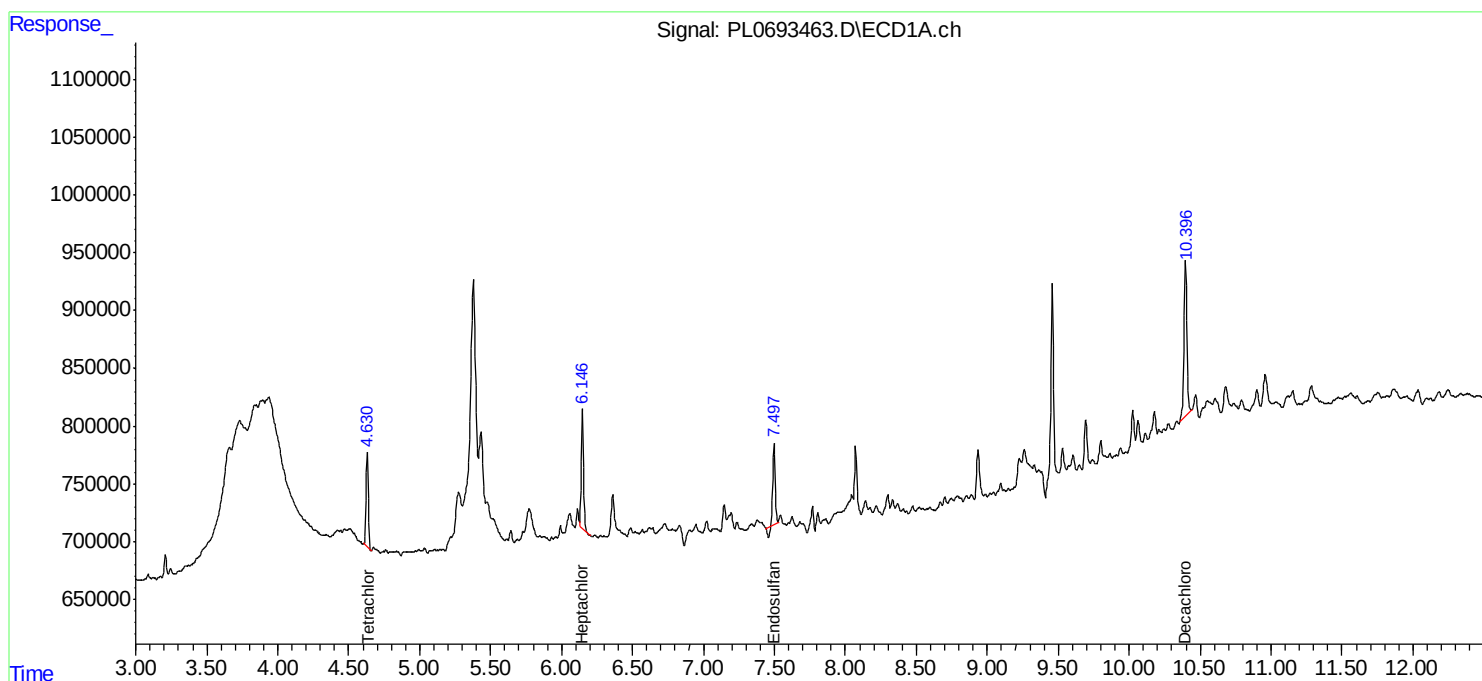


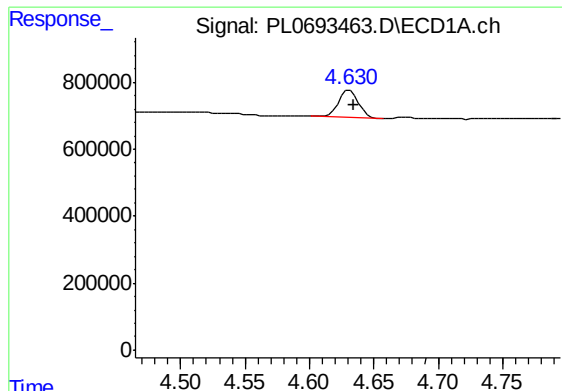

#1 Tetrachloro-m-xylene


R.T.: 4.631 min
Delta R.T.: -0.003 min
Response: 883087
Conc: 1.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
PT-3-082421RE

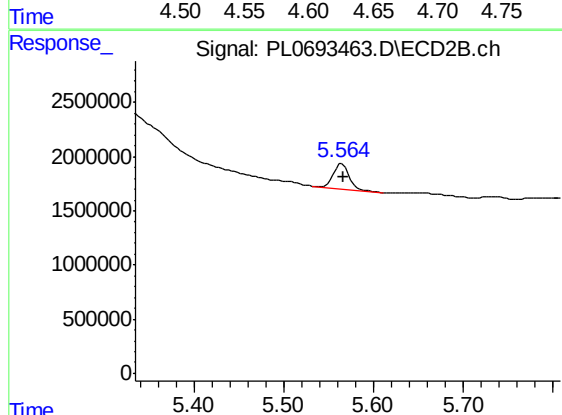


#1 Tetrachloro-m-xylene

R.T.: 5.565 min
Delta R.T.: -0.002 min
Response: 2823861
Conc: 1.97 ng/ml

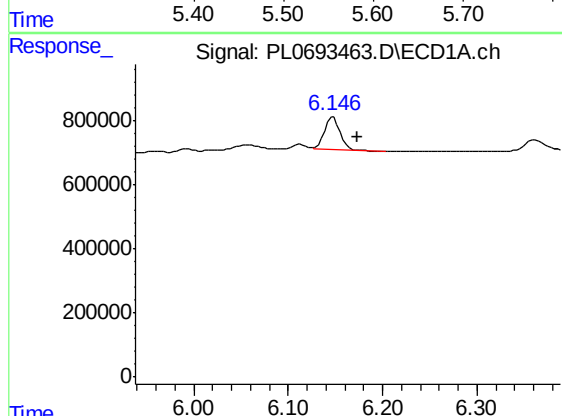


#4 Heptachlor

R.T.: 6.147 min
Delta R.T.: -0.026 min
Response: 1180529
Conc: 1.70 ng/ml

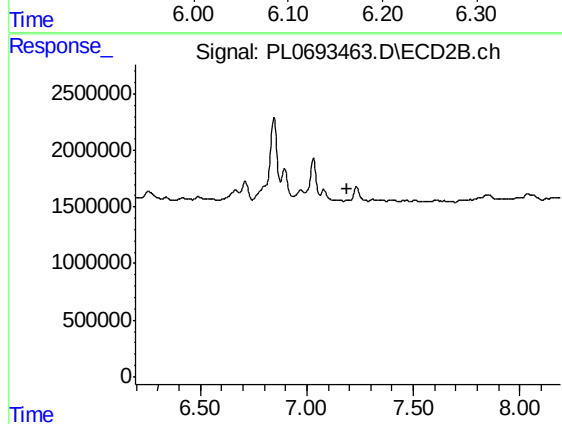

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 7.193 min
Response: 0
Conc: N.D.

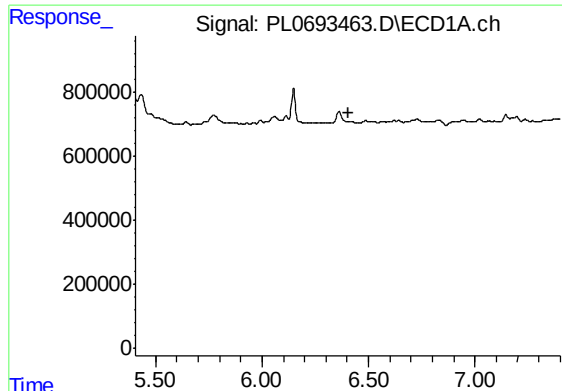

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.404 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PT-3-082421RE

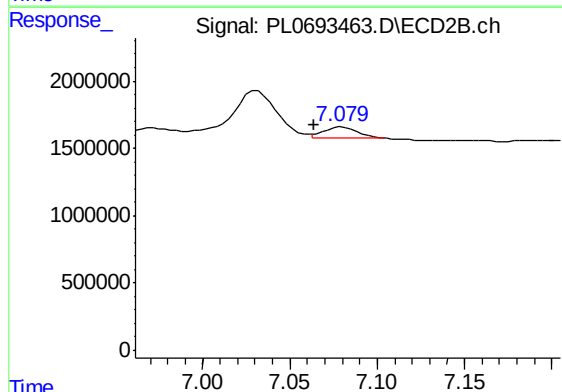


#7 delta-BHC

R.T.: 7.080 min
Delta R.T.: 0.016 min
Response: 1062414
Conc: 0.58 ng/ml

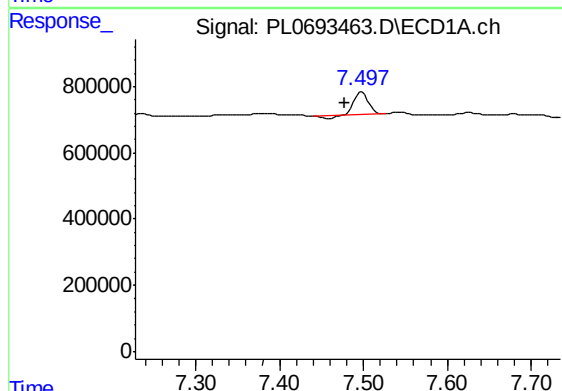


#9 Endosulfan I

R.T.: 7.498 min
Delta R.T.: 0.020 min
Response: 753676
Conc: 1.27 ng/ml

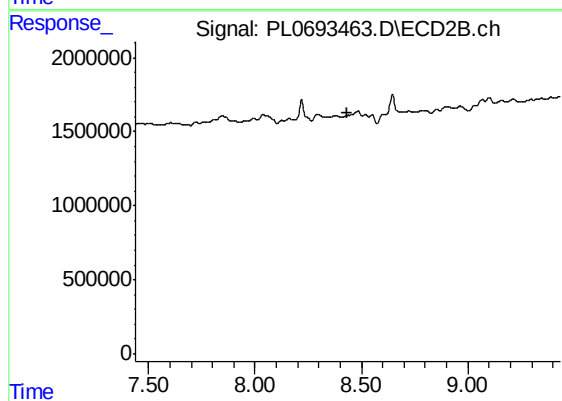

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 8.436 min
Response: 0
Conc: N.D.

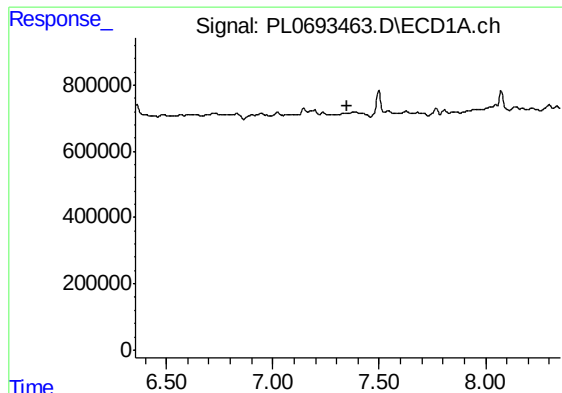

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 7.352 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PT-3-082421RE

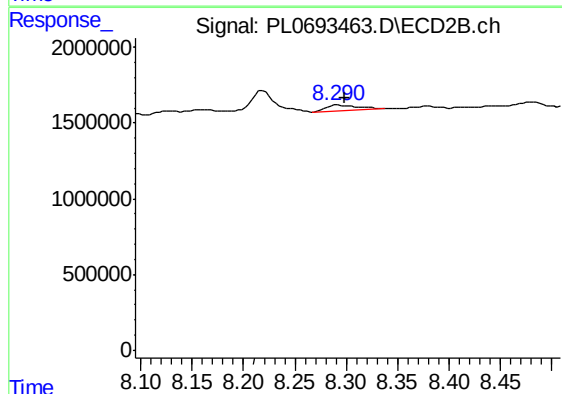


#10 gamma-Chlordane

R.T.: 8.292 min
Delta R.T.: -0.007 min
Response: 724389
Conc: 0.47 ng/ml

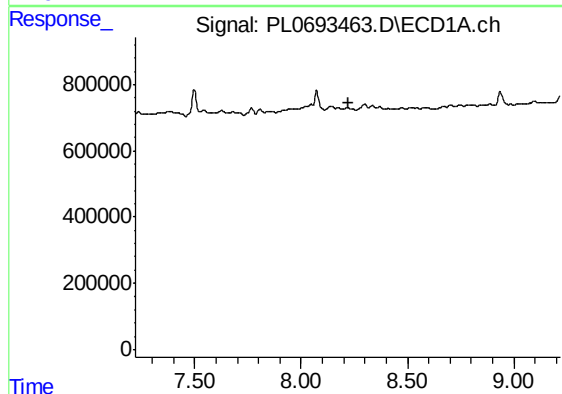


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.220 min
Response: 0
Conc: N.D.

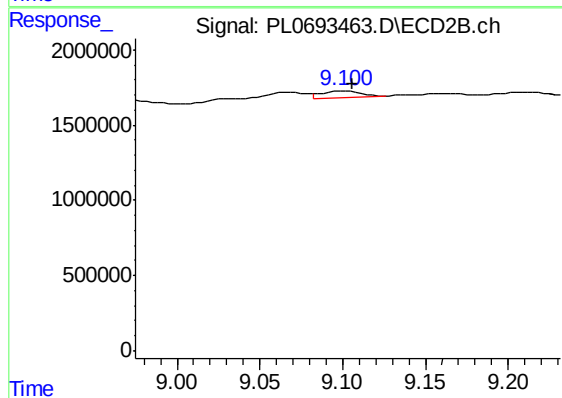

#16 4,4'-DDD


R.T.: 9.102 min
Delta R.T.: -0.005 min
Response: 751423
Conc: 0.61 ng/ml

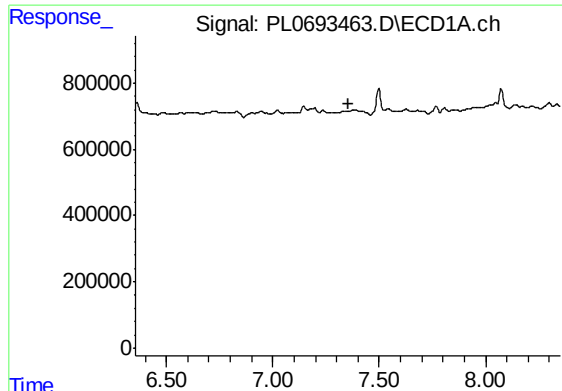

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.354 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PT-3-082421RE

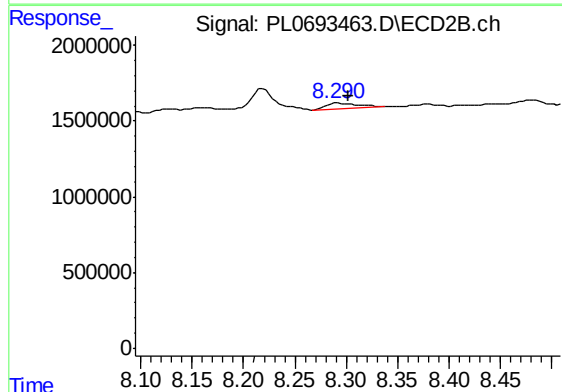


#25 Chlordane-3

R.T.: 8.292 min
Delta R.T.: -0.011 min
Response: 724389
Conc: 3.38 ng/ml

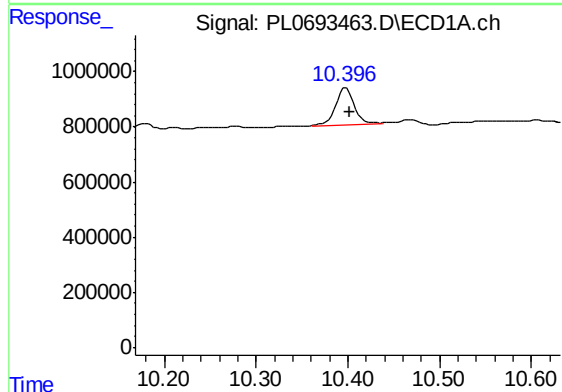

#28 Decachlorobiphenyl

R.T.: 10.398 min
Delta R.T.: -0.004 min
Response: 1860888
Conc: 2.76 ng/ml

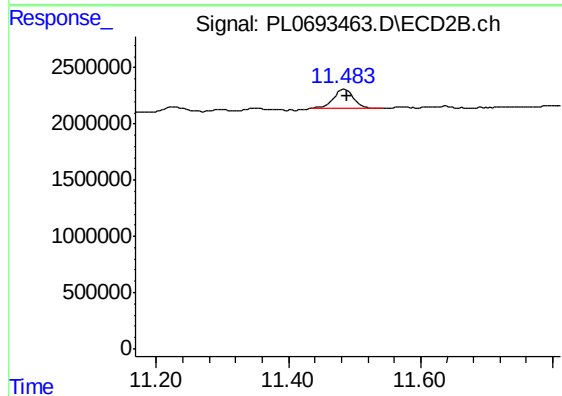

#28 Decachlorobiphenyl

R.T.: 11.485 min
Delta R.T.: -0.003 min
Response: 3712987
Conc: 3.03 ng/ml