

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082620\
 Data File : PL061008.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Aug 2020 14:44
 Operator : DD\AJ
 Sample : L3794-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 26 16:15:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 25 16:59:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.461	4.009	27811242	34957539	15.071	13.450
28)	SA Decachlor...	8.215	9.097	16376322	19481591	9.721	9.233
Target Compounds							
2)	A alpha-BHC	0.000	4.424f	0	2768826	N.D.	0.682 #
9)	A Endosulfan I	5.533f	0.000	5441135	0	2.994	N.D. #
10)	B gamma-Chl...	5.400	6.123	3257093	5355643	1.658	1.724
11)	B alpha-Chl...	5.448	6.197	14830183	9326701	7.599	3.000 #
15)	B Endosulfa...	0.000	6.943	0	3883300	N.D.	1.510 #
23)	Chlordane-1	4.332	0.000	2751908	0	45.071	N.D. #
25)	Chlordane-3	5.400	6.123	3257093	5355643	18.047	13.400 #
26)	Chlordane-4	5.448	6.197	14830183	9326701	99.742	19.401 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082620\
Data File : PL061008.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Aug 2020 14:44
Operator : DD\AJ
Sample : L3794-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 26 16:15:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
Quant Title : GC Extractables
QLast Update : Tue Aug 25 16:59:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

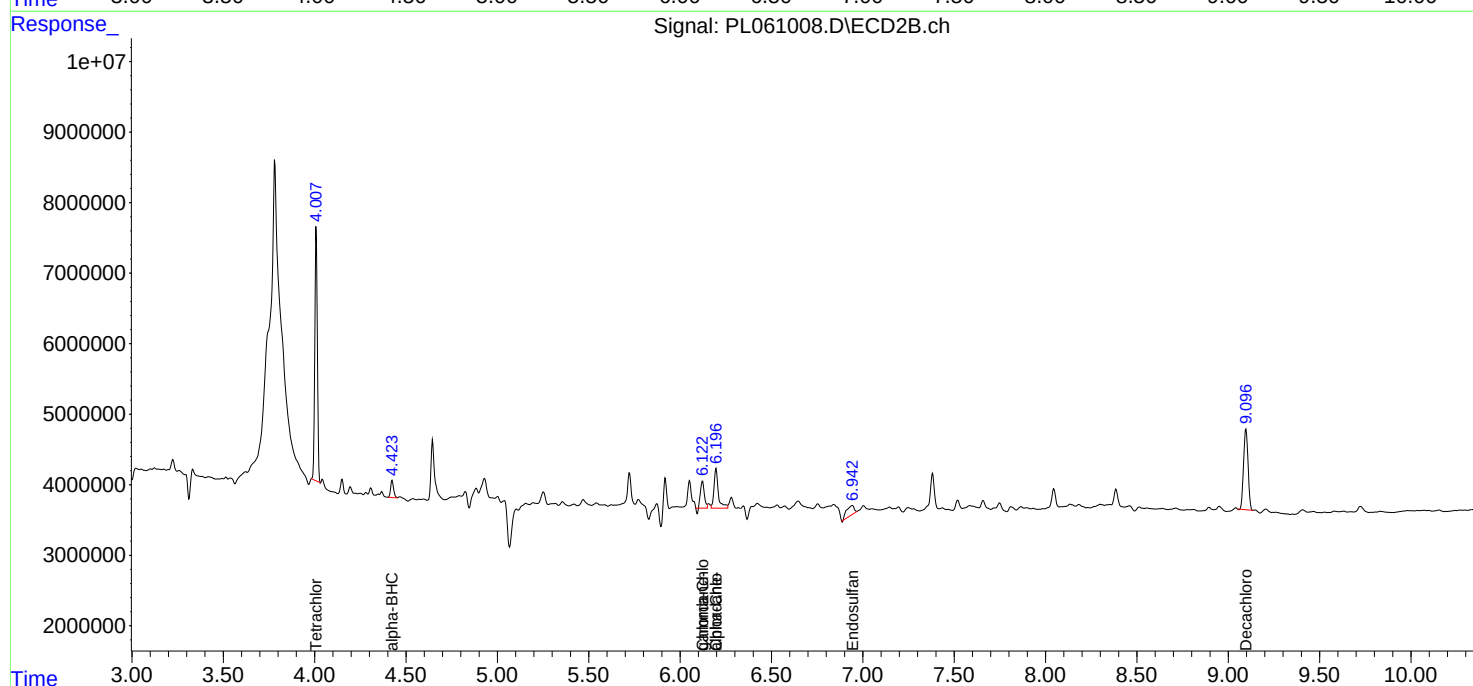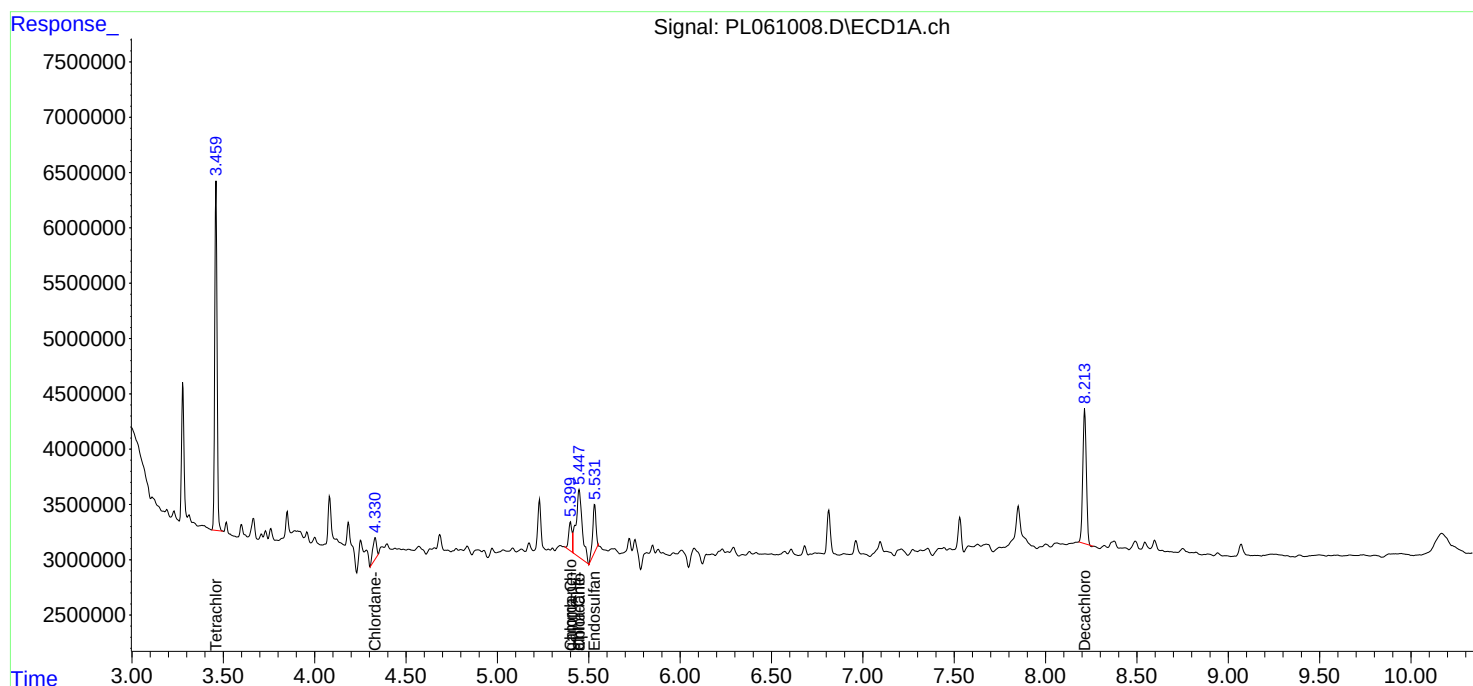


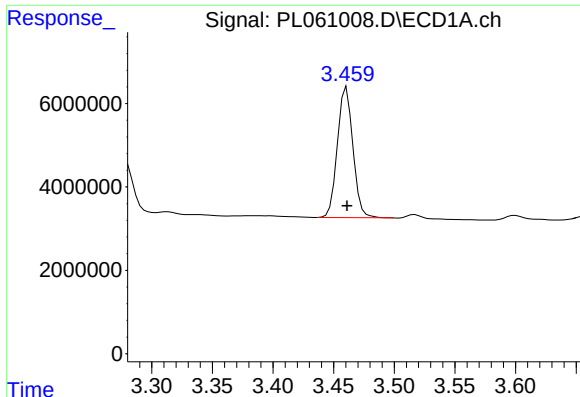

#1 Tetrachloro-m-xylene


R.T.: 3.461 min
Delta R.T.: 0.000 min
Response: 27811242
Conc: 15.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

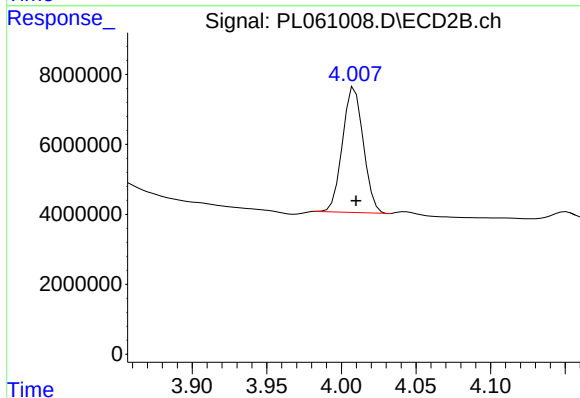


#1 Tetrachloro-m-xylene

R.T.: 4.009 min
Delta R.T.: 0.000 min
Response: 34957539
Conc: 13.45 ng/ml

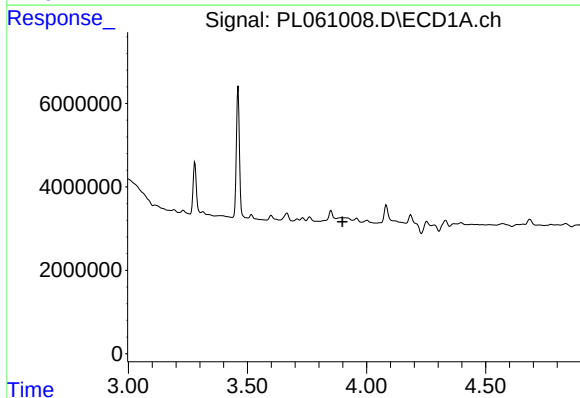


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.898 min
Response: 0
Conc: N.D.

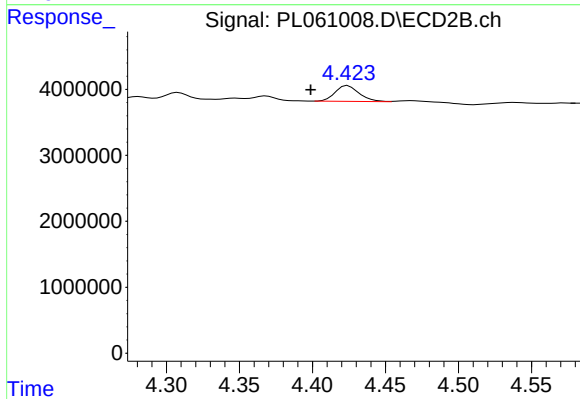

#2 alpha-BHC


R.T.: 4.424 min
Delta R.T.: 0.026 min
Response: 2768826
Conc: 0.68 ng/ml

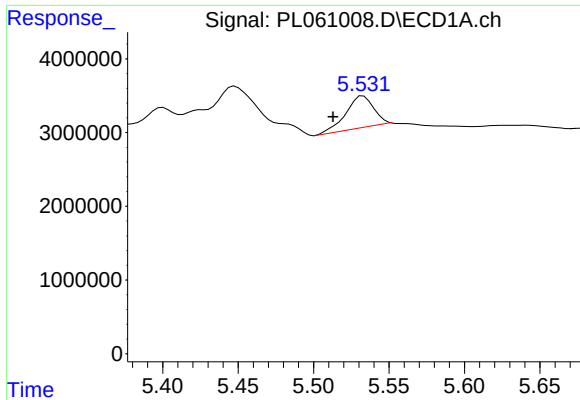

#9 Endosulfan I


R.T.: 5.533 min
Delta R.T.: 0.020 min
Response: 5441135
Conc: 2.99 ng/ml

Instrument :
ECD_L
ClientSampleId :

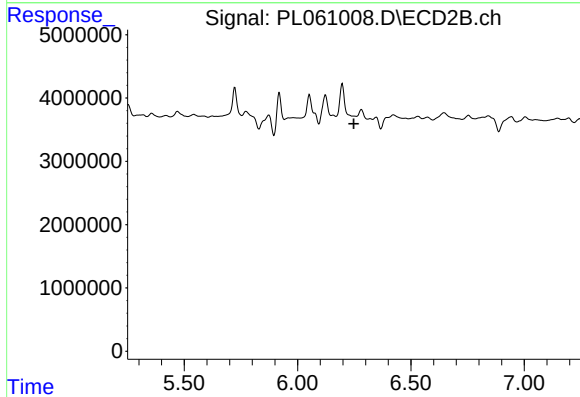


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.248 min
Response: 0
Conc: N.D.

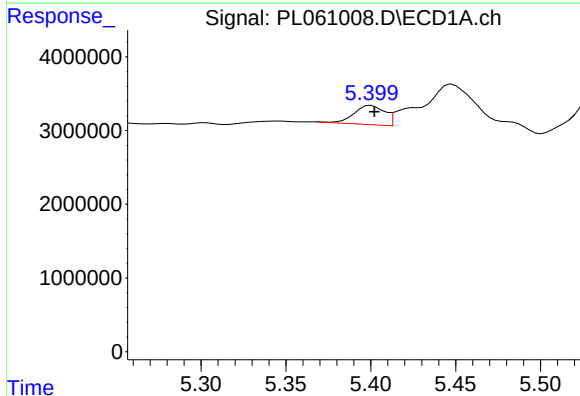


#10 gamma-Chlordane

R.T.: 5.400 min
Delta R.T.: -0.002 min
Response: 3257093
Conc: 1.66 ng/ml

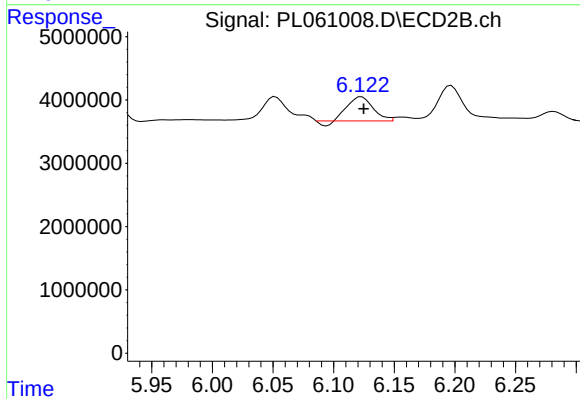

#10 gamma-Chlordane


R.T.: 6.123 min
Delta R.T.: -0.002 min
Response: 5355643
Conc: 1.72 ng/ml

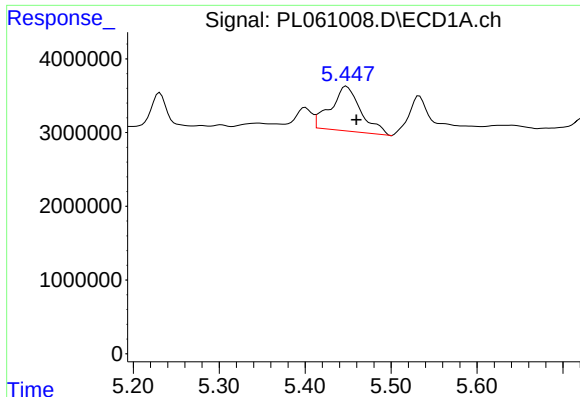

#11 alpha-Chlordane


R.T.: 5.448 min
Delta R.T.: -0.012 min
Response: 14830183
Conc: 7.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

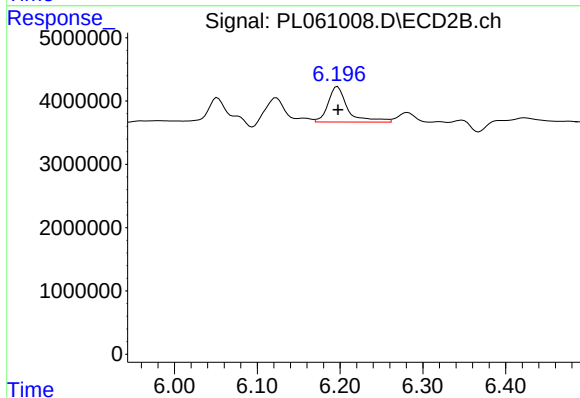


#11 alpha-Chlordane

R.T.: 6.197 min
Delta R.T.: 0.000 min
Response: 9326701
Conc: 3.00 ng/ml

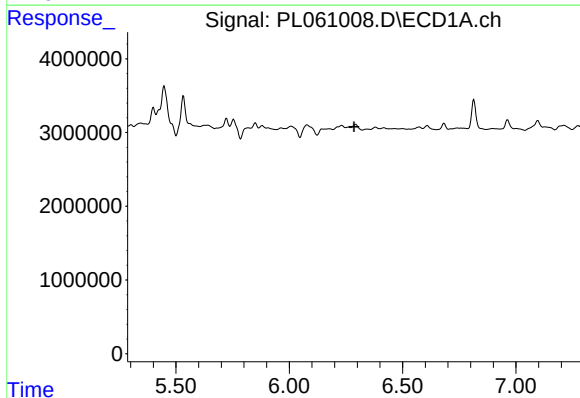


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.286 min
Response: 0
Conc: N.D.

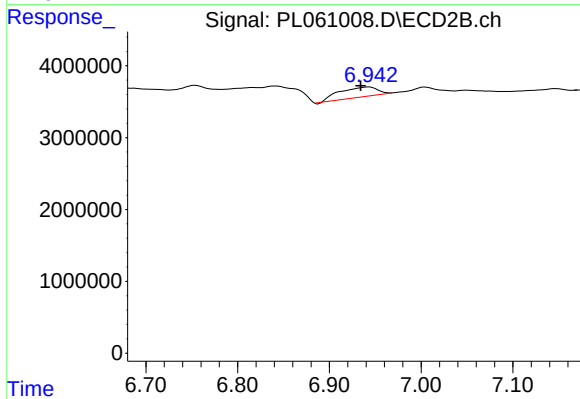

#15 Endosulfan II


R.T.: 6.943 min
Delta R.T.: 0.009 min
Response: 3883300
Conc: 1.51 ng/ml

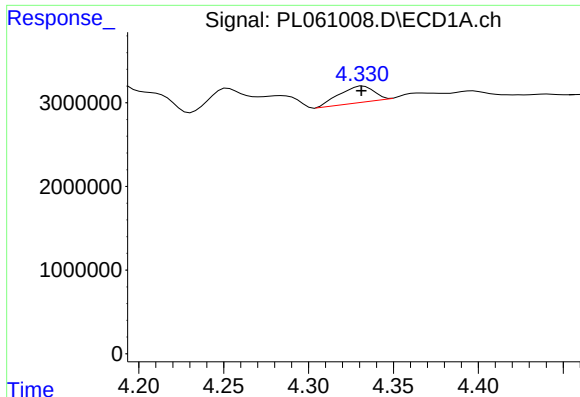

#23 Chlordane-1


R.T.: 4.332 min
Delta R.T.: 0.000 min
Response: 2751908
Conc: 45.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

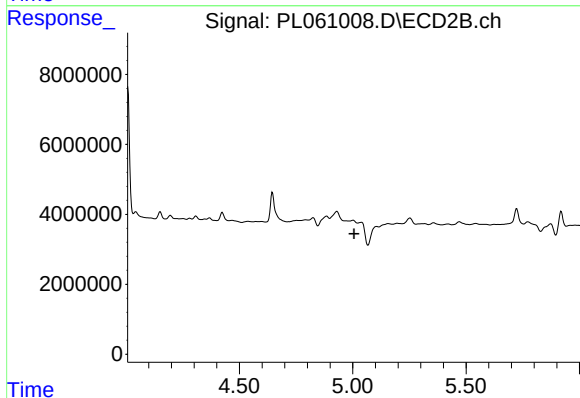


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.007 min
Response: 0
Conc: N.D.

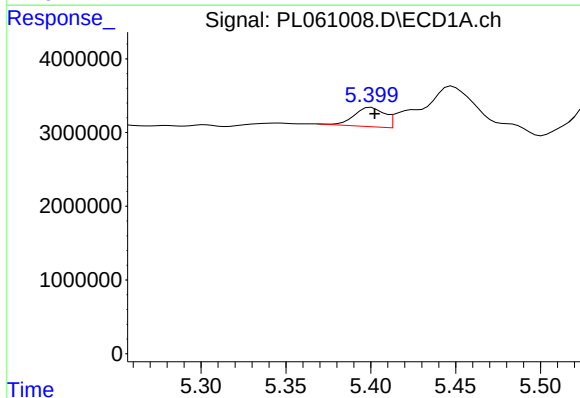


#25 Chlordane-3

R.T.: 5.400 min
Delta R.T.: -0.002 min
Response: 3257093
Conc: 18.05 ng/ml

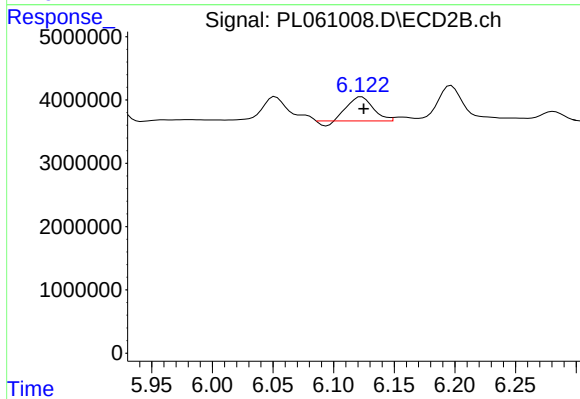

#25 Chlordane-3


R.T.: 6.123 min
Delta R.T.: -0.002 min
Response: 5355643
Conc: 13.40 ng/ml

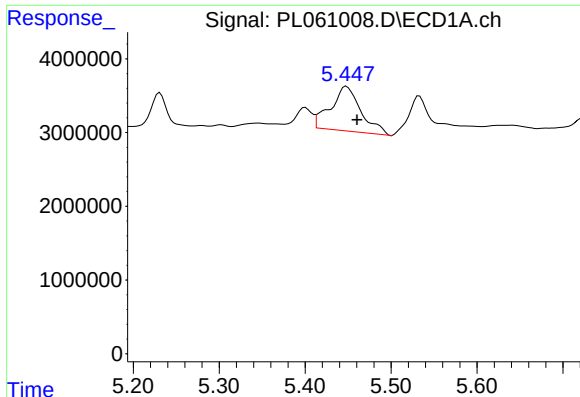

#26 Chlordane-4


R.T.: 5.448 min
Delta R.T.: -0.012 min
Response: 14830183
Conc: 99.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

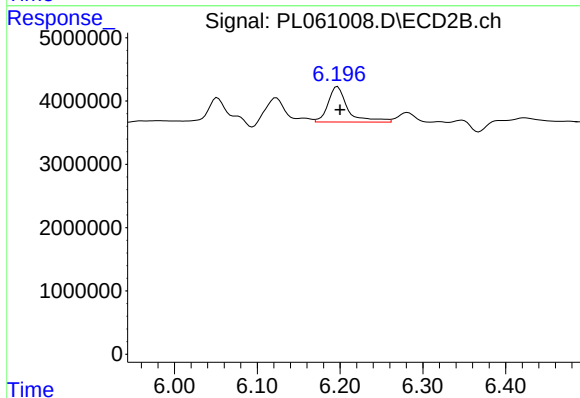


#26 Chlordane-4

R.T.: 6.197 min
Delta R.T.: -0.003 min
Response: 9326701
Conc: 19.40 ng/ml

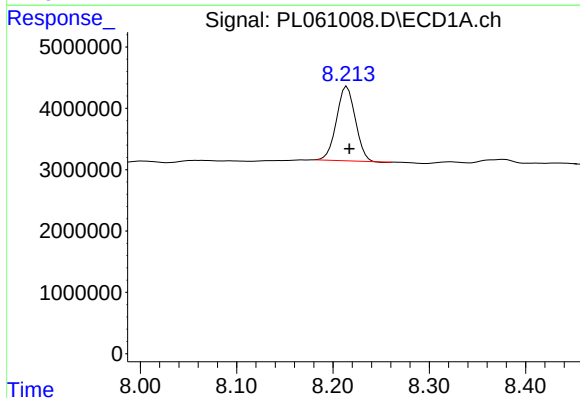

#28 Decachlorobiphenyl

R.T.: 8.215 min
Delta R.T.: -0.003 min
Response: 16376322
Conc: 9.72 ng/ml

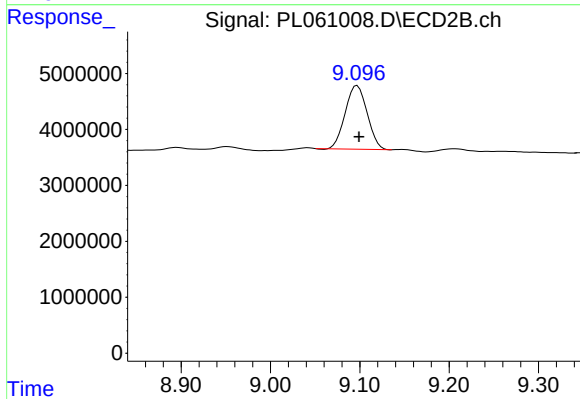

#28 Decachlorobiphenyl

R.T.: 9.097 min
Delta R.T.: -0.002 min
Response: 19481591
Conc: 9.23 ng/ml