

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082620\
 Data File : PL061019.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Aug 2020 17:34
 Operator : DD\AJ
 Sample : L3784-11
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RO-24

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 01:39:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 25 16:59:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.461	4.009	30280145	39679275	16.409	15.267
28) SA Decachlor...	8.216	9.098	25951426	34199552	15.405	16.208
Target Compounds						
15) B Endosulfa...	0.000	6.947	0	2014907	N.D.	0.783 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082620\
Data File : PL061019.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Aug 2020 17:34
Operator : DD\AJ
Sample : L3784-11
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RO-24

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 01:39:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
Quant Title : GC Extractables
QLast Update : Tue Aug 25 16:59:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

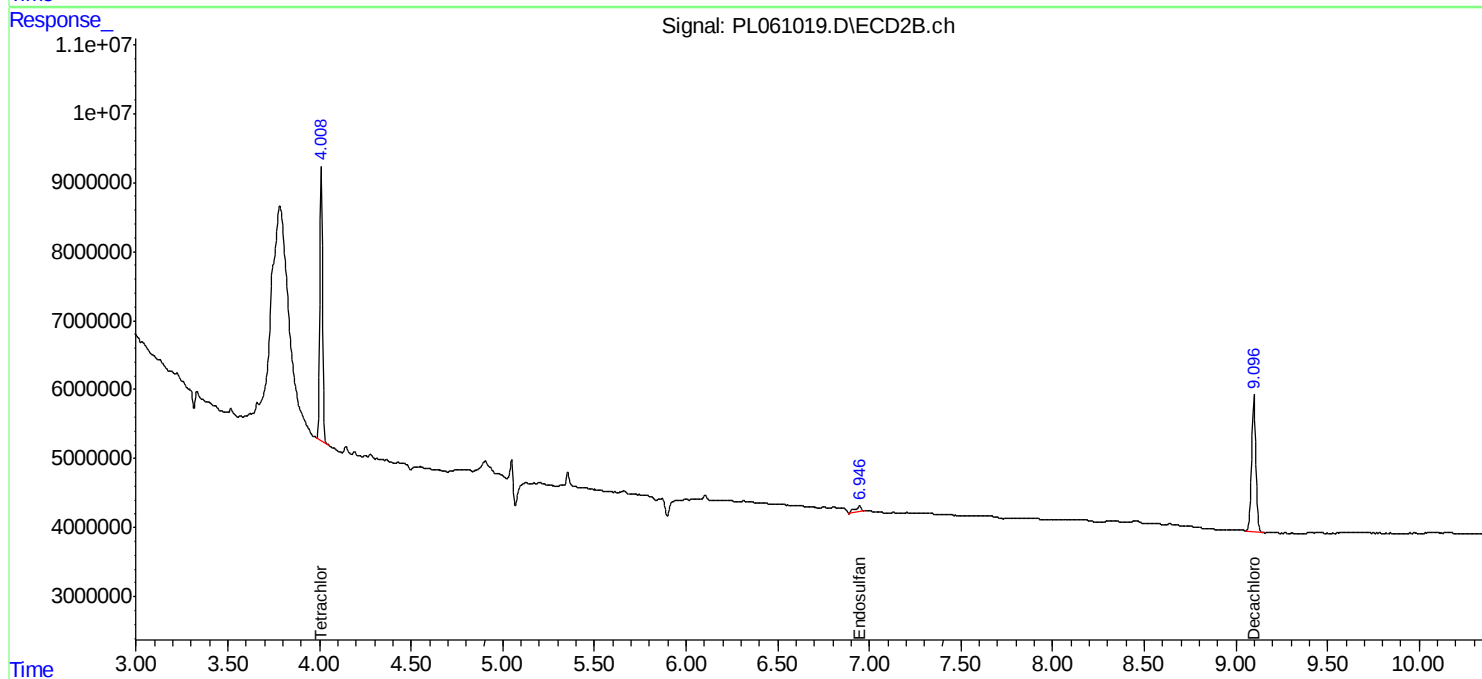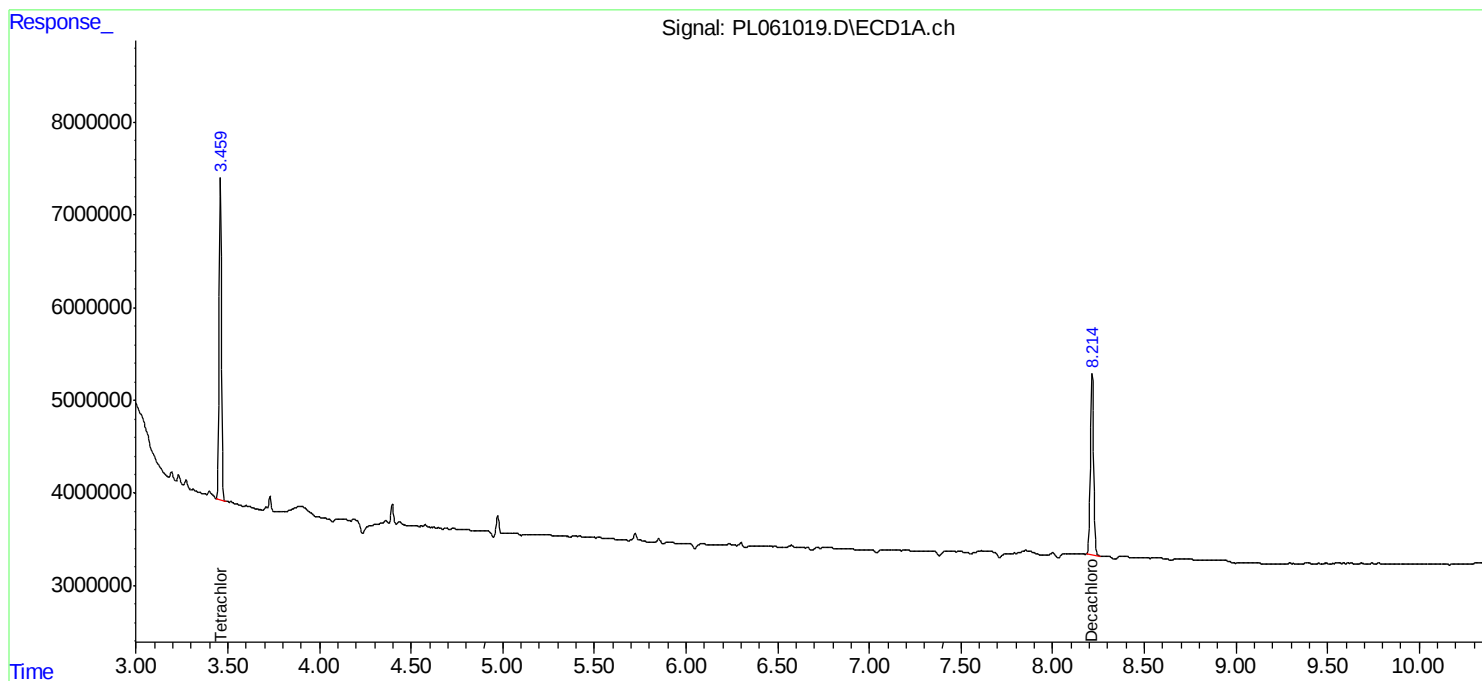


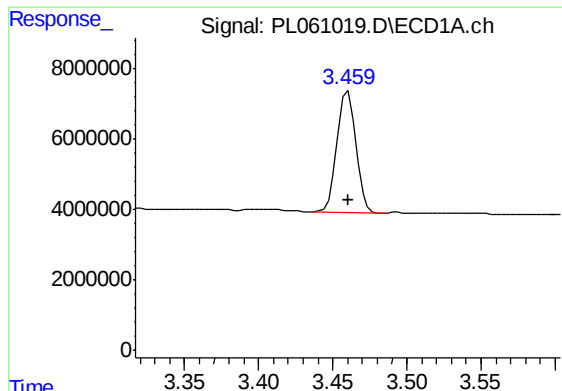

#1 Tetrachloro-m-xylene


R.T.: 3.461 min
Delta R.T.: 0.000 min
Response: 30280145
Conc: 16.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
RO-24

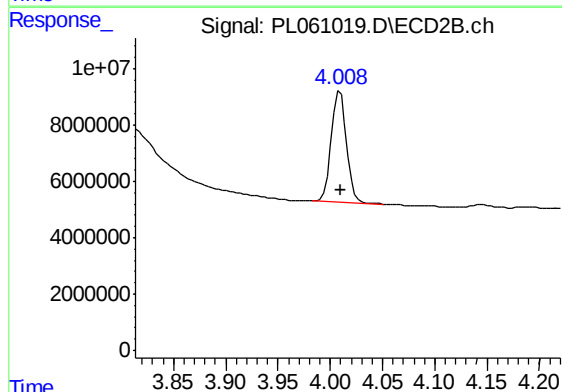


#1 Tetrachloro-m-xylene

R.T.: 4.009 min
Delta R.T.: 0.000 min
Response: 39679275
Conc: 15.27 ng/ml

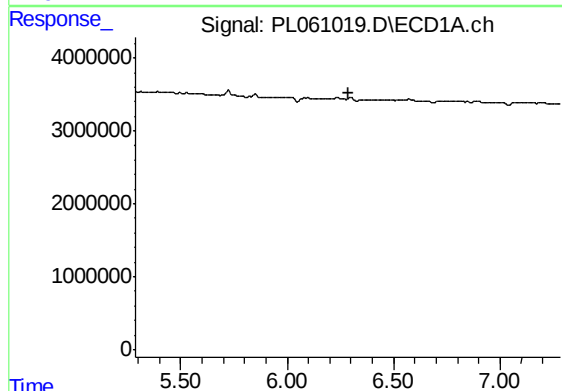


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.286 min
Response: 0
Conc: N.D.

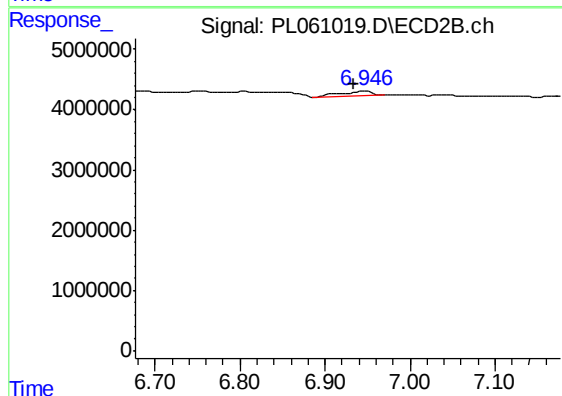

#15 Endosulfan II


R.T.: 6.947 min
Delta R.T.: 0.013 min
Response: 2014907
Conc: 0.78 ng/ml

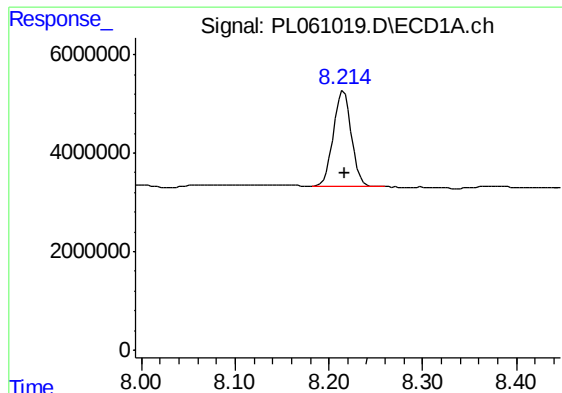

#28 Decachlorobiphenyl

R.T.: 8.216 min
Delta R.T.: -0.002 min
Response: 25951426
Conc: 15.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
RO-24

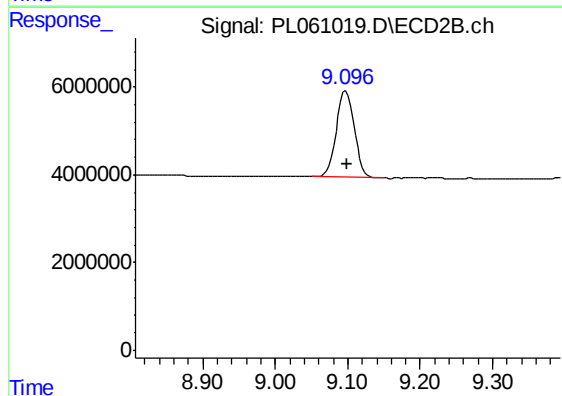

#28 Decachlorobiphenyl

R.T.: 9.098 min
Delta R.T.: -0.002 min
Response: 34199552
Conc: 16.21 ng/ml