

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082620\
 Data File : PL061020.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Aug 2020 17:49
 Operator : DD\AJ
 Sample : L3784-14
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RO-06

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 01:39:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 25 16:59:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.461	4.009	35373011	46377750	19.168	17.844
28)	SA Decachlor...	8.215	9.099	27993384	37260771	16.617	17.659
Target Compounds							
15)	B Endosulfa...	0.000	6.945	0	2319662	N.D.	0.902 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082620\
Data File : PL061020.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Aug 2020 17:49
Operator : DD\AJ
Sample : L3784-14
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RO-06

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 01:39:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082520.M
Quant Title : GC Extractables
QLast Update : Tue Aug 25 16:59:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

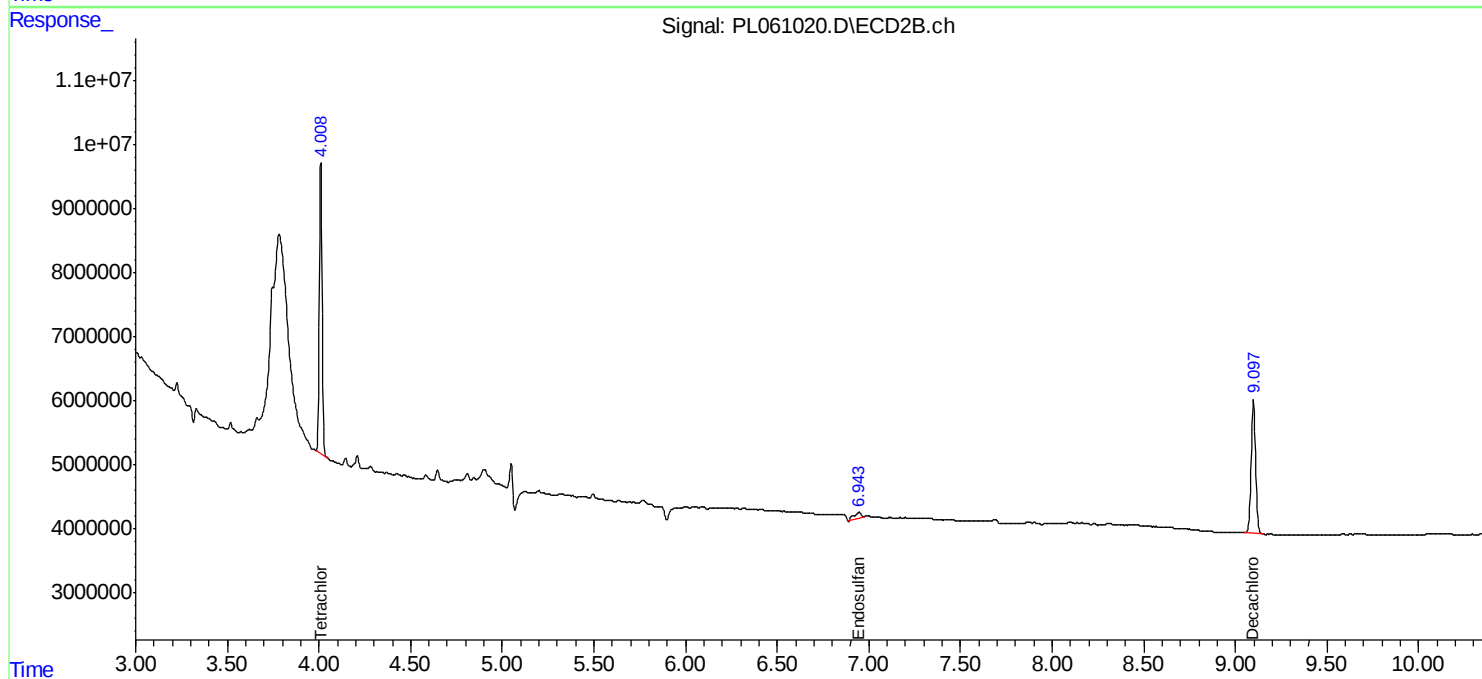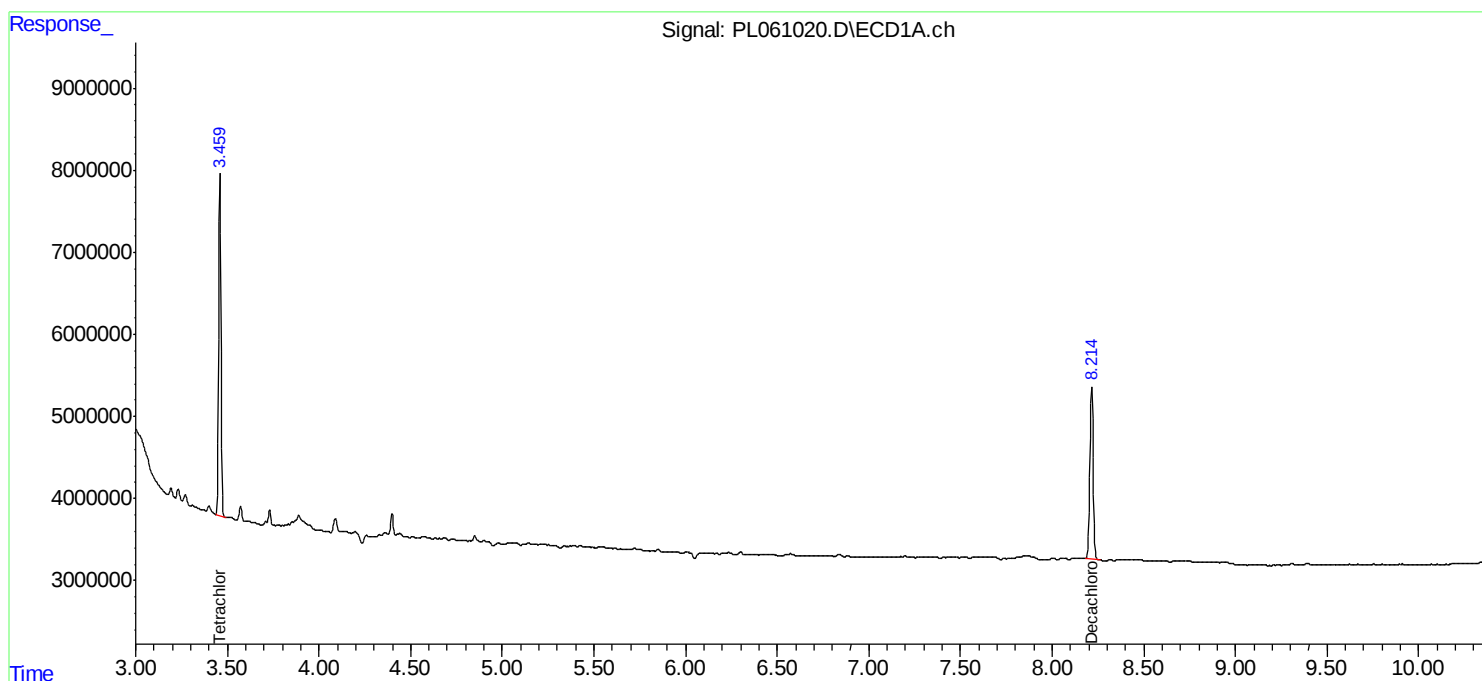


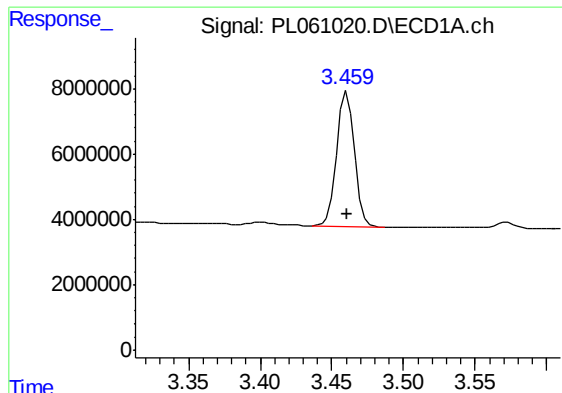

#1 Tetrachloro-m-xylene


R.T.: 3.461 min
Delta R.T.: 0.000 min
Response: 35373011
Conc: 19.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
RO-06

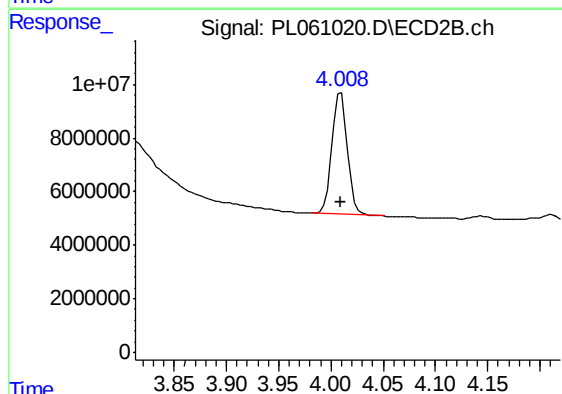


#1 Tetrachloro-m-xylene

R.T.: 4.009 min
Delta R.T.: 0.000 min
Response: 46377750
Conc: 17.84 ng/ml

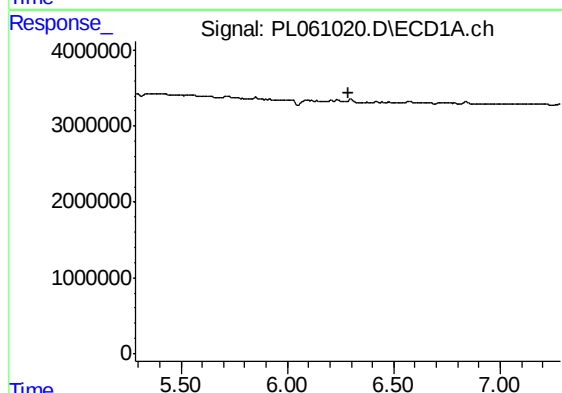


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.286 min
Response: 0
Conc: N.D.

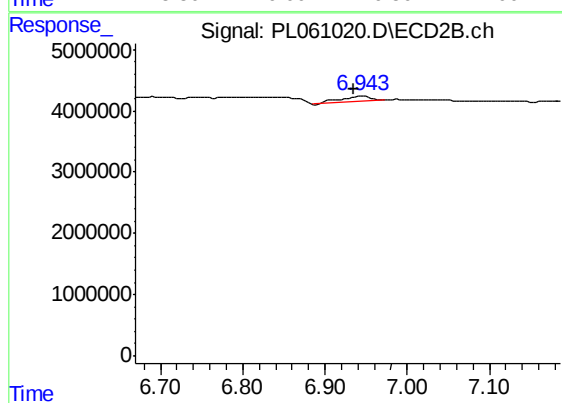

#15 Endosulfan II


R.T.: 6.945 min
Delta R.T.: 0.011 min
Response: 2319662
Conc: 0.90 ng/ml

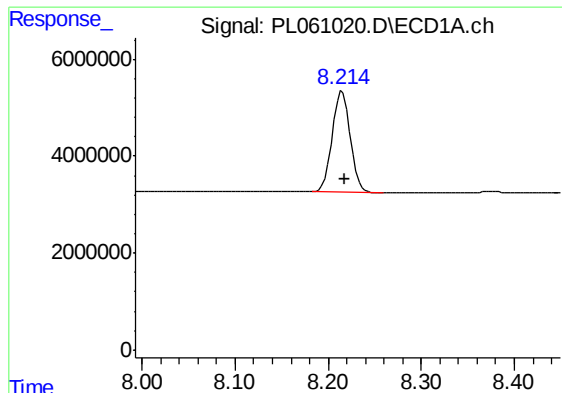

#28 Decachlorobiphenyl

R.T.: 8.215 min
Delta R.T.: -0.002 min
Response: 27993384
Conc: 16.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
RO-06

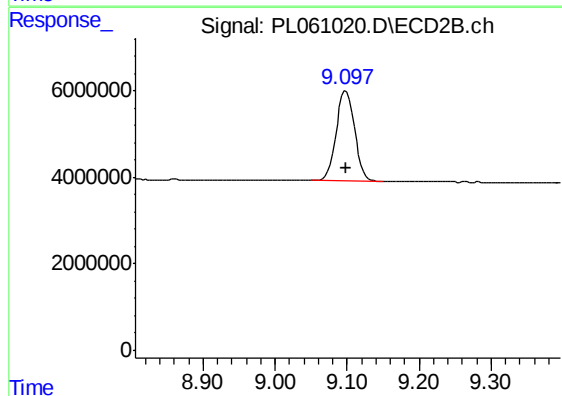

#28 Decachlorobiphenyl

R.T.: 9.099 min
Delta R.T.: 0.000 min
Response: 37260771
Conc: 17.66 ng/ml