

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082719\
 Data File : PL051807.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Aug 2019 13:30
 Operator : SG\AJ
 Sample : PB122568BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB122568BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 00:44:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.322	3.926	162.7E6	40706479	19.015	18.632
28)	SA Decachlor...	7.983	8.956	226.0E6	60222838	18.618	19.785
Target Compounds							
11)	B alpha-Chl...	5.266	0.000	210.9E6	0	14.576	N.D. #
13)	MA Dieldrin	5.544	0.000	162.6E6	0	10.693	N.D. #
14)	MA Endrin	5.774f	0.000	53620072	0	3.676	N.D. #
15)	B Endosulfa...	0.000	6.836	0	9276427	N.D.	2.814 #
16)	A 4,4'-DDD	5.941	0.000	13816859	0	1.128	N.D. #
17)	MA 4,4'-DDT	6.169	0.000	208.7E6	0	16.368	N.D. #
18)	B Endrin al...	6.255f	0.000	29540390	0	2.539	N.D. #
20)	A Methoxychlor	6.738f	0.000	28874527	0	4.259	N.D. #
21)	B Endrin ke...	6.938	0.000	30104100	0	2.128	N.D. #
26)	Chlordane-4	5.266	0.000	210.9E6	0	172.992	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082719\
Data File : PL051807.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Aug 2019 13:30
Operator : SG\AJ
Sample : PB122568BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
PB122568BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 00:44:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

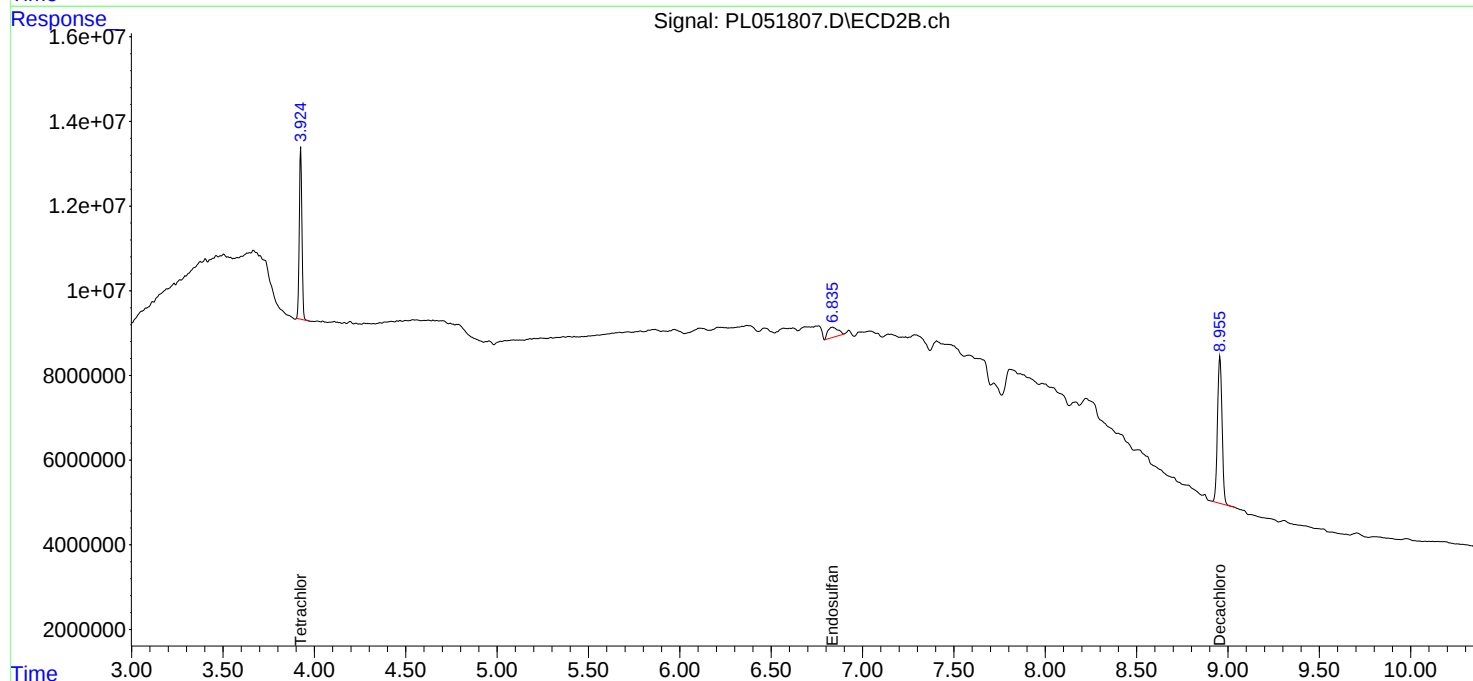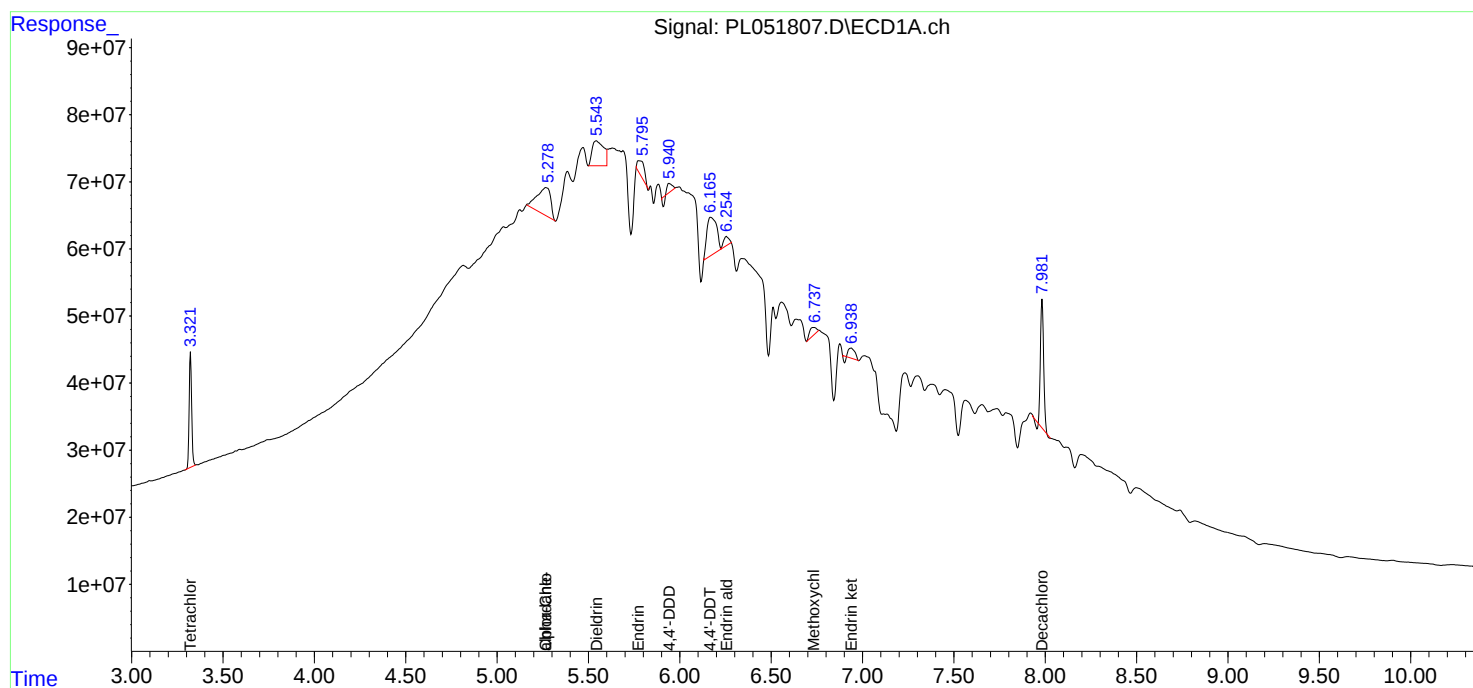


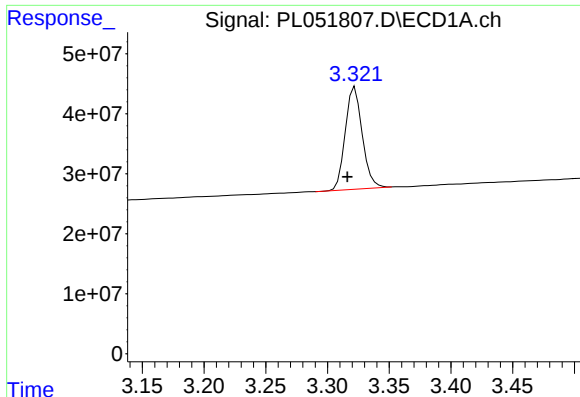

#1 Tetrachloro-m-xylene


R.T.: 3.322 min
Delta R.T.: 0.006 min
Response: 162742984
Conc: 19.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB122568BL

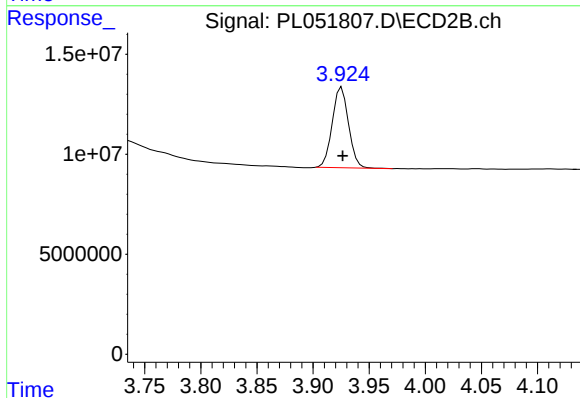


#1 Tetrachloro-m-xylene

R.T.: 3.926 min
Delta R.T.: -0.001 min
Response: 40706479
Conc: 18.63 ng/ml

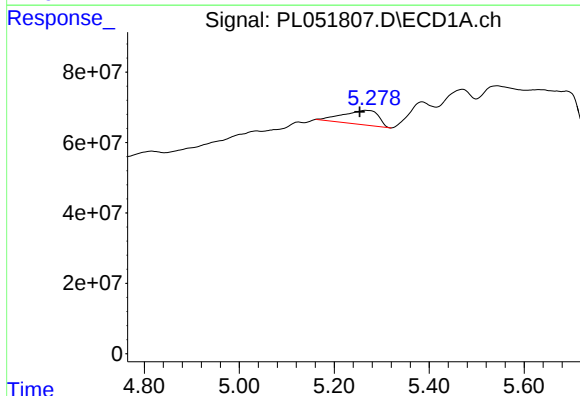


#11 alpha-Chlordane

R.T.: 5.266 min
Delta R.T.: 0.013 min
Response: 210938488
Conc: 14.58 ng/ml

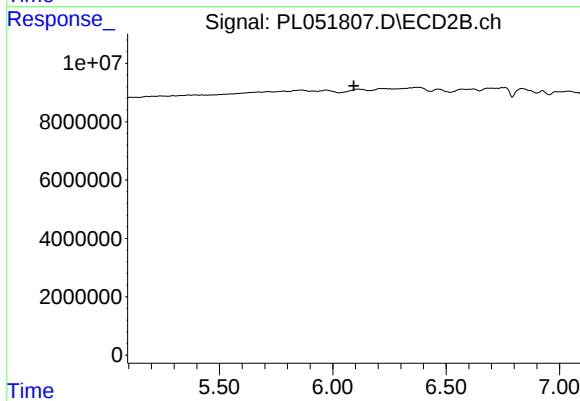

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.093 min
Response: 0
Conc: N.D.

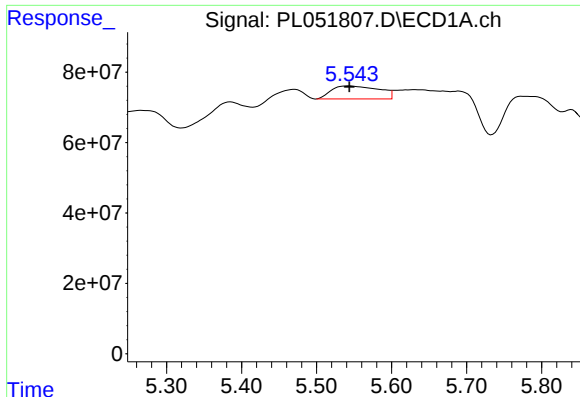

#13 Dieldrin


R.T.: 5.544 min
Delta R.T.: 0.000 min
Response: 162580158
Conc: 10.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB122568BL

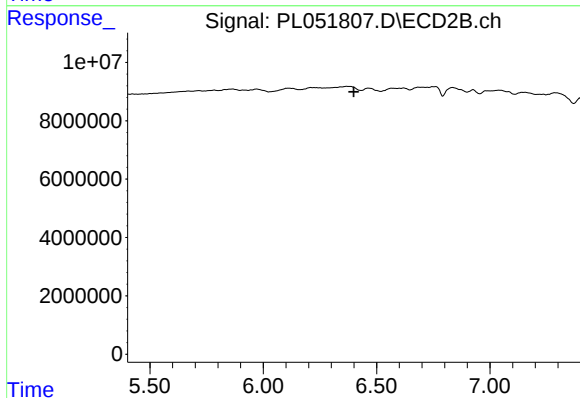


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.399 min
Response: 0
Conc: N.D.

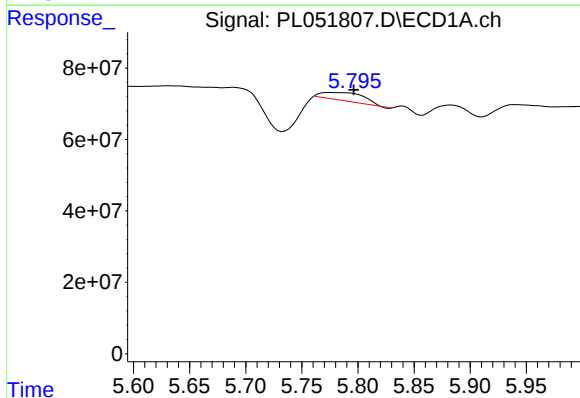


#14 Endrin

R.T.: 5.774 min
Delta R.T.: -0.022 min
Response: 53620072
Conc: 3.68 ng/ml

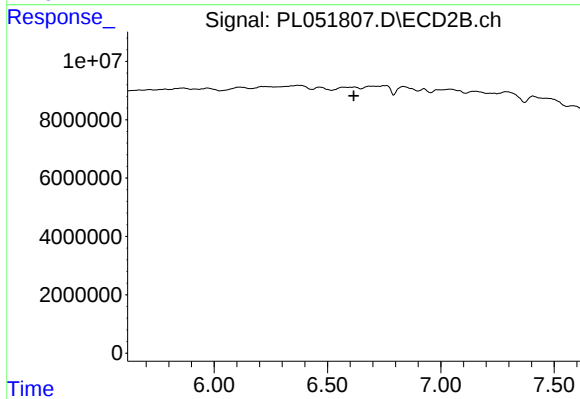

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.616 min
Response: 0
Conc: N.D.

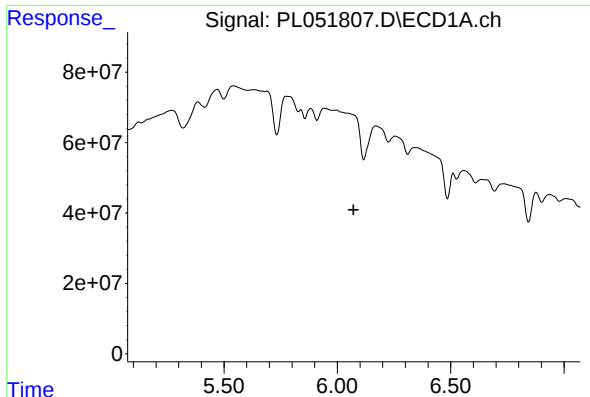

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.072 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB122568BL

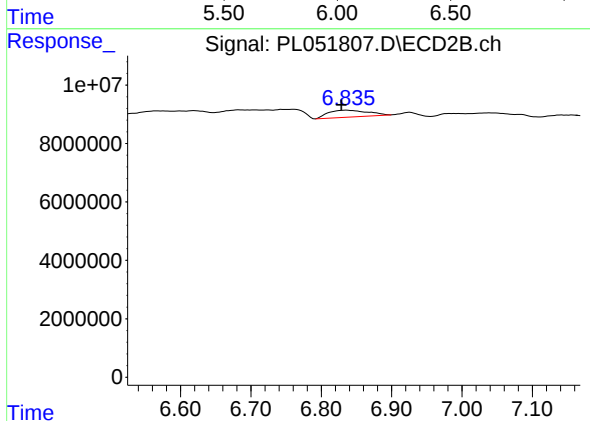


#15 Endosulfan II

R.T.: 6.836 min
Delta R.T.: 0.008 min
Response: 9276427
Conc: 2.81 ng/ml

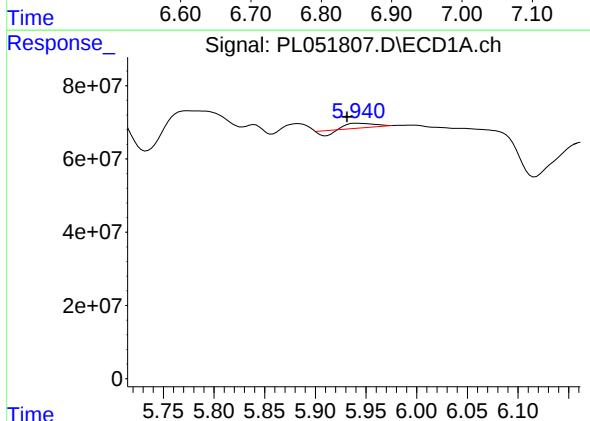


#16 4,4'-DDD

R.T.: 5.941 min
Delta R.T.: 0.010 min
Response: 13816859
Conc: 1.13 ng/ml

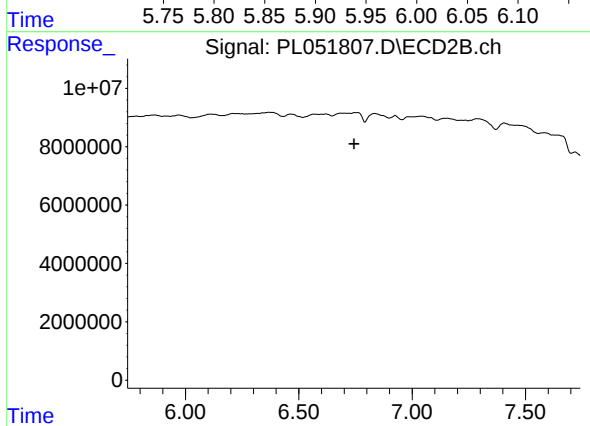

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.744 min
Response: 0
Conc: N.D.

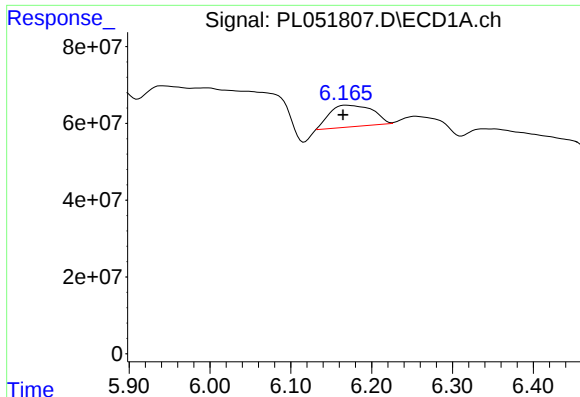

#17 4,4'-DDT


R.T.: 6.169 min
Delta R.T.: 0.004 min
Response: 208718768
Conc: 16.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB122568BL

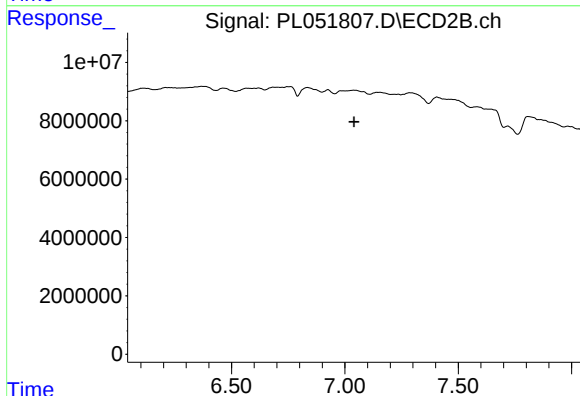


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.041 min
Response: 0
Conc: N.D.

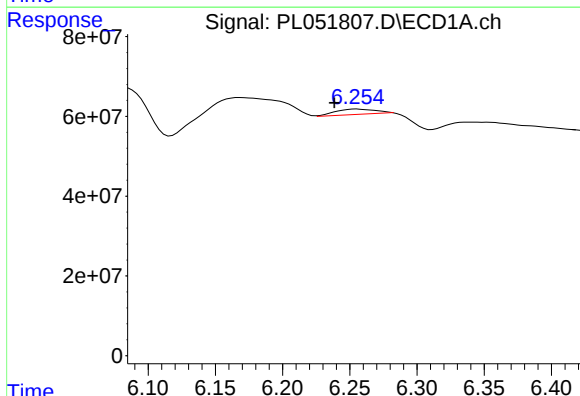


#18 Endrin aldehyde

R.T.: 6.255 min
Delta R.T.: 0.016 min
Response: 29540390
Conc: 2.54 ng/ml

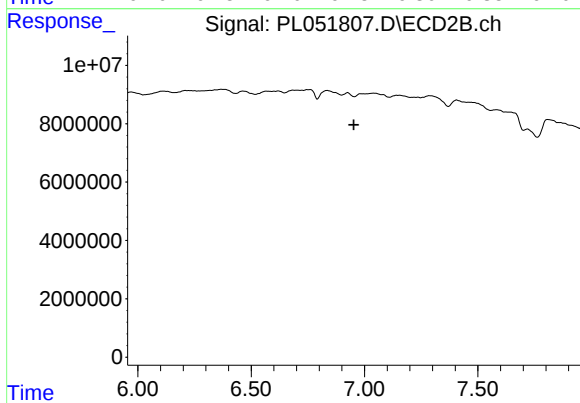

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.953 min
Response: 0
Conc: N.D.

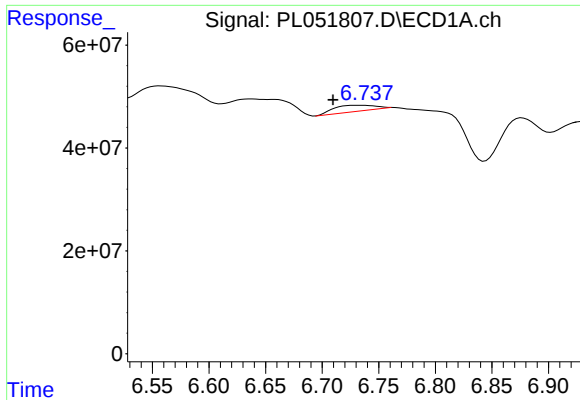

#20 Methoxychlor


R.T.: 6.738 min
Delta R.T.: 0.028 min
Response: 28874527
Conc: 4.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB122568BL

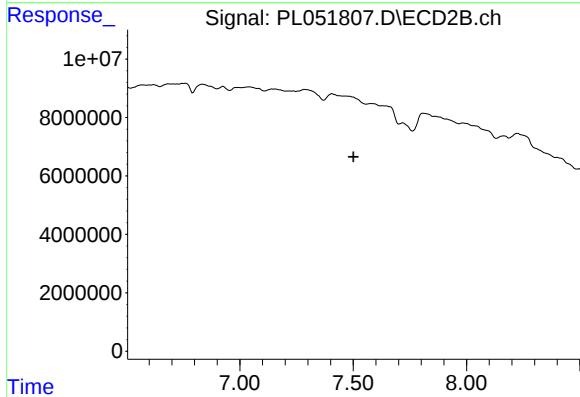


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 7.502 min
Response: 0
Conc: N.D.

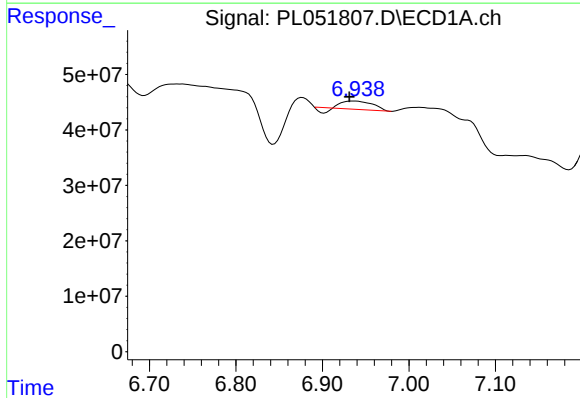


#21 Endrin ketone

R.T.: 6.938 min
Delta R.T.: 0.007 min
Response: 30104100
Conc: 2.13 ng/ml

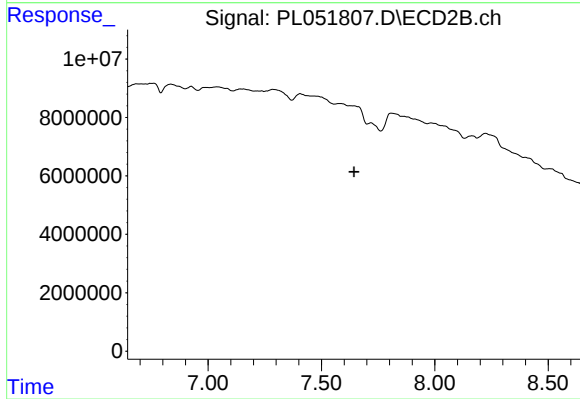

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.644 min
Response: 0
Conc: N.D.

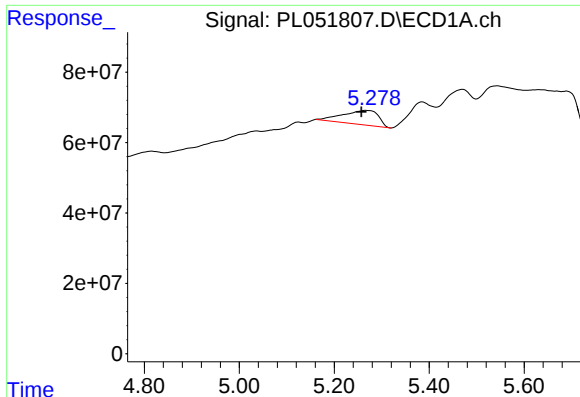

#26 Chlordane-4


R.T.: 5.266 min
Delta R.T.: 0.009 min
Response: 210938488
Conc: 172.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB122568BL

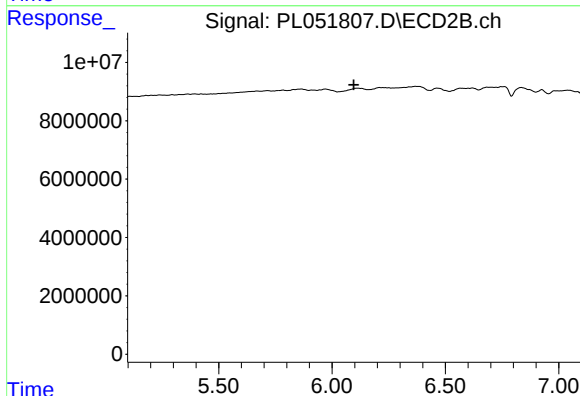


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 6.096 min
Response: 0
Conc: N.D.

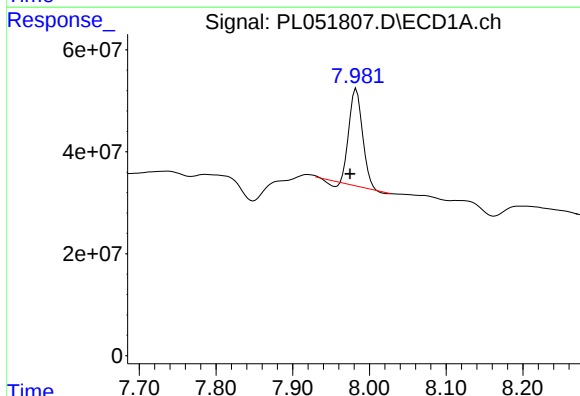

#28 Decachlorobiphenyl

R.T.: 7.983 min
Delta R.T.: 0.008 min
Response: 225984223
Conc: 18.62 ng/ml

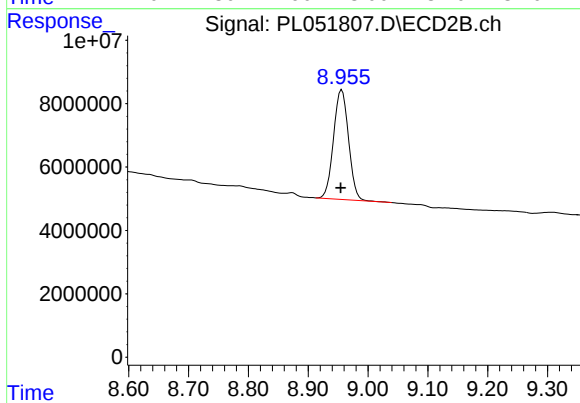

#28 Decachlorobiphenyl

R.T.: 8.956 min
Delta R.T.: 0.002 min
Response: 60222838
Conc: 19.78 ng/ml