

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082719\
 Data File : PL051842.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Aug 2019 22:26
 Operator : SG\AJ
 Sample : K4526-14
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 T9-12-13-G1-G4-(0-1.9)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 00:55:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.314	3.925	88511920	23421965	10.342	10.720
28)	SA Decachlor...	7.972	8.951	144.3E6	36987795	11.886	12.152
Target Compounds							
6)	B beta-BHC	0.000	4.802f	0	5342765	N.D.	3.666 #
13)	MA Dieldrin	5.555	0.000	32681818	0	2.149	N.D. #
15)	B Endosulfa...	0.000	6.817	0	6279328	N.D.	1.905 #
17)	MA 4,4'-DDT	6.156	0.000	26733701	0	2.097	N.D. #
19)	B Endosulfa...	6.437	0.000	9570271	0	0.736	N.D. #
20)	A Methoxychlor	6.686f	0.000	39585515	0	5.839	N.D. #
21)	B Endrin ke...	6.954f	0.000	10259887	0	0.725	N.D. #
27)	Chlordane-5	0.000	6.918f	0	1025973	N.D.	10.407 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082719\
Data File : PL051842.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Aug 2019 22:26
Operator : SG\AJ
Sample : K4526-14
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
T9-12-13-G1-G4-(0-1.9)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 00:55:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

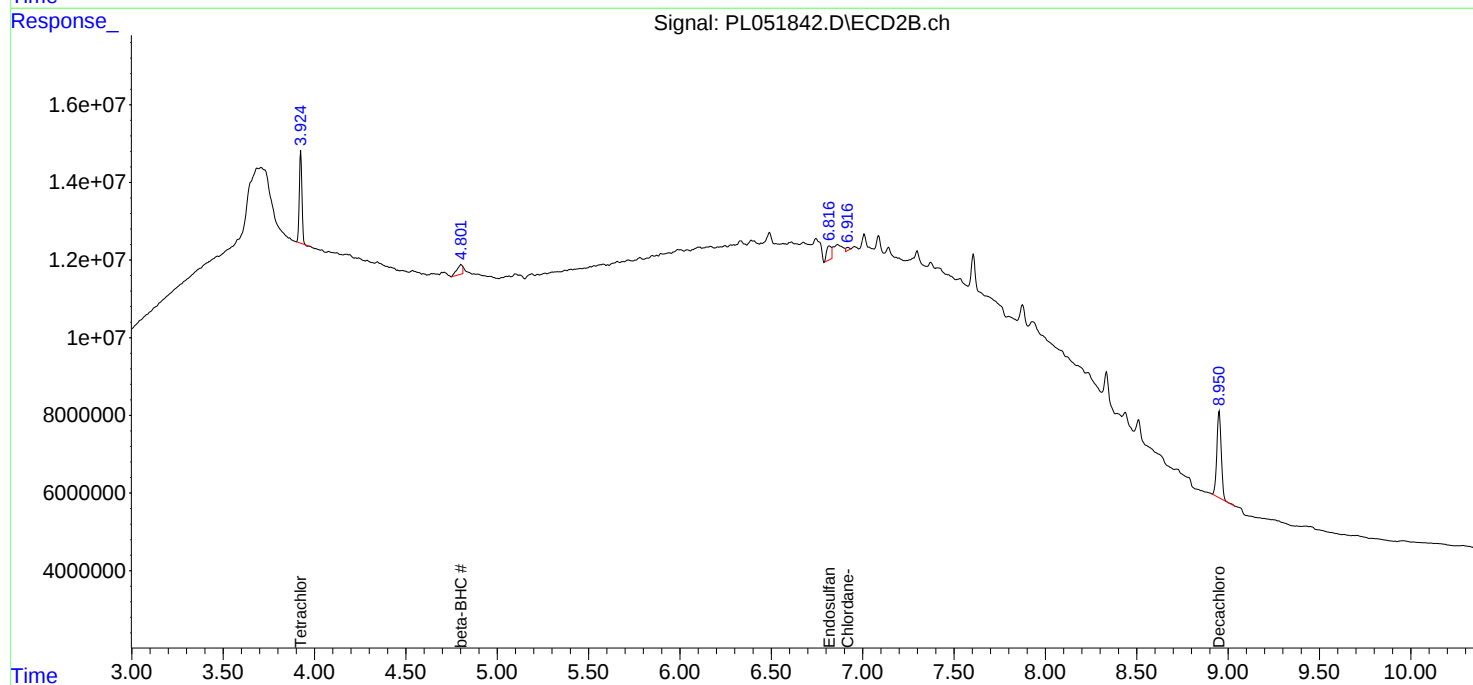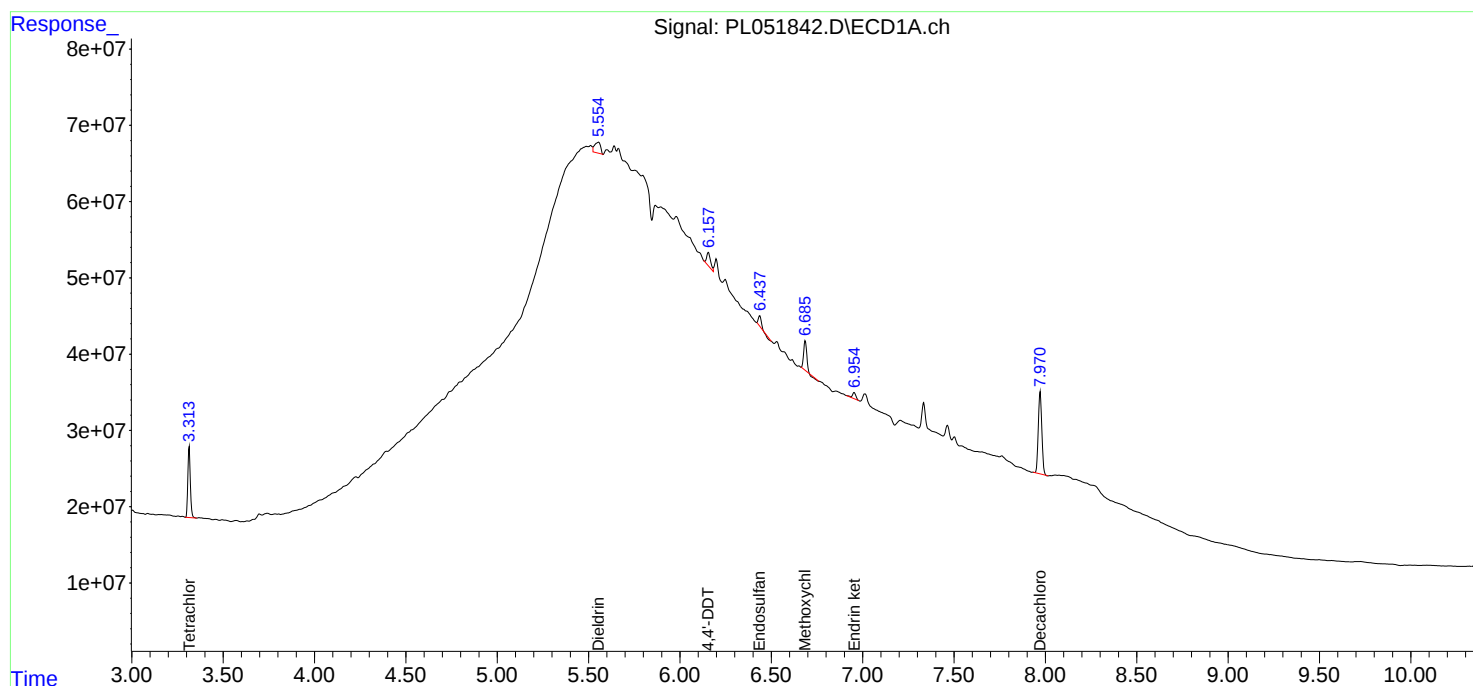


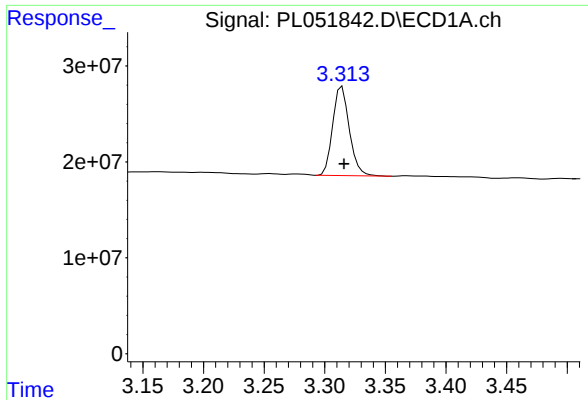

#1 Tetrachloro-m-xylene


R.T.: 3.314 min
Delta R.T.: -0.002 min
Response: 88511920
Conc: 10.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
T9-12-13-G1-G4-(0-1.9)

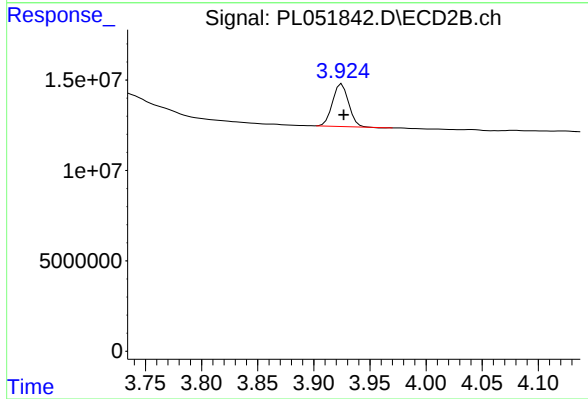


#1 Tetrachloro-m-xylene

R.T.: 3.925 min
Delta R.T.: -0.002 min
Response: 23421965
Conc: 10.72 ng/ml

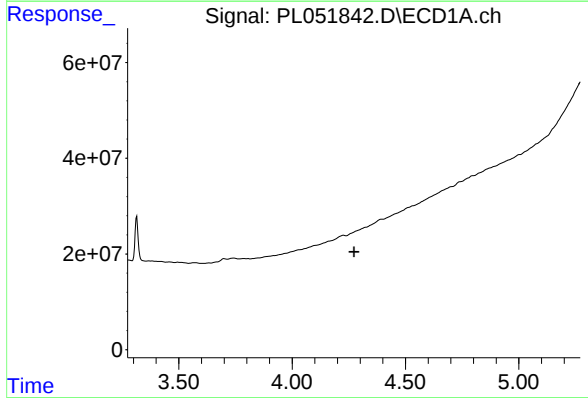


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.273 min
Response: 0
Conc: N.D.

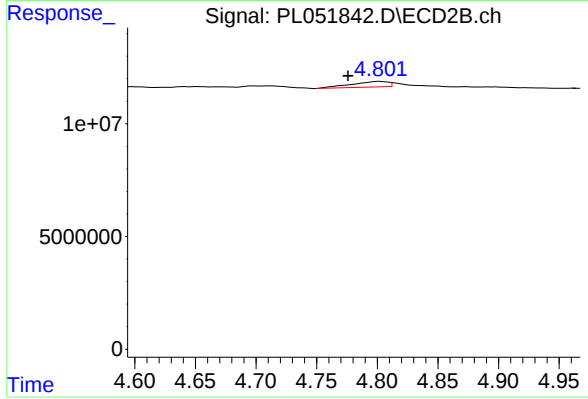

#6 beta-BHC


R.T.: 4.802 min
Delta R.T.: 0.026 min
Response: 5342765
Conc: 3.67 ng/ml

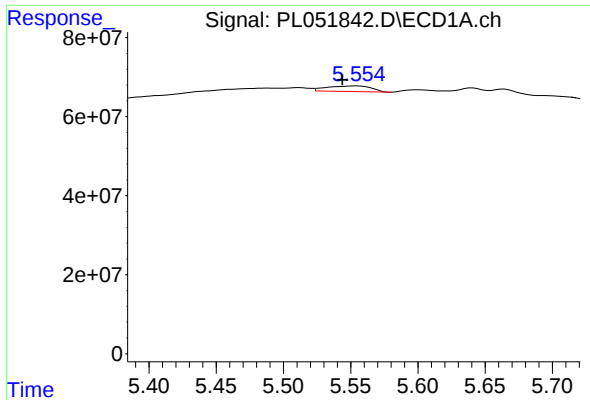

#13 Dieldrin


R.T.: 5.555 min
Delta R.T.: 0.011 min
Response: 32681818
Conc: 2.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
T9-12-13-G1-G4-(0-1.9)

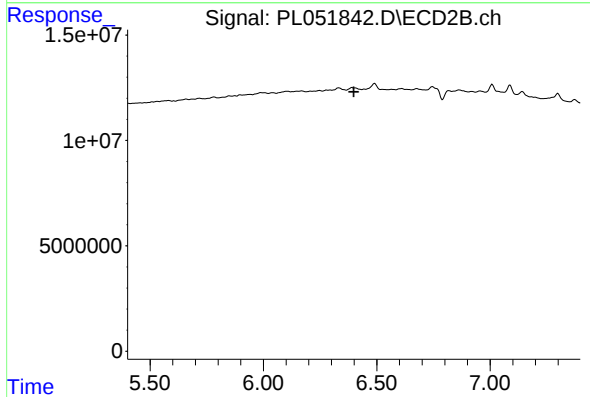


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.399 min
Response: 0
Conc: N.D.

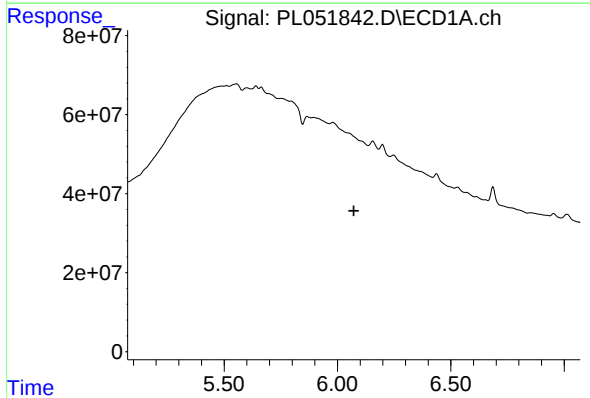


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.072 min
Response: 0
Conc: N.D.

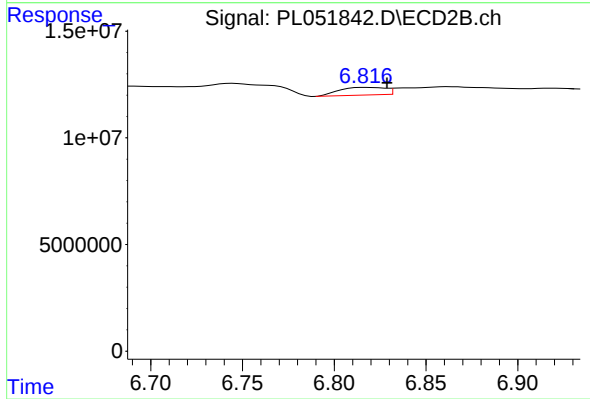

#15 Endosulfan II


R.T.: 6.817 min
Delta R.T.: -0.012 min
Response: 6279328
Conc: 1.91 ng/ml

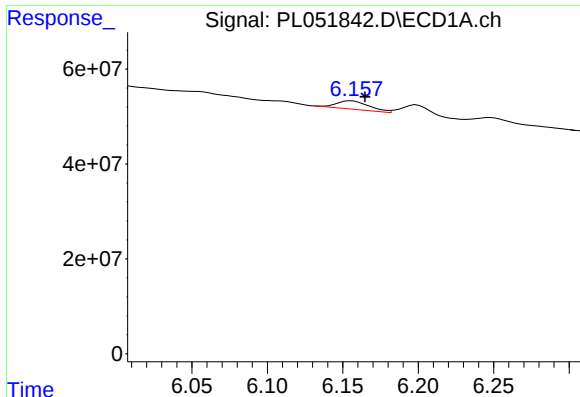

#17 4,4'-DDT


R.T.: 6.156 min
Delta R.T.: -0.009 min
Response: 26733701
Conc: 2.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
T9-12-13-G1-G4-(0-1.9)

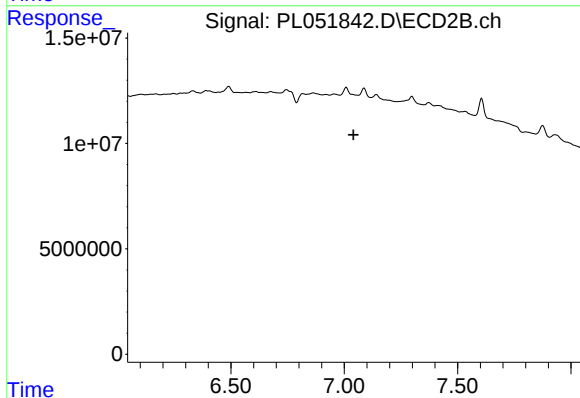


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.041 min
Response: 0
Conc: N.D.

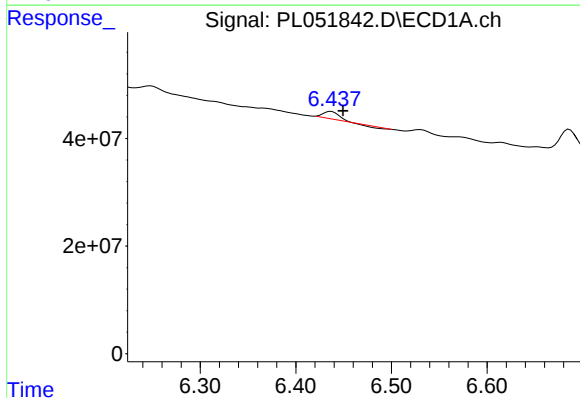


#19 Endosulfan Sulfate

R.T.: 6.437 min
Delta R.T.: -0.013 min
Response: 9570271
Conc: 0.74 ng/ml

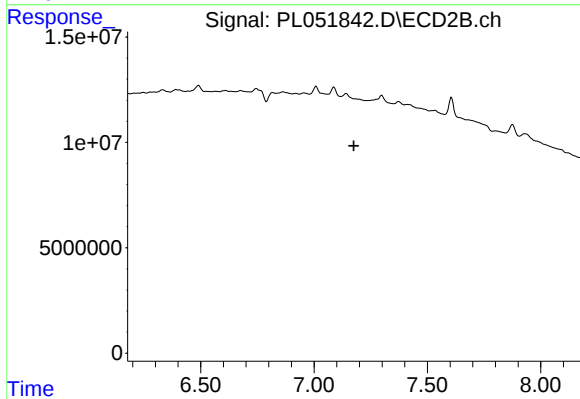

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.176 min
Response: 0
Conc: N.D.

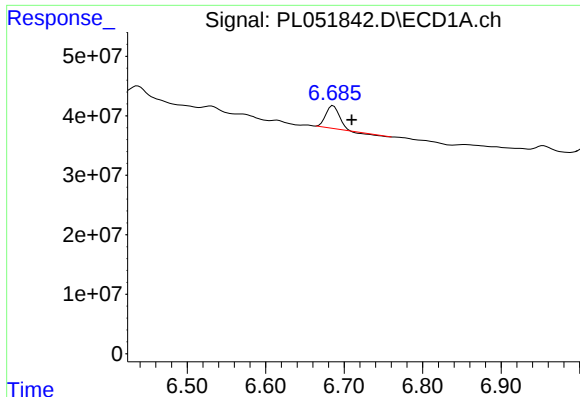

#20 Methoxychlor


R.T.: 6.686 min
Delta R.T.: -0.024 min
Response: 39585515
Conc: 5.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
T9-12-13-G1-G4-(0-1.9)

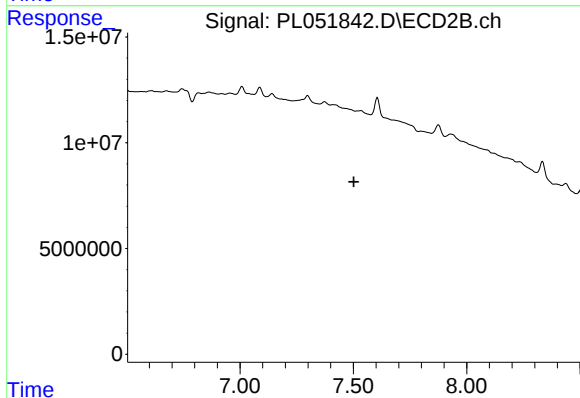


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 7.502 min
Response: 0
Conc: N.D.

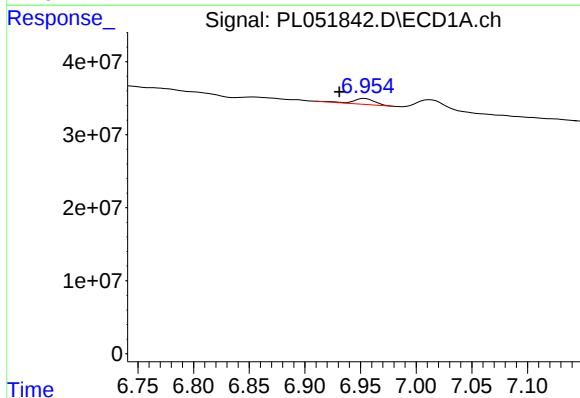


#21 Endrin ketone

R.T.: 6.954 min
Delta R.T.: 0.023 min
Response: 10259887
Conc: 0.73 ng/ml

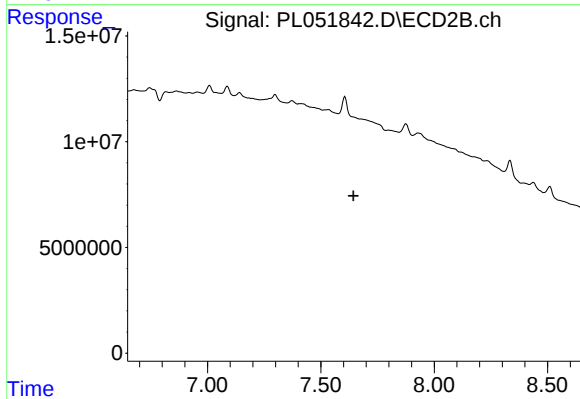

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.644 min
Response: 0
Conc: N.D.

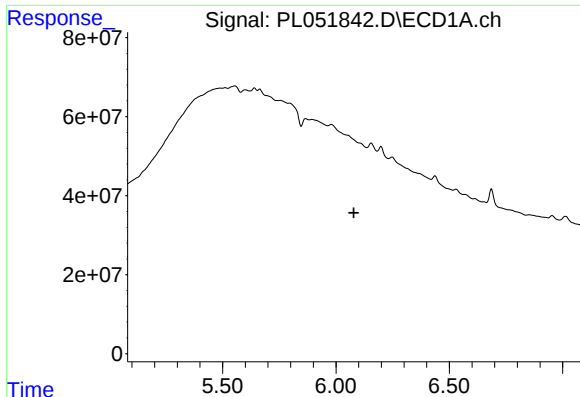

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.079 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
T9-12-13-G1-G4-(0-1.9)

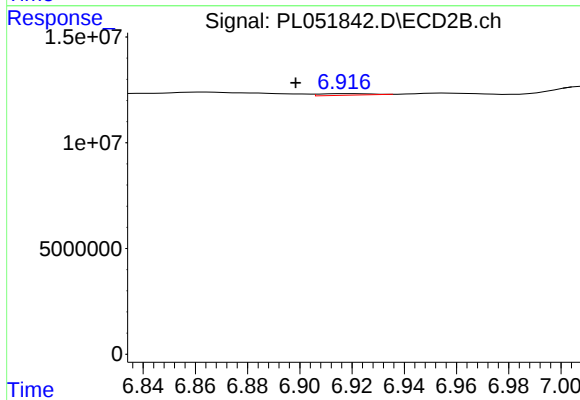


#27 Chlordane-5

R.T.: 6.918 min
Delta R.T.: 0.019 min
Response: 1025973
Conc: 10.41 ng/ml

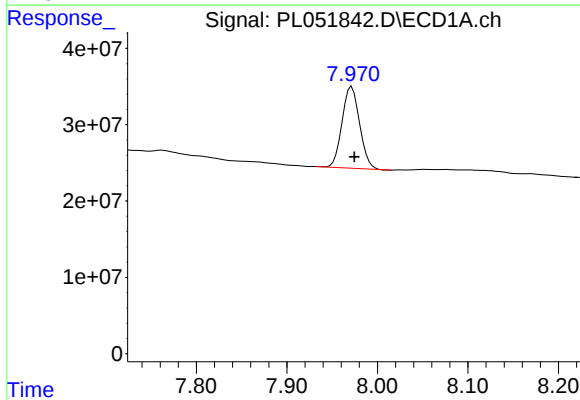

#28 Decachlorobiphenyl

R.T.: 7.972 min
Delta R.T.: -0.003 min
Response: 144272668
Conc: 11.89 ng/ml

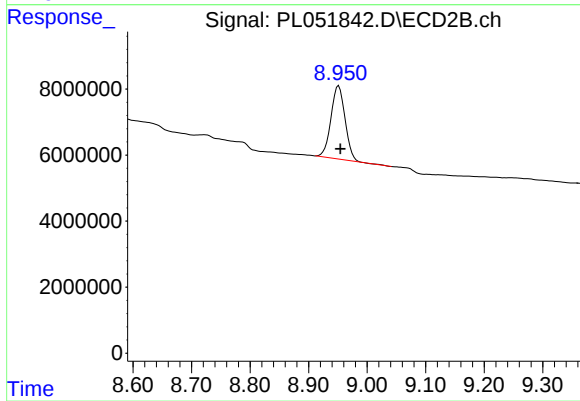

#28 Decachlorobiphenyl

R.T.: 8.951 min
Delta R.T.: -0.003 min
Response: 36987795
Conc: 12.15 ng/ml