

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082719\
 Data File : PL051861.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Aug 2019 02:54
 Operator : SG\AJ
 Sample : K4517-12
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 T4-S-D1-D4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 03:55:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.314	3.925	114.4E6	28135946	13.371	12.878
28)	SA Decachlor...	7.972	8.951	137.8E6	31599165	11.356	10.381
Target Compounds							
6)	B beta-BHC	0.000	4.801f	0	2238533	N.D.	1.536 #
9)	A Endosulfan I	5.331f	0.000	23001243	0	1.711	N.D. #
11)	B alpha-Chl...	5.239	0.000	72557764	0	5.014	N.D. #
13)	MA Dieldrin	5.548	0.000	157.9E6	0	10.384	N.D. #
15)	B Endosulfa...	0.000	6.839	0	7896103	N.D.	2.396 #
26)	Chlordane-4	5.268	0.000	41351349	0	33.912	N.D. #
27)	Chlordane-5	0.000	6.878f	0	1893756	N.D.	19.210 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082719\
Data File : PL051861.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Aug 2019 02:54
Operator : SG\AJ
Sample : K4517-12
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
T4-S-D1-D4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 03:55:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

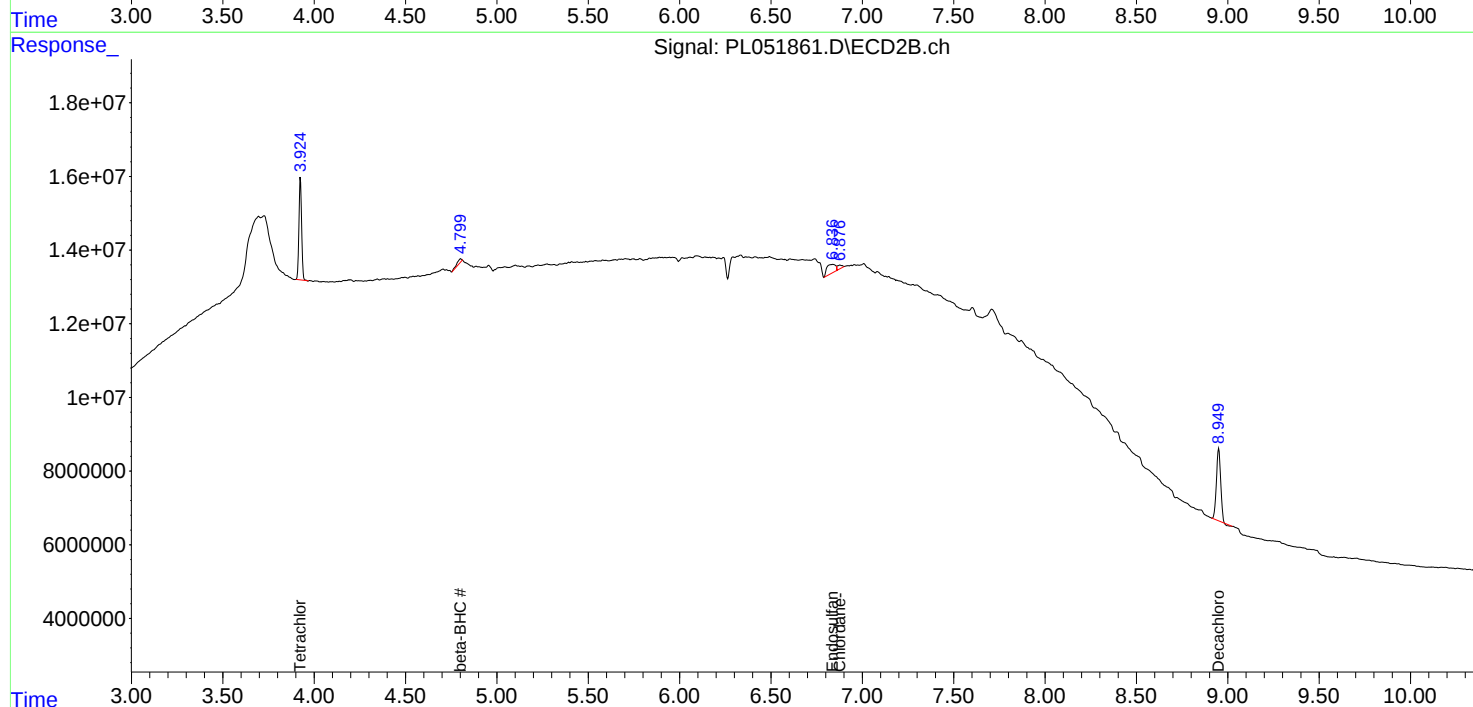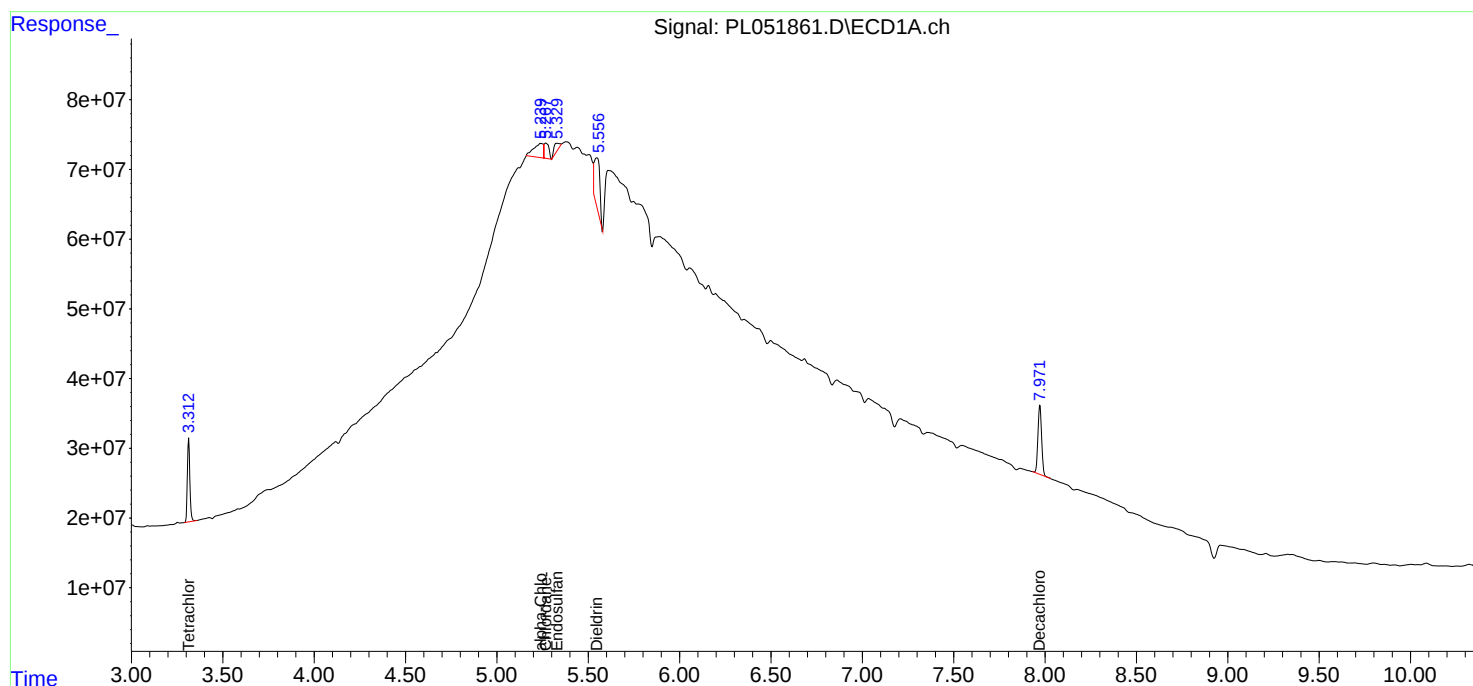


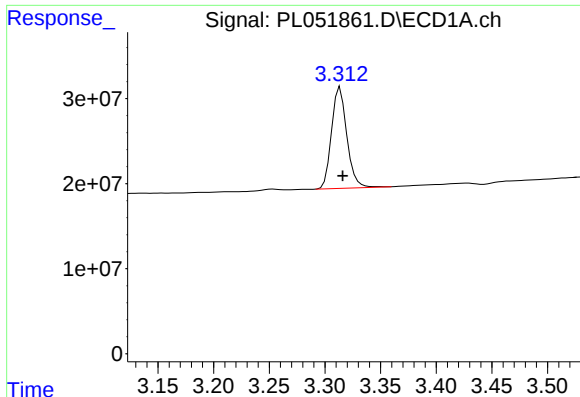

#1 Tetrachloro-m-xylene


R.T.: 3.314 min
Delta R.T.: -0.002 min
Response: 114439329
Conc: 13.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
T4-S-D1-D4

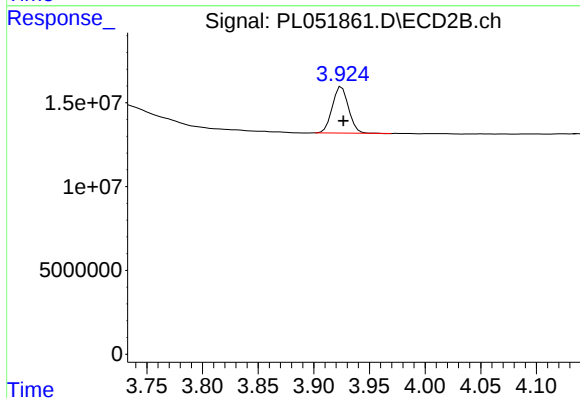


#1 Tetrachloro-m-xylene

R.T.: 3.925 min
Delta R.T.: -0.002 min
Response: 28135946
Conc: 12.88 ng/ml

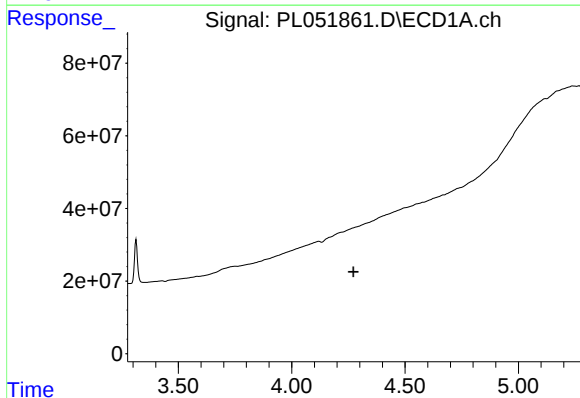


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.273 min
Response: 0
Conc: N.D.

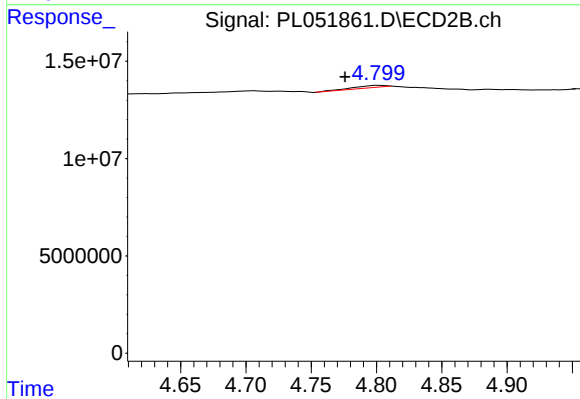

#6 beta-BHC


R.T.: 4.801 min
Delta R.T.: 0.025 min
Response: 2238533
Conc: 1.54 ng/ml

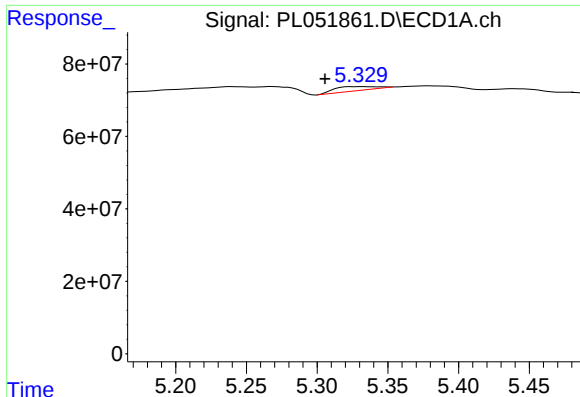

#9 Endosulfan I


R.T.: 5.331 min
Delta R.T.: 0.026 min
Response: 23001243
Conc: 1.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
T4-S-D1-D4

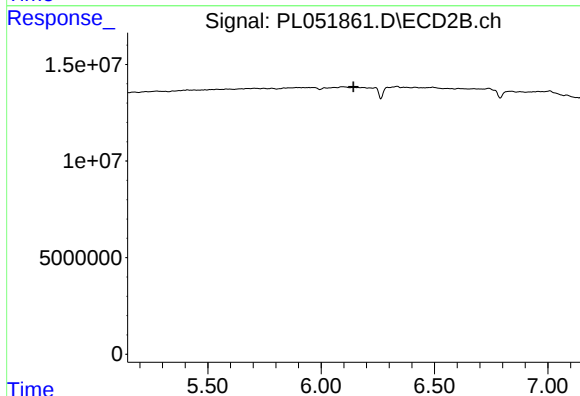


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.143 min
Response: 0
Conc: N.D.

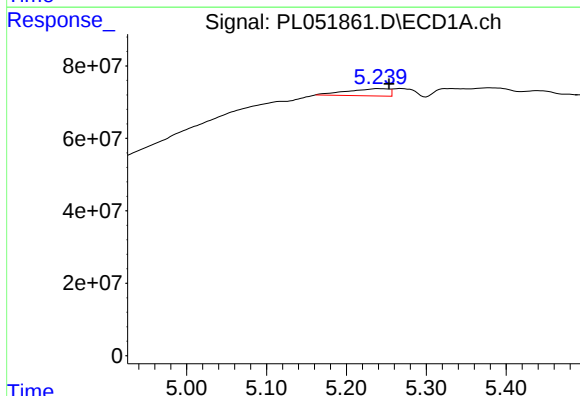


#11 alpha-Chlordane

R.T.: 5.239 min
Delta R.T.: -0.014 min
Response: 72557764
Conc: 5.01 ng/ml

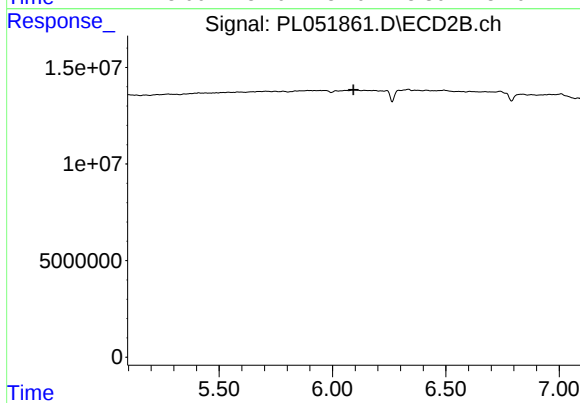

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.093 min
Response: 0
Conc: N.D.

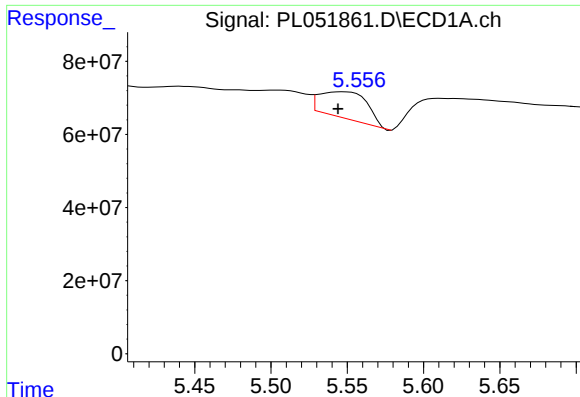

#13 Dieldrin


R.T.: 5.548 min
Delta R.T.: 0.004 min
Response: 157891947
Conc: 10.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
T4-S-D1-D4

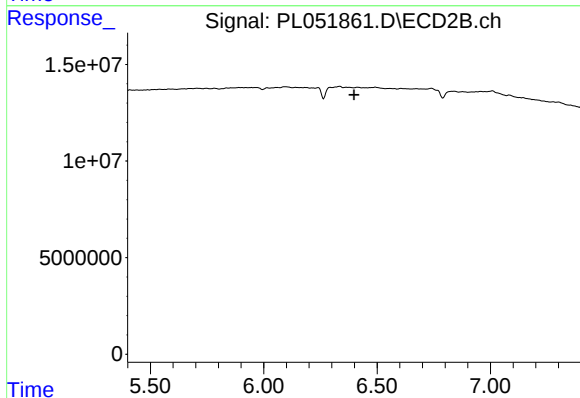


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.399 min
Response: 0
Conc: N.D.

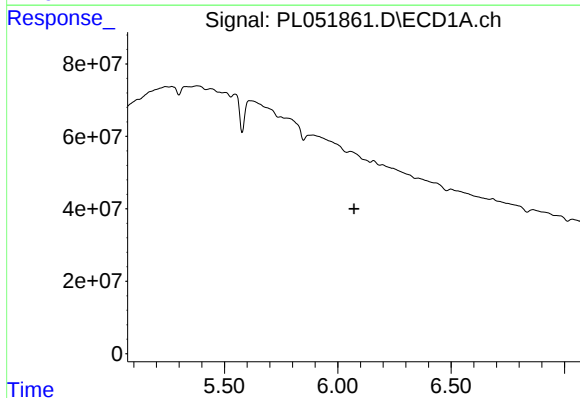


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.072 min
Response: 0
Conc: N.D.

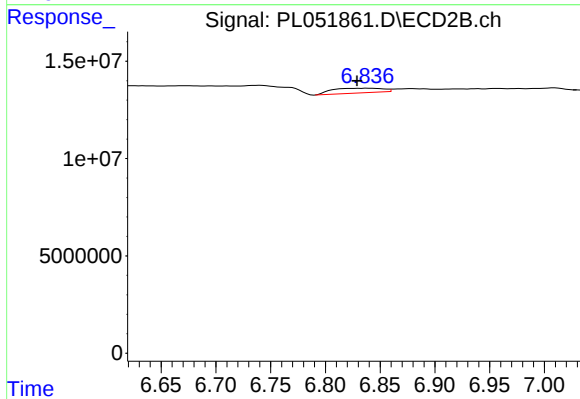

#15 Endosulfan II


R.T.: 6.839 min
Delta R.T.: 0.010 min
Response: 7896103
Conc: 2.40 ng/ml

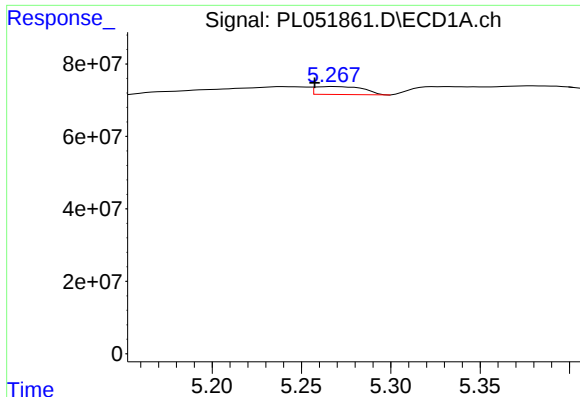

#26 Chlordane-4


R.T.: 5.268 min
Delta R.T.: 0.011 min
Response: 41351349
Conc: 33.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
T4-S-D1-D4

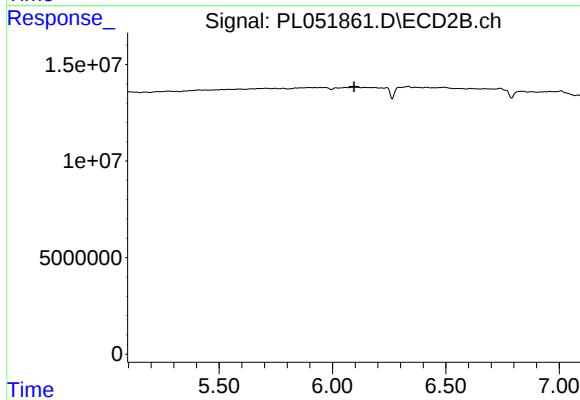


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.096 min
Response: 0
Conc: N.D.

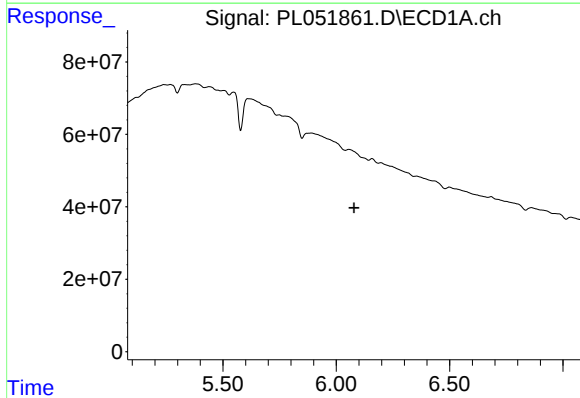


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.079 min
Response: 0
Conc: N.D.

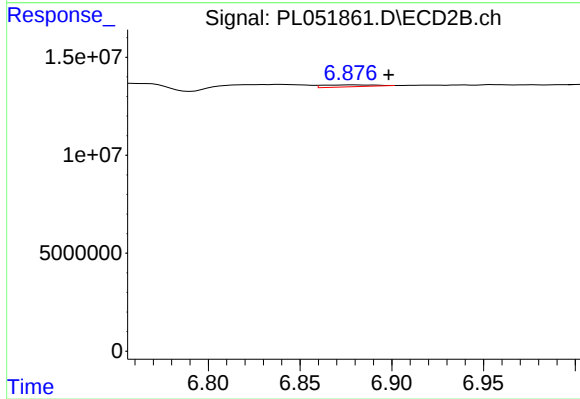

#27 Chlordane-5


R.T.: 6.878 min
Delta R.T.: -0.021 min
Response: 1893756
Conc: 19.21 ng/ml

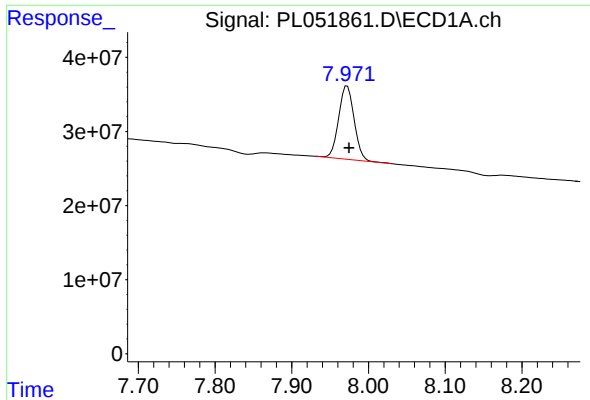

#28 Decachlorobiphenyl

R.T.: 7.972 min
Delta R.T.: -0.002 min
Response: 137833651
Conc: 11.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
T4-S-D1-D4

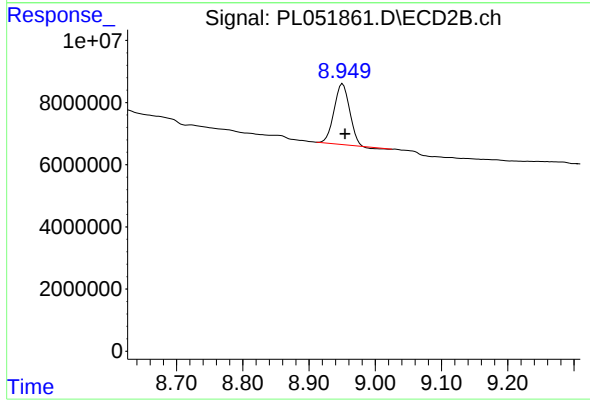

#28 Decachlorobiphenyl

R.T.: 8.951 min
Delta R.T.: -0.003 min
Response: 31599165
Conc: 10.38 ng/ml