

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082719\
 Data File : PL051877.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Aug 2019 06:40
 Operator : SG\AJ
 Sample : K4543-03
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-2-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 07:01:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.314	3.925	84258471	20747211	9.845	9.496
28)	SA Decachlor...	7.973	8.952	87922252	24532751	7.244	8.060
Target Compounds							
6)	B beta-BHC	0.000	4.800f	0	2720376	N.D.	1.867 #
8)	B Heptachlo...	4.981	0.000	6397787	0	0.457	N.D. #
10)	B gamma-Chl...	5.197	0.000	3116437	0	0.209	N.D. #
15)	B Endosulfa...	0.000	6.836	0	8965241	N.D.	2.720 #
23)	Chlordane-1	4.167	0.000	13651289	0	42.373	N.D. #
25)	Chlordane-3	5.197	0.000	3116437	0	2.400	N.D. #
27)	Chlordane-5	0.000	6.877f	0	2538911	N.D.	25.754 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082719\
Data File : PL051877.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Aug 2019 06:40
Operator : SG\AJ
Sample : K4543-03
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-2-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 07:01:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

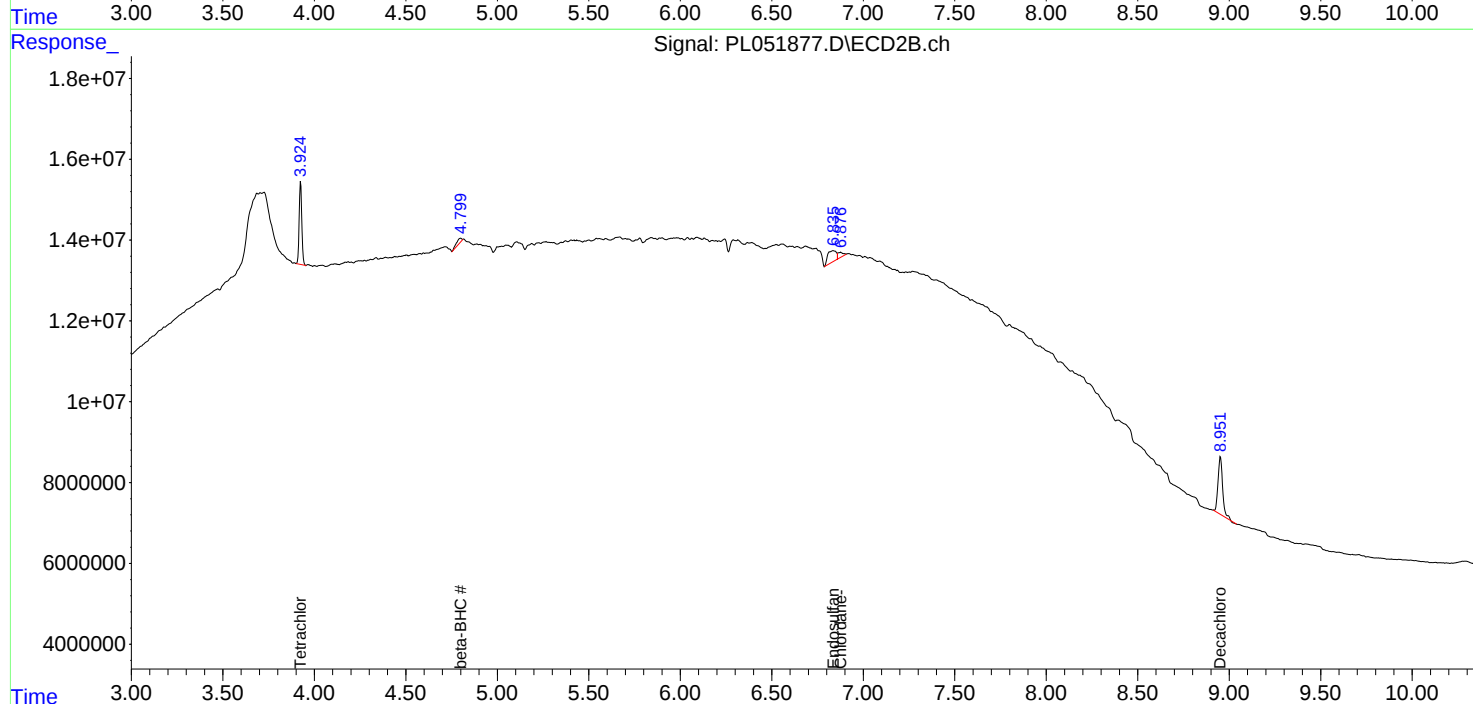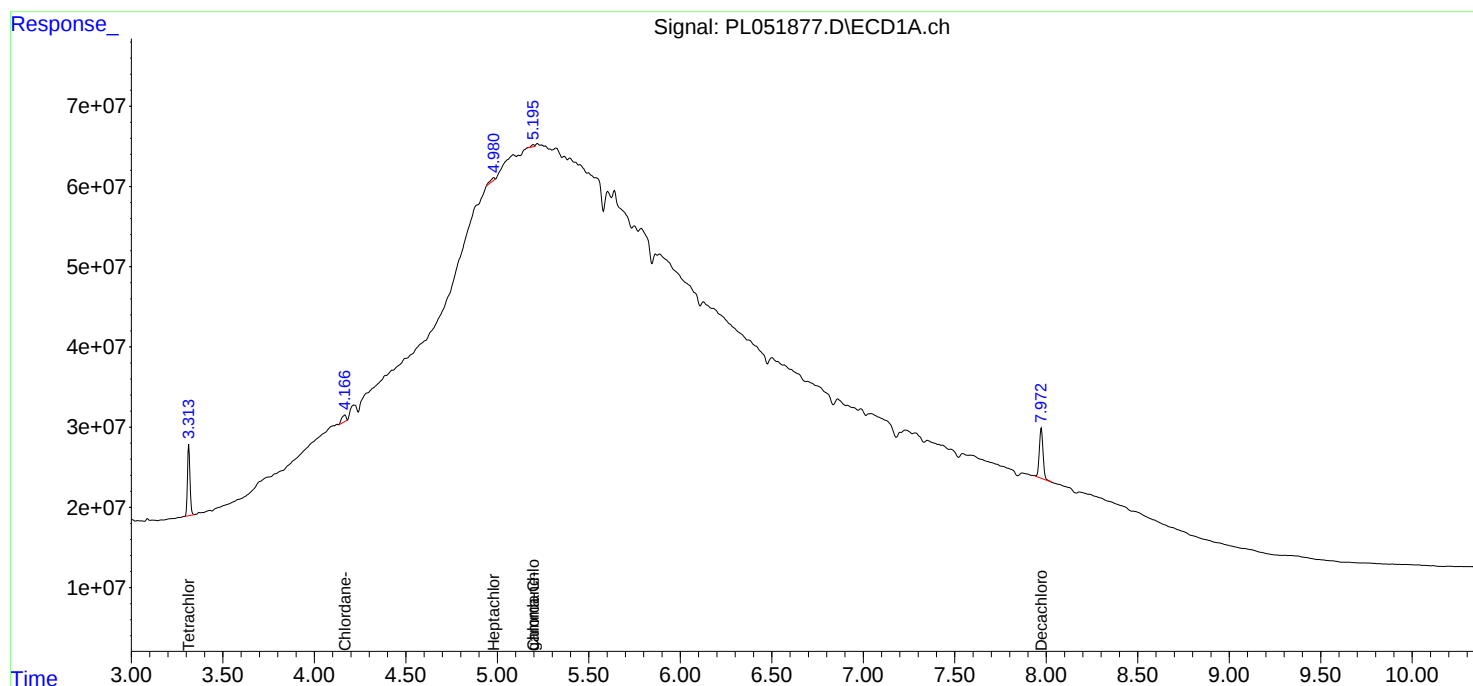


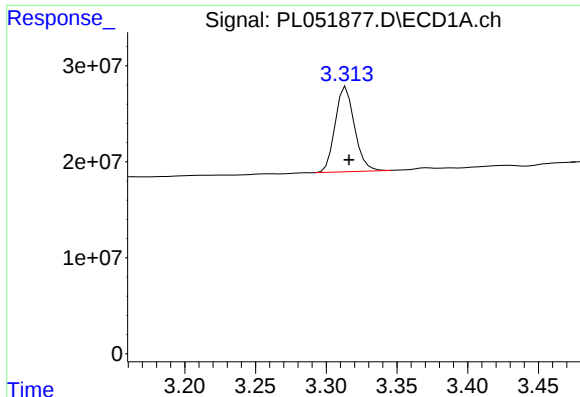

#1 Tetrachloro-m-xylene


R.T.: 3.314 min
Delta R.T.: -0.002 min
Response: 84258471
Conc: 9.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2-S

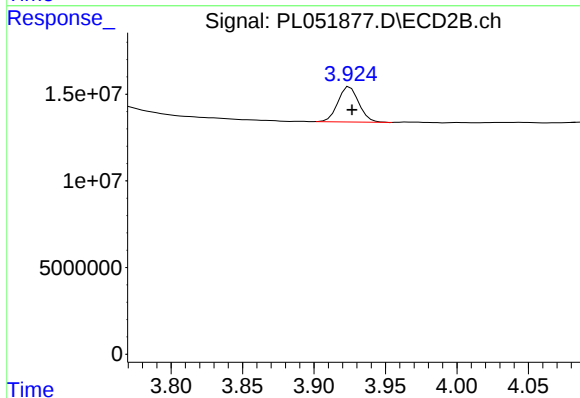


#1 Tetrachloro-m-xylene

R.T.: 3.925 min
Delta R.T.: -0.001 min
Response: 20747211
Conc: 9.50 ng/ml

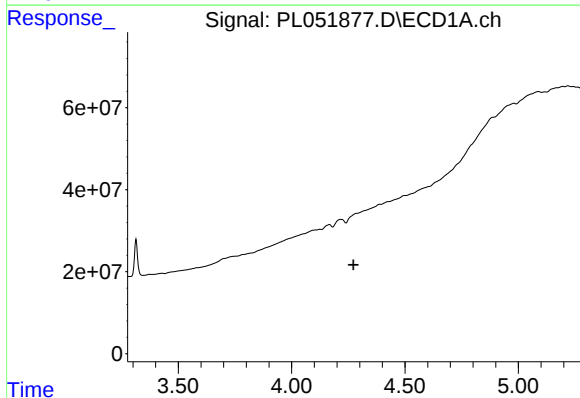


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.273 min
Response: 0
Conc: N.D.

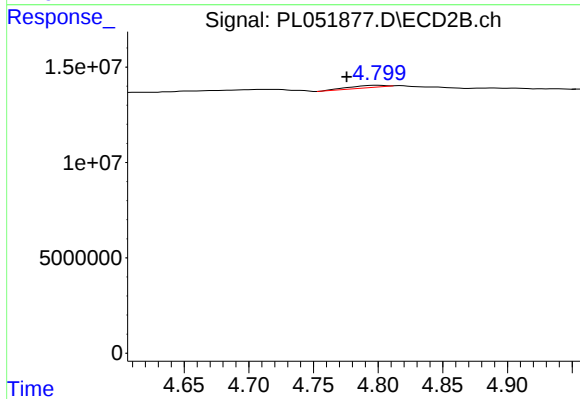

#6 beta-BHC


R.T.: 4.800 min
Delta R.T.: 0.024 min
Response: 2720376
Conc: 1.87 ng/ml

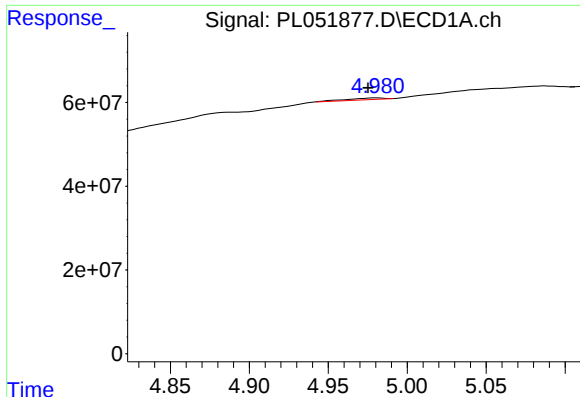

#8 Heptachlor epoxide


R.T.: 4.981 min
Delta R.T.: 0.006 min
Response: 6397787
Conc: 0.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2-S

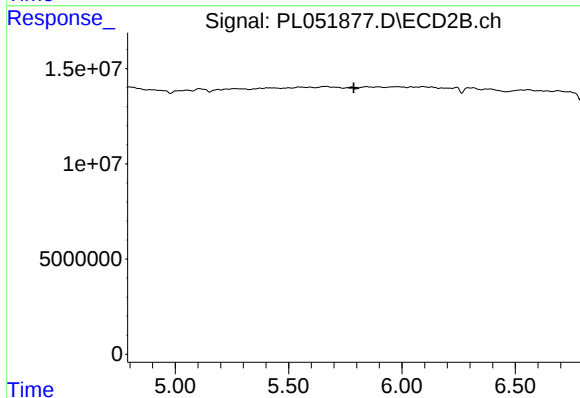


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.787 min
Response: 0
Conc: N.D.

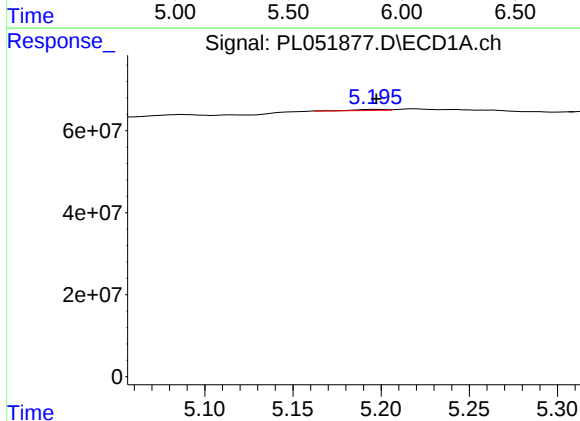


#10 gamma-Chlordane

R.T.: 5.197 min
Delta R.T.: 0.000 min
Response: 3116437
Conc: 0.21 ng/ml

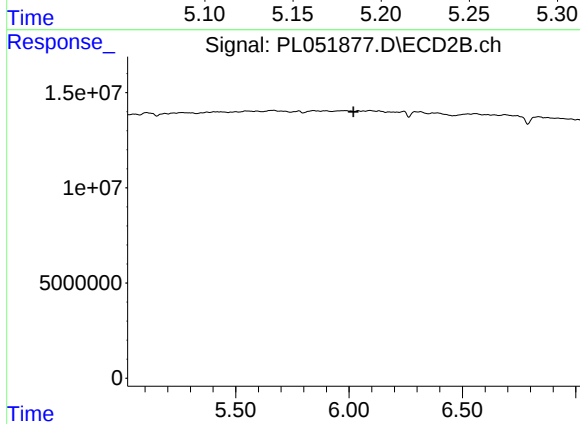

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.020 min
Response: 0
Conc: N.D.

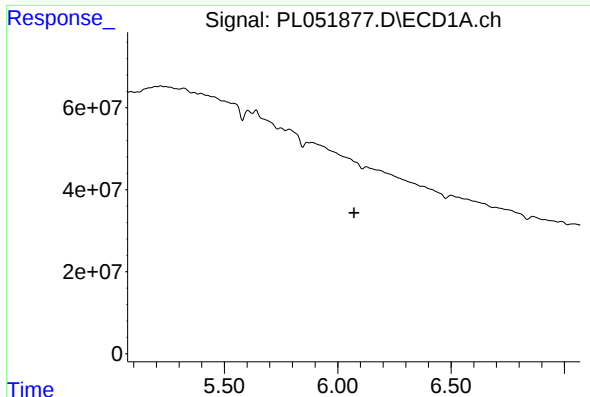

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.072 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-2-S

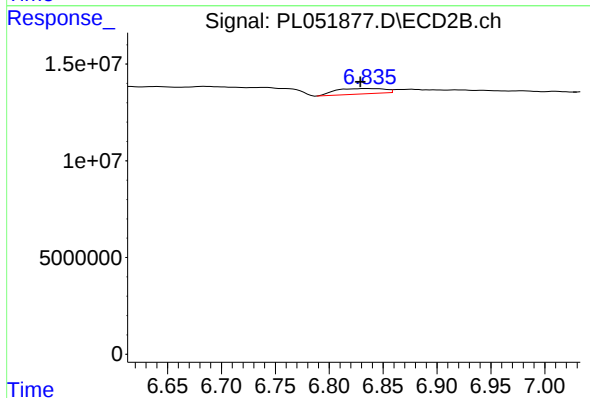


#15 Endosulfan II

R.T.: 6.836 min
Delta R.T.: 0.008 min
Response: 8965241
Conc: 2.72 ng/ml

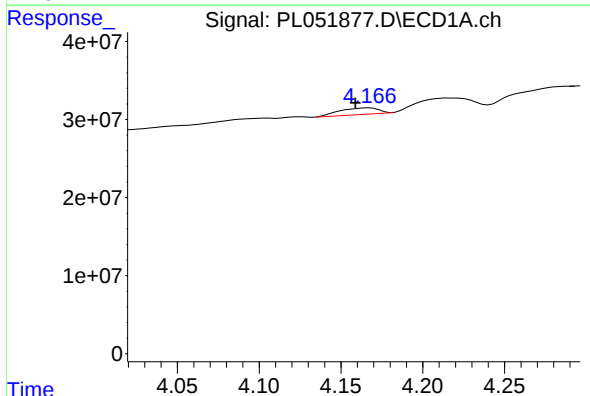


#23 Chlordane-1

R.T.: 4.167 min
Delta R.T.: 0.009 min
Response: 13651289
Conc: 42.37 ng/ml

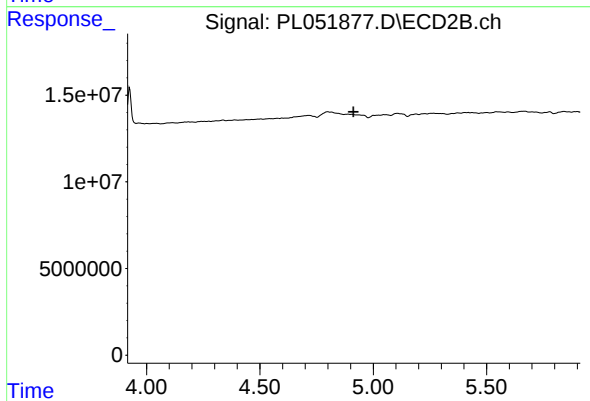

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.913 min
Response: 0
Conc: N.D.

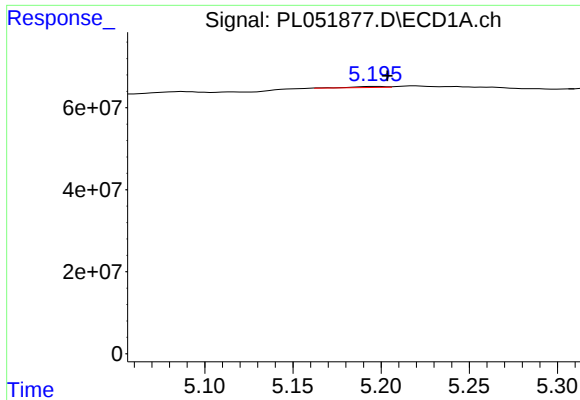

#25 Chlordane-3


R.T.: 5.197 min
Delta R.T.: -0.007 min
Response: 3116437
Conc: 2.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2-S

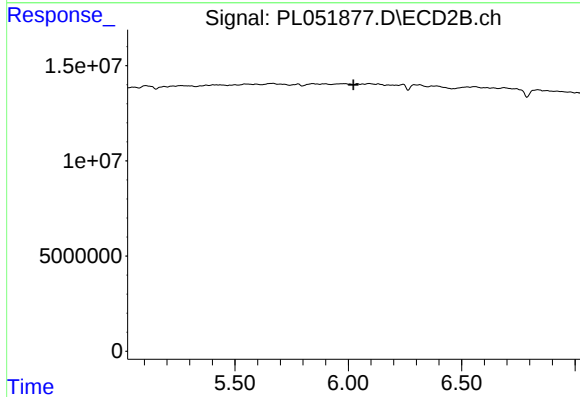


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

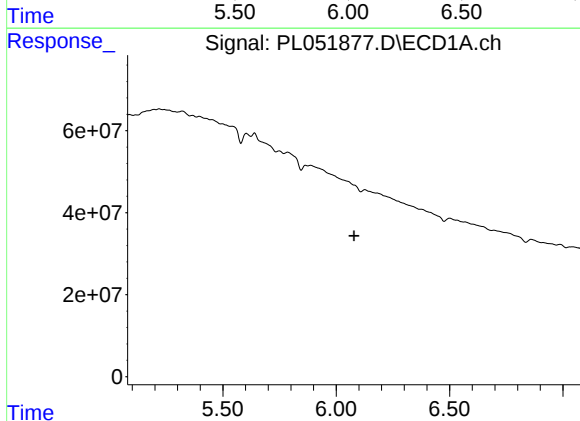


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.079 min
Response: 0
Conc: N.D.

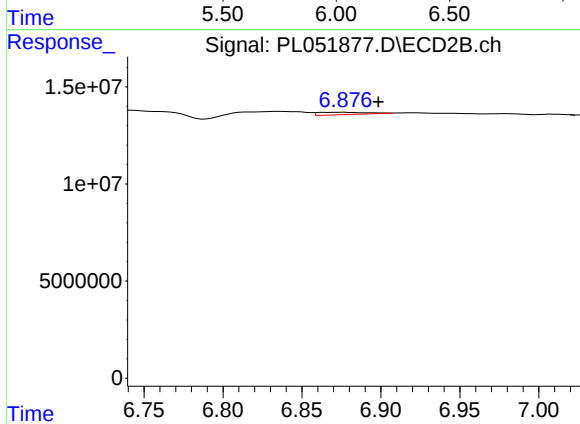

#27 Chlordane-5


R.T.: 6.877 min
Delta R.T.: -0.022 min
Response: 2538911
Conc: 25.75 ng/ml

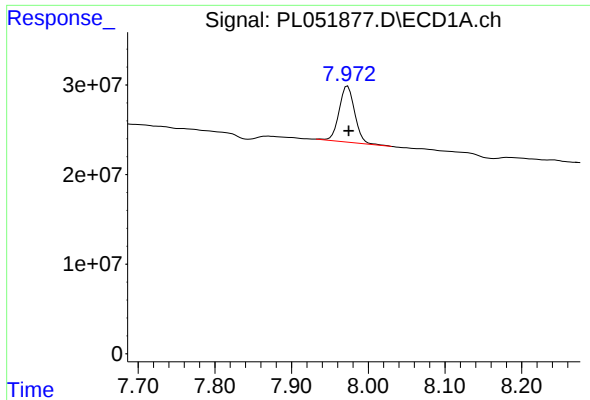

#28 Decachlorobiphenyl

R.T.: 7.973 min
Delta R.T.: -0.002 min
Response: 87922252
Conc: 7.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2-S

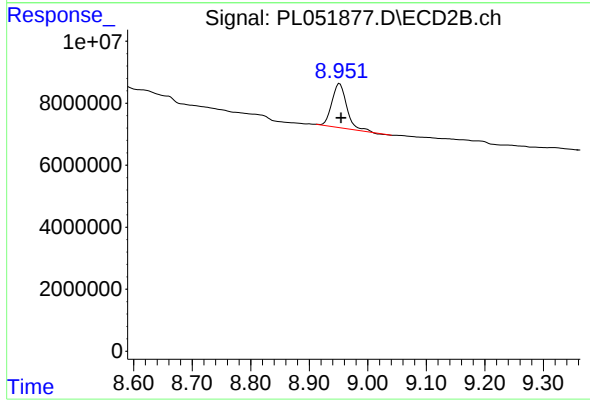

#28 Decachlorobiphenyl

R.T.: 8.952 min
Delta R.T.: -0.002 min
Response: 24532751
Conc: 8.06 ng/ml