

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082719\
 Data File : PL051878.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Aug 2019 06:54
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 07:01:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.314	3.925	187.1E6	44841505	21.863	20.524
28)	SA Decachlor...	7.973	8.953	229.5E6	61957142	18.904	20.355
Target Compounds							
6)	B beta-BHC	0.000	4.804f	0	4566040	N.D.	3.133 #
9)	A Endosulfan I	5.319	0.000	20861690	0	1.552	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082719\
Data File : PL051878.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Aug 2019 06:54
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 07:01:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

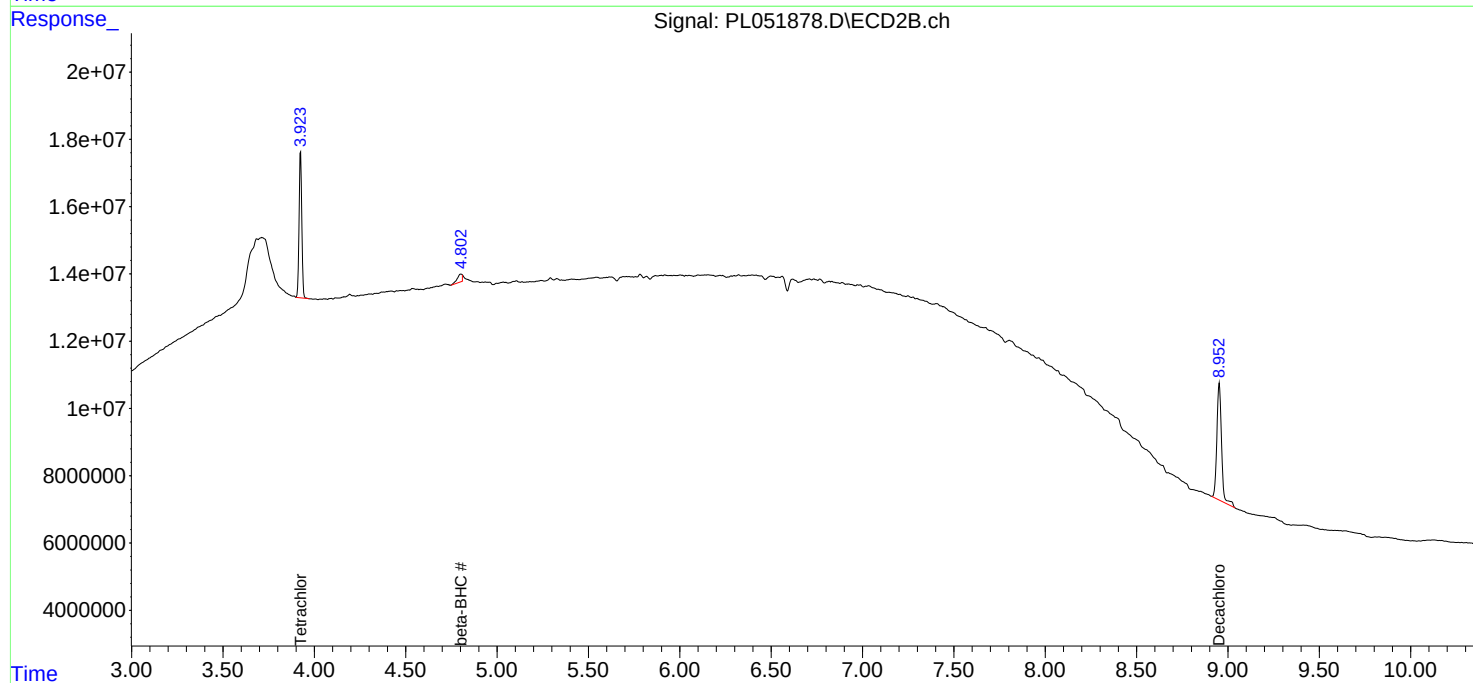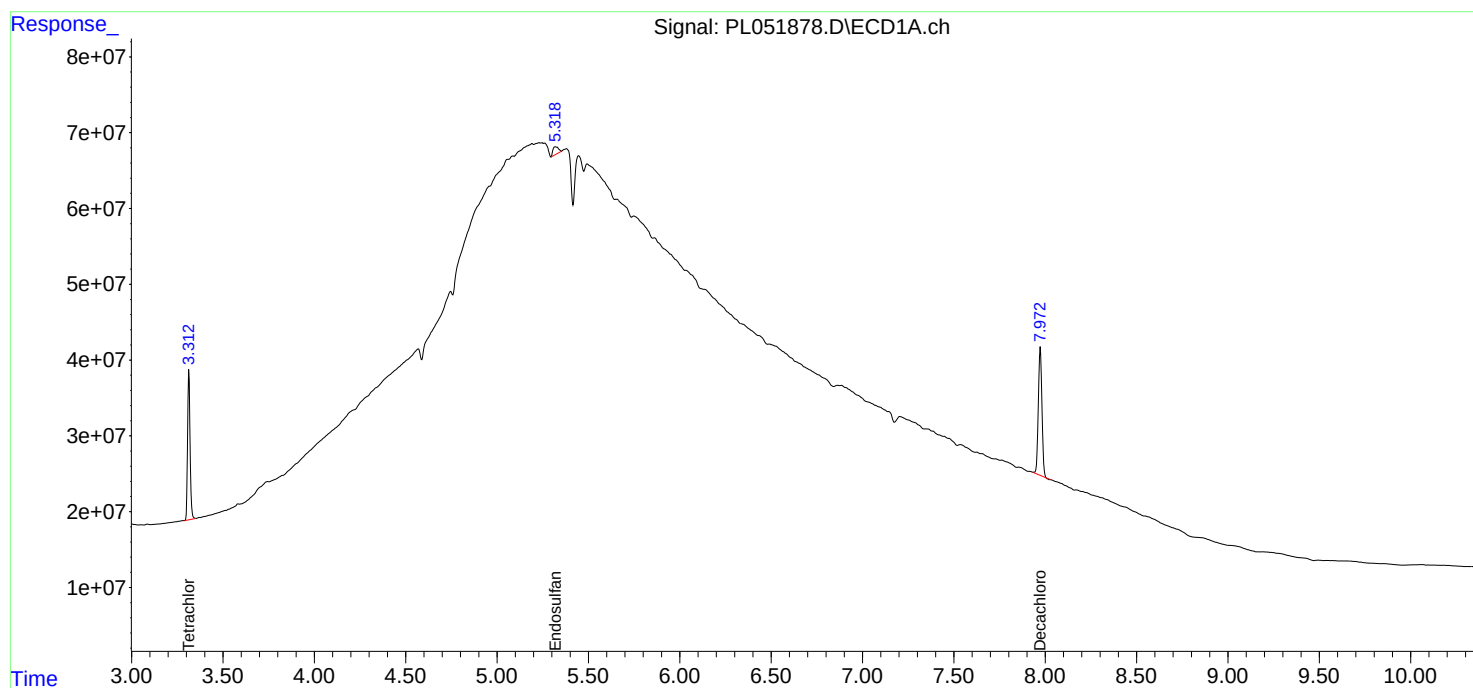


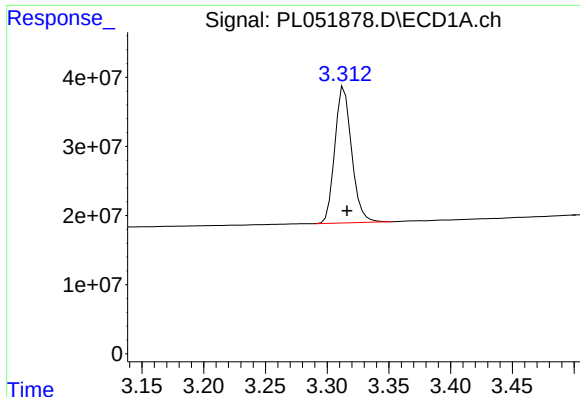

#1 Tetrachloro-m-xylene


R.T.: 3.314 min
Delta R.T.: -0.002 min
Response: 187112993
Conc: 21.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

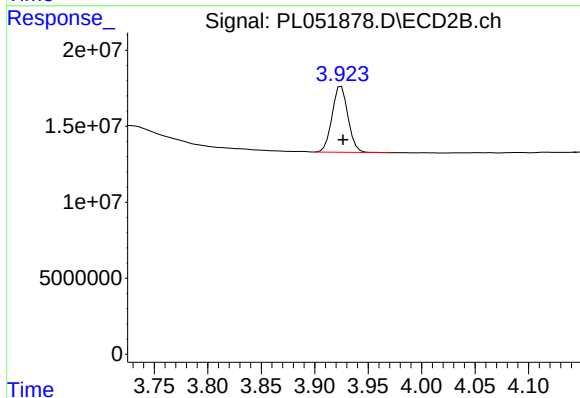


#1 Tetrachloro-m-xylene

R.T.: 3.925 min
Delta R.T.: -0.002 min
Response: 44841505
Conc: 20.52 ng/ml

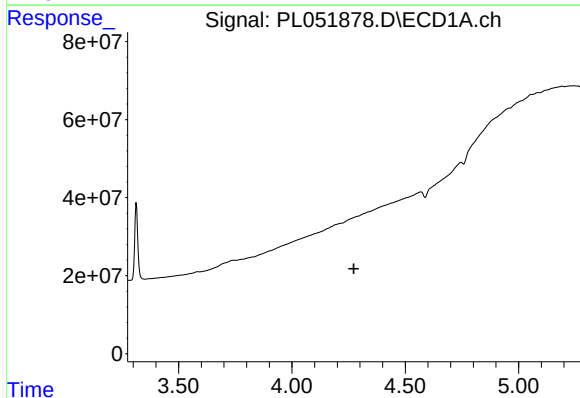


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.273 min
Response: 0
Conc: N.D.

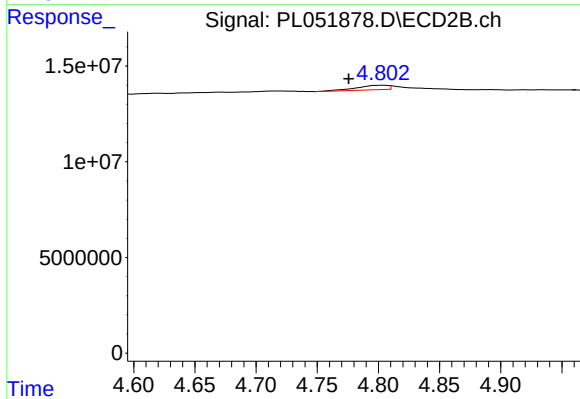

#6 beta-BHC


R.T.: 4.804 min
Delta R.T.: 0.028 min
Response: 4566040
Conc: 3.13 ng/ml

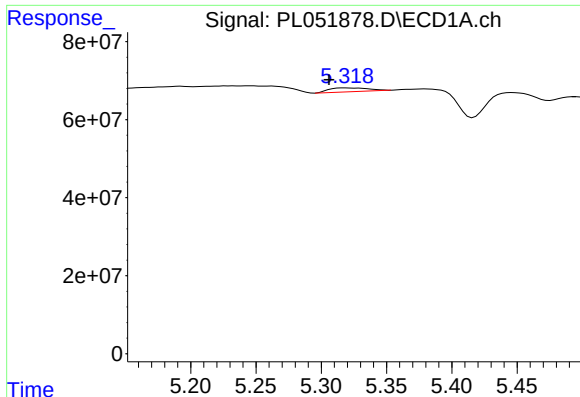

#9 Endosulfan I


R.T.: 5.319 min
Delta R.T.: 0.013 min
Response: 20861690
Conc: 1.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

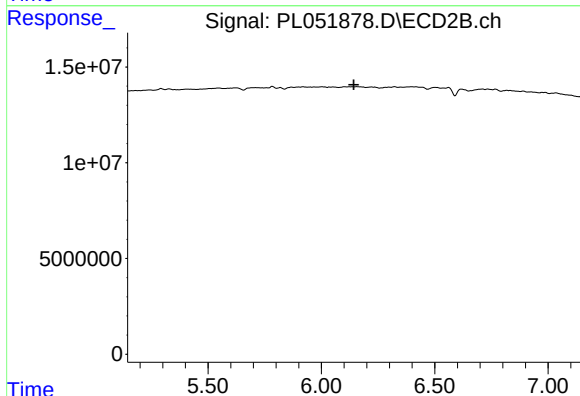


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 6.143 min
Response: 0
Conc: N.D.

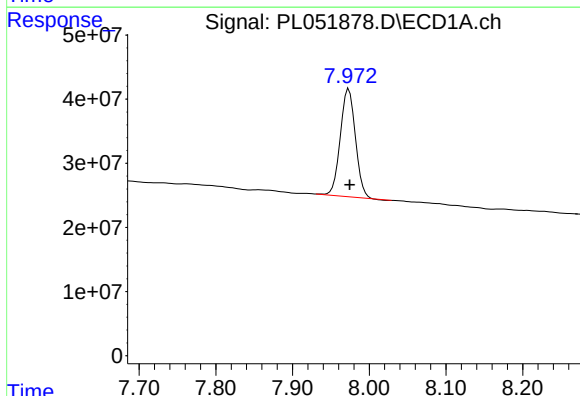

#28 Decachlorobiphenyl

R.T.: 7.973 min
Delta R.T.: -0.001 min
Response: 229451682
Conc: 18.90 ng/ml

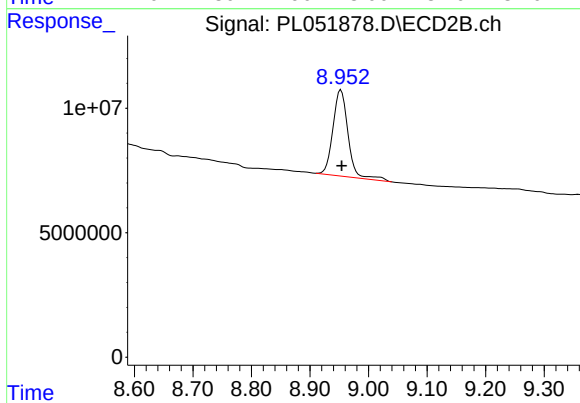

#28 Decachlorobiphenyl

R.T.: 8.953 min
Delta R.T.: -0.001 min
Response: 61957142
Conc: 20.35 ng/ml