

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082719\
 Data File : PL051810.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Aug 2019 14:34
 Operator : SG\AJ
 Sample : K4525-19
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 T9-12-13-C-(0-1.9)

Manual Integrations
 APPROVED

Ankita
 8/28/2019 5:04:03 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 00:45:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.314	3.925	204.3E6	49546216	23.875	22.678
28)	SA Decachlor...	7.973	8.952	255.0E6	60406705	21.009	19.845
Target Compounds							
17)	MA 4,4'-DDT	6.160	7.037	12159364	1293804	0.954m	0.442m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082719\
Data File : PL051810.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Aug 2019 14:34
Operator : SG\AJ
Sample : K4525-19
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
T9-12-13-C-(0-1.9)


Manual Integrations
APPROVED

Ankita
8/28/2019 5:04:03 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 00:45:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

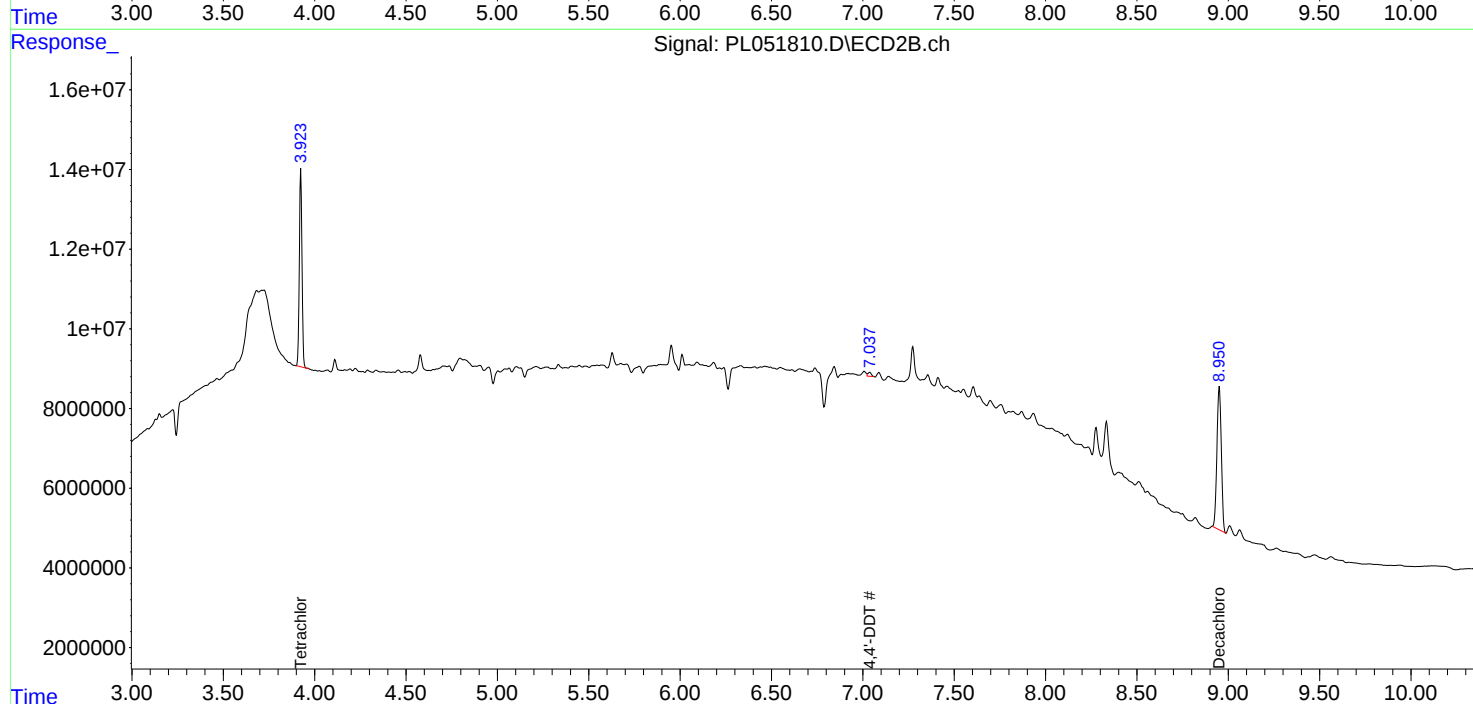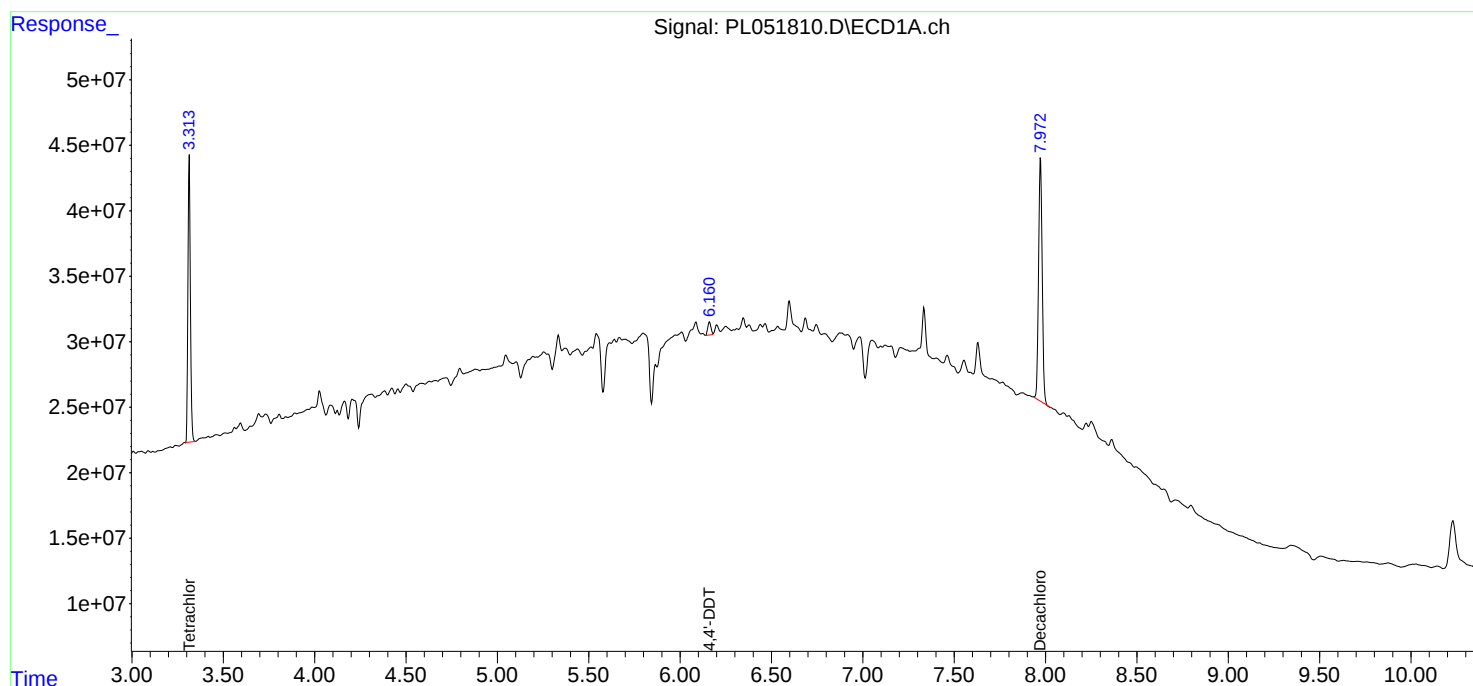

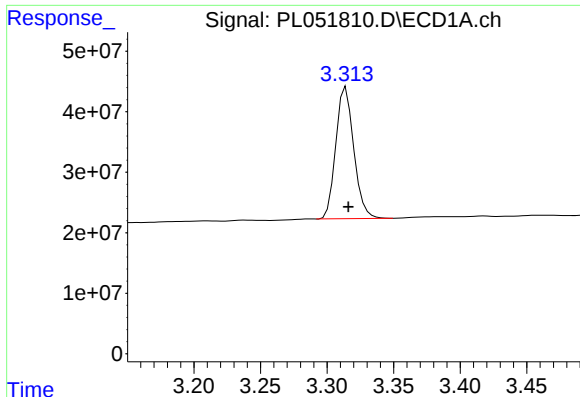


#1 Tetrachloro-m-xylene

R.T.: 3.314 min
Delta R.T.: -0.002 min
Response: 204340155
Conc: 23.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
T9-12-13-C-(0-1.9)


Manual Integrations
APPROVED

Ankita
8/28/2019 5:04:03 PM

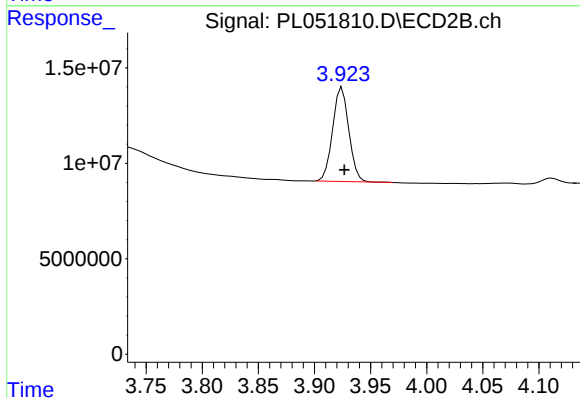


#1 Tetrachloro-m-xylene

R.T.: 3.925 min
Delta R.T.: -0.002 min
Response: 49546216
Conc: 22.68 ng/ml

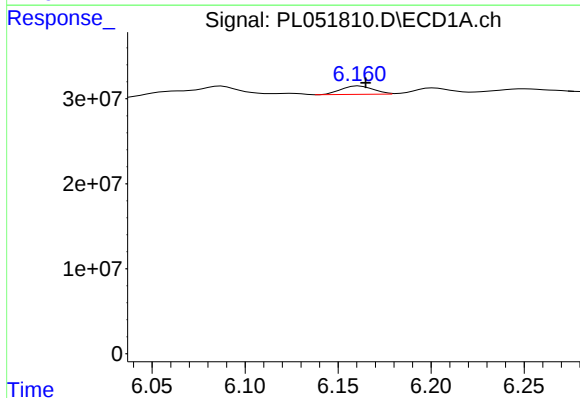


#17 4,4'-DDT

R.T.: 6.160 min
Delta R.T.: -0.005 min
Response: 12159364
Conc: 0.95 ng/ml m

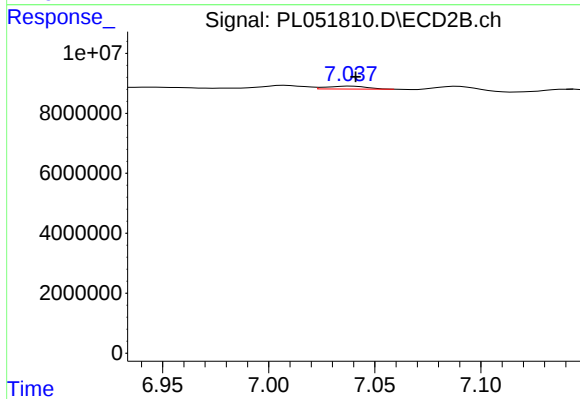

#17 4,4'-DDT

R.T.: 7.037 min
Delta R.T.: -0.004 min
Response: 1293804
Conc: 0.44 ng/ml m

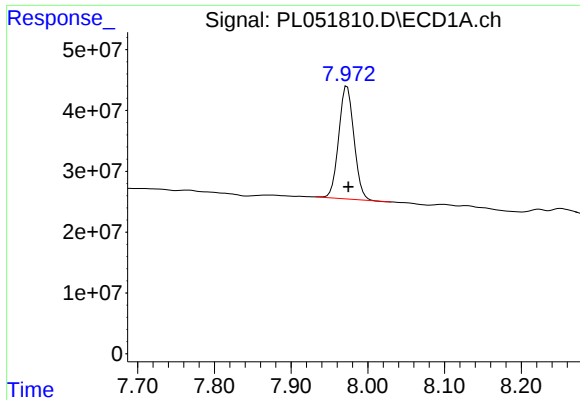


#28 Decachlorobiphenyl

R.T.: 7.973 min
Delta R.T.: -0.002 min
Response: 255005852
Conc: 21.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
T9-12-13-C-(0-1.9)

Manual Integrations
APPROVED

Ankita
8/28/2019 5:04:03 PM

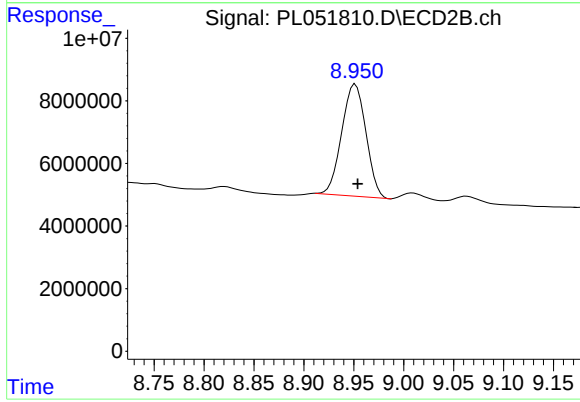

#28 Decachlorobiphenyl

R.T.: 8.952 min
Delta R.T.: -0.003 min
Response: 60406705
Conc: 19.85 ng/ml