

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082719\
 Data File : PL051821.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Aug 2019 17:28
 Operator : SG\AJ
 Sample : K4506-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RO-COMP

Manual Integrations
 APPROVED

Ankita
 8/28/2019 3:39:19 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 00:49:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.314	3.925	128.5E6	36231113	15.017	16.583
28)	SA Decachlor...	7.972	8.952	124.3E6	31927534	10.240	10.489
Target Compounds							
14)	MA Endrin	5.797	6.609	107.1E6	17251788	7.343m	5.704

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082719\
Data File : PL051821.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Aug 2019 17:28
Operator : SG\AJ
Sample : K4506-01
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
RO-COMP


Manual Integrations
APPROVED

Ankita
8/28/2019 3:39:19 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 00:49:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

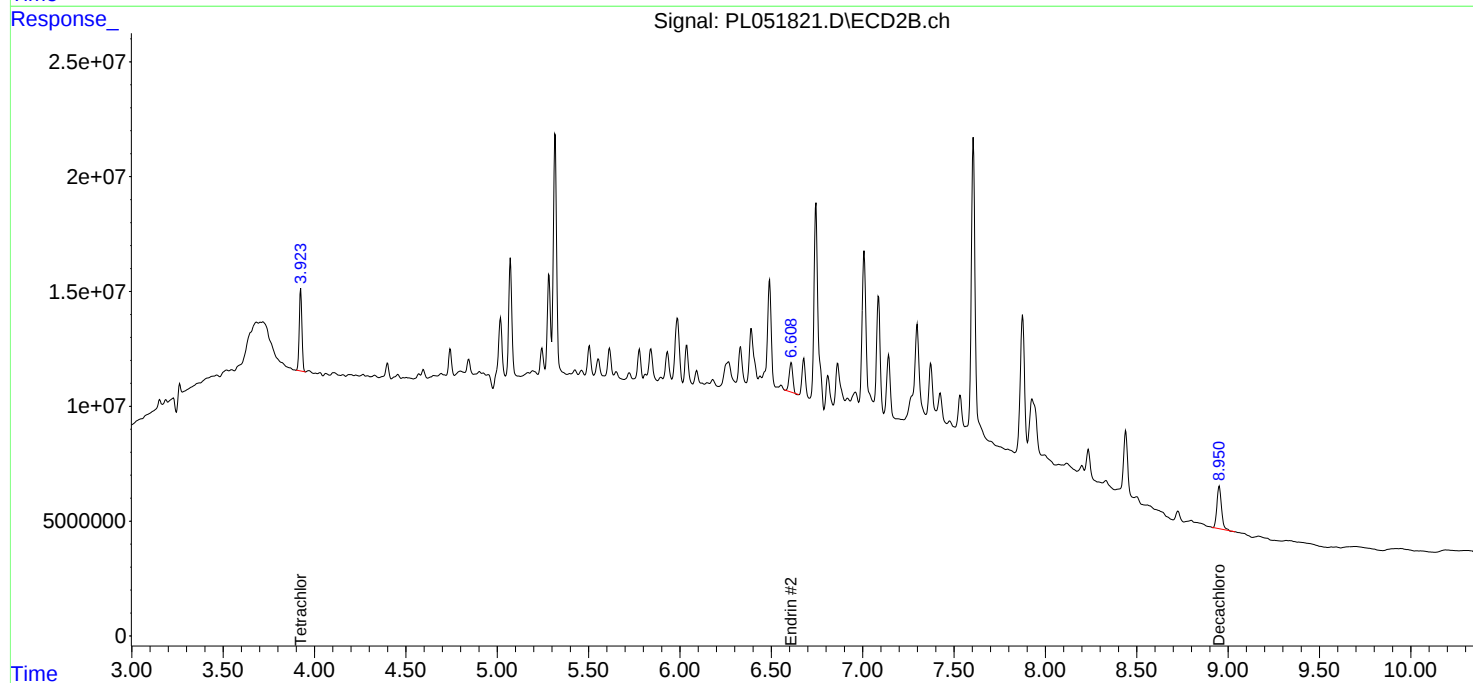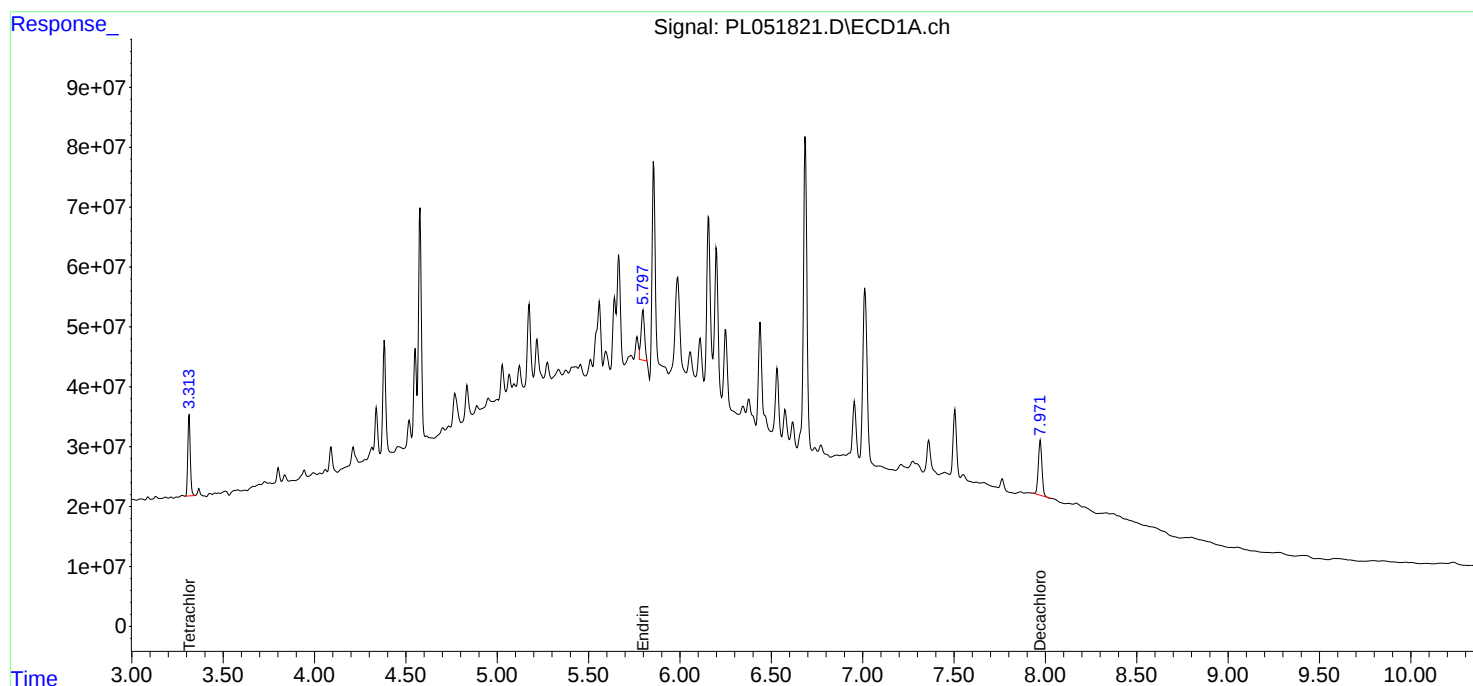

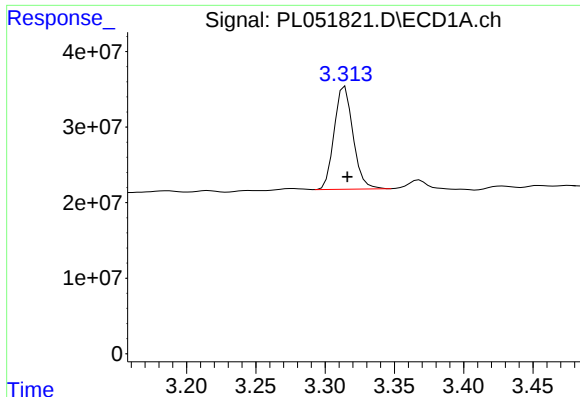


#1 Tetrachloro-m-xylene

R.T.: 3.314 min
Delta R.T.: -0.002 min
Response: 128525938
Conc: 15.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
RO-COMP


Manual Integrations
APPROVED

Ankita
8/28/2019 3:39:19 PM

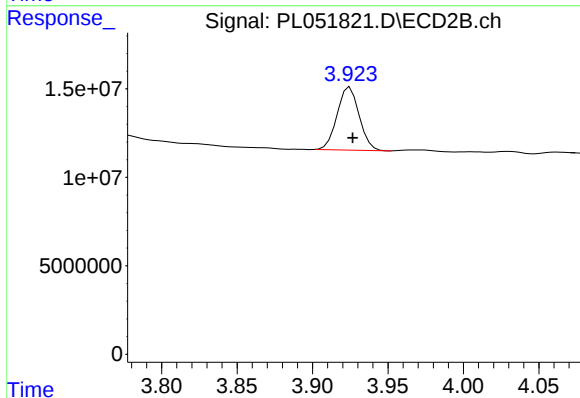


#1 Tetrachloro-m-xylene

R.T.: 3.925 min
Delta R.T.: -0.002 min
Response: 36231113
Conc: 16.58 ng/ml

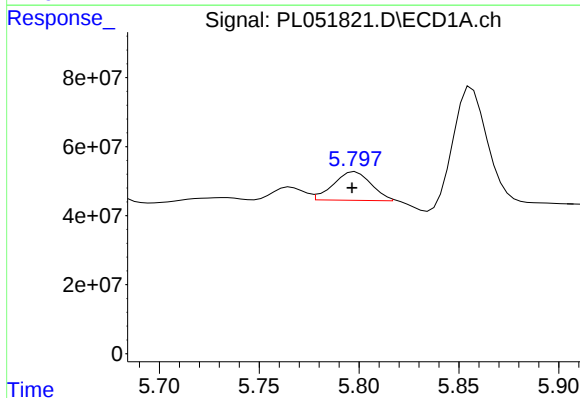


#14 Endrin

R.T.: 5.797 min
Delta R.T.: 0.000 min
Response: 107098354
Conc: 7.34 ng/ml m

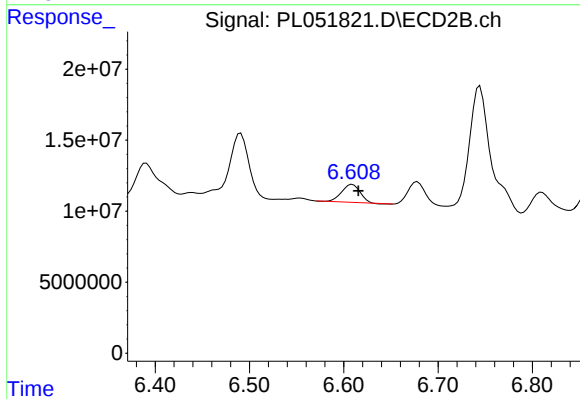

#14 Endrin

R.T.: 6.609 min
Delta R.T.: -0.007 min
Response: 17251788
Conc: 5.70 ng/ml

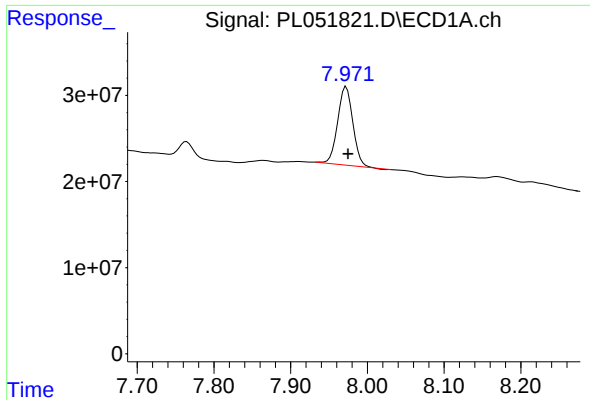


#28 Decachlorobiphenyl

R.T.: 7.972 min
Delta R.T.: -0.002 min
Response: 124294296
Conc: 10.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
RO-COMP

Manual Integrations
APPROVED

Ankita
8/28/2019 3:39:19 PM

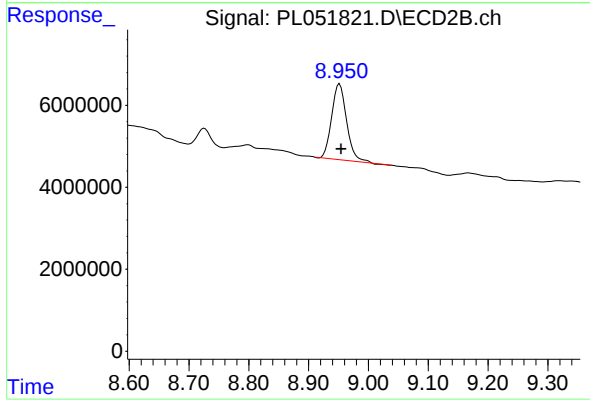

#28 Decachlorobiphenyl

R.T.: 8.952 min
Delta R.T.: -0.002 min
Response: 31927534
Conc: 10.49 ng/ml