

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082719\
 Data File : PL051865.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Aug 2019 03:51
 Operator : SG\AJ
 Sample : K4517-18
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 T4-S-E

Manual Integrations
 APPROVED

Ankita
 8/28/2019 3:41:29 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 04:23:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.314	3.925	115.8E6	31101669	13.535	14.235
28)	SA Decachlor...	7.972	8.951	190.7E6	41871068	15.714	13.756
Target Compounds							
10)	B gamma-Chl...	5.196	6.019	9248947	7203572	0.619m	1.973 #
11)	B alpha-Chl...	5.251	6.092	25071213	5809580	1.732m	1.683
14)	MA Endrin	5.801	6.610	45100100	9276559	3.092m	3.067m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082719\
Data File : PL051865.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Aug 2019 03:51
Operator : SG\AJ
Sample : K4517-18
Misc :
ALS Vial : 53 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
T4-S-E


Manual Integrations
APPROVED

Ankita
8/28/2019 3:41:29 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 04:23:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

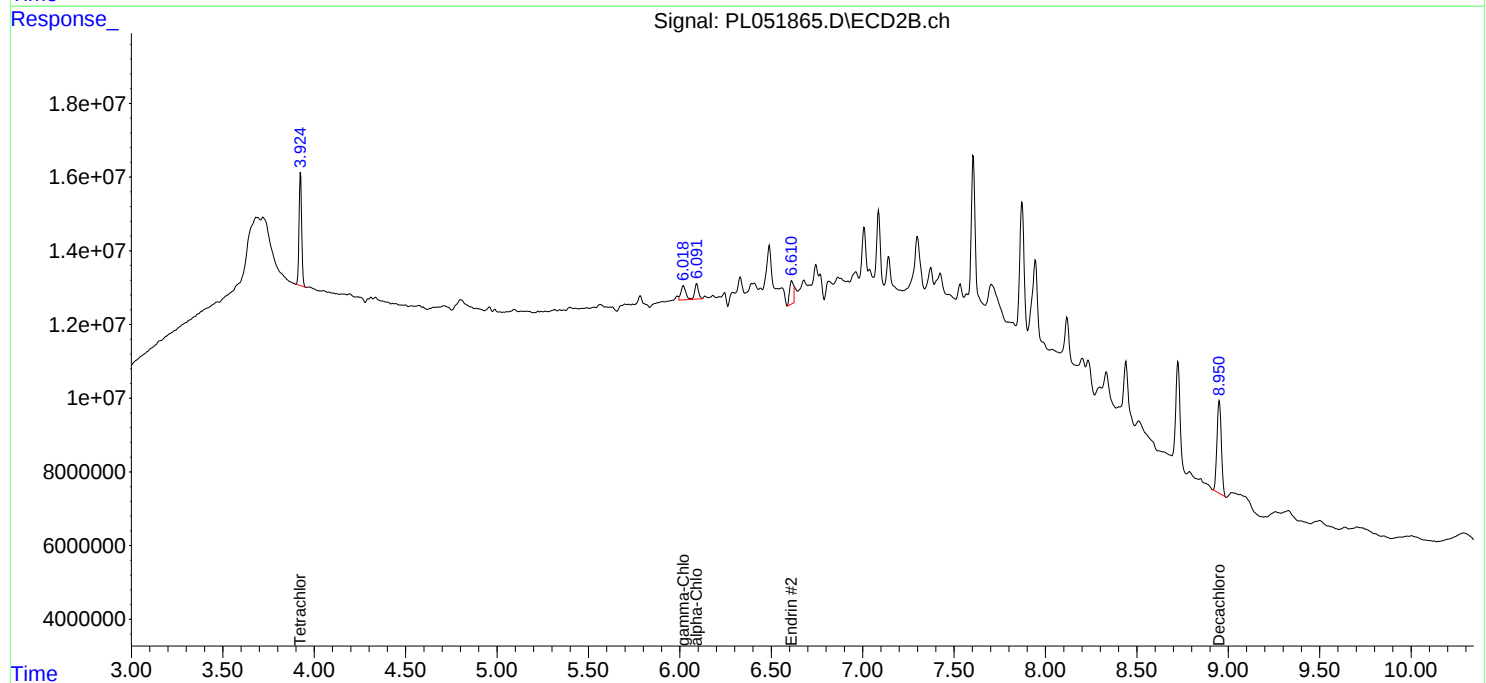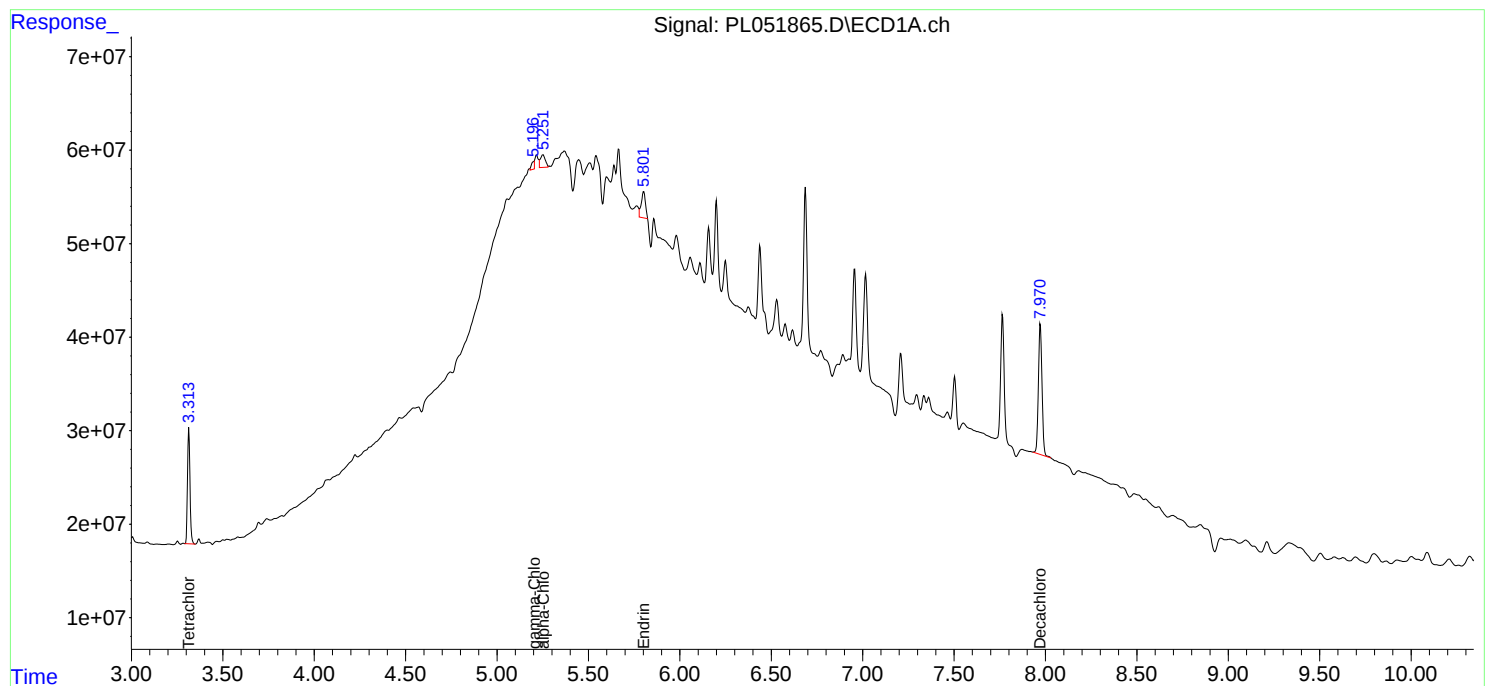

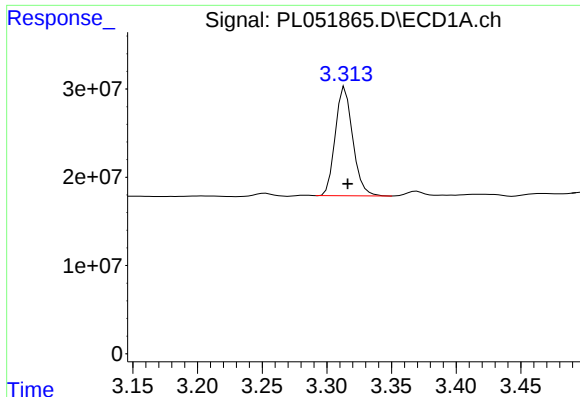


#1 Tetrachloro-m-xylene

R.T.: 3.314 min
Delta R.T.: -0.002 min
Response: 115840064
Conc: 13.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
T4-S-E


Manual Integrations
APPROVED

Ankita
8/28/2019 3:41:29 PM

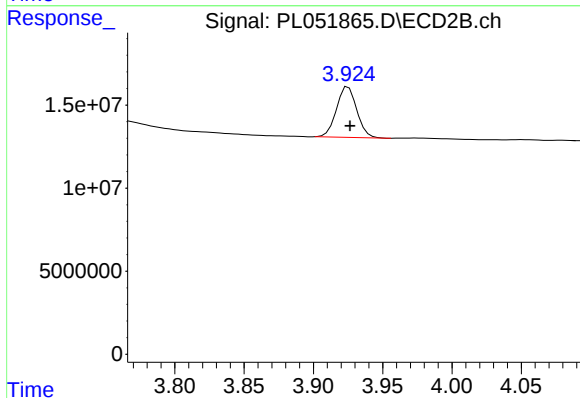


#1 Tetrachloro-m-xylene

R.T.: 3.925 min
Delta R.T.: -0.001 min
Response: 31101669
Conc: 14.24 ng/ml

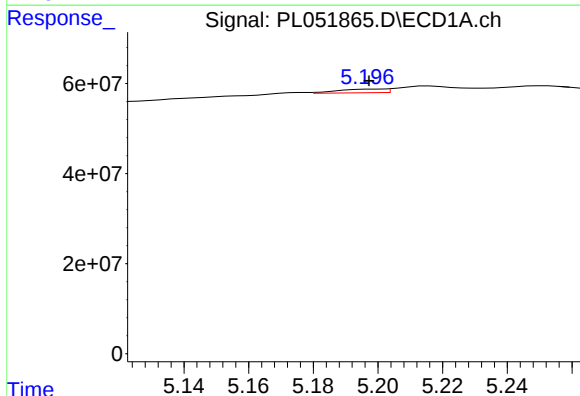


#10 gamma-Chlordane

R.T.: 5.196 min
Delta R.T.: -0.001 min
Response: 9248947
Conc: 0.62 ng/ml m

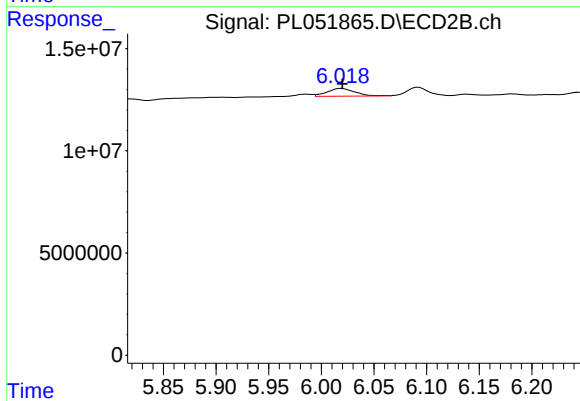

#10 gamma-Chlordane

R.T.: 6.019 min
Delta R.T.: -0.001 min
Response: 7203572
Conc: 1.97 ng/ml

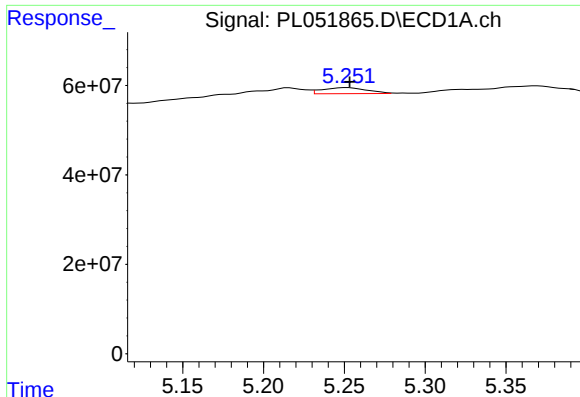


#11 alpha-Chlordane

R.T.: 5.251 min
Delta R.T.: -0.002 min
Response: 25071213
Conc: 1.73 ng/ml m

Instrument :
ECD_L
ClientSampleId :
T4-S-E


Manual Integrations
APPROVED

Ankita
8/28/2019 3:41:29 PM

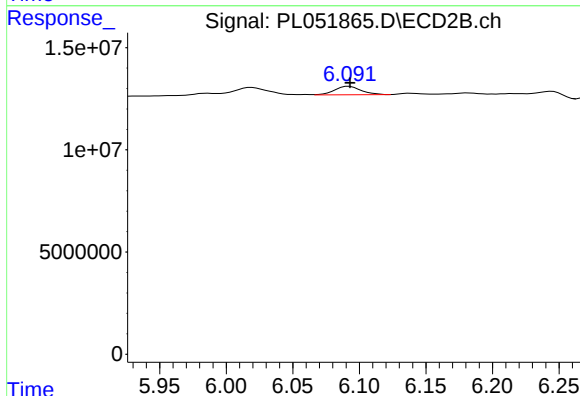


#11 alpha-Chlordane

R.T.: 6.092 min
Delta R.T.: 0.000 min
Response: 5809580
Conc: 1.68 ng/ml

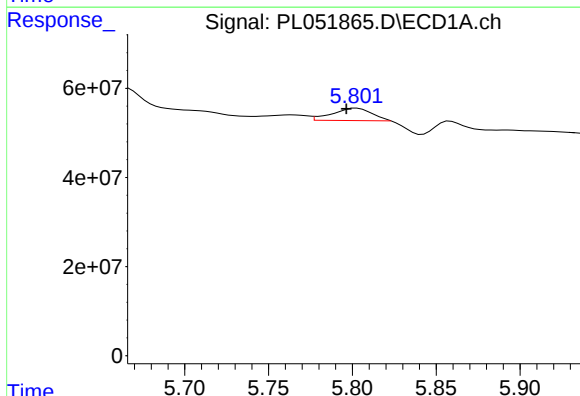


#14 Endrin

R.T.: 5.801 min
Delta R.T.: 0.005 min
Response: 45100100
Conc: 3.09 ng/ml m

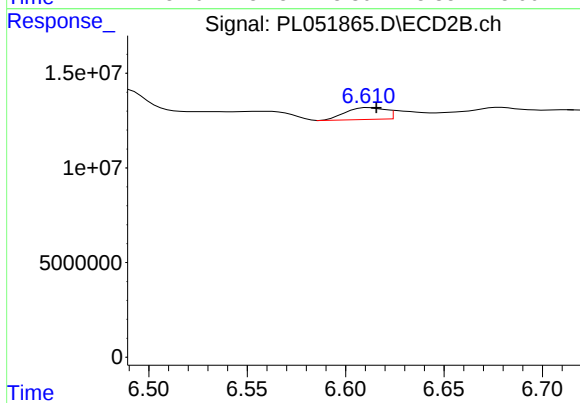

#14 Endrin

R.T.: 6.610 min
Delta R.T.: -0.005 min
Response: 9276559
Conc: 3.07 ng/ml m

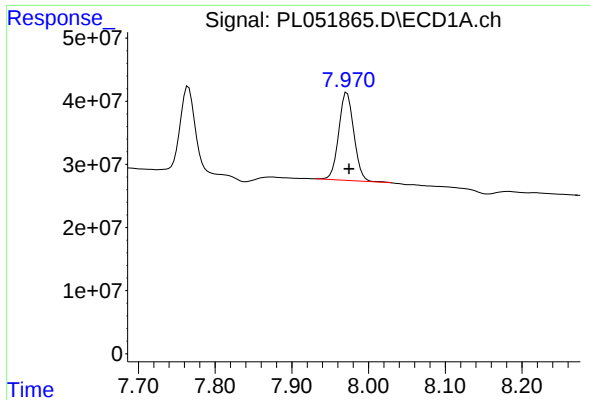


#28 Decachlorobiphenyl

R.T.: 7.972 min
Delta R.T.: -0.003 min
Response: 190730301
Conc: 15.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
T4-S-E

Manual Integrations
APPROVED

Ankita
8/28/2019 3:41:29 PM

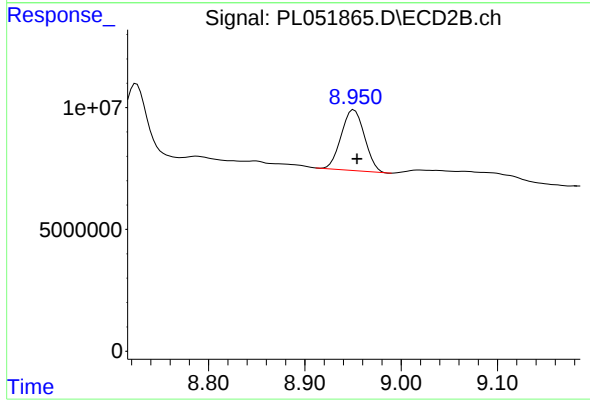

#28 Decachlorobiphenyl

R.T.: 8.951 min
Delta R.T.: -0.003 min
Response: 41871068
Conc: 13.76 ng/ml