

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082719\
 Data File : PL051880.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Aug 2019 07:54
 Operator : SG\AJ
 Sample : K4093-03 5X
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PL-02-082619

Manual Integrations
 APPROVED

Ankita
 8/28/2019 5:04:29 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 13:42:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.321	3.926	35560113	6840784	4.155	3.131
28)	SA Decachlor...	7.982	8.957	30410077	6763116	2.505	2.222
Target Compounds							
17)	MA 4,4'-DDT	6.170	7.042	10442344	3072889	0.819m	1.050 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082719\
Data File : PL051880.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Aug 2019 07:54
Operator : SG\AJ
Sample : K4093-03 5X
Misc :
ALS Vial : 66 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PL-02-082619


Manual Integrations
APPROVED

Ankita
8/28/2019 5:04:29 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 13:42:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

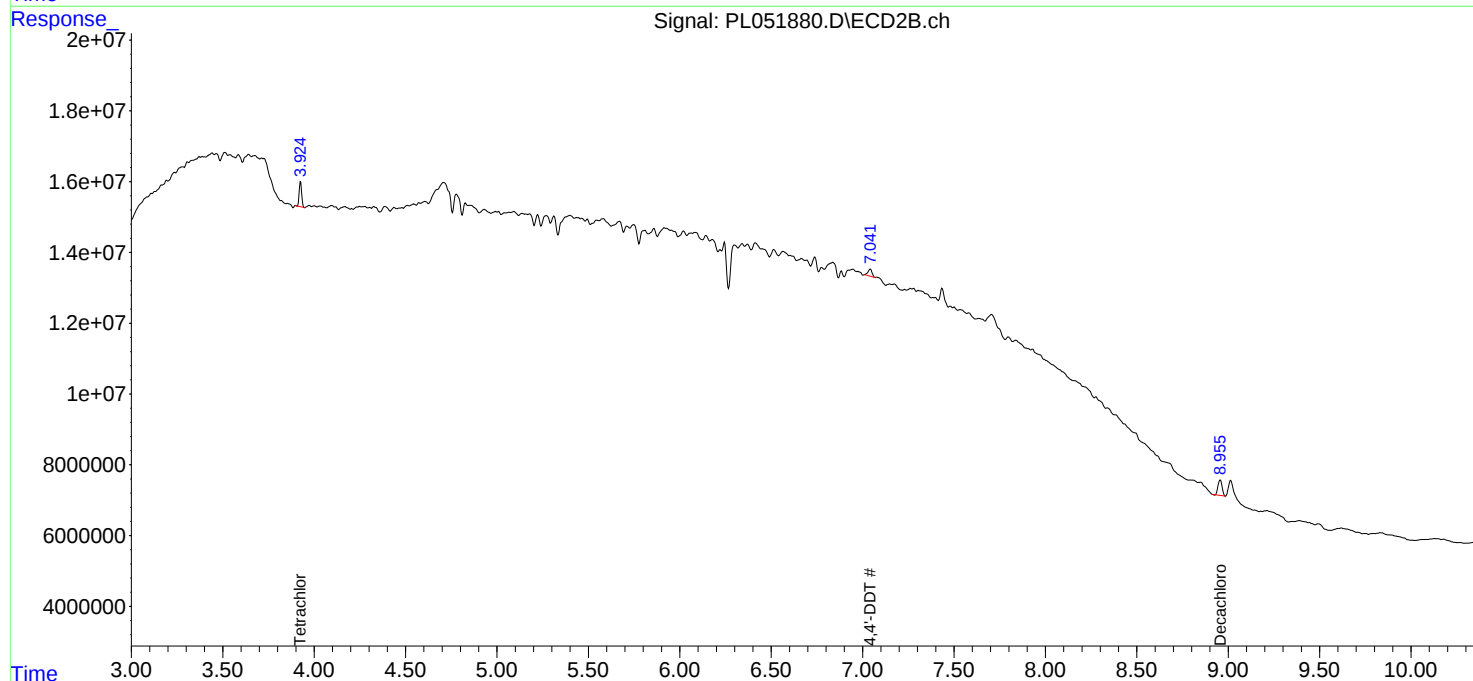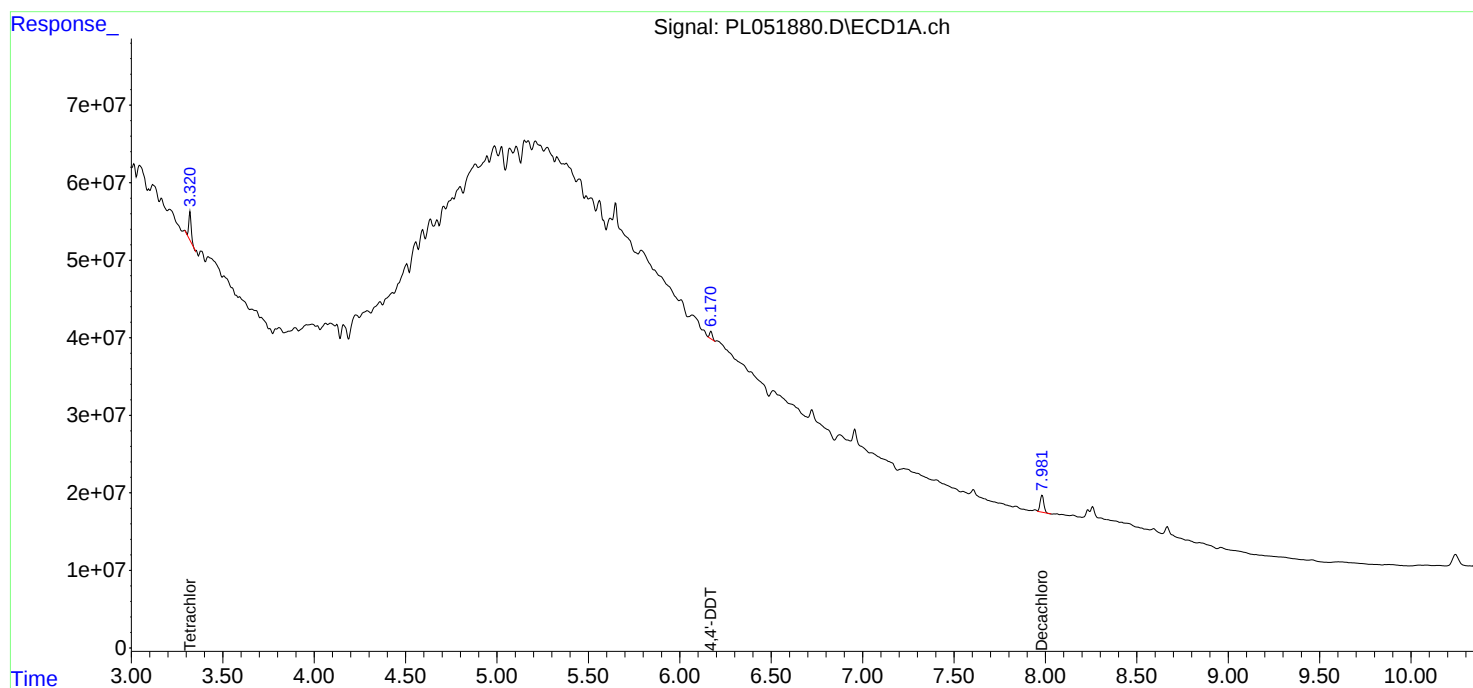

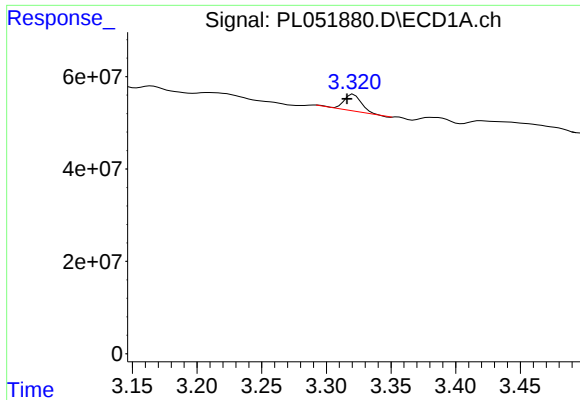


#1 Tetrachloro-m-xylene

R.T.: 3.321 min
Delta R.T.: 0.005 min
Response: 35560113
Conc: 4.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
PL-02-082619


Manual Integrations
APPROVED

Ankita
8/28/2019 5:04:29 PM

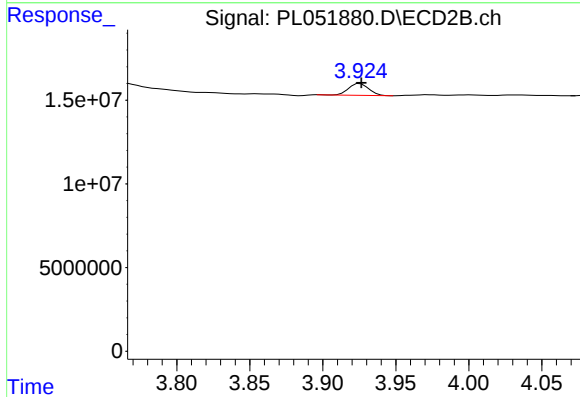


#1 Tetrachloro-m-xylene

R.T.: 3.926 min
Delta R.T.: 0.000 min
Response: 6840784
Conc: 3.13 ng/ml

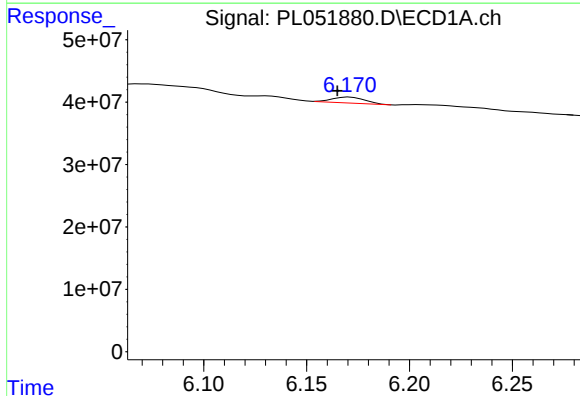


#17 4,4'-DDT

R.T.: 6.170 min
Delta R.T.: 0.005 min
Response: 10442344
Conc: 0.82 ng/ml m

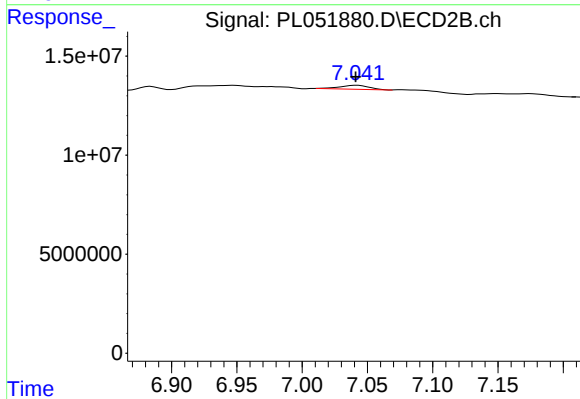

#17 4,4'-DDT

R.T.: 7.042 min
Delta R.T.: 0.001 min
Response: 3072889
Conc: 1.05 ng/ml

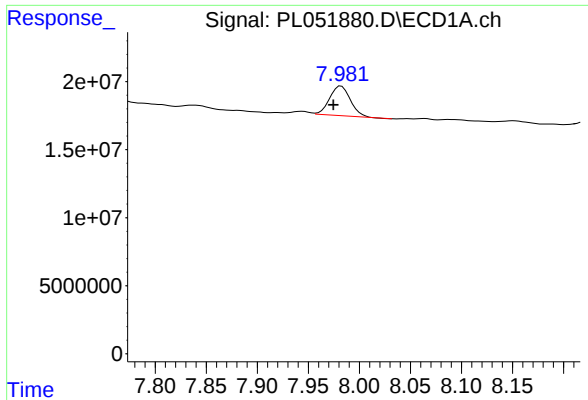


#28 Decachlorobiphenyl

R.T.: 7.982 min
Delta R.T.: 0.008 min
Response: 30410077
Conc: 2.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
PL-02-082619

Manual Integrations
APPROVED

Ankita
8/28/2019 5:04:29 PM

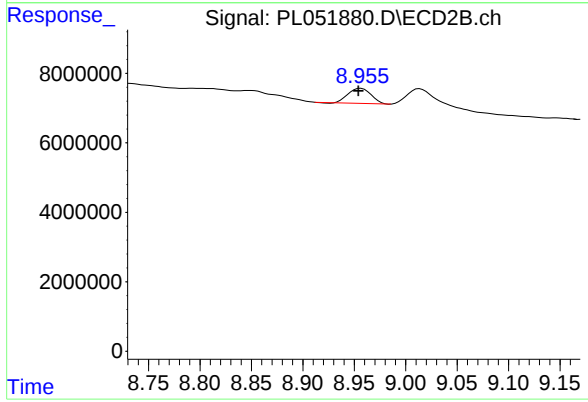

#28 Decachlorobiphenyl

R.T.: 8.957 min
Delta R.T.: 0.002 min
Response: 6763116
Conc: 2.22 ng/ml