

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082724\
 Data File : PL091355.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Aug 2024 18:32
 Operator : AR\AJ
 Sample : P3737-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-3

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/28/2024
 Supervised By :Ankita Jodhani 08/28/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 05:35:46 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081324.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 14 13:09:19 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	2.785	45279081	46608367	21.088	23.877
2)	SA Decachlor...	9.055	7.921	31632698	37733106	20.749	19.921
Target Compounds							
18)	B Endrin al...	6.923	6.120	852879	856404	0.534m	0.550

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082724\
Data File : PL091355.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Aug 2024 18:32
Operator : AR\AJ
Sample : P3737-03
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
COMP-3


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 08/28/2024
Supervised By : Ankita Jodhani 08/28/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 05:35:46 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081324.M
Quant Title : GC Extractables
QLast Update : Wed Aug 14 13:09:19 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

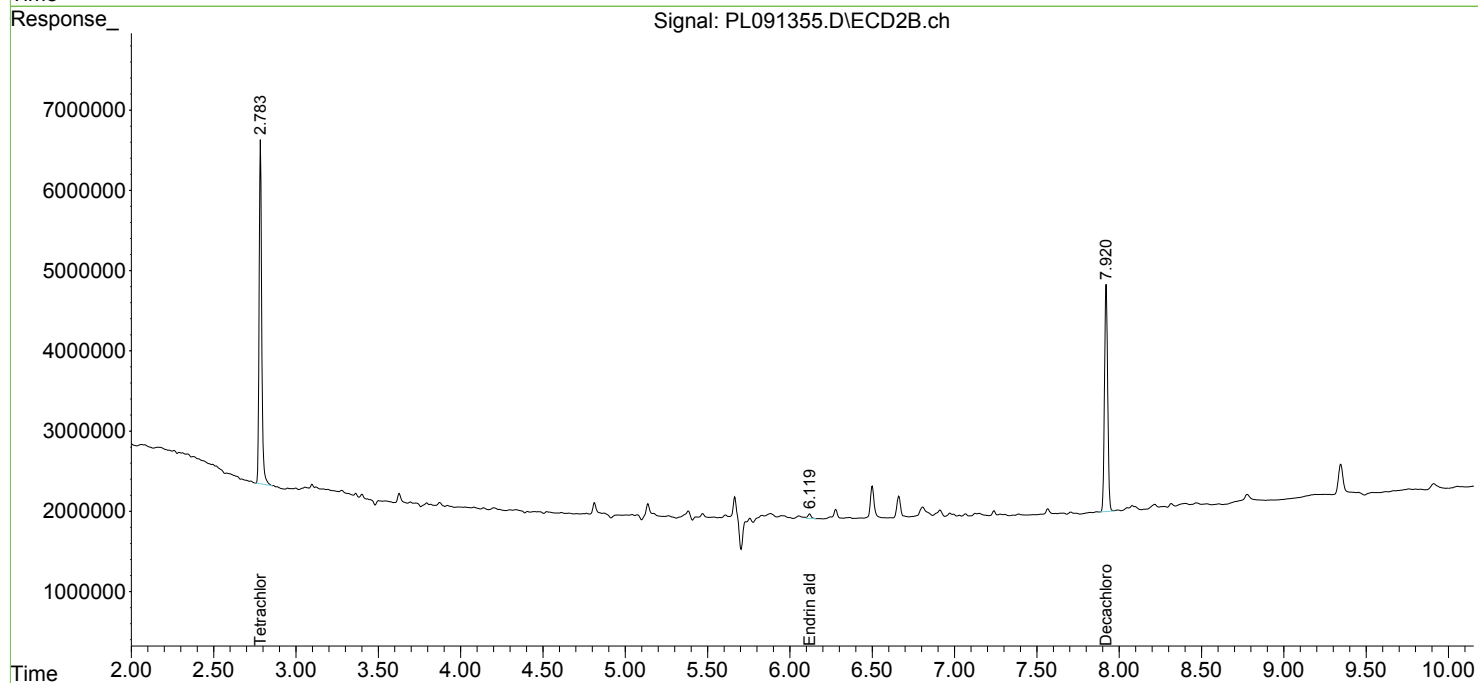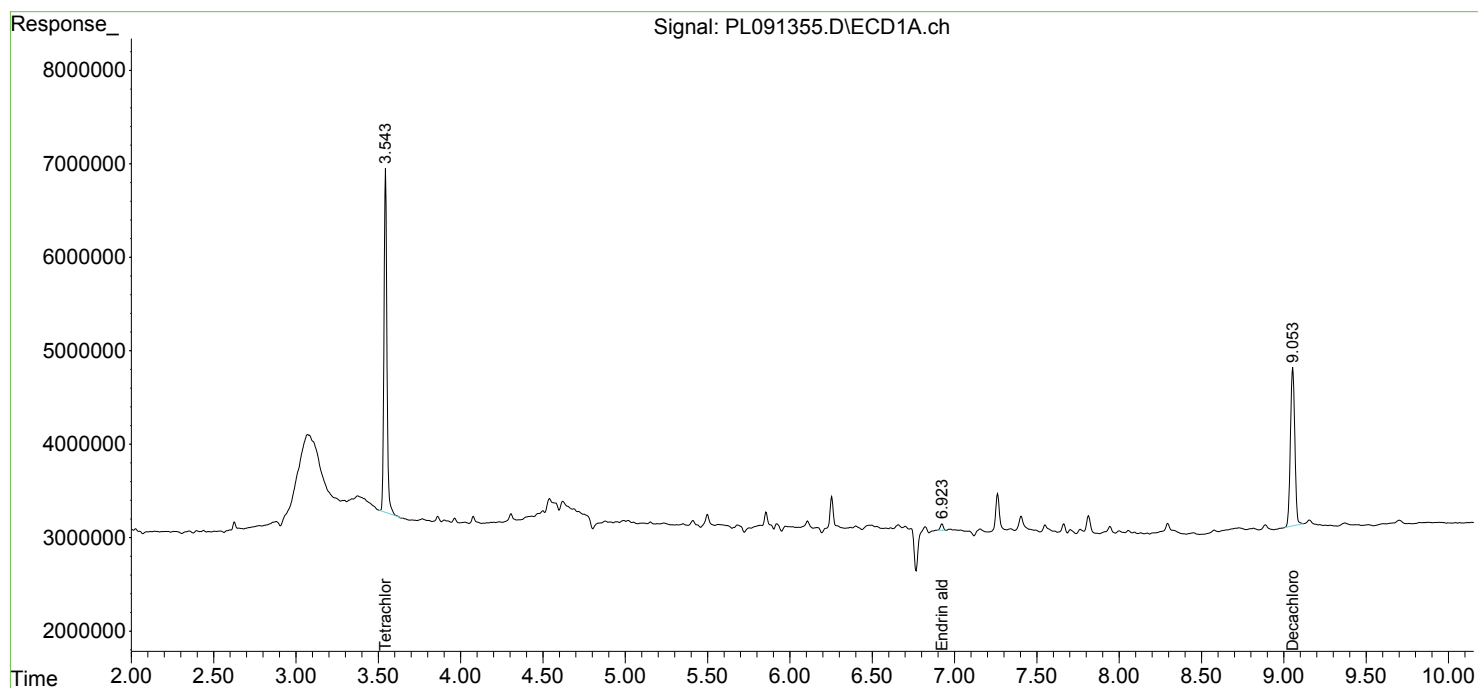

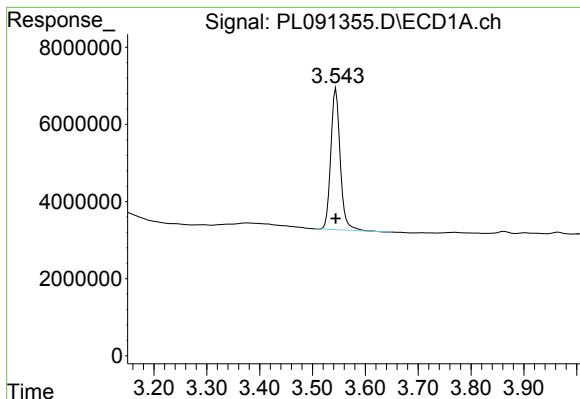


#1 Tetrachloro-m-xylene

R.T.: 3.544 min
Delta R.T.: 0.000 min
Response: 45279081
Conc: 21.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-3


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/28/2024
Supervised By :Ankita Jodhani 08/28/2024

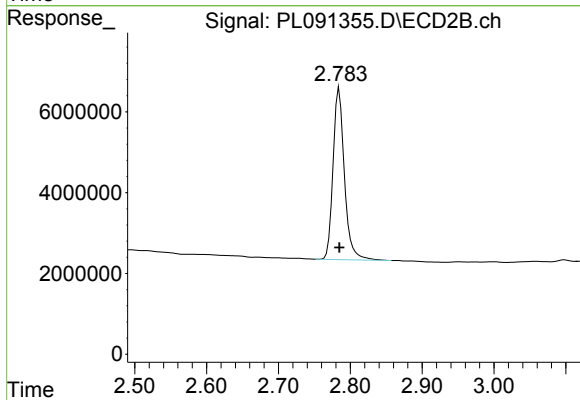


#1 Tetrachloro-m-xylene

R.T.: 2.785 min
Delta R.T.: 0.000 min
Response: 46608367
Conc: 23.88 ng/ml

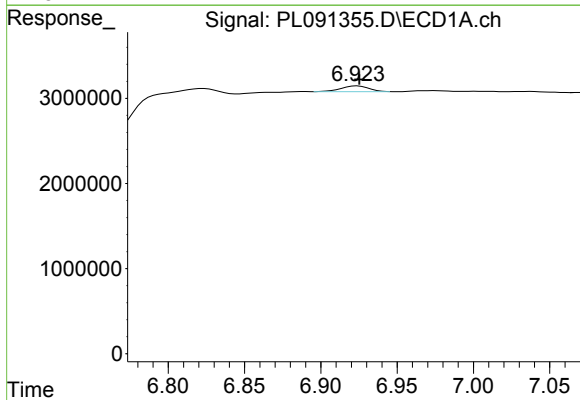


#18 Endrin aldehyde

R.T.: 6.923 min
Delta R.T.: -0.003 min
Response: 852879
Conc: 0.53 ng/ml m

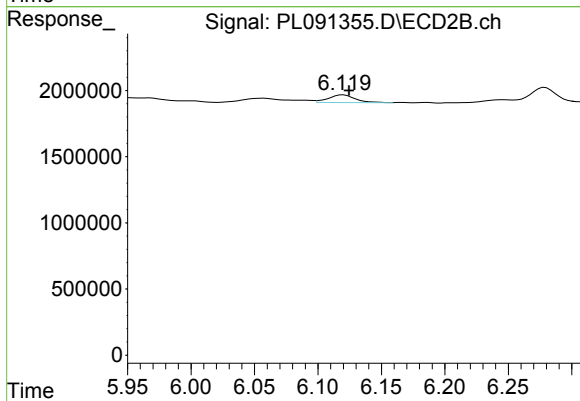

#18 Endrin aldehyde

R.T.: 6.120 min
Delta R.T.: -0.004 min
Response: 856404
Conc: 0.55 ng/ml

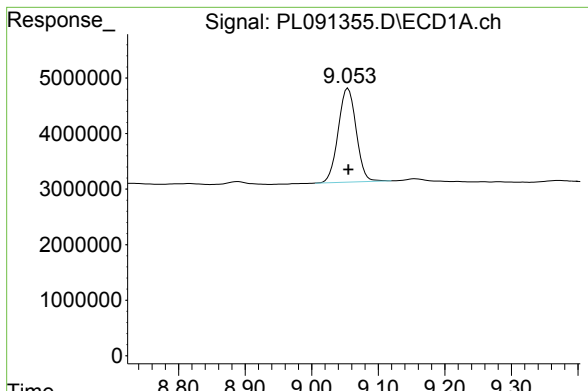


#28 Decachlorobiphenyl

R.T.: 9.055 min
Delta R.T.: 0.000 min
Response: 31632698
Conc: 20.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-3

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/28/2024
Supervised By :Ankita Jodhani 08/28/2024

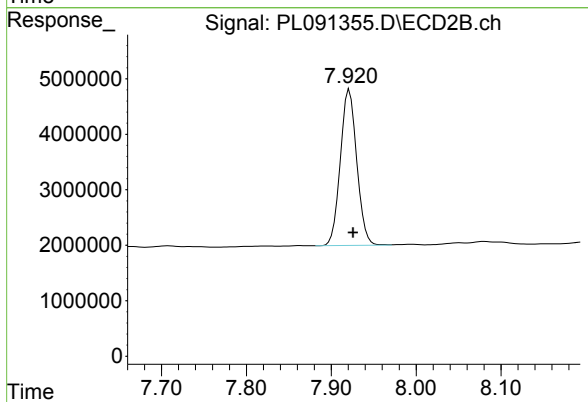

#28 Decachlorobiphenyl

R.T.: 7.921 min
Delta R.T.: -0.005 min
Response: 37733106
Conc: 19.92 ng/ml