

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082818\
 Data File : PL039557.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Aug 2018 14:34
 Operator : AJ\SJ
 Sample : PB112431BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 29 00:57:47 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.304	3.906	146.3E6	62312301	20.931	23.243
28)	SA Decachlor...	7.958	8.892	141.0E6	56593346	20.082	24.387
Target Compounds							
6)	B beta-BHC	4.216f	0.000	14471435	0	3.115	N.D. #
8)	B Heptachlo...	4.916f	0.000	2765100	0	0.290	N.D. #
9)	A Endosulfan I	5.254f	0.000	7035207	0	0.803	N.D. #
10)	B gamma-Chl...	5.254f	0.000	7035207	0	0.712	N.D. #
11)	B alpha-Chl...	5.254	0.000	7035207	0	0.732	N.D. #
25)	Chlordane-3	5.254	0.000	7035207	0	6.441	N.D. #
26)	Chlordane-4	5.254	0.000	7035207	0	7.040	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082818\
Data File : PL039557.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Aug 2018 14:34
Operator : AJ\SJ
Sample : PB112431BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 29 00:57:47 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

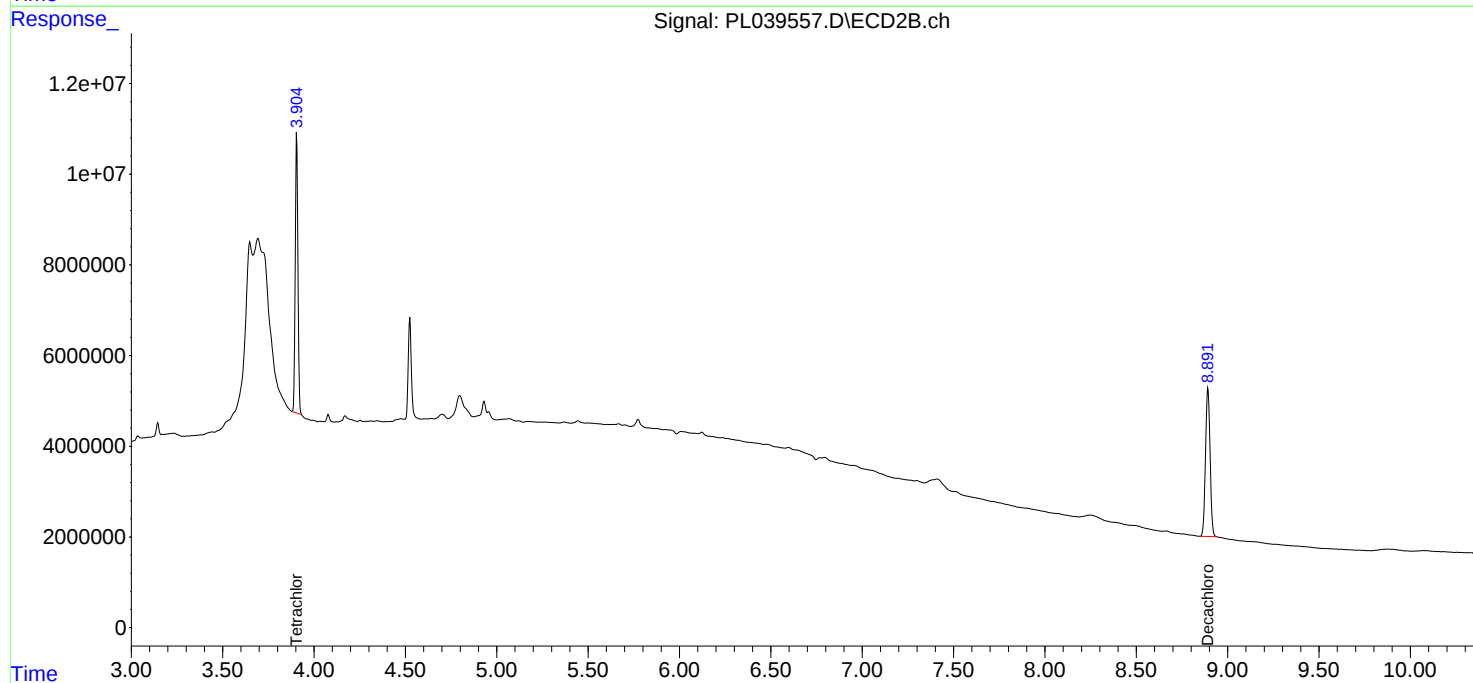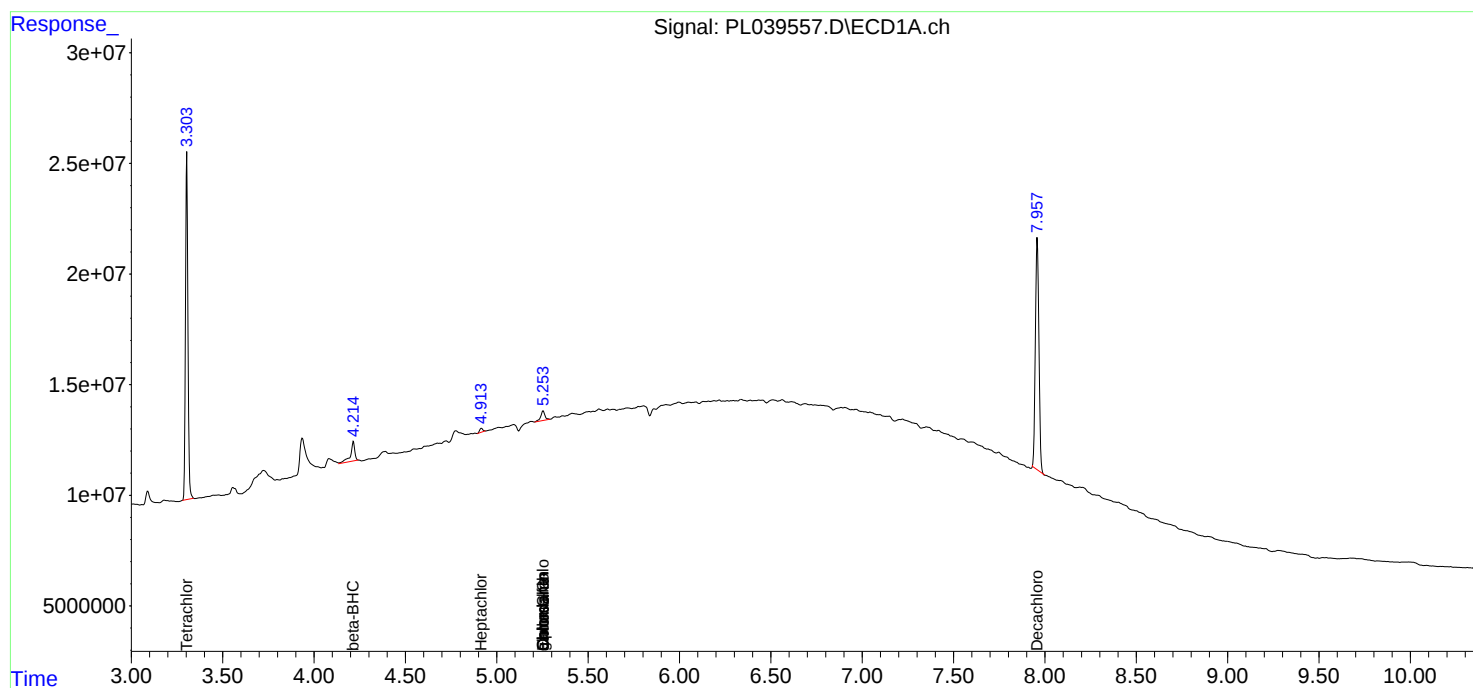


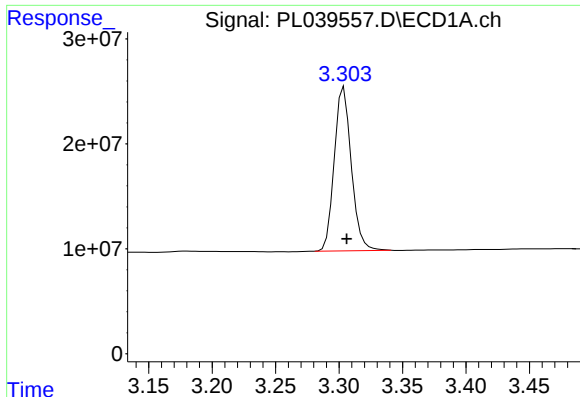

#1 Tetrachloro-m-xylene


R.T.: 3.304 min
Delta R.T.: -0.002 min
Response: 146318748
Conc: 20.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

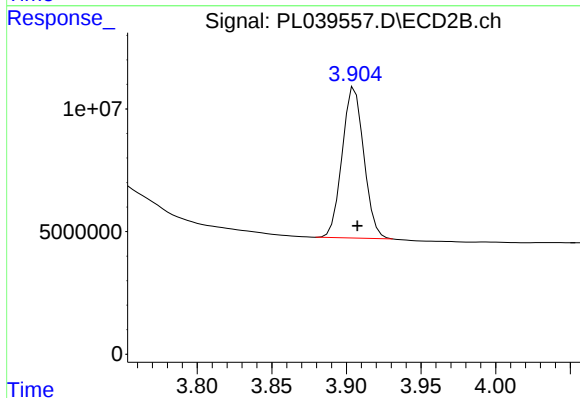


#1 Tetrachloro-m-xylene

R.T.: 3.906 min
Delta R.T.: -0.002 min
Response: 62312301
Conc: 23.24 ng/ml

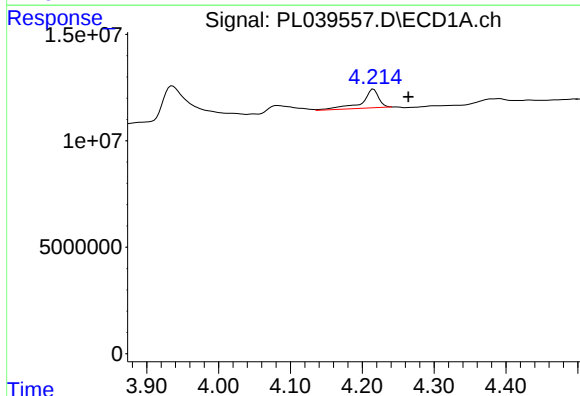


#6 beta-BHC

R.T.: 4.216 min
Delta R.T.: -0.048 min
Response: 14471435
Conc: 3.12 ng/ml

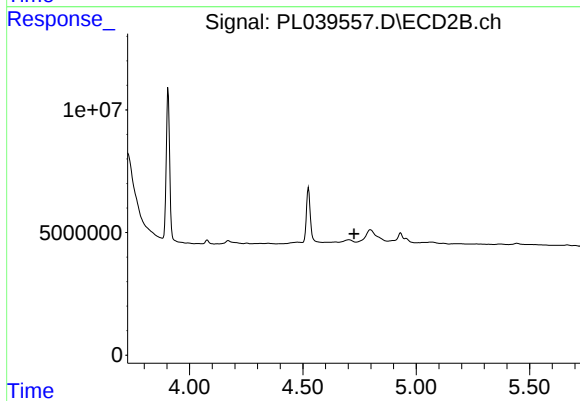

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

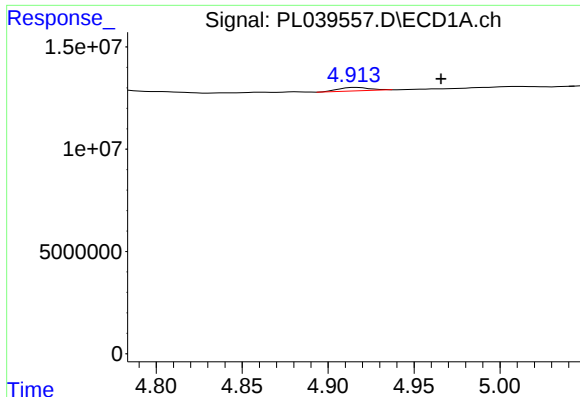

#8 Heptachlor epoxide


R.T.: 4.916 min
Delta R.T.: -0.049 min
Response: 2765100
Conc: 0.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

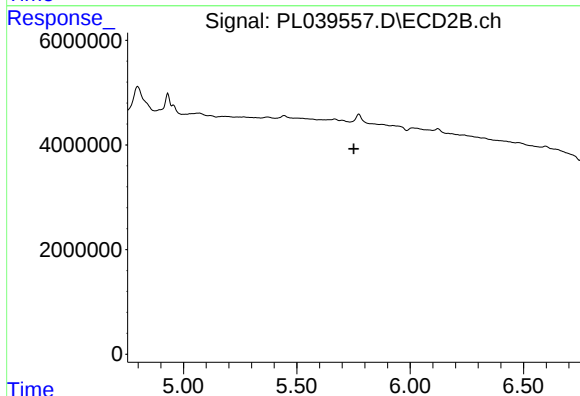


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.751 min
Response: 0
Conc: N.D.

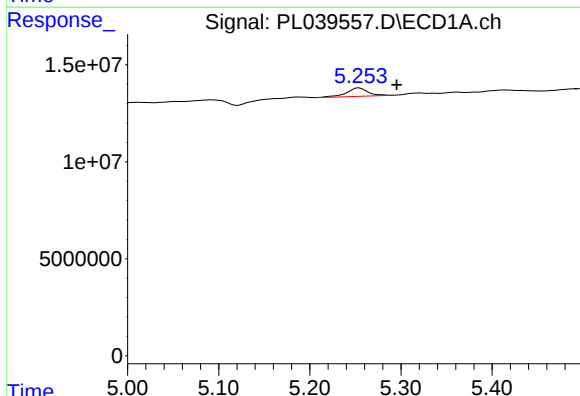


#9 Endosulfan I

R.T.: 5.254 min
Delta R.T.: -0.041 min
Response: 7035207
Conc: 0.80 ng/ml

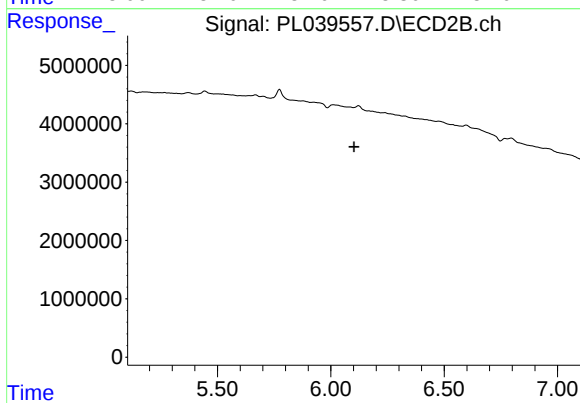

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.102 min
Response: 0
Conc: N.D.

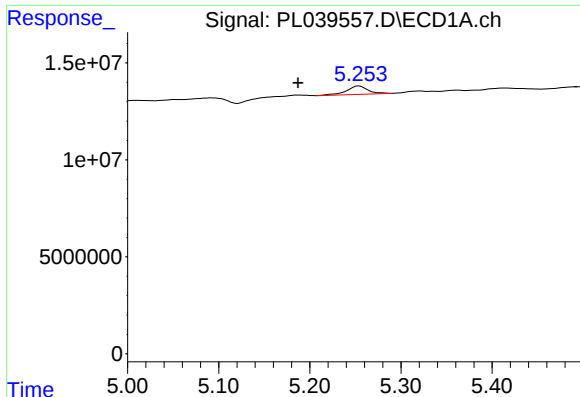

#10 gamma-Chlordane


R.T.: 5.254 min
Delta R.T.: 0.067 min
Response: 7035207
Conc: 0.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

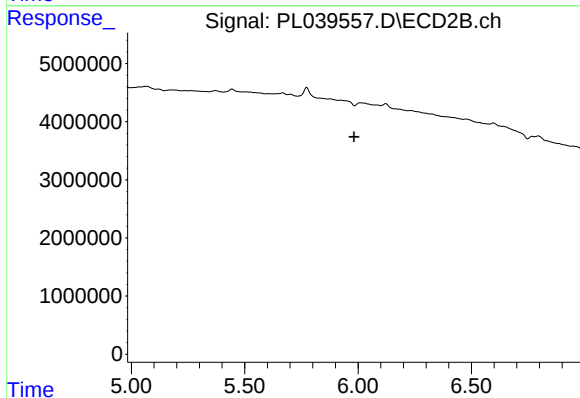


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

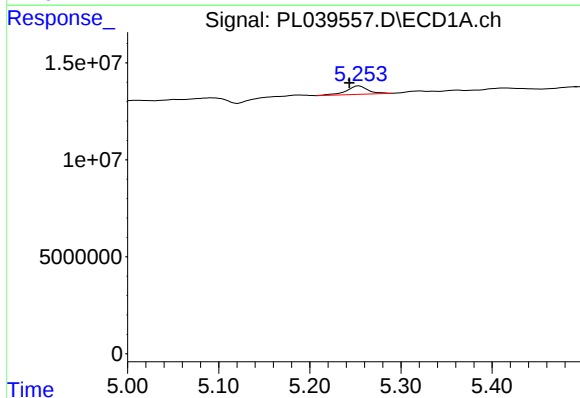


#11 alpha-Chlordane

R.T.: 5.254 min
Delta R.T.: 0.011 min
Response: 7035207
Conc: 0.73 ng/ml

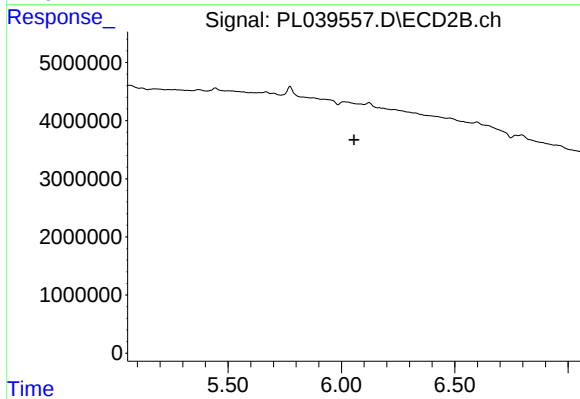

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.056 min
Response: 0
Conc: N.D.

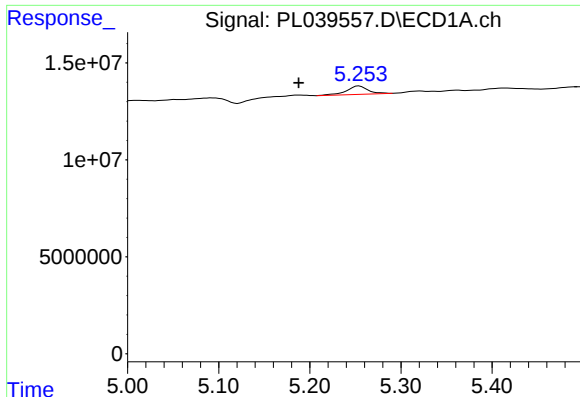

#25 Chlordane-3


R.T.: 5.254 min
Delta R.T.: 0.066 min
Response: 7035207
Conc: 6.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

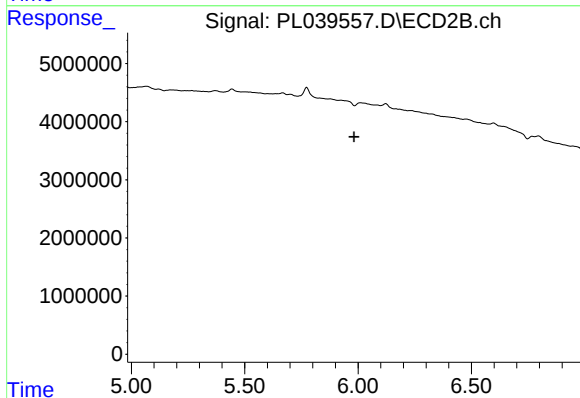


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

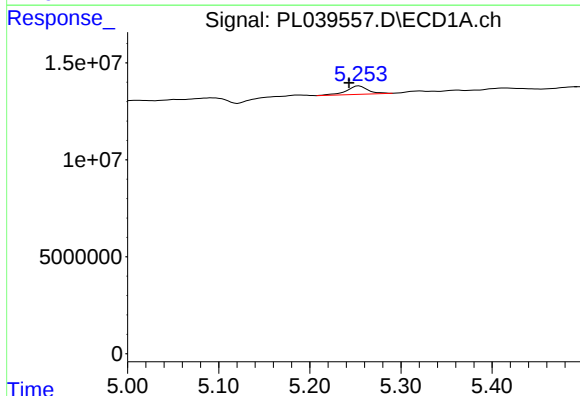


#26 Chlordane-4

R.T.: 5.254 min
Delta R.T.: 0.011 min
Response: 7035207
Conc: 7.04 ng/ml

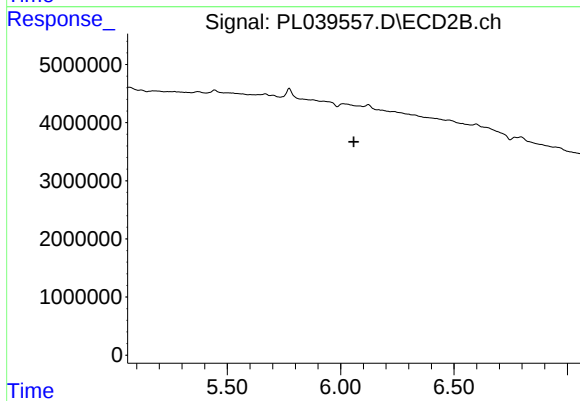

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.058 min
Response: 0
Conc: N.D.

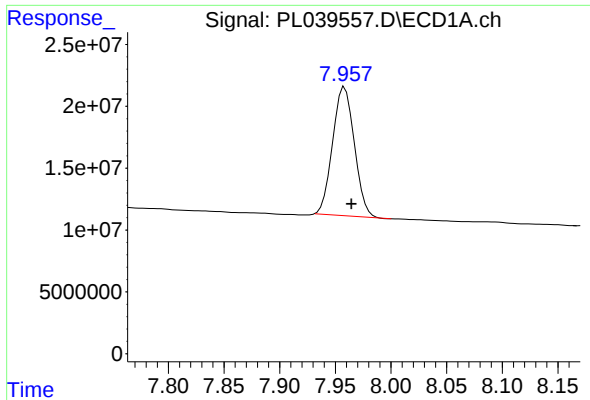

#28 Decachlorobiphenyl

R.T.: 7.958 min
Delta R.T.: -0.006 min
Response: 141043811
Conc: 20.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

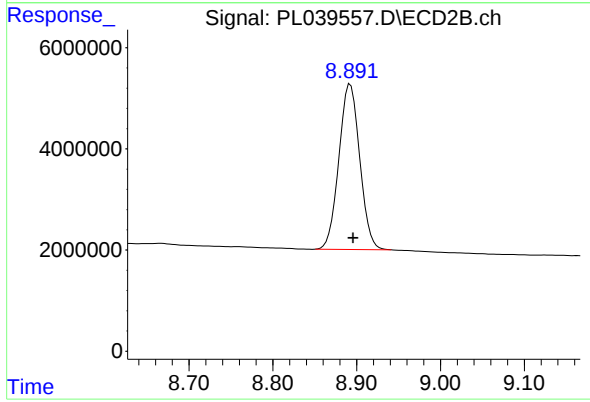

#28 Decachlorobiphenyl

R.T.: 8.892 min
Delta R.T.: -0.003 min
Response: 56593346
Conc: 24.39 ng/ml