

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082818\
 Data File : PL039560.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Aug 2018 15:16
 Operator : AJ\SJ
 Sample : J4277-09
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 29 00:59:00 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.302	3.905	96438637	40094292	13.796	14.956
28)	SA Decachlor...	7.957	8.892	92240674	42842610	13.133	18.462 #
Target Compounds							
2)	A alpha-BHC	3.686f	0.000	508292	0	0.043	N.D. #
3)	MA gamma-BHC...	3.959f	0.000	7824234	0	0.738	N.D. #
9)	A Endosulfan I	5.322	0.000	3178492	0	0.363	N.D. #
10)	B gamma-Chl...	5.200	0.000	19924460	0	2.017	N.D. #
11)	B alpha-Chl...	5.237	0.000	19482174	0	2.028	N.D. #
12)	B 4,4'-DDE	5.405	0.000	5154426	0	0.538	N.D. #
23)	Chlordane-1	4.142	0.000	9148006	0	28.896	N.D. #
24)	Chlordane-2	4.628	0.000	6888768	0	19.705	N.D. #
25)	Chlordane-3	5.200	0.000	19924460	0	18.241	N.D. #
26)	Chlordane-4	5.237	0.000	19482174	0	19.495	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082818\
Data File : PL039560.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Aug 2018 15:16
Operator : AJ\SJ
Sample : J4277-09
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 29 00:59:00 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

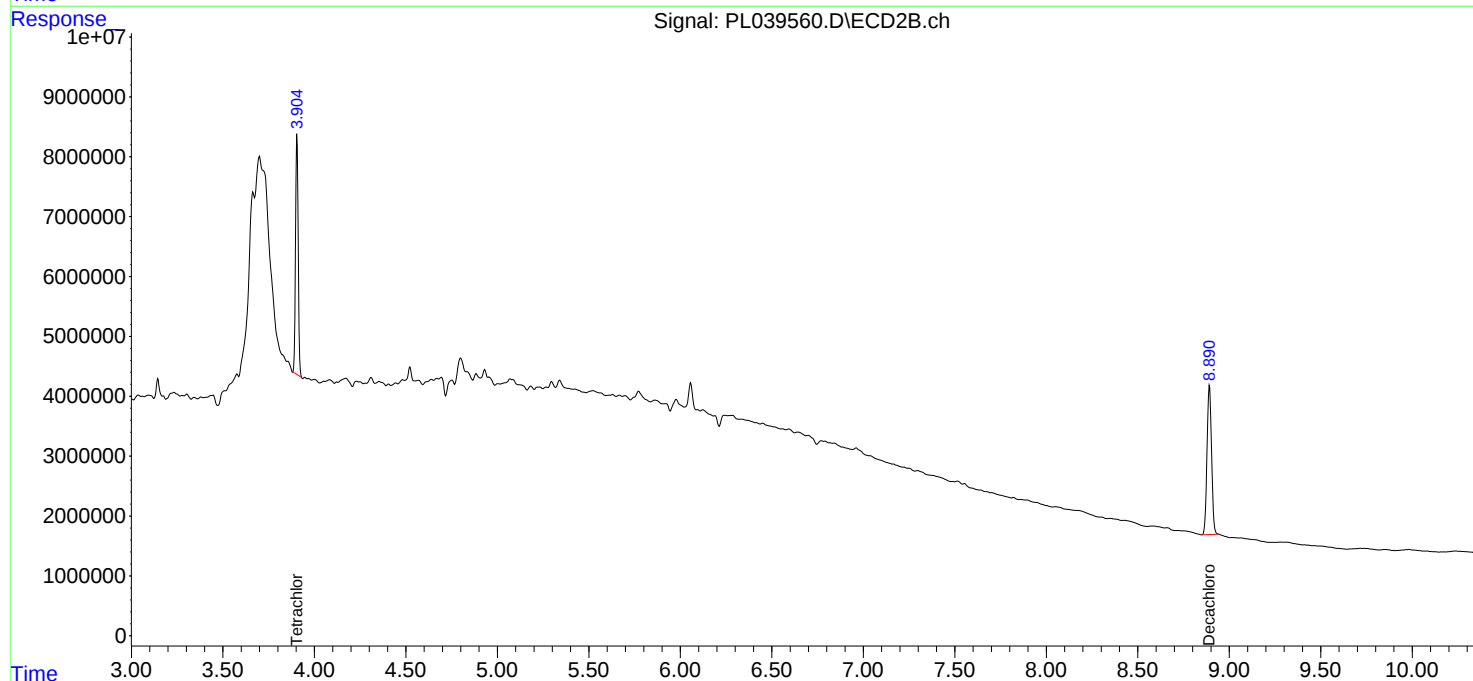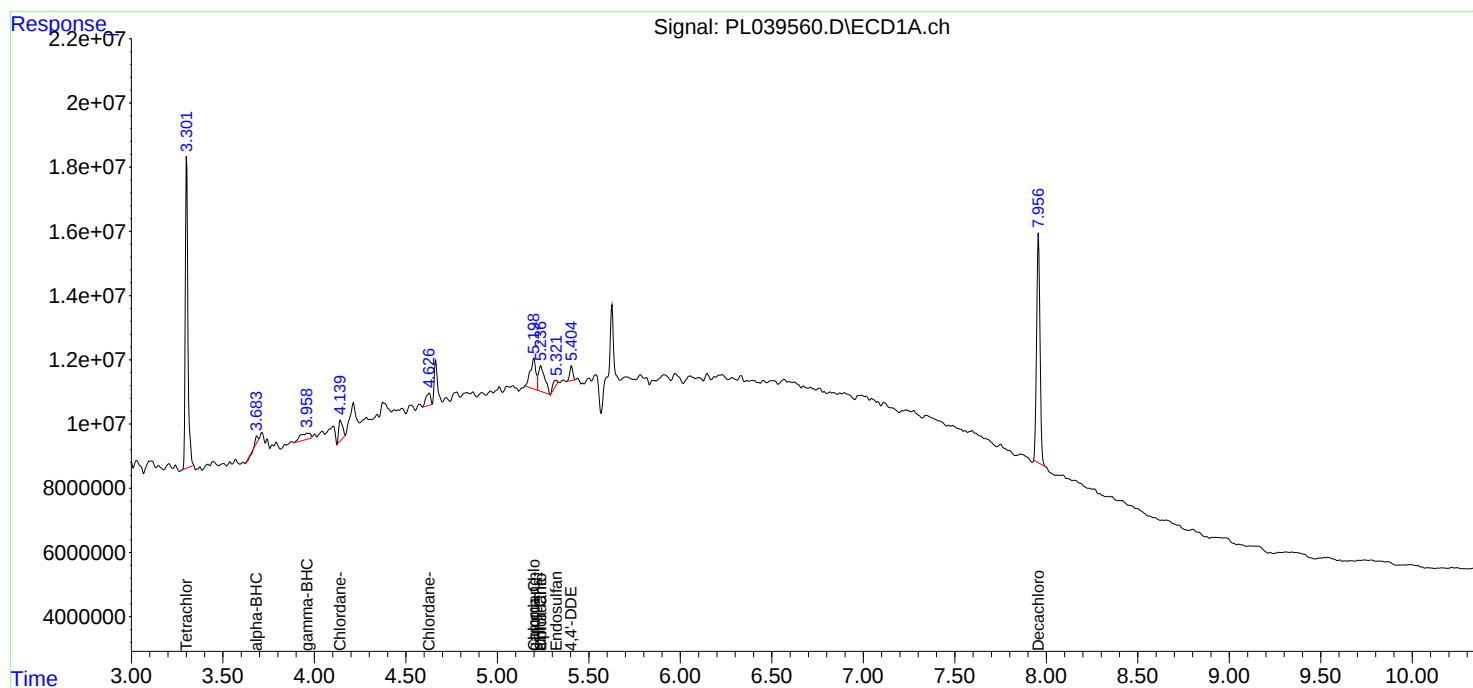


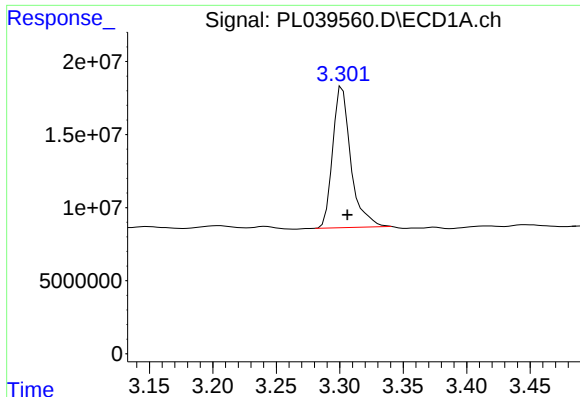

#1 Tetrachloro-m-xylene


R.T.: 3.302 min
Delta R.T.: -0.004 min
Response: 96438637
Conc: 13.80 ng/ml

Instrument :
ECD_L
ClientSampleId :

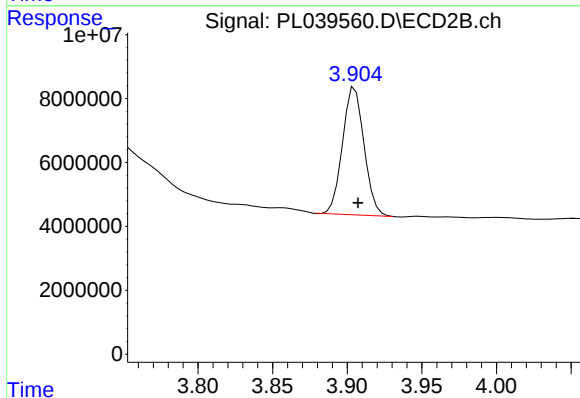


#1 Tetrachloro-m-xylene

R.T.: 3.905 min
Delta R.T.: -0.002 min
Response: 40094292
Conc: 14.96 ng/ml

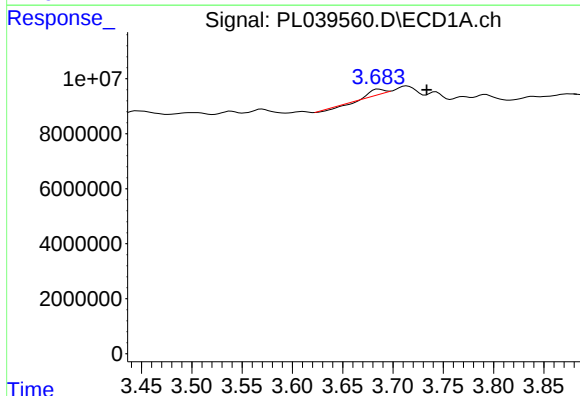


#2 alpha-BHC

R.T.: 3.686 min
Delta R.T.: -0.048 min
Response: 508292
Conc: 0.04 ng/ml

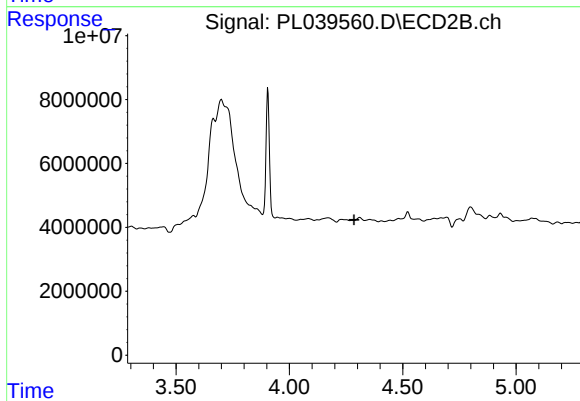

#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 4.285 min
Response: 0
Conc: N.D.

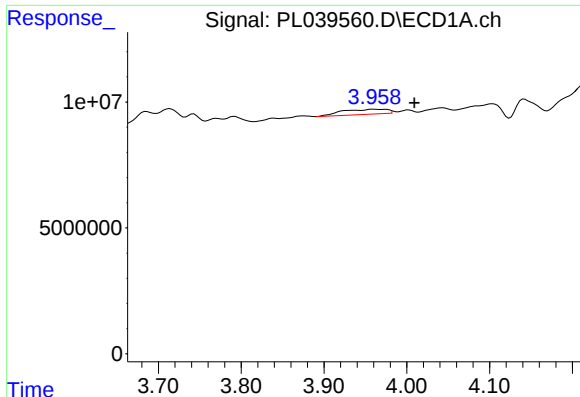

#3 gamma-BHC (Lindane)


R.T.: 3.959 min

Delta R.T.: -0.050 min

Response: 7824234

Conc: 0.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

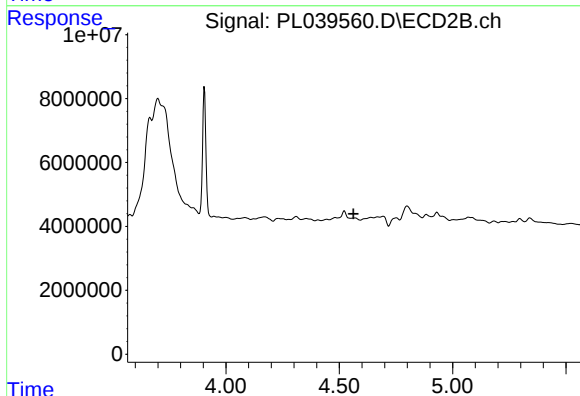


#3 gamma-BHC (Lindane)

R.T.: 0.000 min

Exp R.T. : 4.563 min

Response: 0

Conc: N.D.

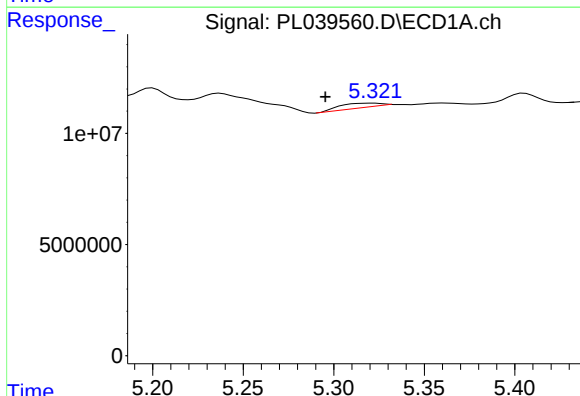


#9 Endosulfan I

R.T.: 5.322 min

Delta R.T.: 0.027 min

Response: 3178492

Conc: 0.36 ng/ml

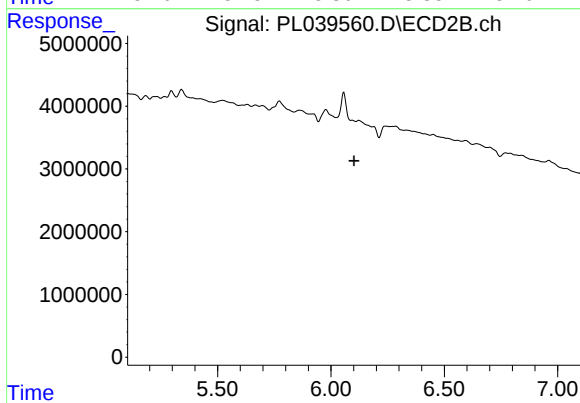


#9 Endosulfan I

R.T.: 0.000 min

Exp R.T. : 6.102 min

Response: 0


Conc: N.D.

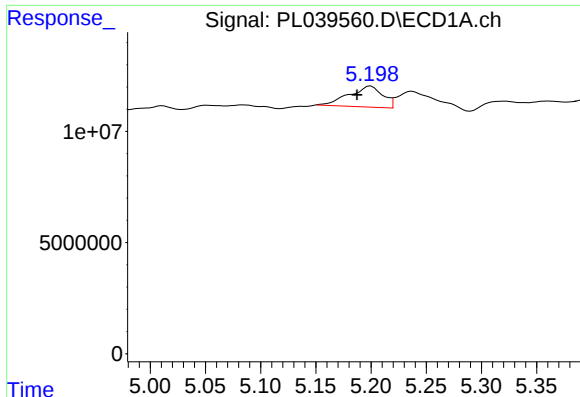

#10 gamma-Chlordane


R.T.: 5.200 min
Delta R.T.: 0.013 min
Response: 19924460
Conc: 2.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

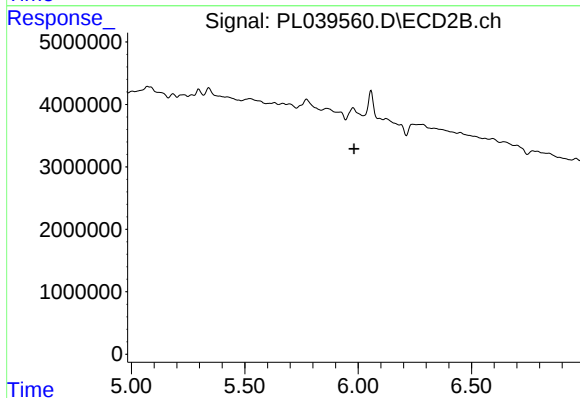


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

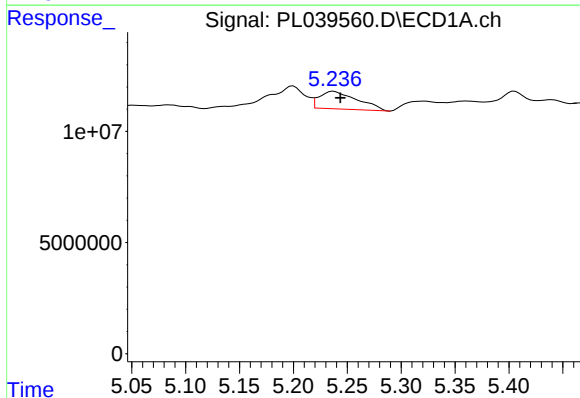


#11 alpha-Chlordane

R.T.: 5.237 min
Delta R.T.: -0.006 min
Response: 19482174
Conc: 2.03 ng/ml

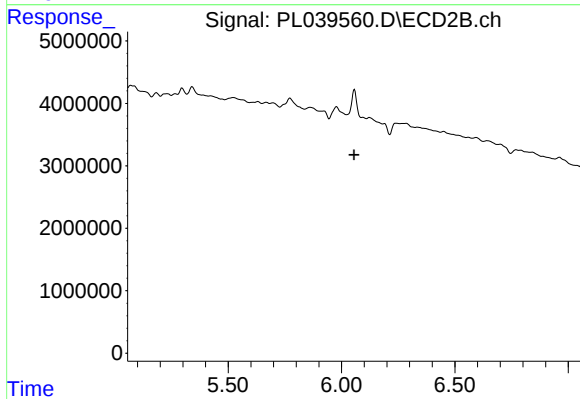

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.056 min
Response: 0
Conc: N.D.

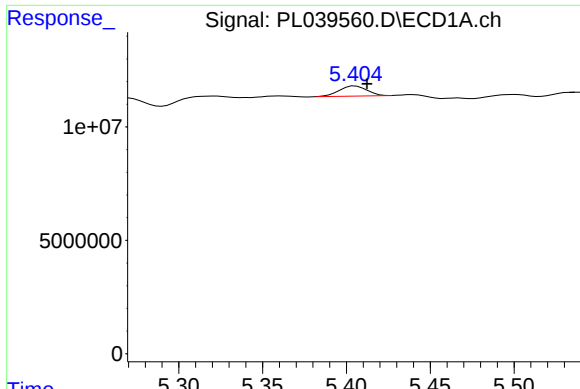

#12 4,4'-DDE


R.T.: 5.405 min
Delta R.T.: -0.007 min
Response: 5154426
Conc: 0.54 ng/ml

Instrument :
ECD_L
ClientSampleId :

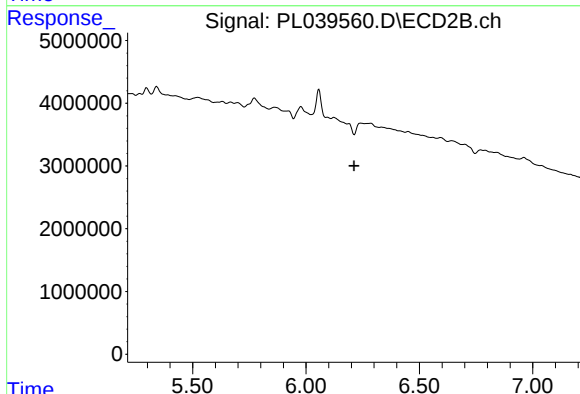


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.212 min
Response: 0
Conc: N.D.

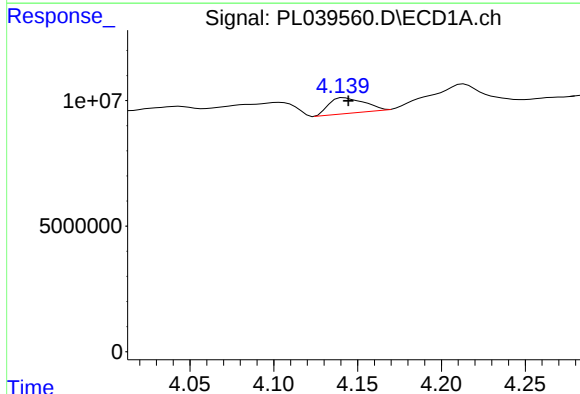


#23 Chlordane-1

R.T.: 4.142 min
Delta R.T.: -0.003 min
Response: 9148006
Conc: 28.90 ng/ml

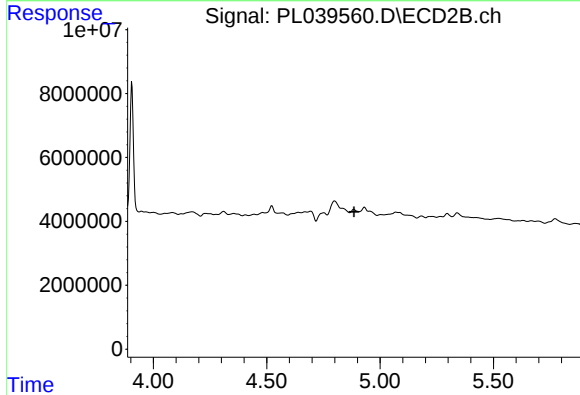

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.885 min
Response: 0
Conc: N.D.

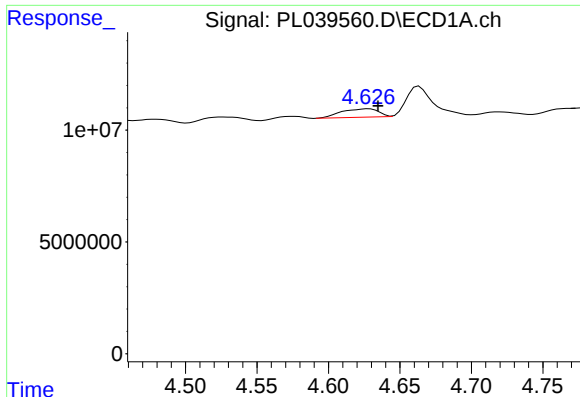

#24 Chlordane-2


R.T.: 4.628 min
Delta R.T.: -0.006 min
Response: 6888768
Conc: 19.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

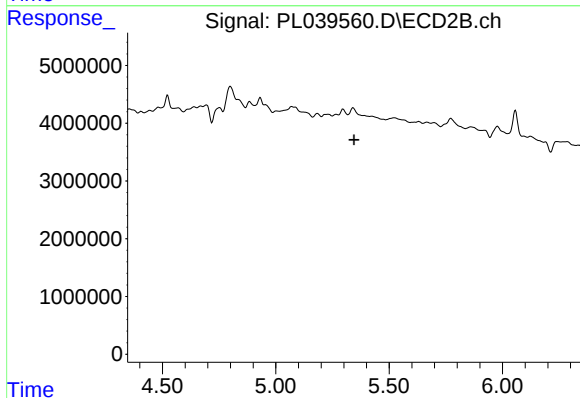


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.346 min
Response: 0
Conc: N.D.

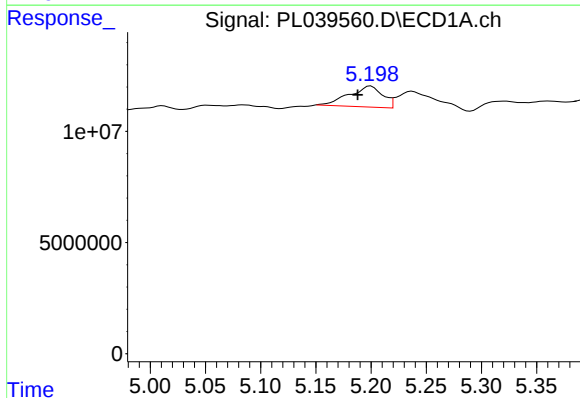


#25 Chlordane-3

R.T.: 5.200 min
Delta R.T.: 0.012 min
Response: 19924460
Conc: 18.24 ng/ml

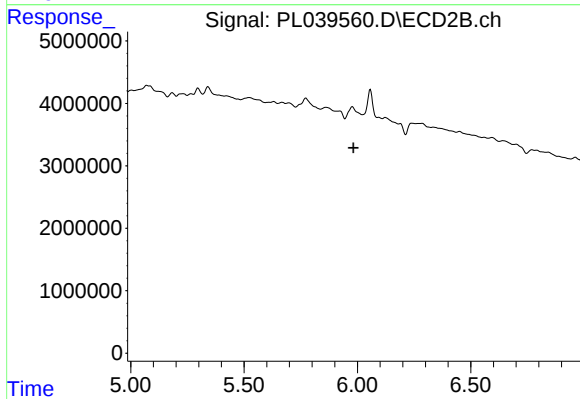

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

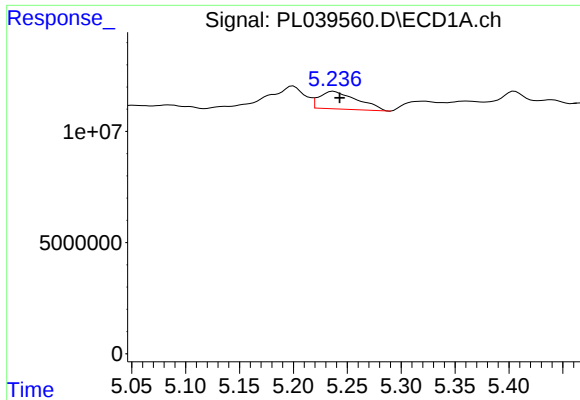

#26 Chlordane-4


R.T.: 5.237 min
Delta R.T.: -0.006 min
Response: 19482174
Conc: 19.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

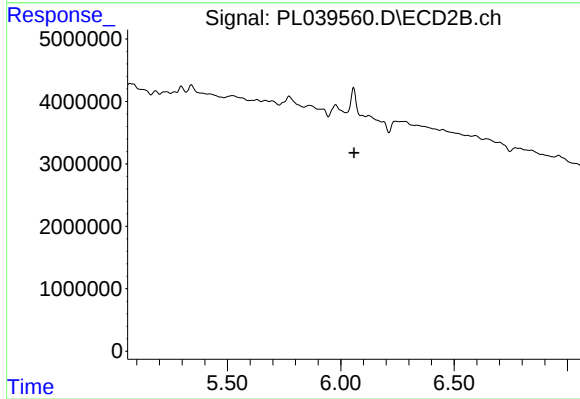


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.058 min
Response: 0
Conc: N.D.

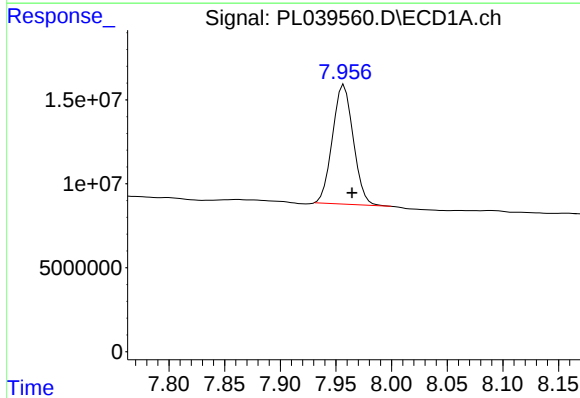

#28 Decachlorobiphenyl

R.T.: 7.957 min
Delta R.T.: -0.007 min
Response: 92240674
Conc: 13.13 ng/ml

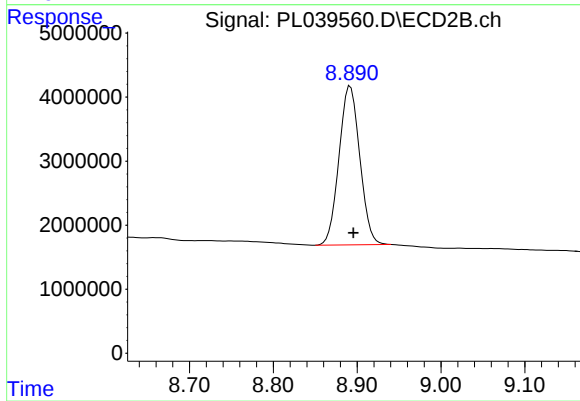

#28 Decachlorobiphenyl

R.T.: 8.892 min
Delta R.T.: -0.004 min
Response: 42842610
Conc: 18.46 ng/ml